

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 20:22
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 23:18:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 23 23:13:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.563	167.1E6	241.1E6	73.087	73.029
28)	SA Decachlor...	8.765	7.629	138.8E6	166.1E6	73.103	72.904
Target Compounds							
23)	Chlordane-1	4.466	3.528	71862085	76857134	729.265	730.370
24)	Chlordane-2	4.999	4.094	76003755	83361172	729.348	725.930
25)	Chlordane-3	5.708	4.713	315.5E6	246.0E6	731.802	729.043
26)	Chlordane-4	5.786	4.773	381.1E6	263.5E6	730.672	728.029
27)	Chlordane-5	6.642	5.434	62363892	67511016	731.393	730.467



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 20:22
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 23:18:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Wed Nov 23 23:13:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

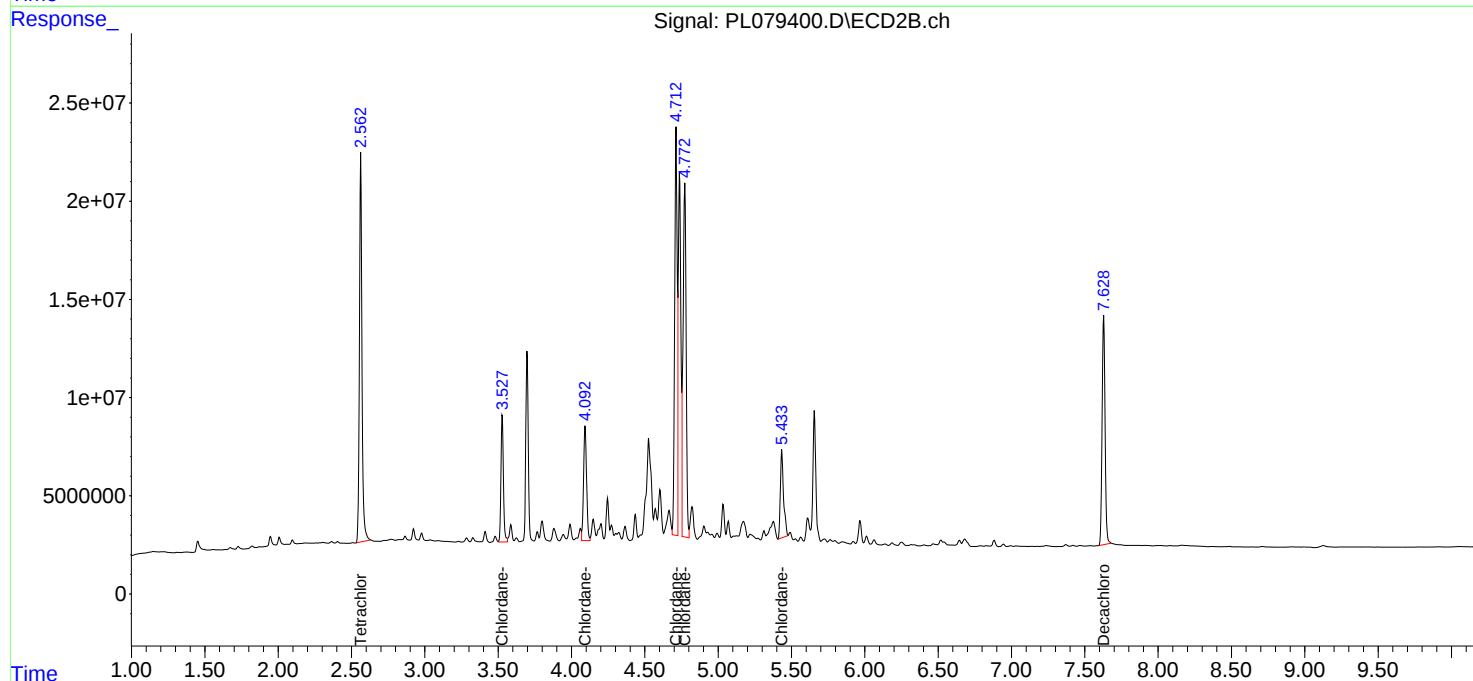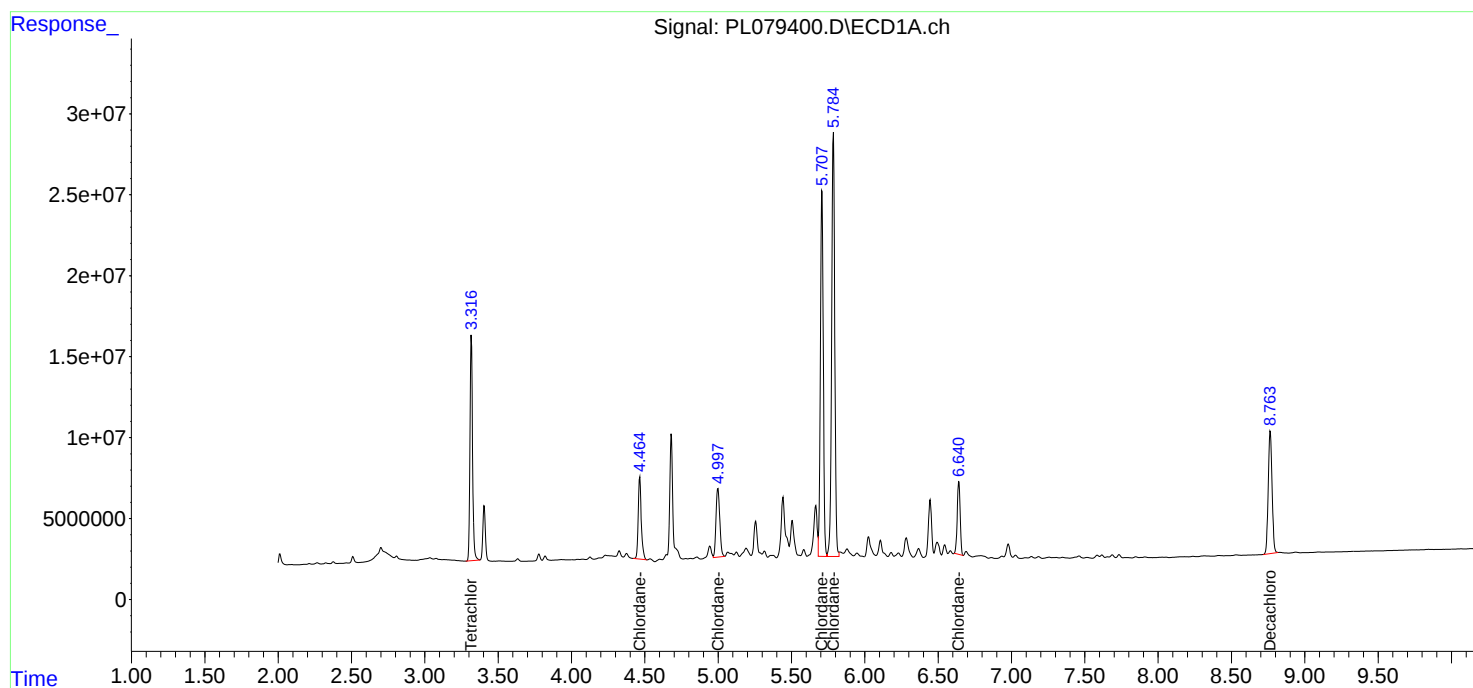


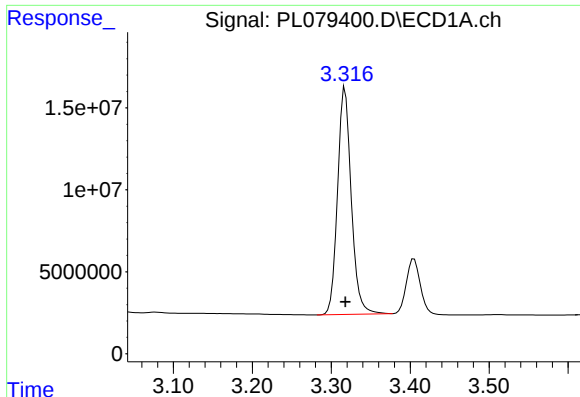

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 167086680
Conc: 73.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

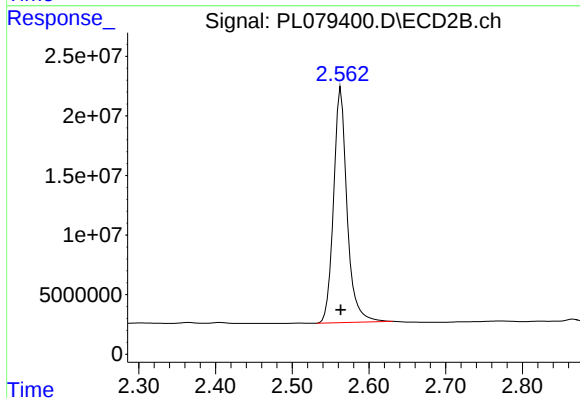


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 241059839
Conc: 73.03 ng/ml

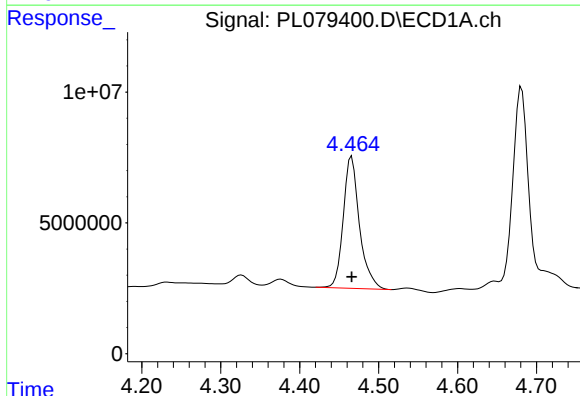


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 71862085
Conc: 729.26 ng/ml

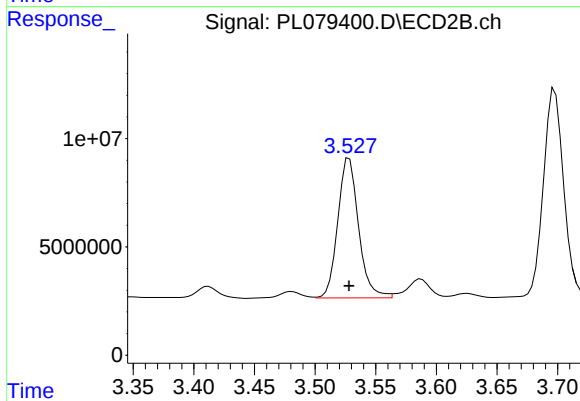

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 76857134
Conc: 730.37 ng/ml

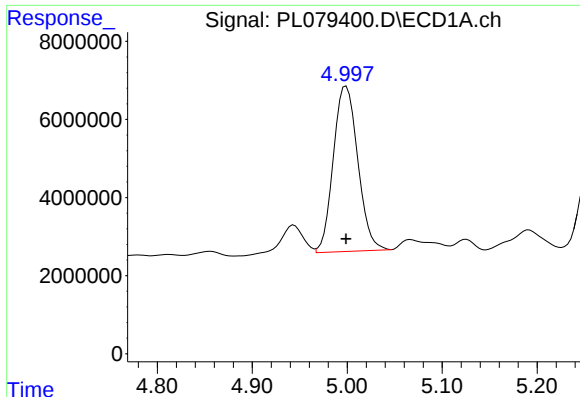

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 76003755
Conc: 729.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

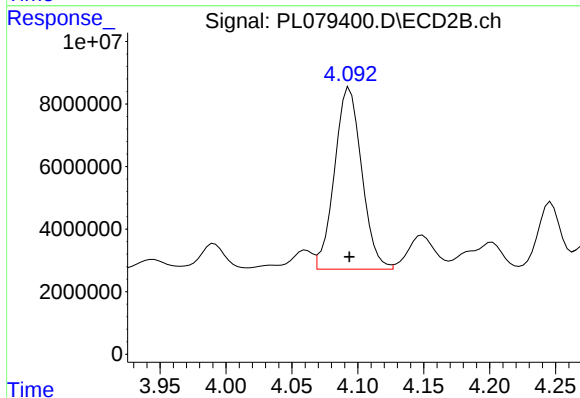


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 83361172
Conc: 725.93 ng/ml

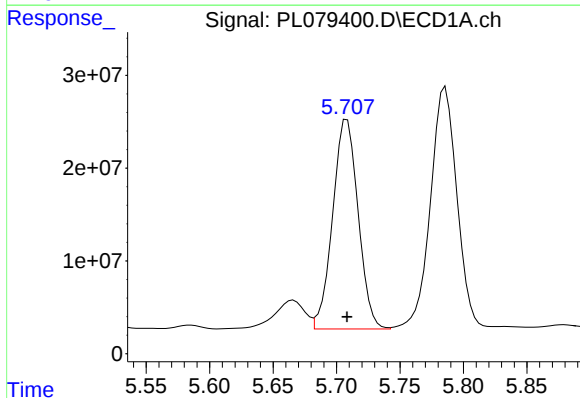


#25 Chlordane-3

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 315508468
Conc: 731.80 ng/ml

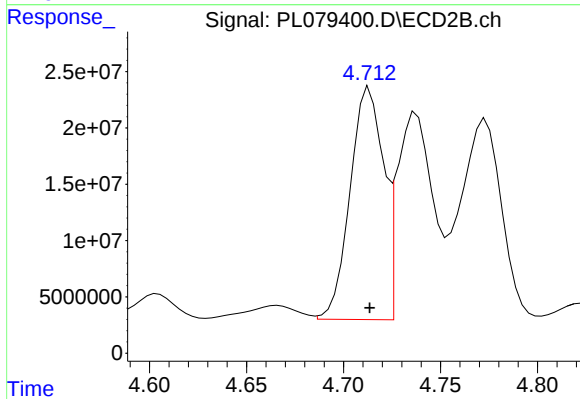

#25 Chlordane-3


R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 245958874
Conc: 729.04 ng/ml

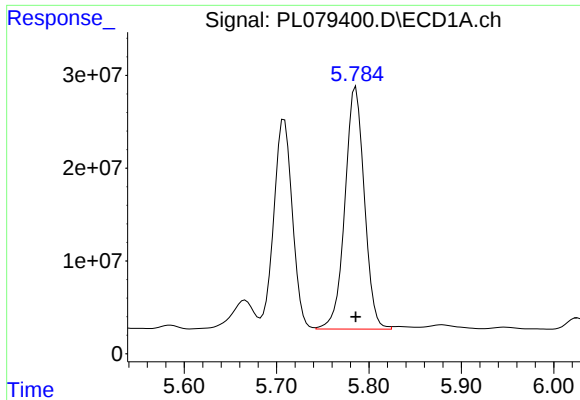

#26 Chlordane-4


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 381056267
Conc: 730.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

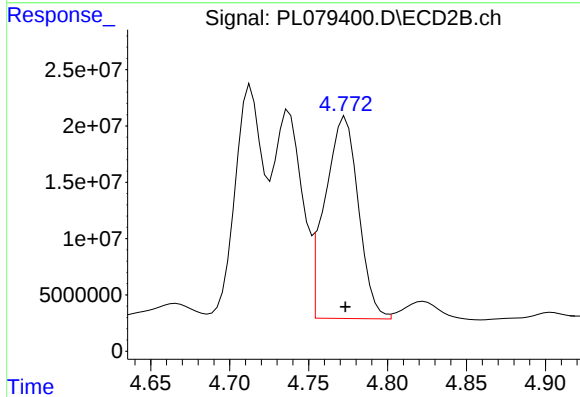


#26 Chlordane-4

R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 263538499
Conc: 728.03 ng/ml

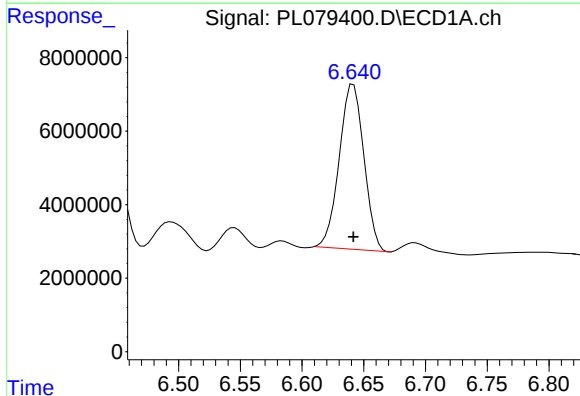


#27 Chlordane-5

R.T.: 6.642 min
Delta R.T.: 0.000 min
Response: 62363892
Conc: 731.39 ng/ml

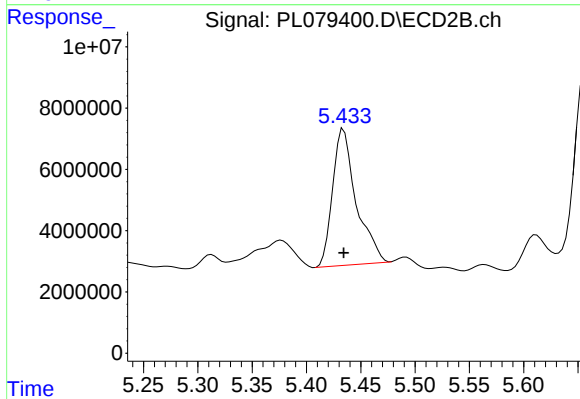

#27 Chlordane-5


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 67511016
Conc: 730.47 ng/ml

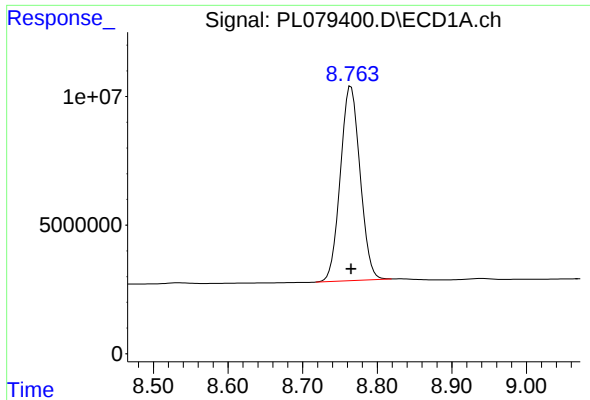

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 138807885
Conc: 73.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

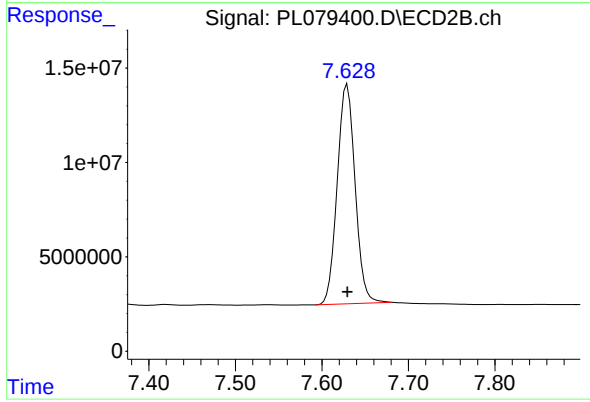

#28 Decachlorobiphenyl

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 166073669
Conc: 72.90 ng/ml