

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 20:36
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 23:14:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 23 23:13:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.563	113.8E6	166.0E6	50.000	50.000
28)	SA Decachlor...	8.765	7.630	97499641	117.7E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.465	3.528	49190961	53369941	500.000	500.000
24)	Chlordane-2	4.999	4.094	53371039	59416403	500.000	500.000
25)	Chlordane-3	5.709	4.713	212.7E6	170.4E6	500.000	500.000
26)	Chlordane-4	5.786	4.773	259.8E6	183.4E6	500.000	500.000
27)	Chlordane-5	6.642	5.434	42412551	47070936	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 20:36
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 23:14:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Wed Nov 23 23:13:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

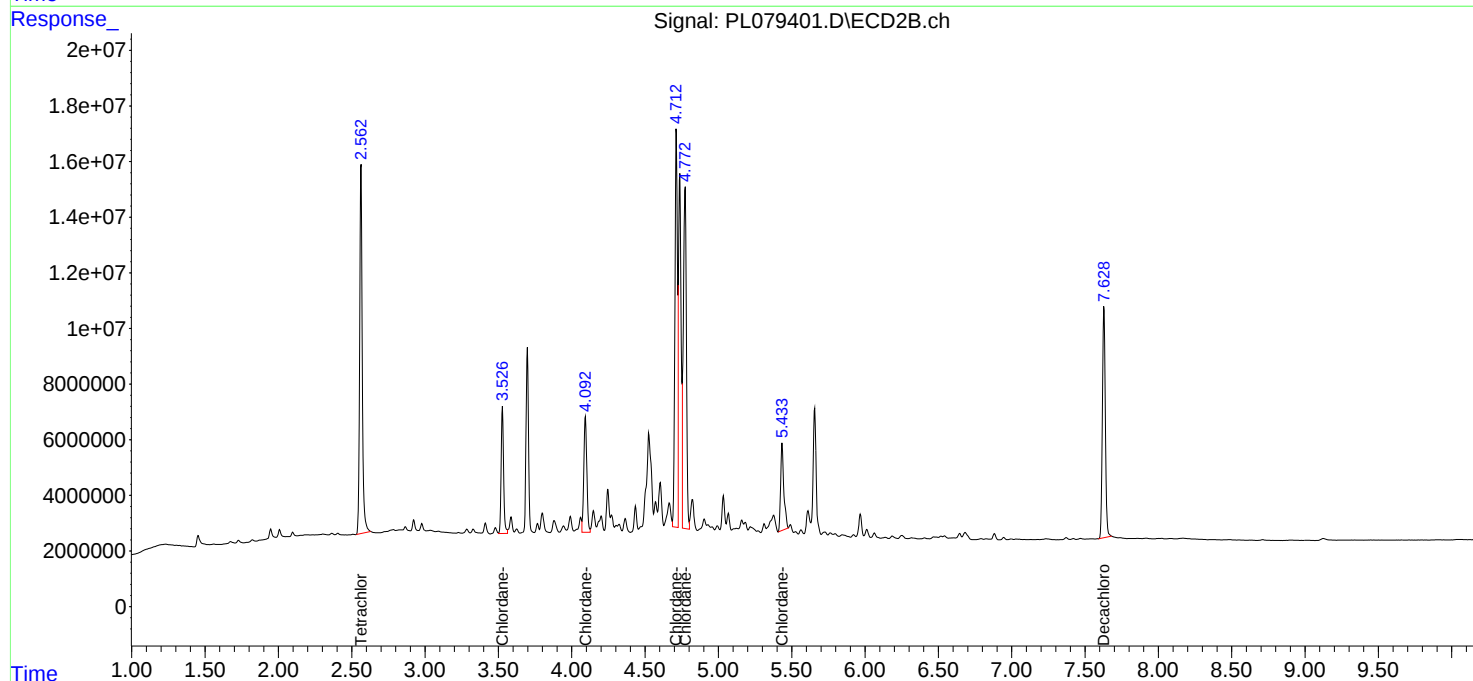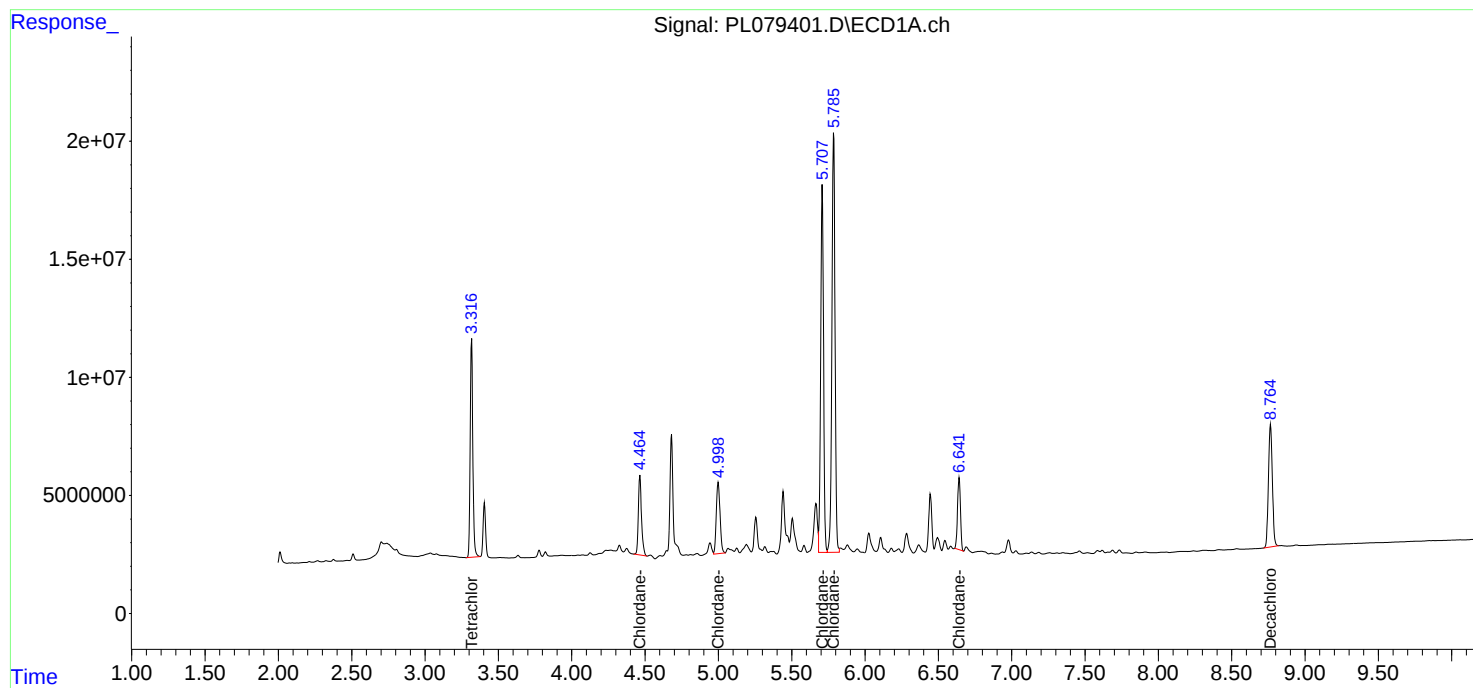


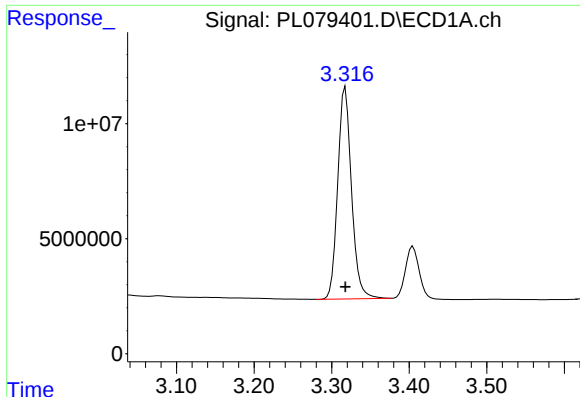

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 113759544
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

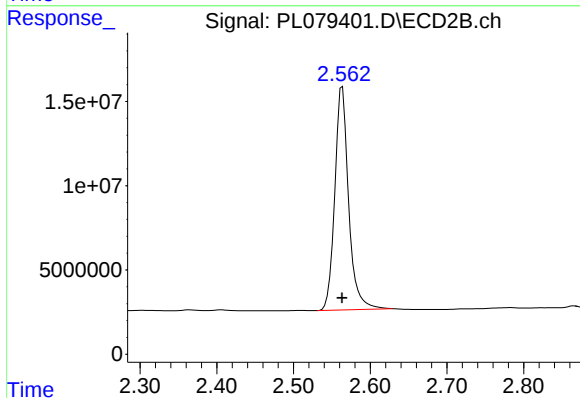


#1 Tetrachloro-m-xylene

R.T.: 2.563 min
Delta R.T.: 0.000 min
Response: 166019208
Conc: 50.00 ng/ml

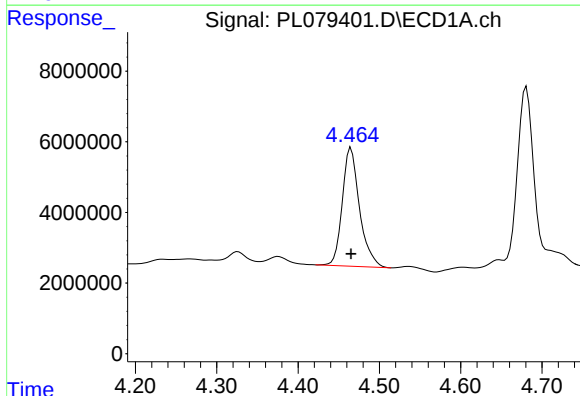


#23 Chlordane-1

R.T.: 4.465 min
Delta R.T.: 0.000 min
Response: 49190961
Conc: 500.00 ng/ml

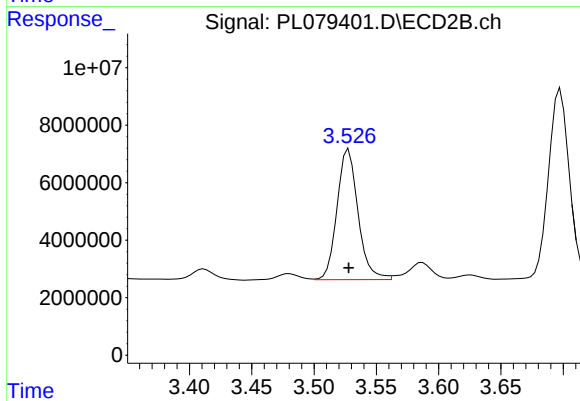

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 53369941
Conc: 500.00 ng/ml

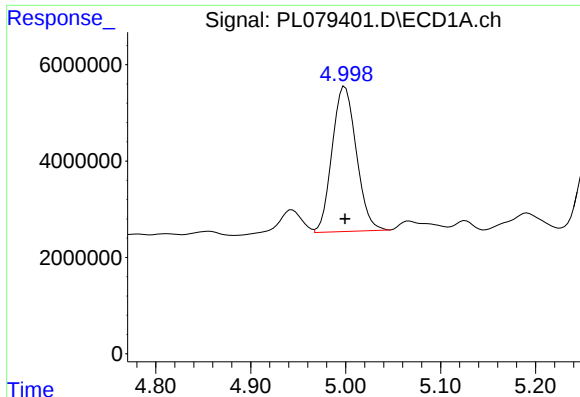

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 53371039
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

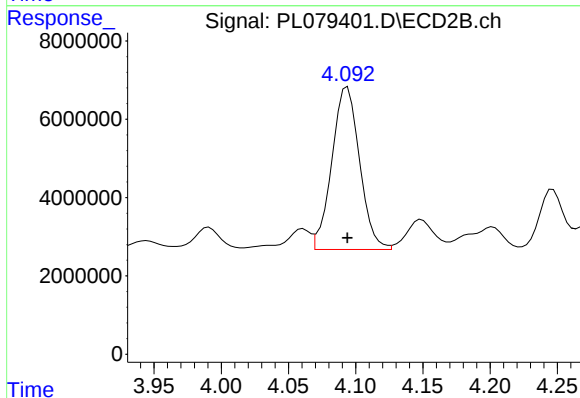


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 59416403
Conc: 500.00 ng/ml

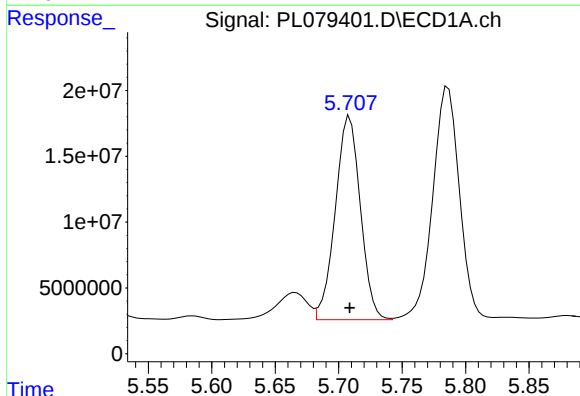


#25 Chlordane-3

R.T.: 5.709 min
Delta R.T.: 0.000 min
Response: 212747527
Conc: 500.00 ng/ml

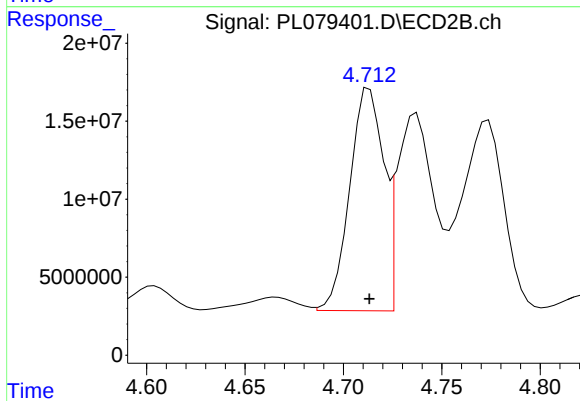

#25 Chlordane-3


R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 170438845
Conc: 500.00 ng/ml

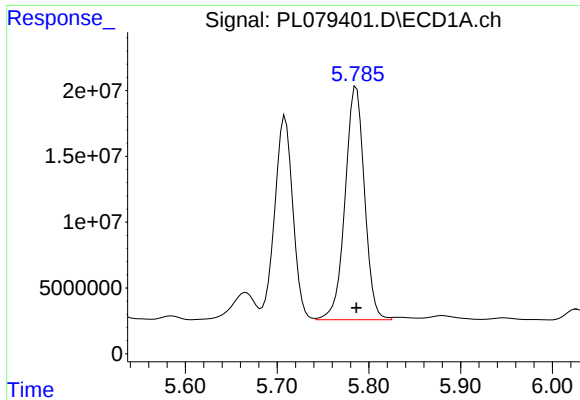

#26 Chlordane-4


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 259834284
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

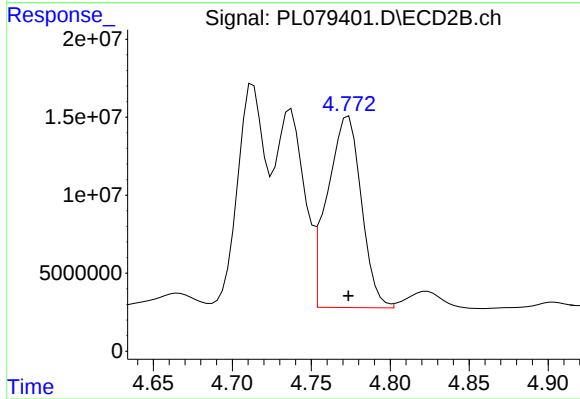


#26 Chlordane-4

R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 183418490
Conc: 500.00 ng/ml

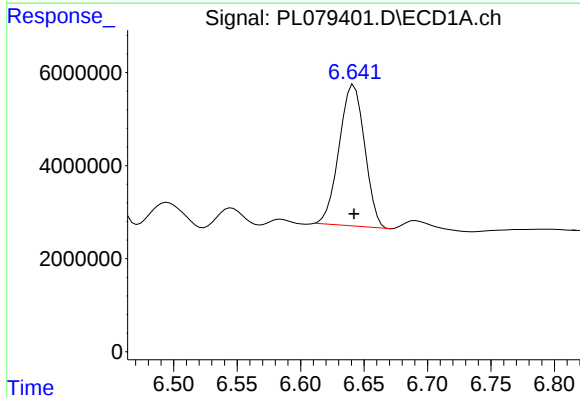


#27 Chlordane-5

R.T.: 6.642 min
Delta R.T.: 0.000 min
Response: 42412551
Conc: 500.00 ng/ml

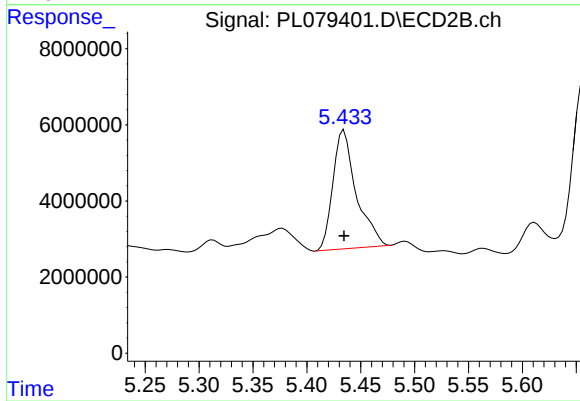

#27 Chlordane-5


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 47070936
Conc: 500.00 ng/ml

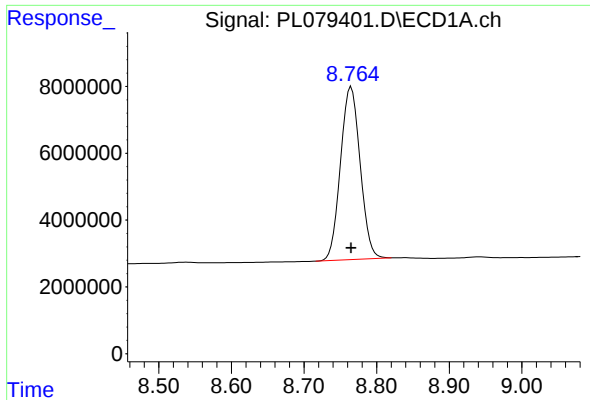

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 97499641
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

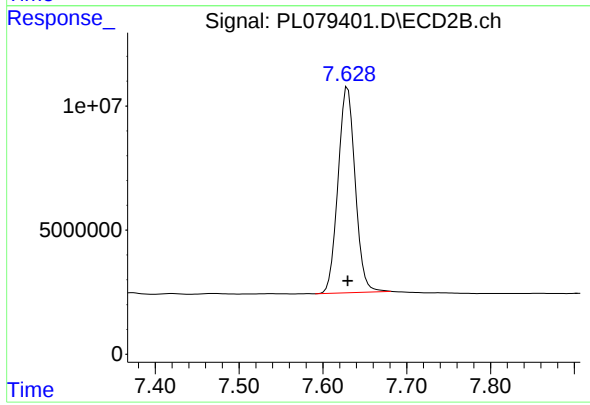

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 117749475
Conc: 50.00 ng/ml