

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 20:50
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 23:20:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 23 23:13:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.564	53992555	79541954	23.948	24.317
28)	SA Decachlor...	8.765	7.630	47584109	58592091	25.045	25.537
Target Compounds							
23)	Chlordane-1	4.466	3.528	23170408	26212186	238.684	249.319
24)	Chlordane-2	4.998	4.094	26131721	30141274	250.574	259.243
25)	Chlordane-3	5.708	4.713	97782817	81519317	232.187	243.670
26)	Chlordane-4	5.786	4.773	121.3E6	88592386	236.657	246.033
27)	Chlordane-5	6.641	5.434	19566145	22519179	234.278	245.212



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 20:50
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 23:20:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Wed Nov 23 23:13:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

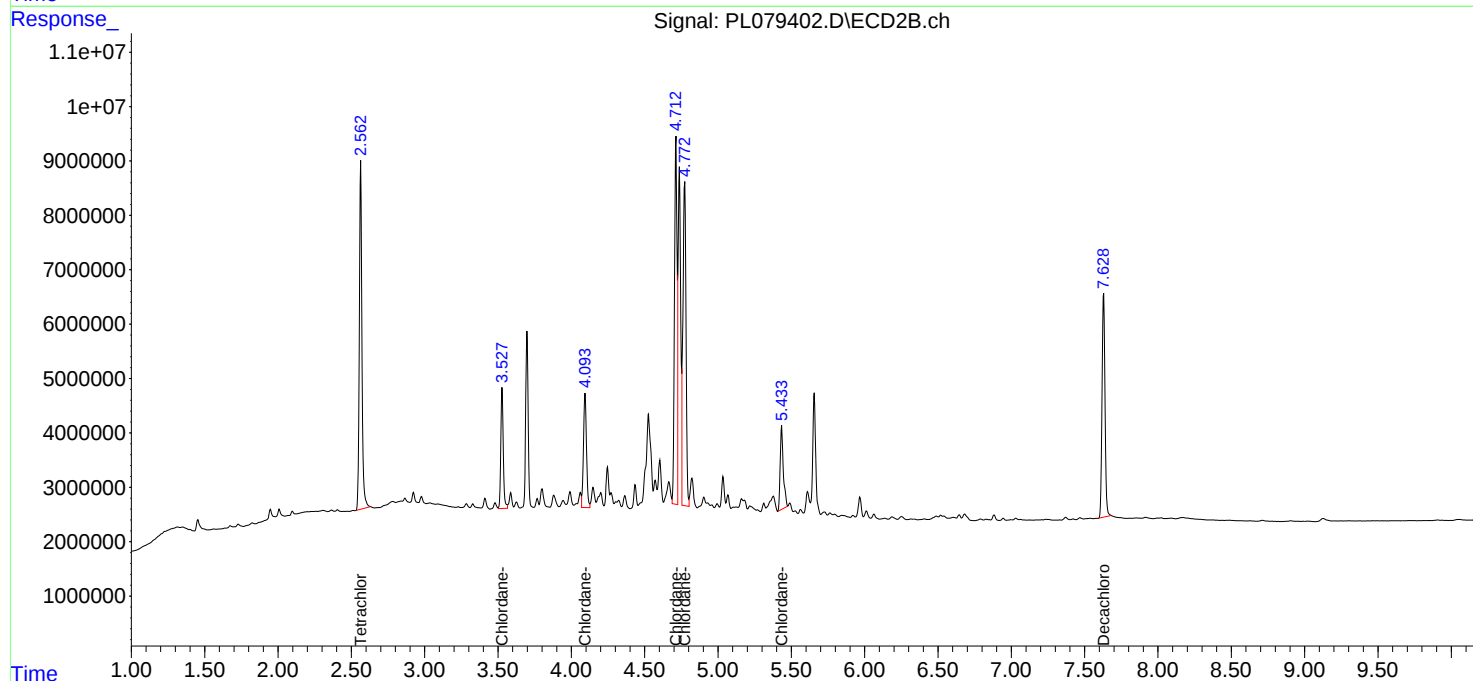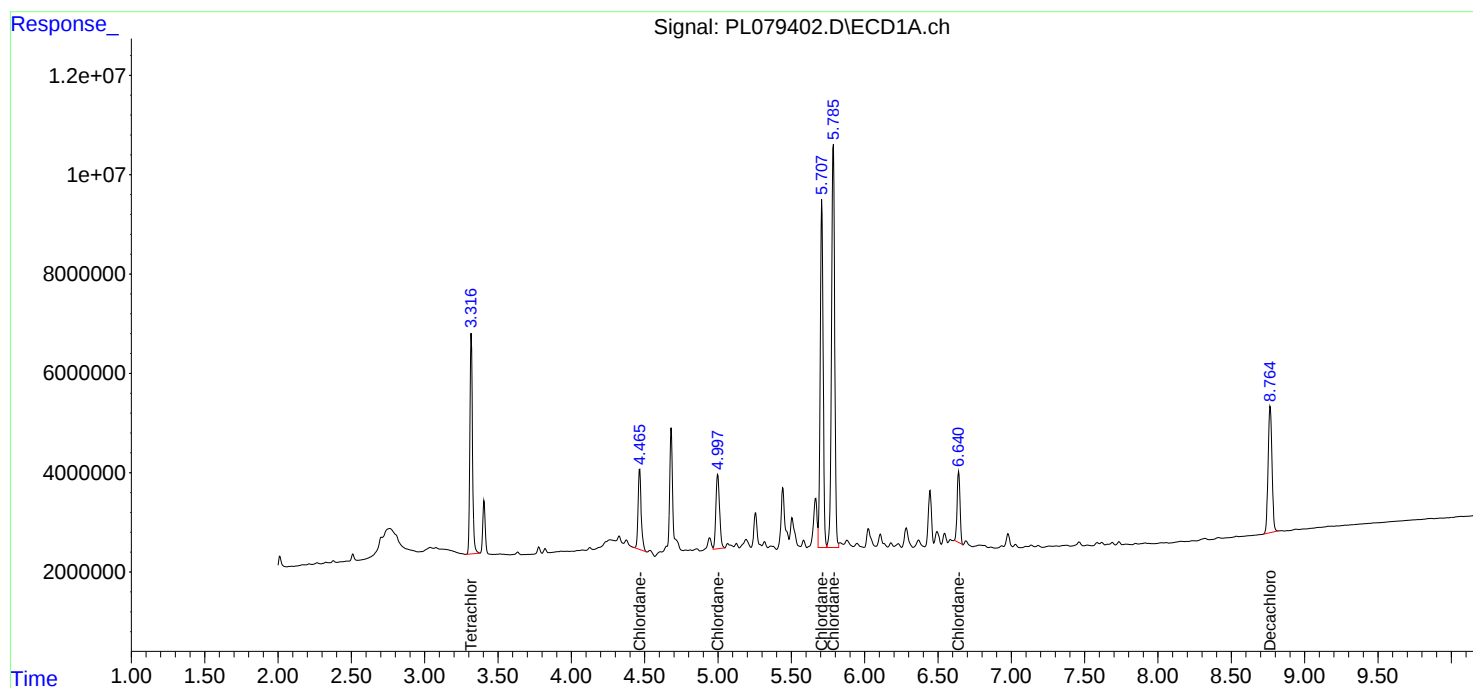


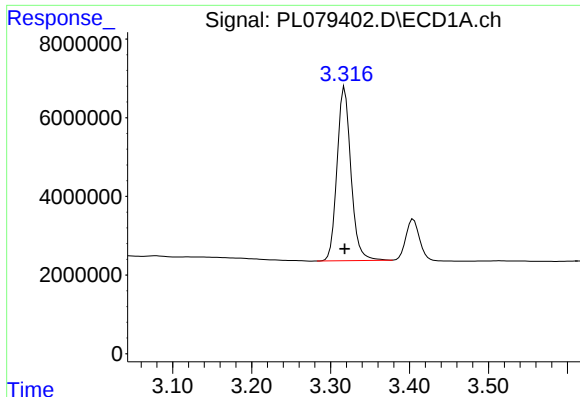

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 53992555
Conc: 23.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

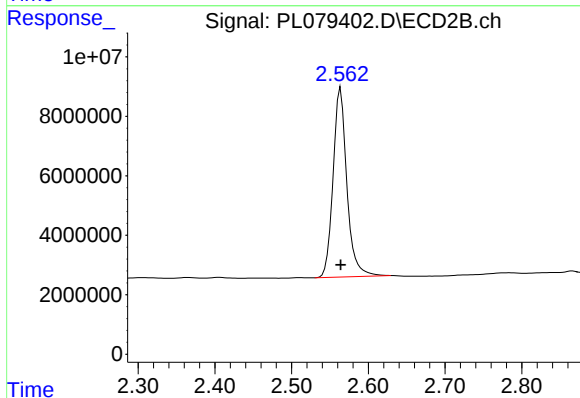


#1 Tetrachloro-m-xylene

R.T.: 2.564 min
Delta R.T.: 0.000 min
Response: 79541954
Conc: 24.32 ng/ml

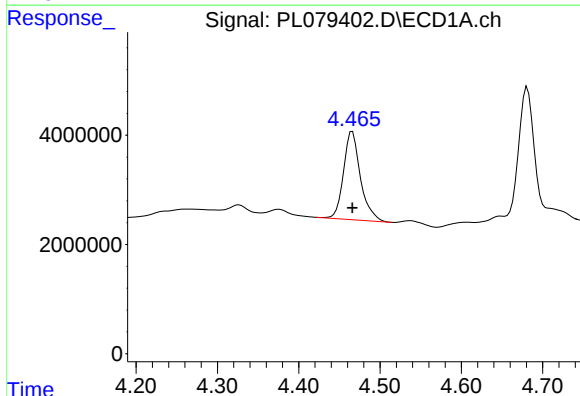


#23 Chlordane-1

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 23170408
Conc: 238.68 ng/ml

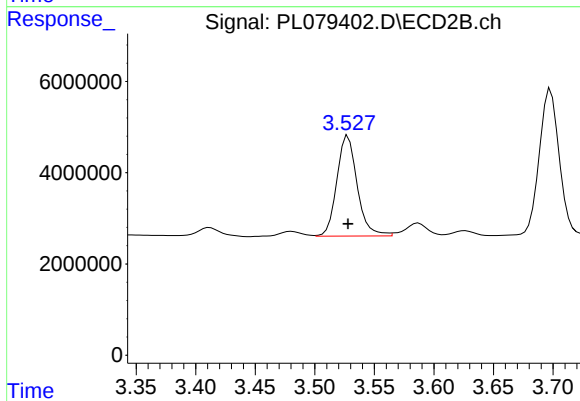

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 26212186
Conc: 249.32 ng/ml

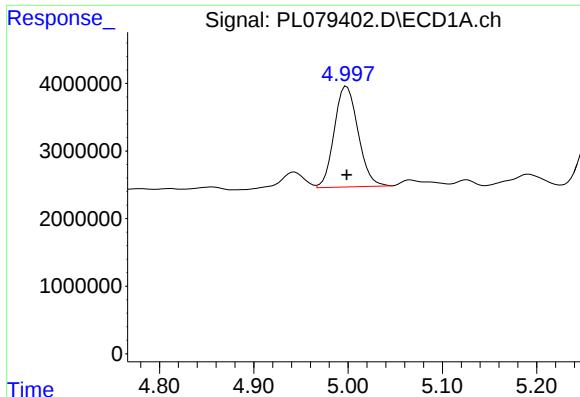

#24 Chlordane-2


R.T.: 4.998 min
Delta R.T.: 0.000 min
Response: 26131721
Conc: 250.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

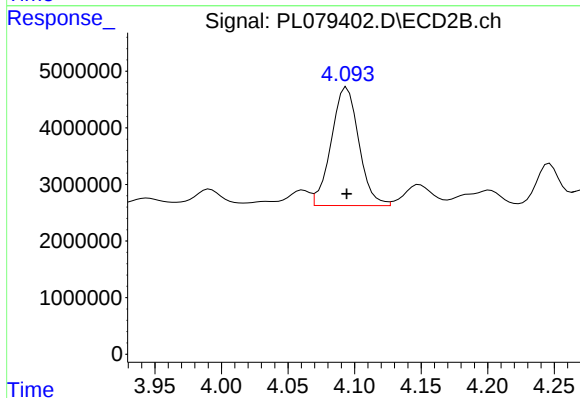


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.000 min
Response: 30141274
Conc: 259.24 ng/ml

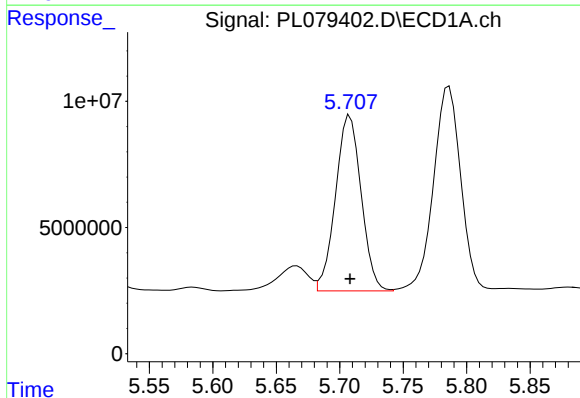


#25 Chlordane-3

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 97782817
Conc: 232.19 ng/ml

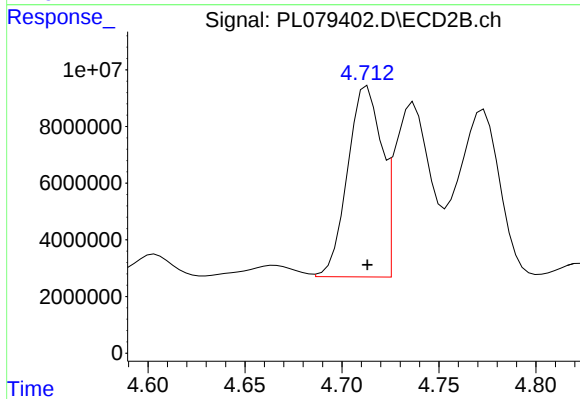

#25 Chlordane-3


R.T.: 4.713 min
Delta R.T.: 0.000 min
Response: 81519317
Conc: 243.67 ng/ml

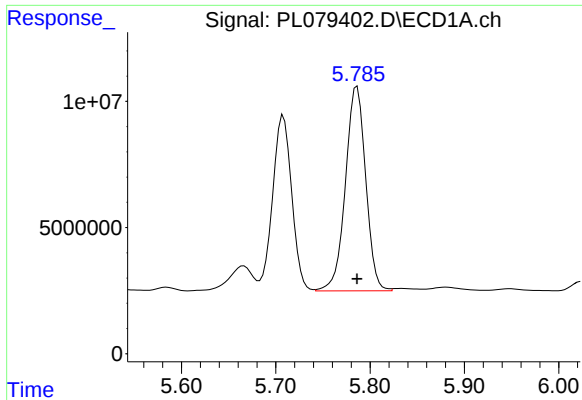

#26 Chlordane-4


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 121263131
Conc: 236.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

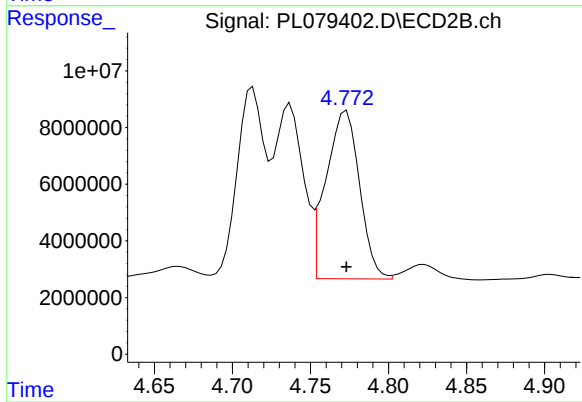


#26 Chlordane-4

R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 88592386
Conc: 246.03 ng/ml

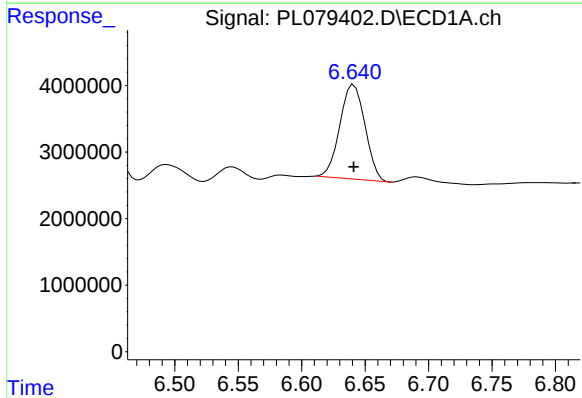


#27 Chlordane-5

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 19566145
Conc: 234.28 ng/ml

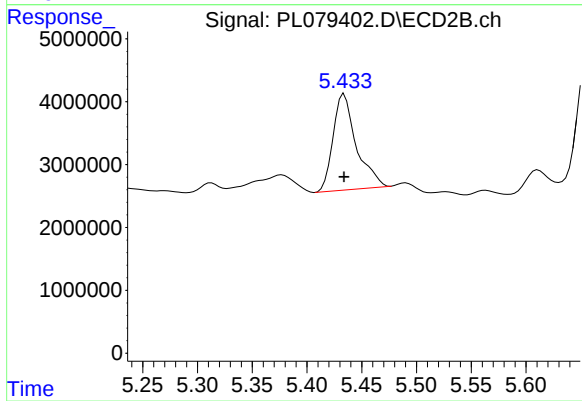

#27 Chlordane-5


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 22519179
Conc: 245.21 ng/ml

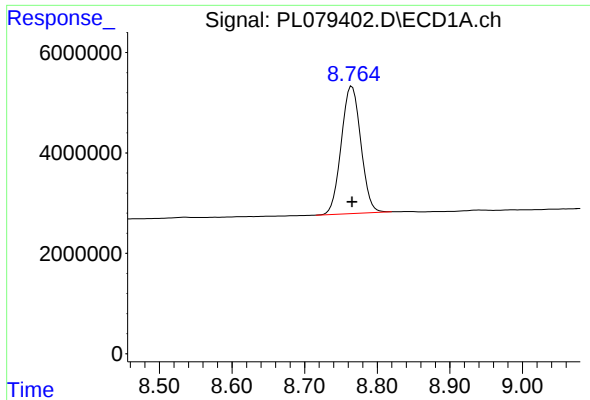

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 47584109
Conc: 25.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

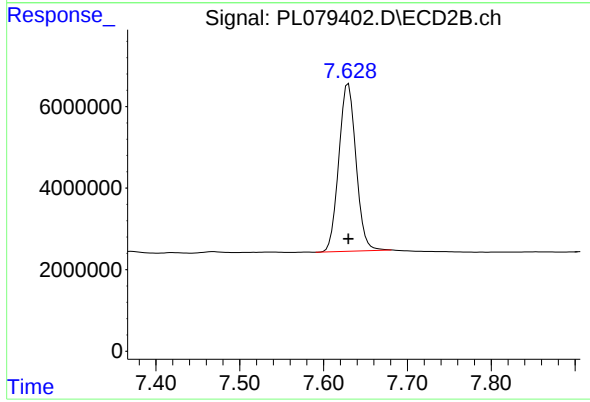

#28 Decachlorobiphenyl

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 58592091
Conc: 25.54 ng/ml