

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
 Data File : PL079410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 23:08
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL112322CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 23:25:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 23 23:23:32 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	2.564	115.2E6	164.3E6	51.747	50.563
28)	SA Decachlor...	8.765	7.629	97642731	115.5E6	51.101	49.116
Target Compounds							
23)	Chlordane-1	4.465	3.528	49609387	52680551	525.891	495.308
24)	Chlordane-2	4.997	4.094	53698235	58390145	509.602	498.709
25)	Chlordane-3	5.708	4.714	213.8E6	166.5E6	514.969	497.962
26)	Chlordane-4	5.786	4.774	257.5E6	180.0E6	506.051	496.839
27)	Chlordane-5	6.641	5.434	42583158	46268221	532.472	514.679



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112322\
Data File : PL079410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 23:08
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL112322CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 23:25:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112322.M
Quant Title : GC Extractables
QLast Update : Wed Nov 23 23:23:32 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

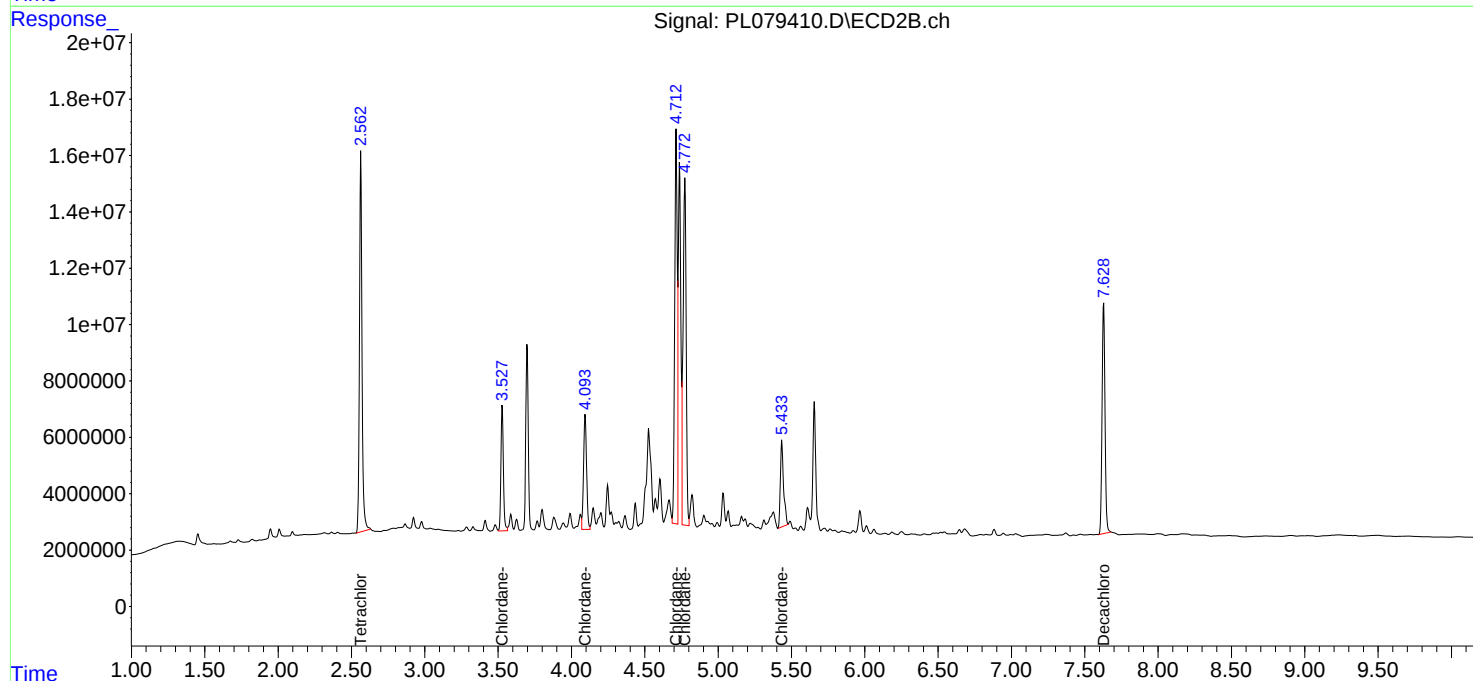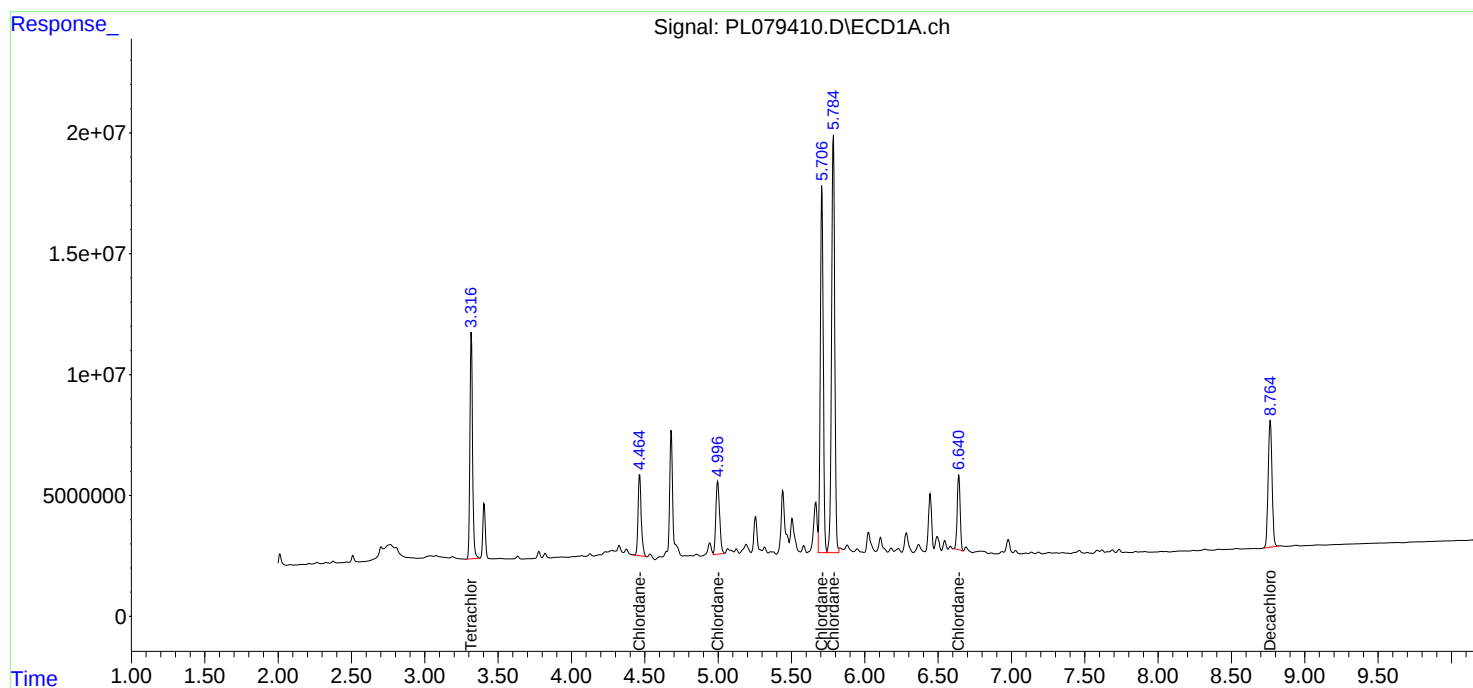


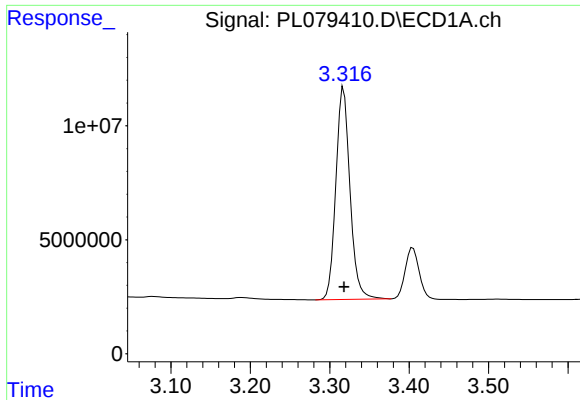

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 115208634
Conc: 51.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112322CHLOR

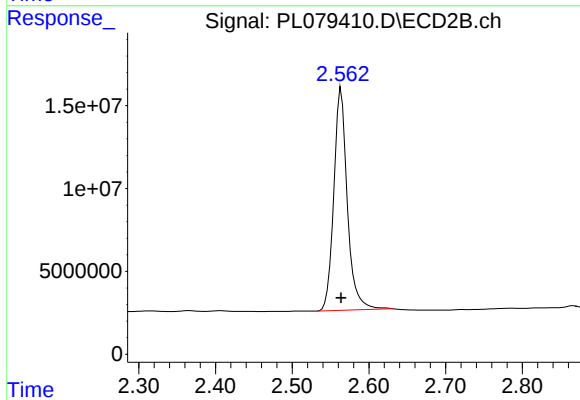


#1 Tetrachloro-m-xylene

R.T.: 2.564 min
Delta R.T.: 0.000 min
Response: 164252704
Conc: 50.56 ng/ml

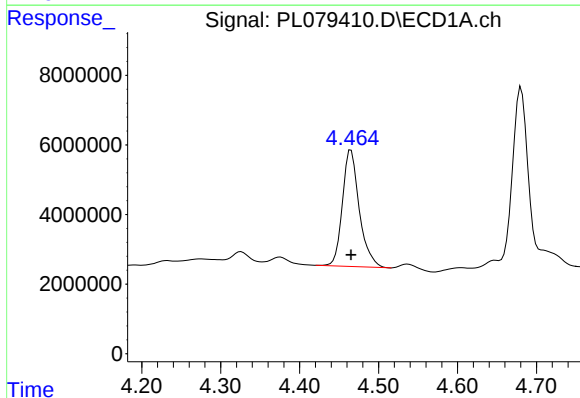


#23 Chlordane-1

R.T.: 4.465 min
Delta R.T.: 0.000 min
Response: 49609387
Conc: 525.89 ng/ml

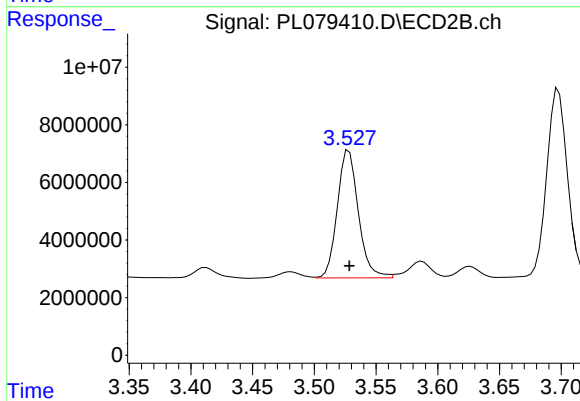

#23 Chlordane-1


R.T.: 3.528 min
Delta R.T.: 0.000 min
Response: 52680551
Conc: 495.31 ng/ml

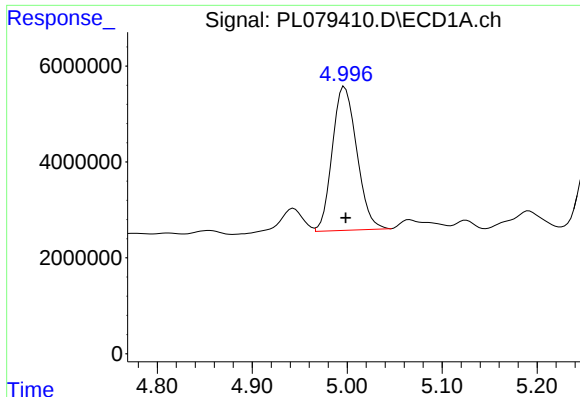

#24 Chlordane-2


R.T.: 4.997 min
Delta R.T.: -0.001 min
Response: 53698235
Conc: 509.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112322CHLOR

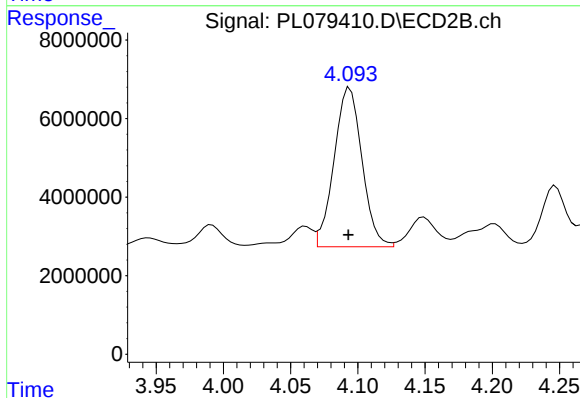


#24 Chlordane-2

R.T.: 4.094 min
Delta R.T.: 0.001 min
Response: 58390145
Conc: 498.71 ng/ml

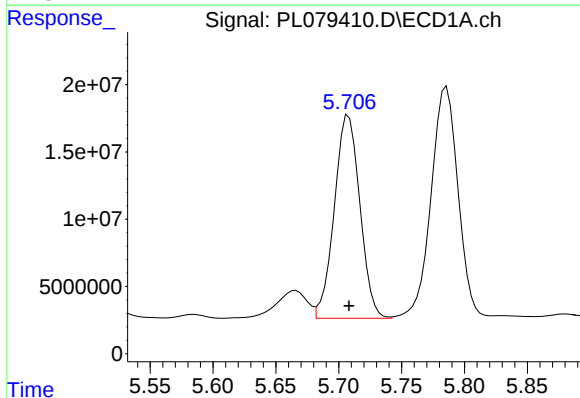


#25 Chlordane-3

R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 213830056
Conc: 514.97 ng/ml

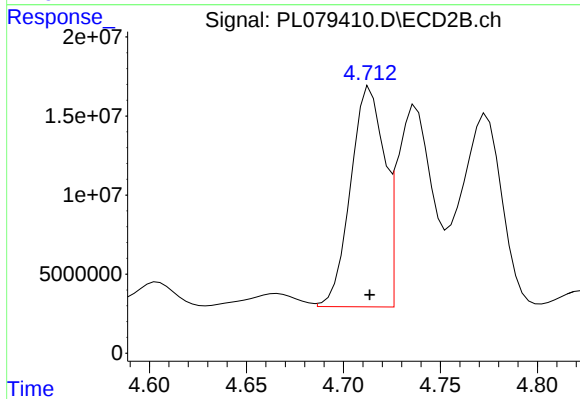

#25 Chlordane-3


R.T.: 4.714 min
Delta R.T.: 0.000 min
Response: 166470570
Conc: 497.96 ng/ml

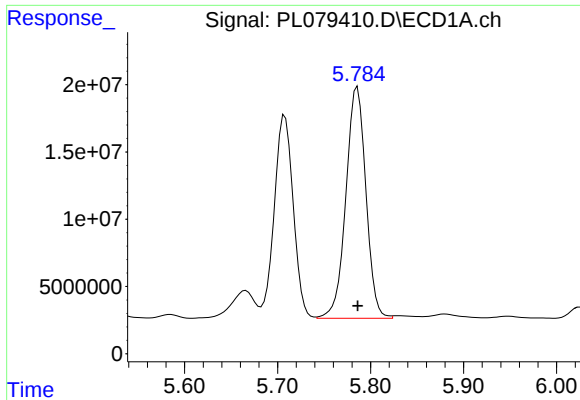

#26 Chlordane-4


R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 257474954
Conc: 506.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112322CHLOR

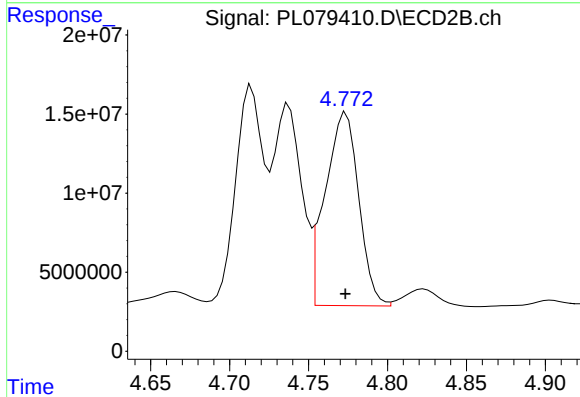


#26 Chlordane-4

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 180036240
Conc: 496.84 ng/ml

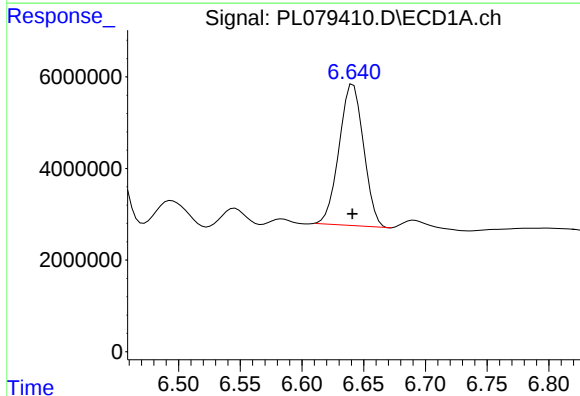


#27 Chlordane-5

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 42583158
Conc: 532.47 ng/ml

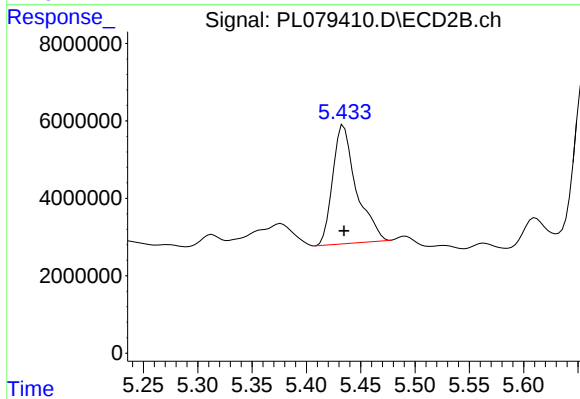

#27 Chlordane-5


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 46268221
Conc: 514.68 ng/ml

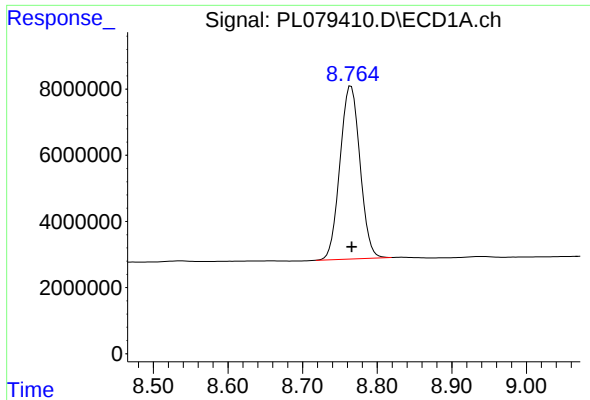

#28 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.000 min
Response: 97642731
Conc: 51.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112322CHLOR

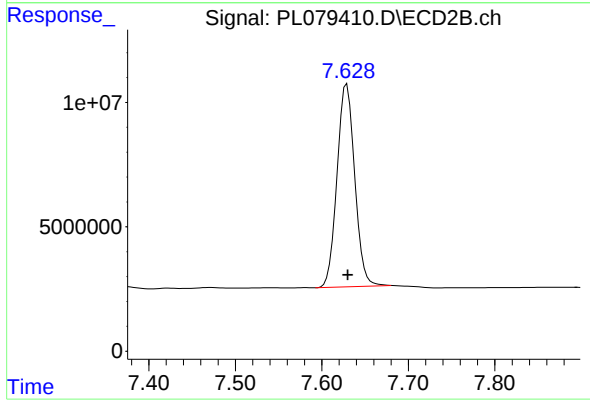

#28 Decachlorobiphenyl

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 115463973
Conc: 49.12 ng/ml