

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 16:43
 Operator : DD\AJ
 Sample : L4592-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-01-112020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:41:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.417	3.950	19837377	28986217	11.648	8.881
28)	SA Decachlor...	8.134	8.994	18726811	24767081	10.028	10.410
Target Compounds							
11)	B alpha-Chl...	0.000	6.122	0	9394852	N.D.	2.604 #
26)	Chlordane-4	0.000	6.122	0	9394852	N.D.	17.516 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 16:43
Operator : DD\AJ
Sample : L4592-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-01-112020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:41:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

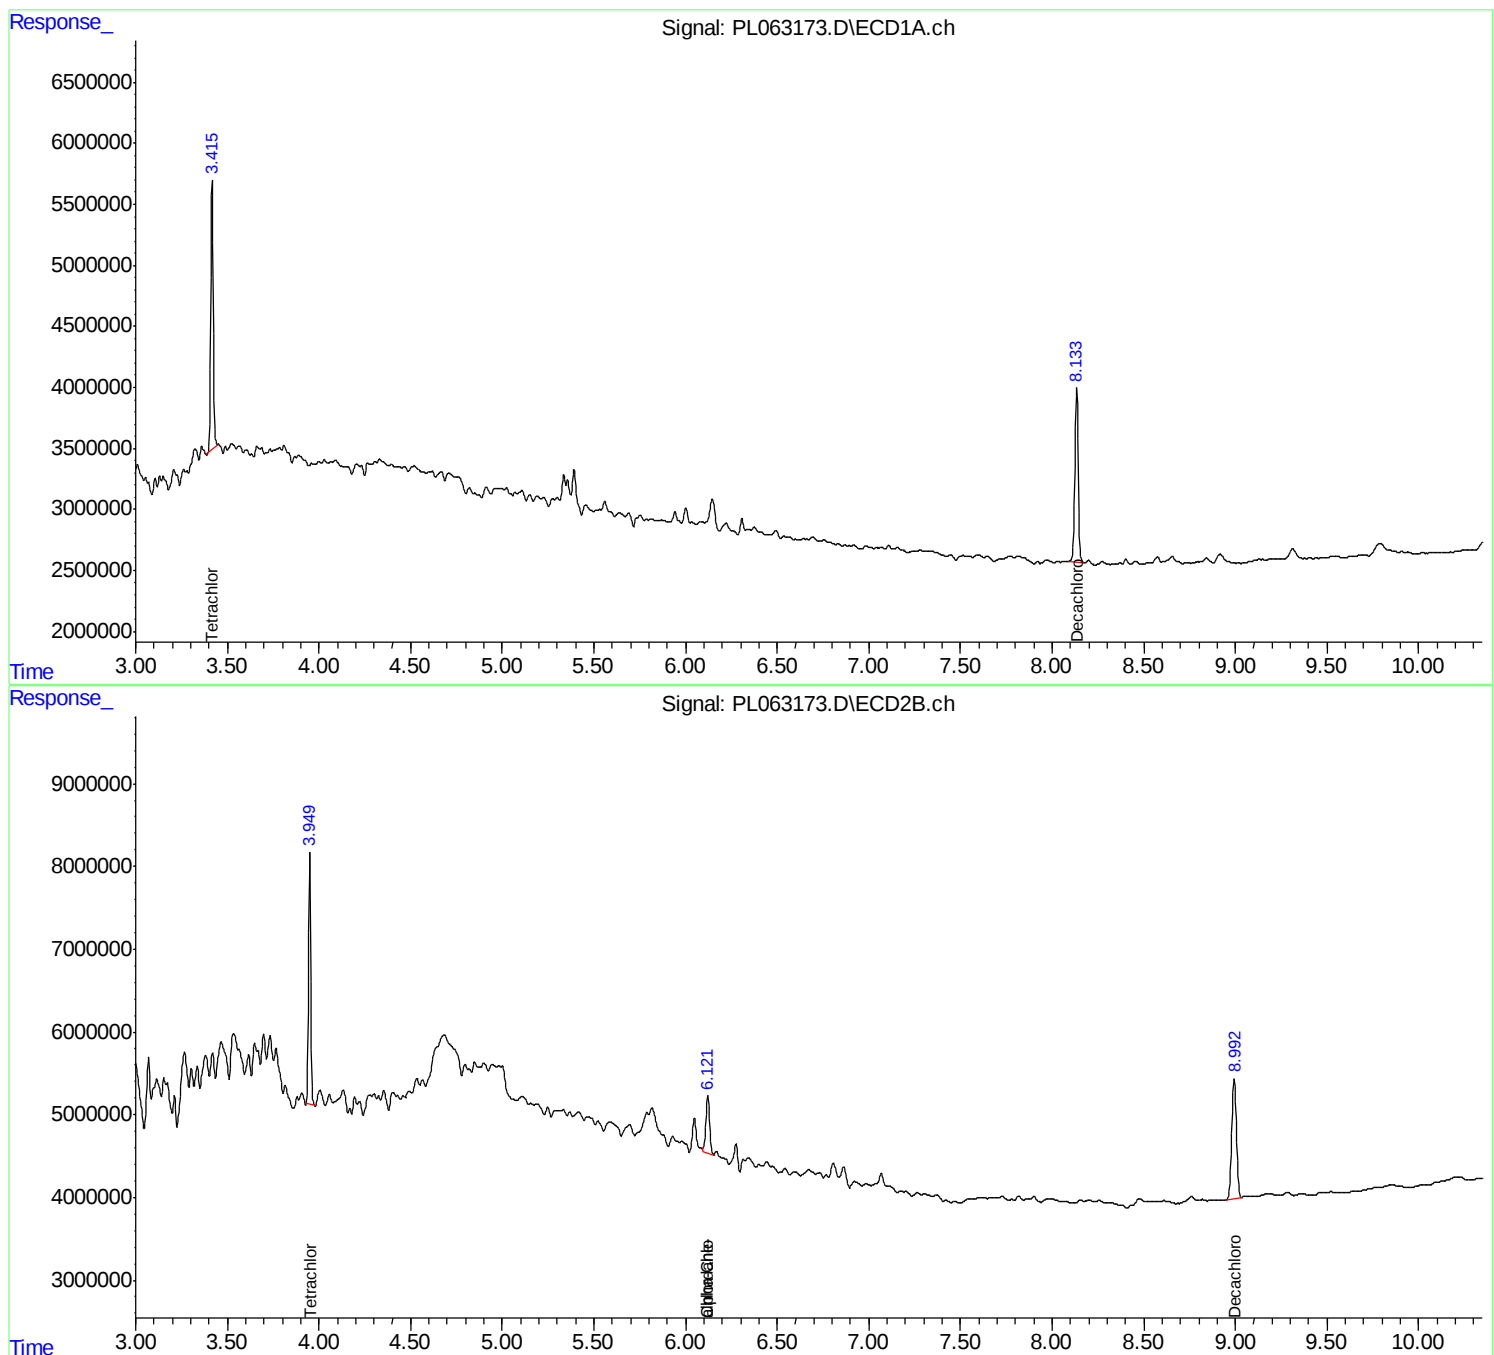


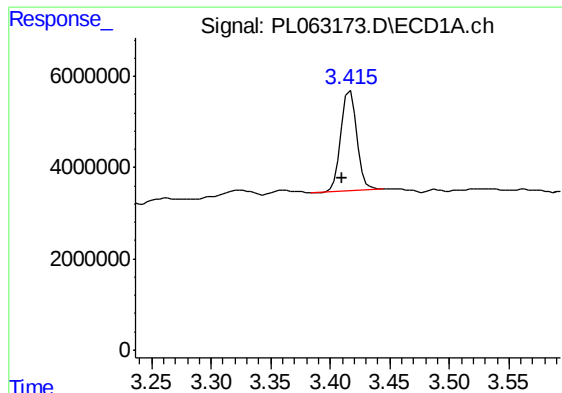

#1 Tetrachloro-m-xylene


R.T.: 3.417 min
Delta R.T.: 0.007 min
Response: 19837377
Conc: 11.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-01-112020

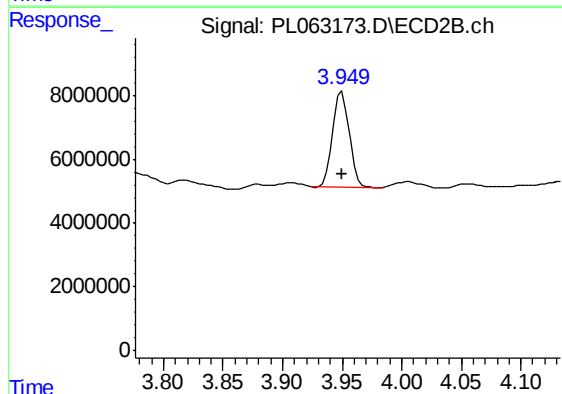


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 28986217
Conc: 8.88 ng/ml

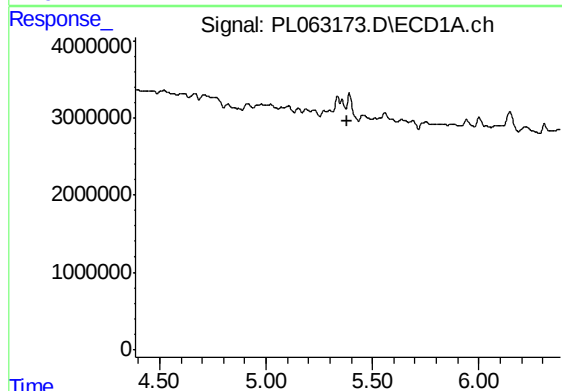


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

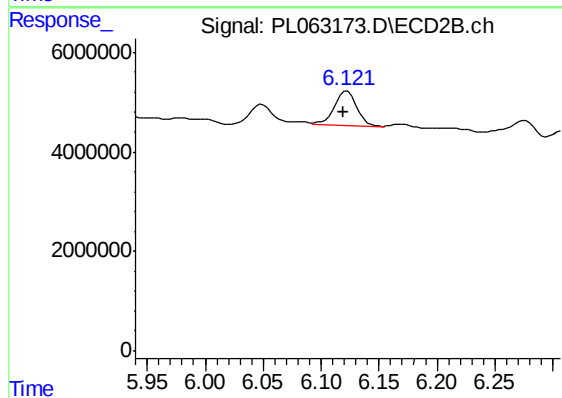

#11 alpha-Chlordane


R.T.: 6.122 min
Delta R.T.: 0.003 min
Response: 9394852
Conc: 2.60 ng/ml

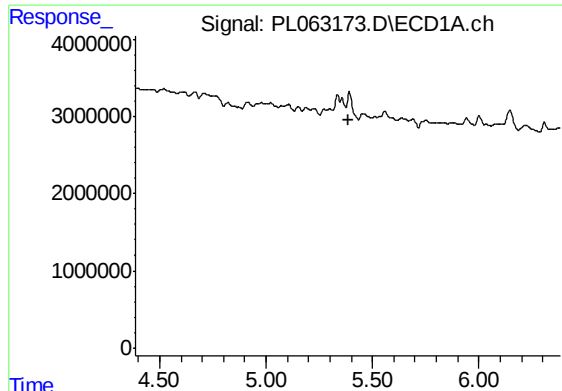

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.385 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-01-112020

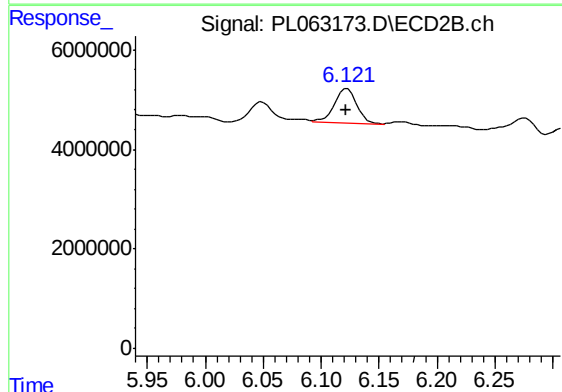


#26 Chlordane-4

R.T.: 6.122 min
Delta R.T.: 0.000 min
Response: 9394852
Conc: 17.52 ng/ml

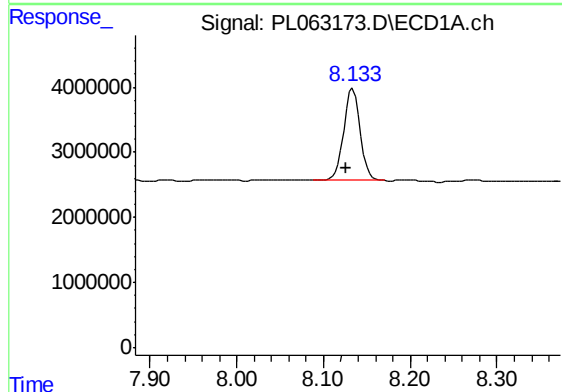

#28 Decachlorobiphenyl

R.T.: 8.134 min
Delta R.T.: 0.008 min
Response: 18726811
Conc: 10.03 ng/ml

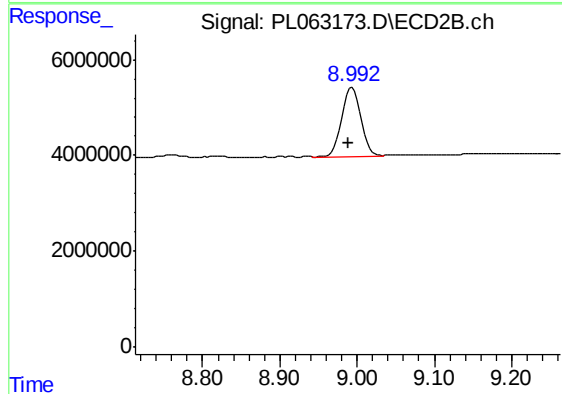

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.004 min
Response: 24767081
Conc: 10.41 ng/ml