

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 16:57
 Operator : DD\AJ
 Sample : L4538-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KENS-B2-111920-0-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:41:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.949	34188811	58620756	20.075	17.961
28)	SA Decachlor...	8.125	8.989	23072397	28488714	12.355	11.974
Target Compounds							
7)	B delta-BHC	0.000	5.001	0 11073395	N.D.	2.908	#
8)	B Heptachlo...	0.000	5.824	0 9236737	N.D.	2.652	#
15)	B Endosulfa...	0.000	6.870f	0 7816120	N.D.	2.364	#
19)	B Endosulfa...	0.000	7.200	0 7003466	N.D.	2.572	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 16:57
Operator : DD\AJ
Sample : L4538-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-0-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:41:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

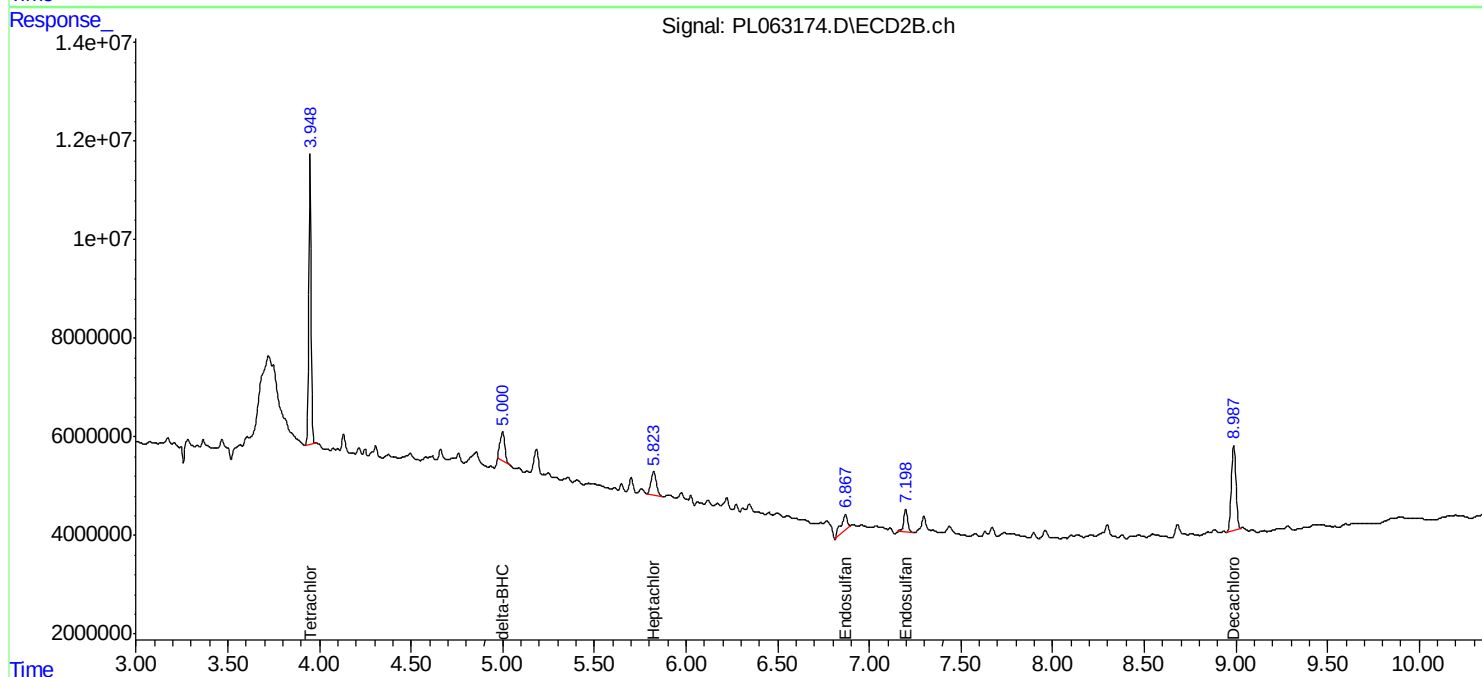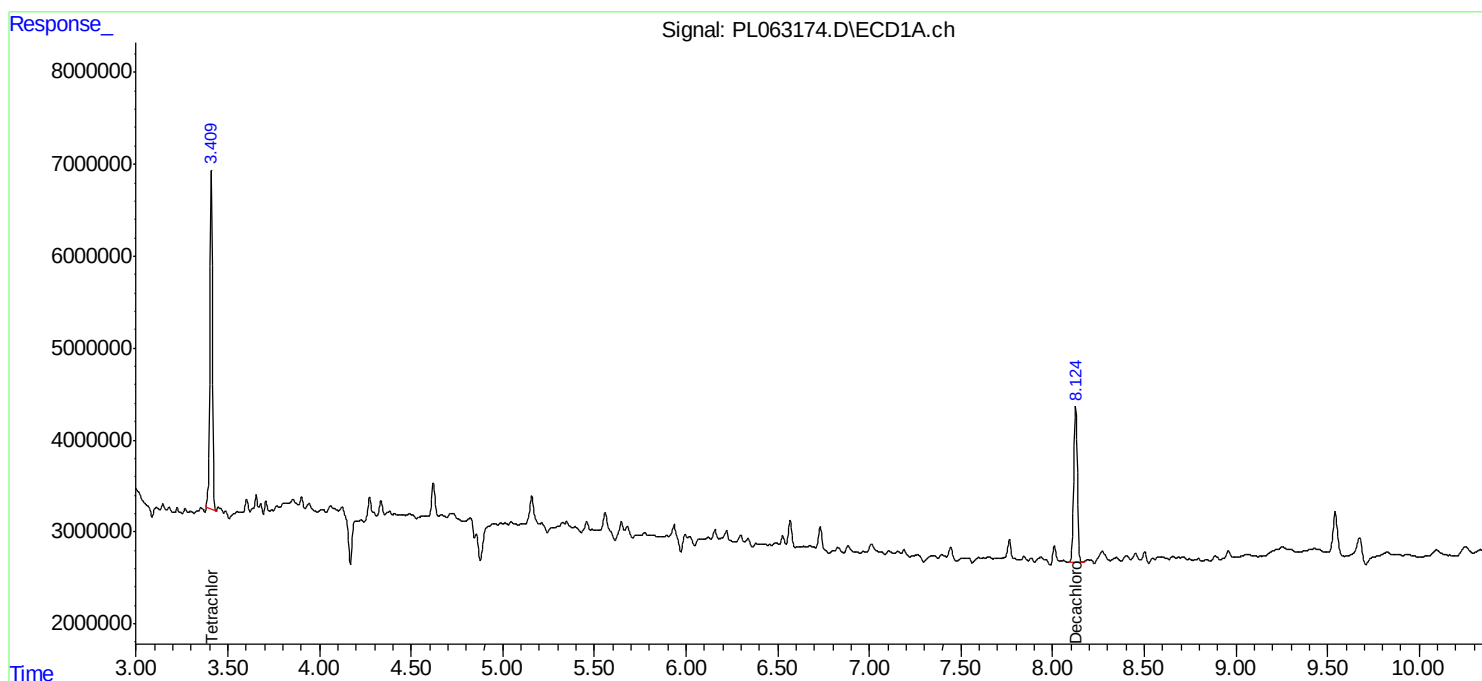


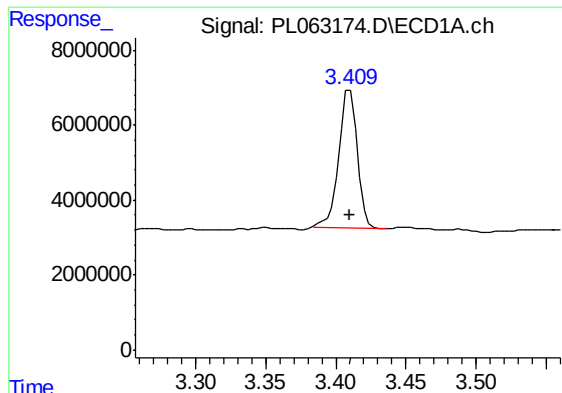

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 34188811
Conc: 20.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-0-2

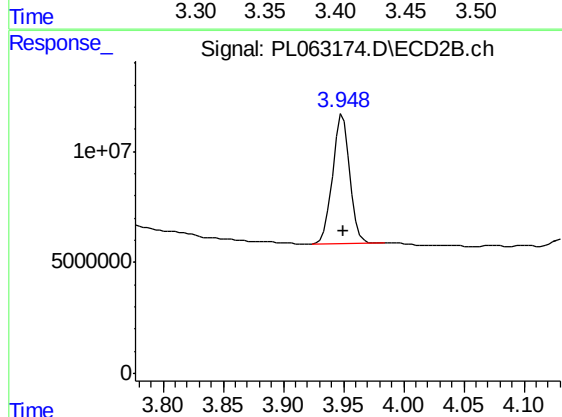


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 58620756
Conc: 17.96 ng/ml

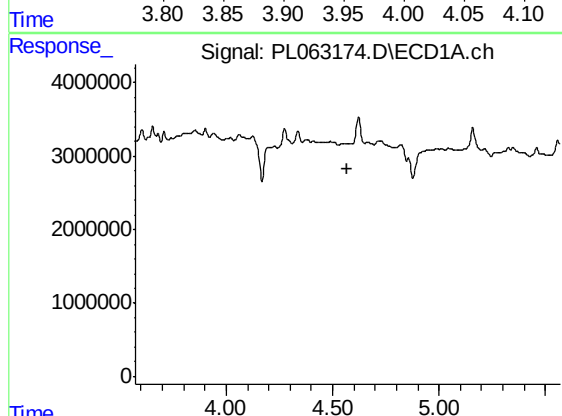


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.572 min
Response: 0
Conc: N.D.

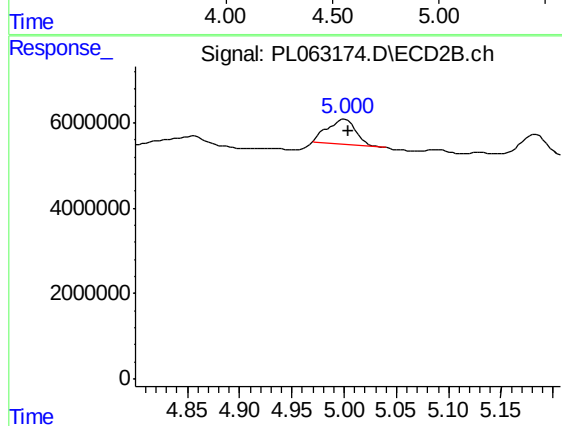

#7 delta-BHC


R.T.: 5.001 min
Delta R.T.: -0.004 min
Response: 11073395
Conc: 2.91 ng/ml

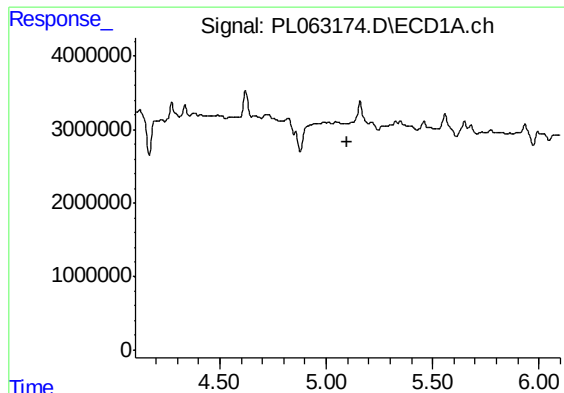

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.101 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-0-2

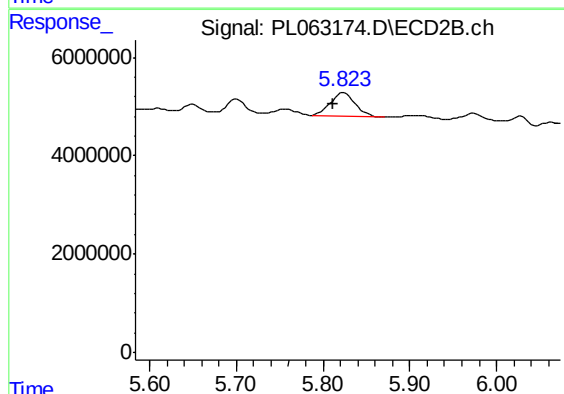


#8 Heptachlor epoxide

R.T.: 5.824 min
Delta R.T.: 0.013 min
Response: 9236737
Conc: 2.65 ng/ml

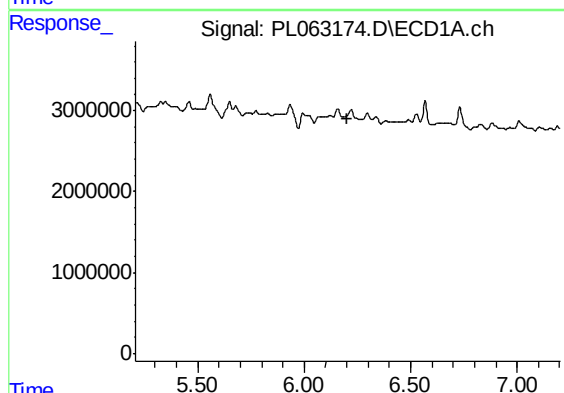


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

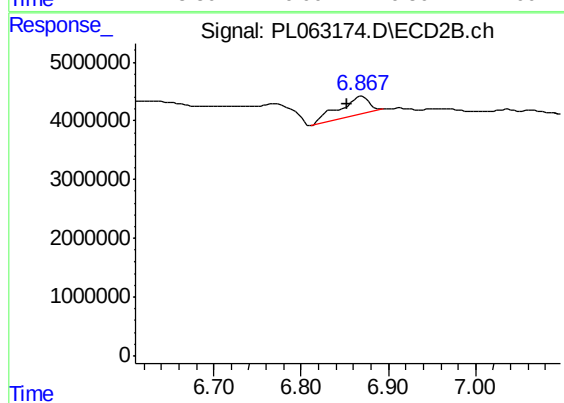

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.017 min
Response: 7816120
Conc: 2.36 ng/ml

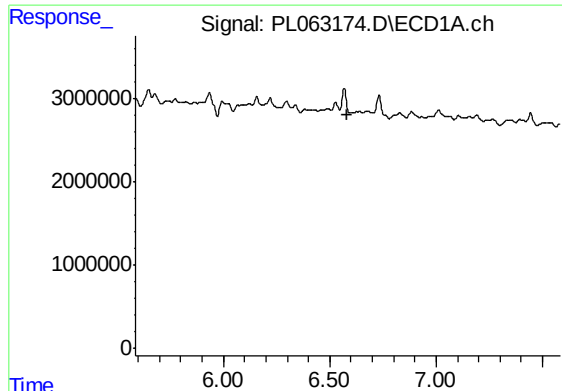

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.584 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-0-2

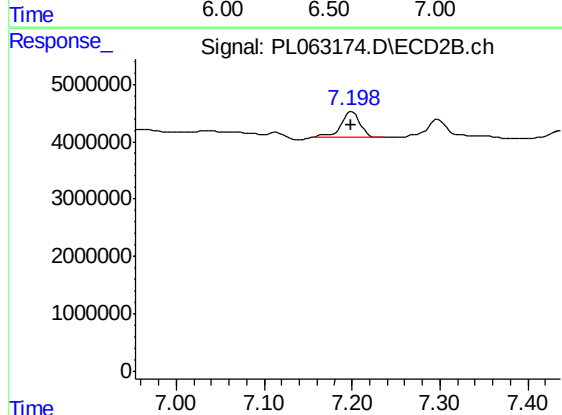


#19 Endosulfan Sulfate

R.T.: 7.200 min
Delta R.T.: 0.002 min
Response: 7003466
Conc: 2.57 ng/ml

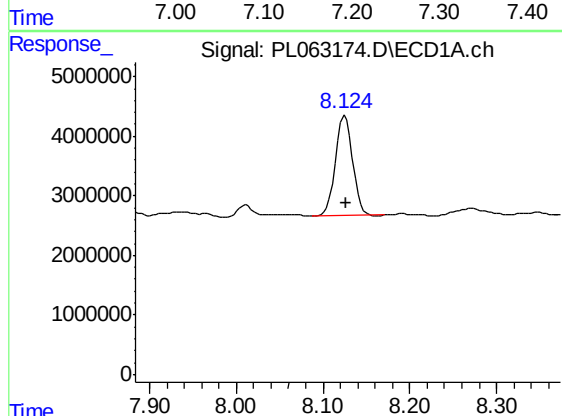

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: 0.000 min
Response: 23072397
Conc: 12.36 ng/ml

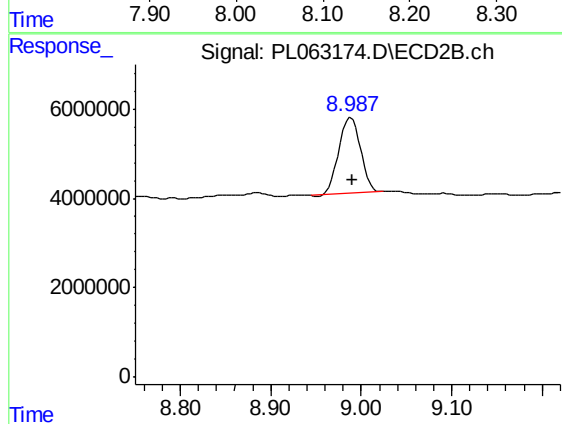

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 28488714
Conc: 11.97 ng/ml