

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 17:25
 Operator : DD\AJ
 Sample : L4844-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-112020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:41:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.409	3.949	19412179	11770839	11.398	3.607 #
28) SA	Decachlor...	8.125	8.988	19928108	19742478	10.671	8.298
Target Compounds							
2) A	alpha-BHC	0.000	4.359f	0	25823200	N.D.	5.307 #
6) B	beta-BHC	0.000	4.811f	0	10246007	N.D.	5.025 #
9) A	Endosulfan I	5.426	0.000	4069735	0	2.404	N.D. #
10) B	gamma-Chl...	0.000	6.019f	0	4453846	N.D.	1.259 #
14) MA	Endrin	0.000	6.671f	0	26960077	N.D.	9.130 #
23)	Chlordane-1	0.000	4.947	0	5396453	N.D.	48.891 #
25)	Chlordane-3	0.000	6.019f	0	4453846	N.D.	10.043 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063176.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 17:25
Operator : DD\AJ
Sample : L4844-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:41:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

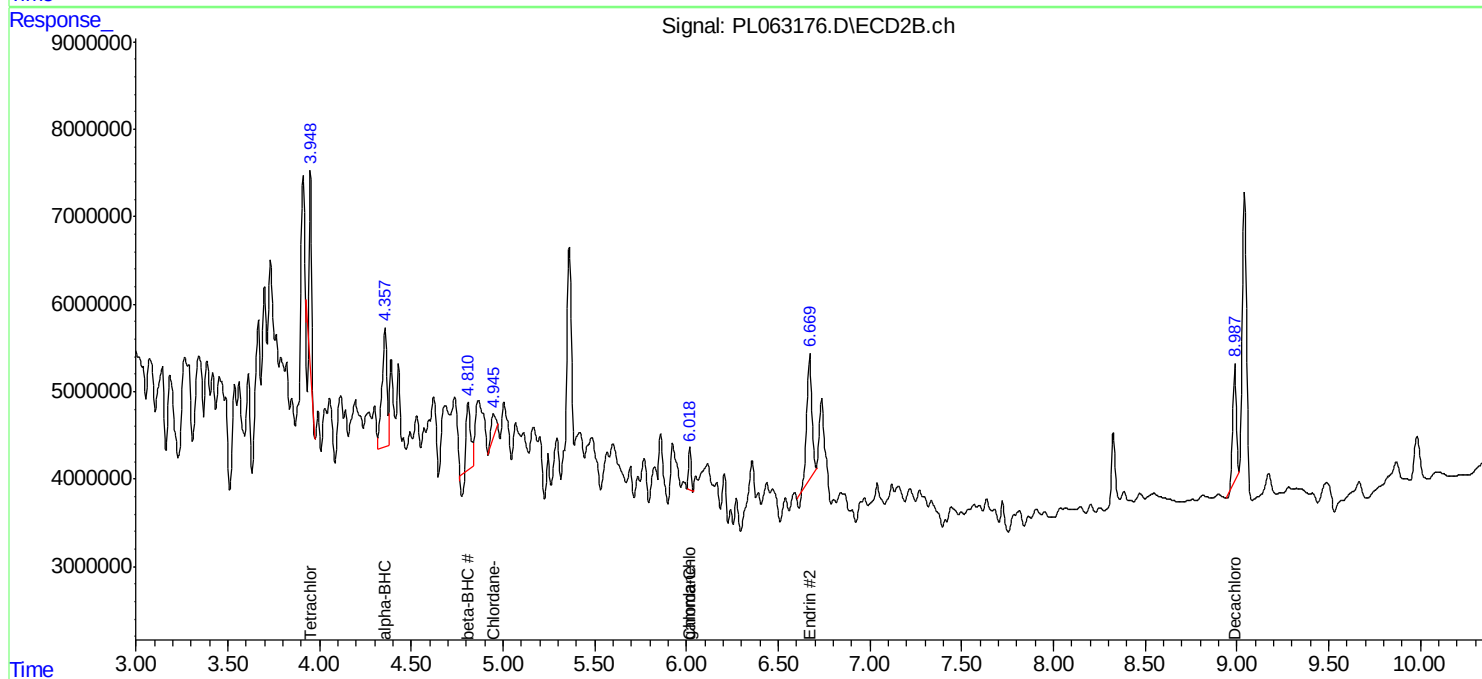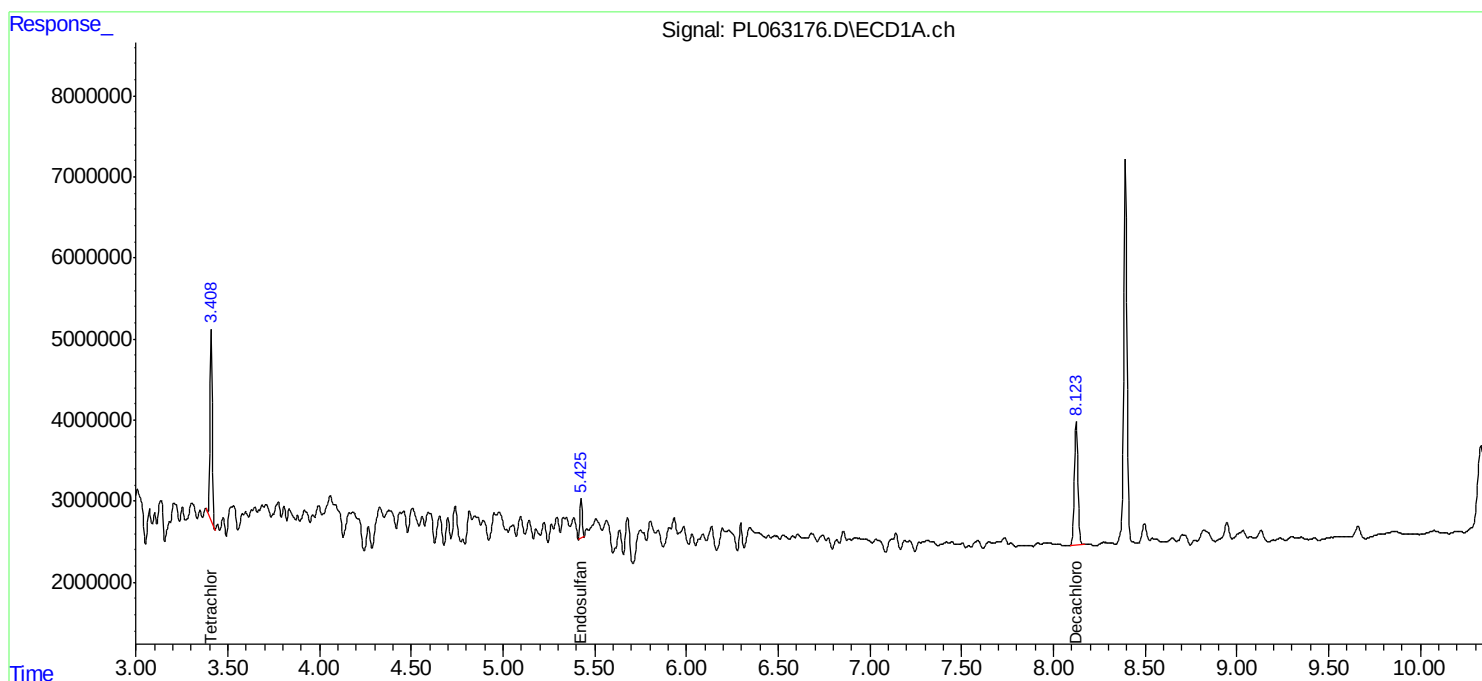


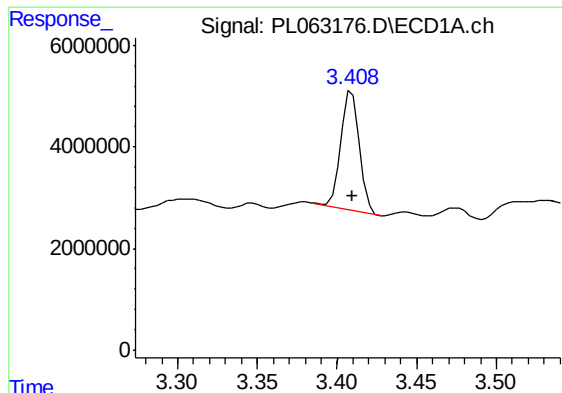

#1 Tetrachloro-m-xylene


R.T.: 3.409 min
Delta R.T.: 0.000 min
Response: 19412179
Conc: 11.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

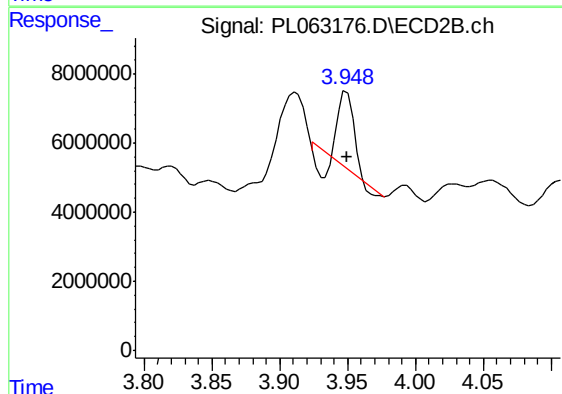


#1 Tetrachloro-m-xylene

R.T.: 3.949 min
Delta R.T.: 0.000 min
Response: 11770839
Conc: 3.61 ng/ml

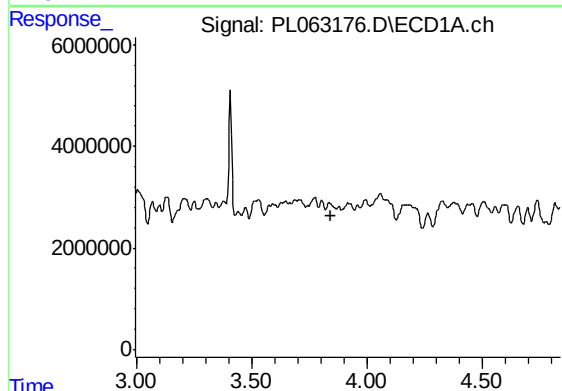


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.842 min
Response: 0
Conc: N.D.

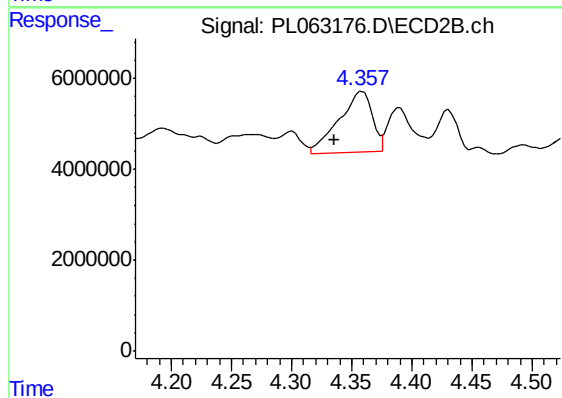

#2 alpha-BHC


R.T.: 4.359 min
Delta R.T.: 0.023 min
Response: 25823200
Conc: 5.31 ng/ml

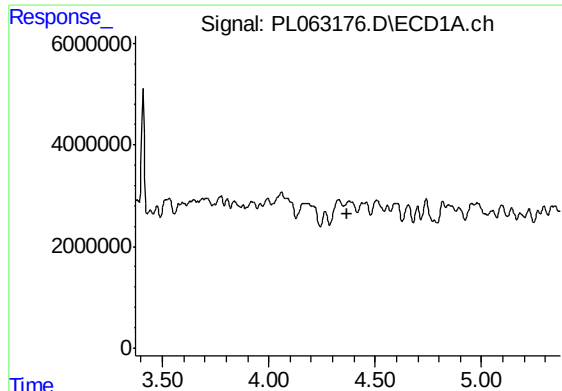

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

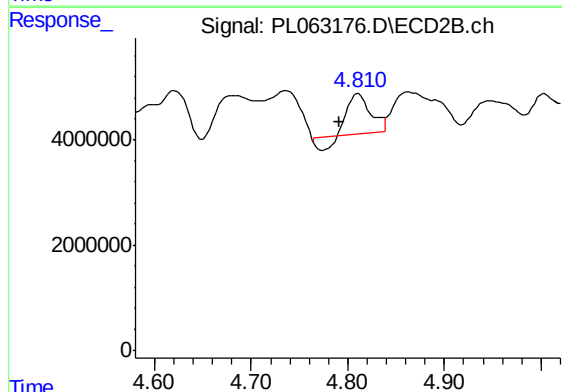


#6 beta-BHC

R.T.: 4.811 min
Delta R.T.: 0.020 min
Response: 10246007
Conc: 5.03 ng/ml

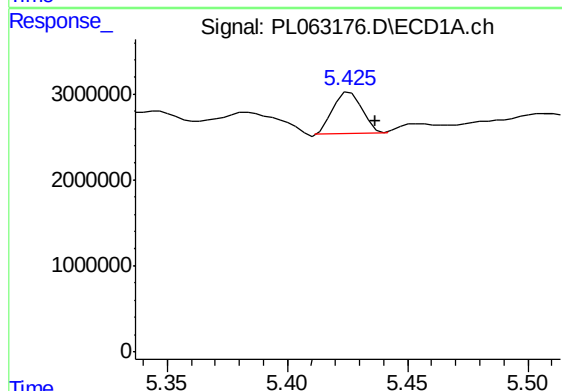


#9 Endosulfan I

R.T.: 5.426 min
Delta R.T.: -0.011 min
Response: 4069735
Conc: 2.40 ng/ml

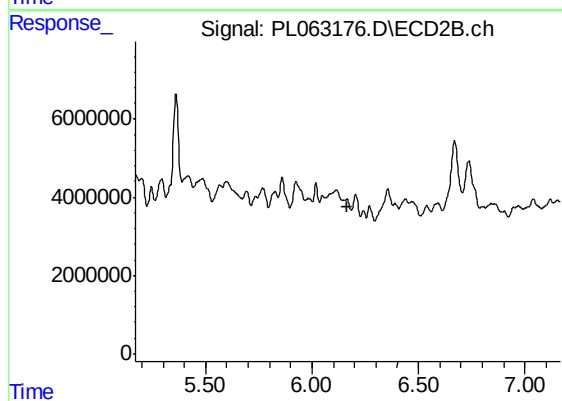

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.167 min
Response: 0
Conc: N.D.

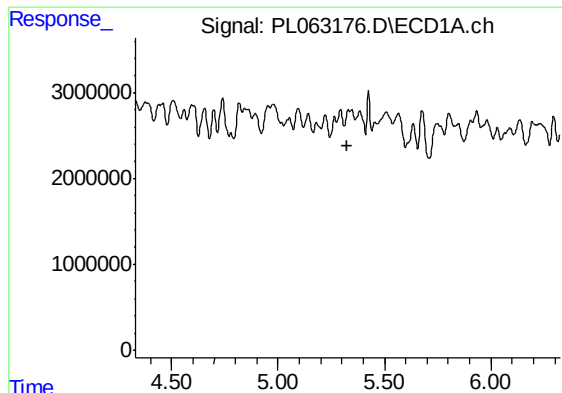

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

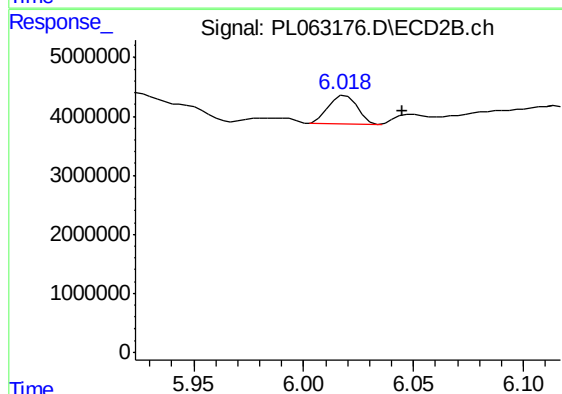


#10 gamma-Chlordane

R.T.: 6.019 min
Delta R.T.: -0.026 min
Response: 4453846
Conc: 1.26 ng/ml

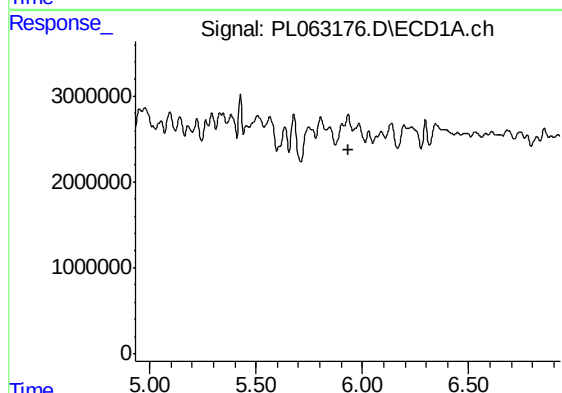


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.932 min
Response: 0
Conc: N.D.

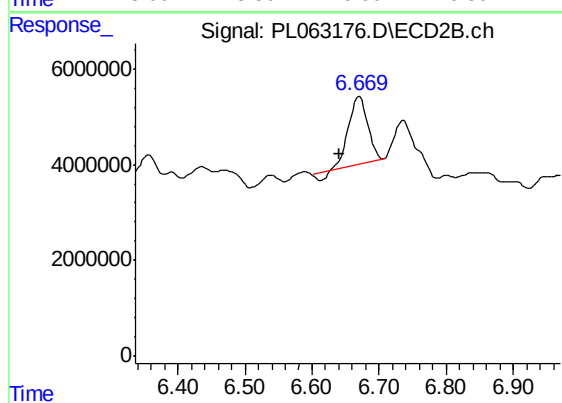

#14 Endrin


R.T.: 6.671 min
Delta R.T.: 0.029 min
Response: 26960077
Conc: 9.13 ng/ml

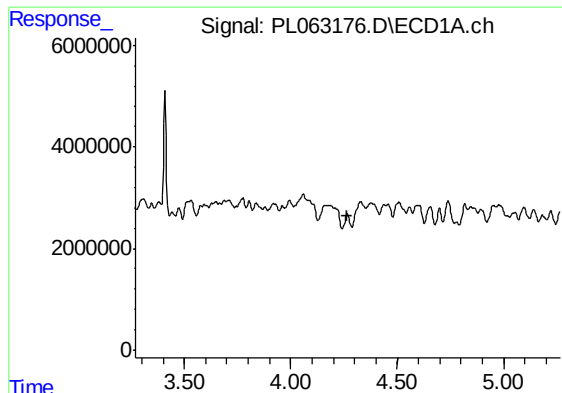

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

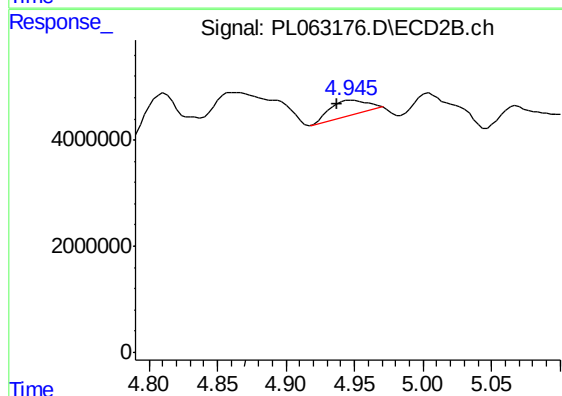


#23 Chlordane-1

R.T.: 4.947 min
Delta R.T.: 0.010 min
Response: 5396453
Conc: 48.89 ng/ml

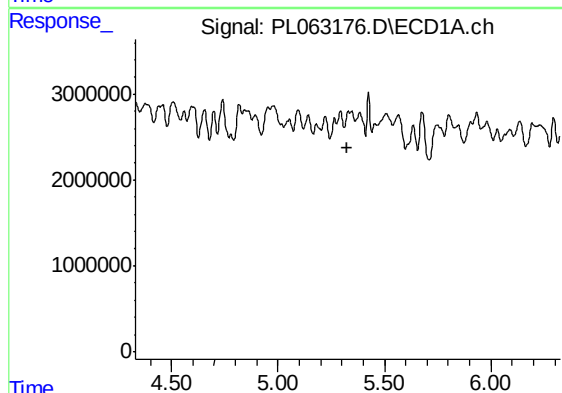


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

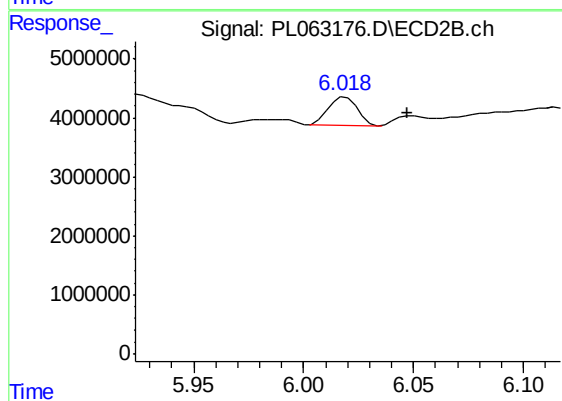

#25 Chlordane-3


R.T.: 6.019 min
Delta R.T.: -0.028 min
Response: 4453846
Conc: 10.04 ng/ml

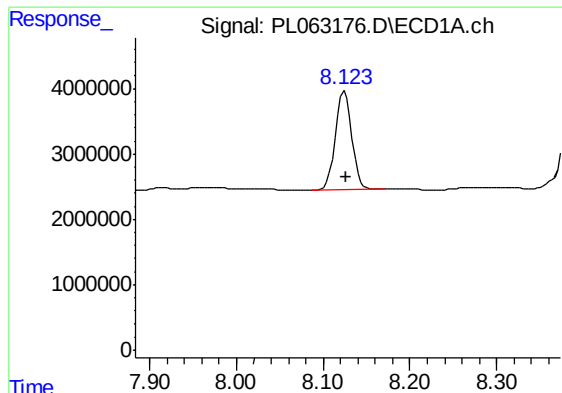

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.001 min
Response: 19928108
Conc: 10.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-112020

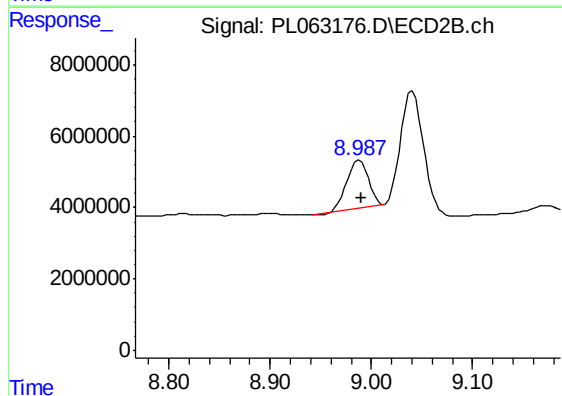

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.001 min
Response: 19742478
Conc: 8.30 ng/ml