

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 17:39
 Operator : DD\AJ
 Sample : L4845-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PH-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:42:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.410	3.950	32665602	58051348	19.180	17.787
28) SA Decachlor...	8.124	8.987	24759253	27686938	13.258	11.637
Target Compounds						
9) A Endosulfan I	5.458f	0.000	728801	0	0.431	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 17:39
Operator : DD\AJ
Sample : L4845-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PH-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:42:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

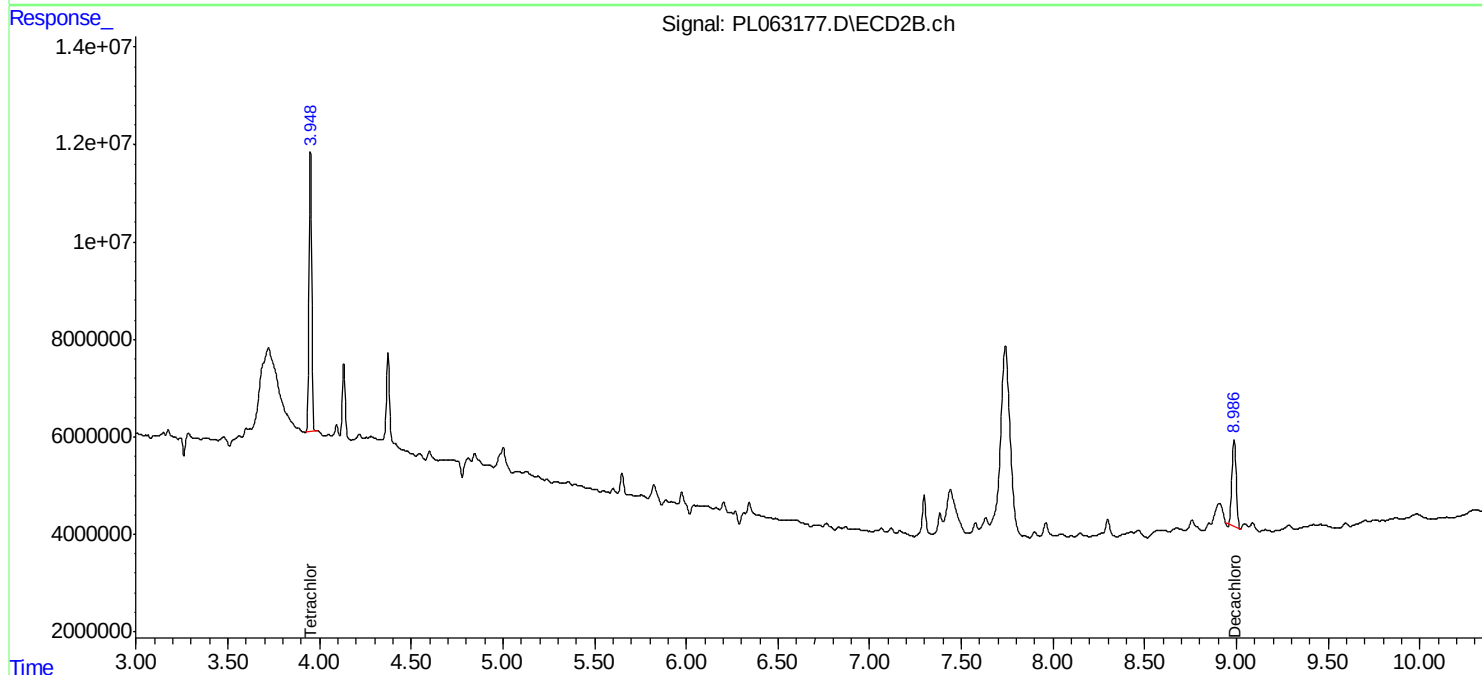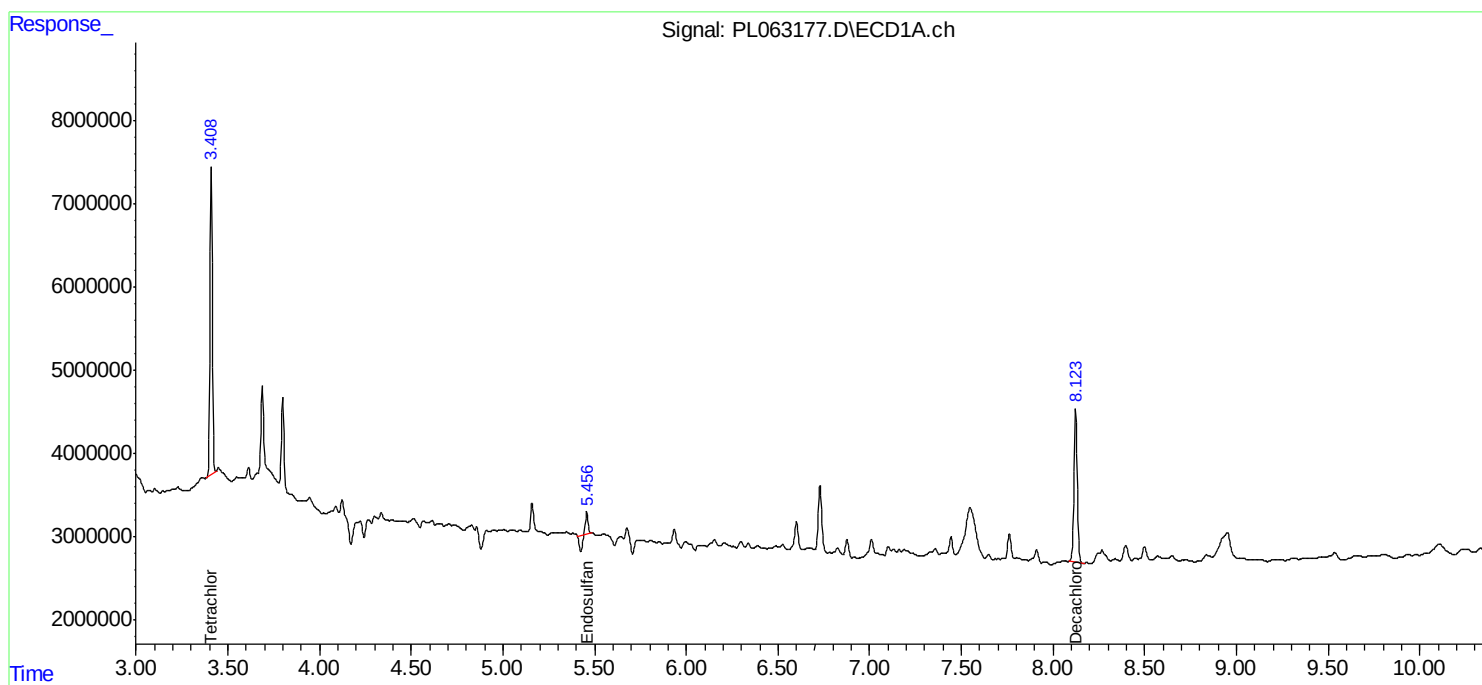


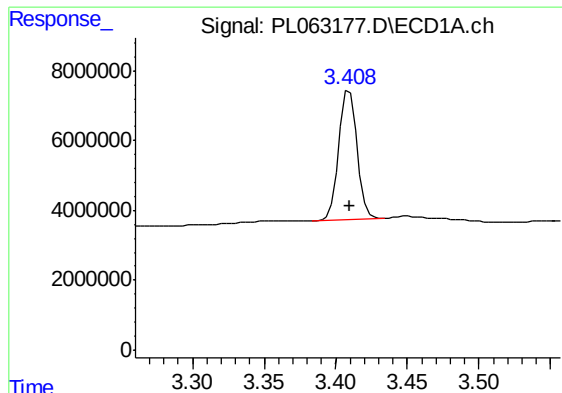

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 32665602
Conc: 19.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PH-TP

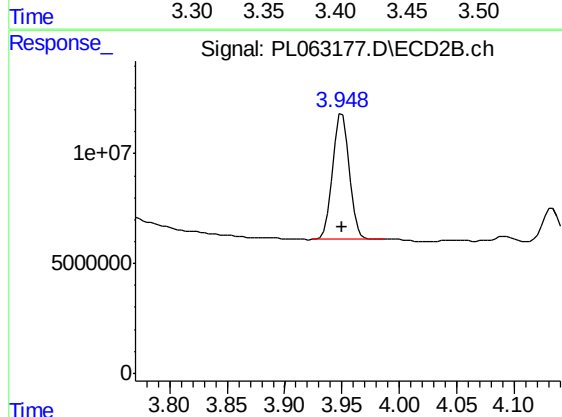


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 58051348
Conc: 17.79 ng/ml

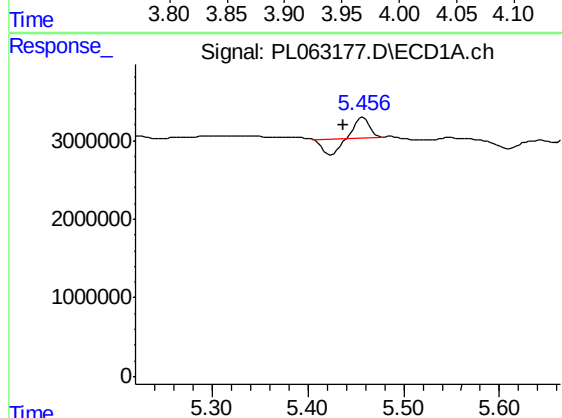


#9 Endosulfan I

R.T.: 5.458 min
Delta R.T.: 0.021 min
Response: 728801
Conc: 0.43 ng/ml

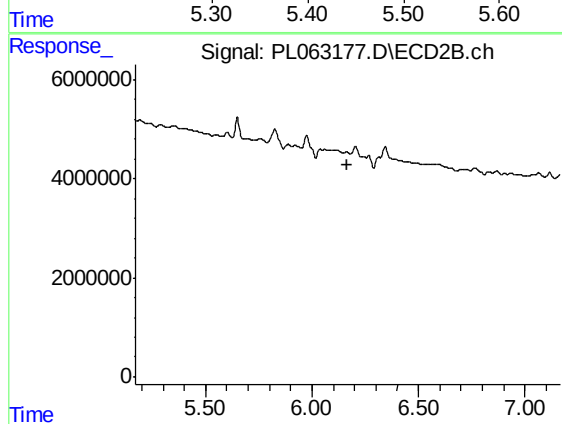

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.167 min
Response: 0
Conc: N.D.

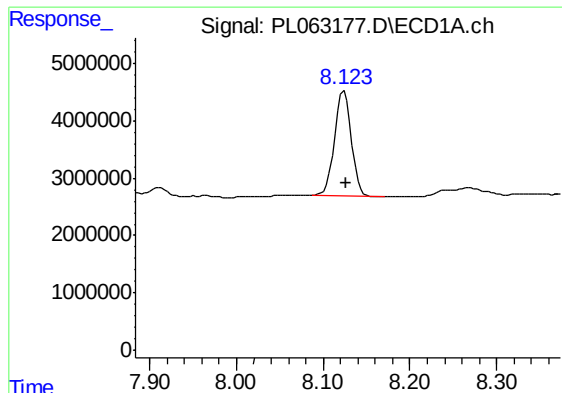

#28 Decachlorobiphenyl

R.T.: 8.124 min
Delta R.T.: -0.002 min
Response: 24759253
Conc: 13.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PH-TP

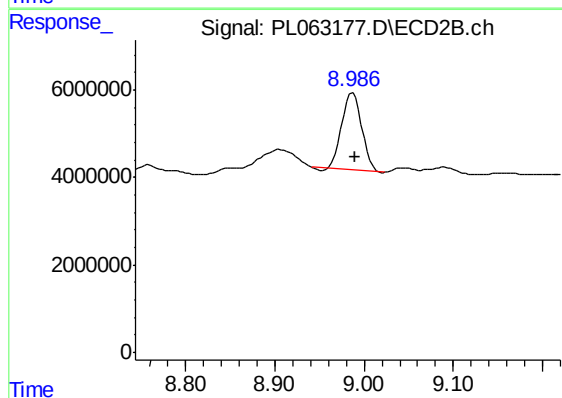

#28 Decachlorobiphenyl

R.T.: 8.987 min
Delta R.T.: -0.002 min
Response: 27686938
Conc: 11.64 ng/ml