

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 17:54
 Operator : DD\AJ
 Sample : L4846-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RCA-EDISON-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:42:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.950	33203816	59252054	19.496	18.154
28)	SA Decachlor...	8.125	8.988	28913879	36471334	15.483	15.329
Target Compounds							
4)	MA Heptachlor	0.000	5.131	0	6700122	N.D.	1.608 #
15)	B Endosulfa...	6.221f	6.871f	29419956	48318626	16.007	14.615
27)	Chlordane-5	6.221	0.000	29419956	0	505.317	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 17:54
Operator : DD\AJ
Sample : L4846-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RCA-EDISON-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:42:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

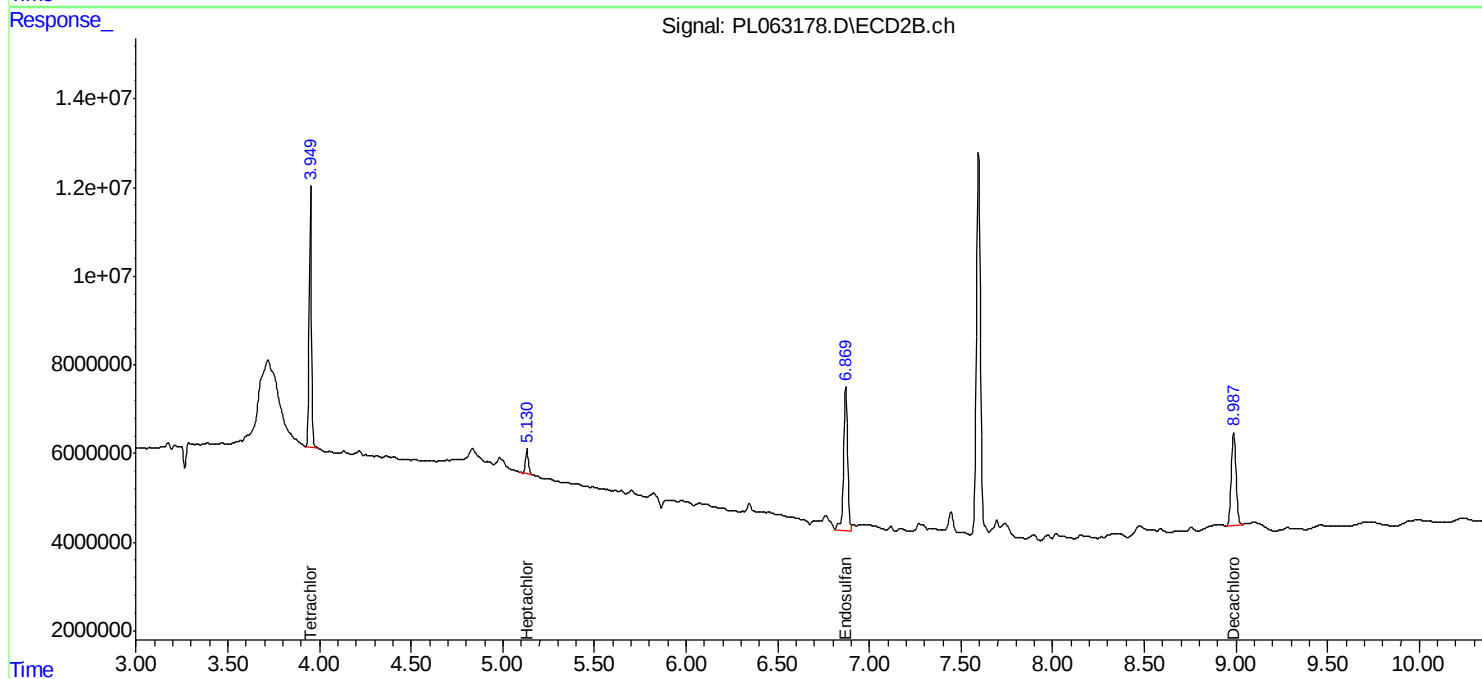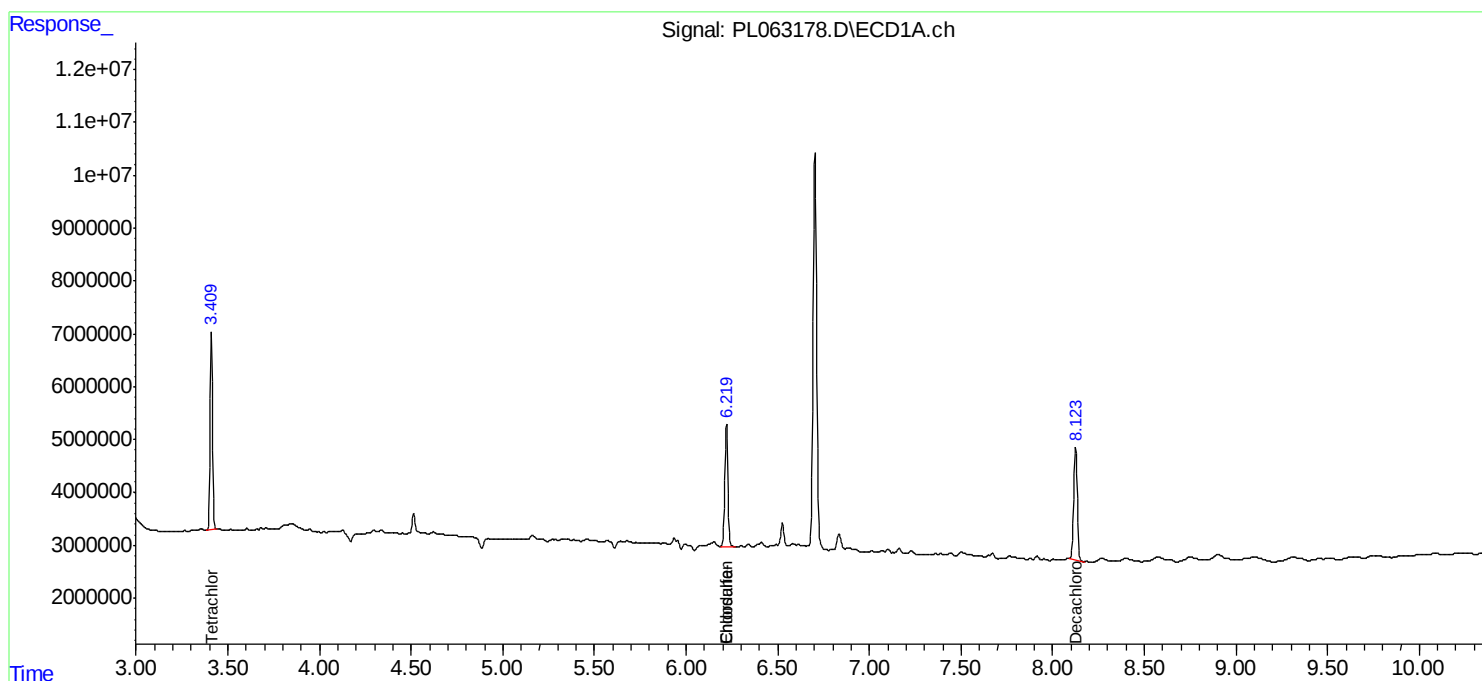


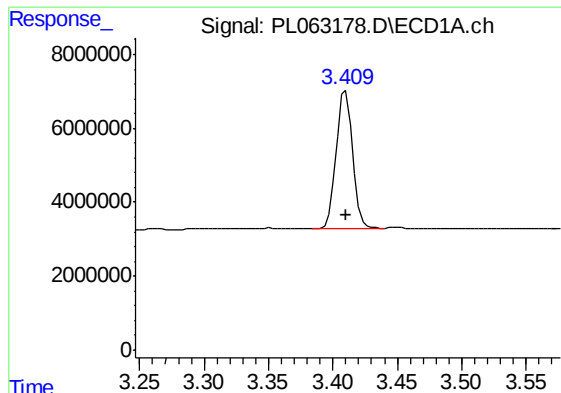

#1 Tetrachloro-m-xylene


R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 33203816
Conc: 19.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
RCA-EDISON-3

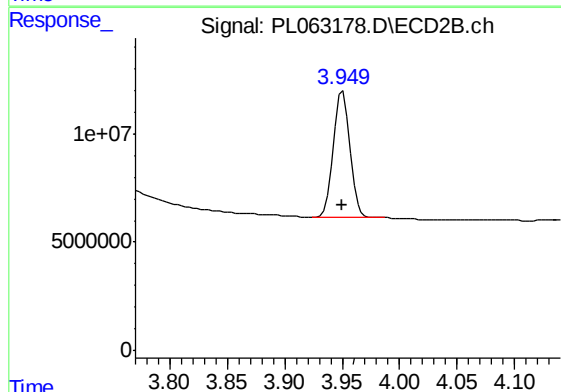


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 59252054
Conc: 18.15 ng/ml

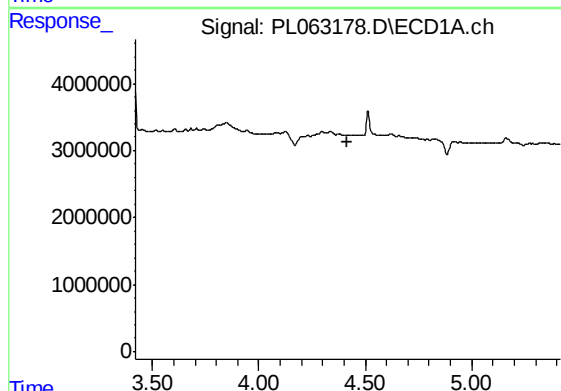


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

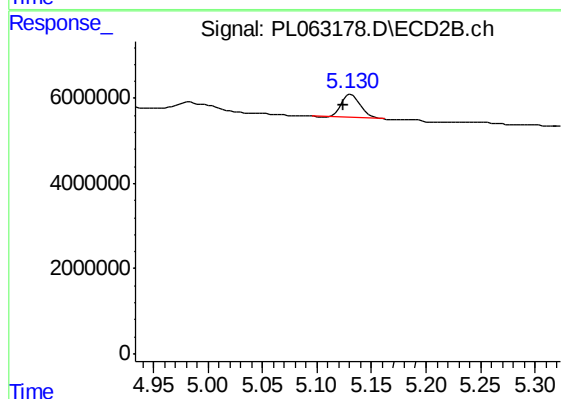

#4 Heptachlor


R.T.: 5.131 min
Delta R.T.: 0.007 min
Response: 6700122
Conc: 1.61 ng/ml

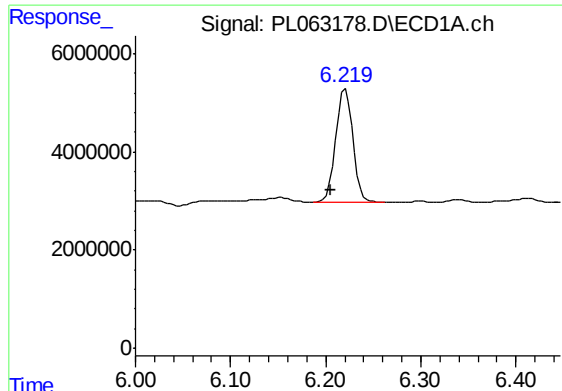

#15 Endosulfan II


R.T.: 6.221 min
Delta R.T.: 0.016 min
Response: 29419956
Conc: 16.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
RCA-EDISON-3

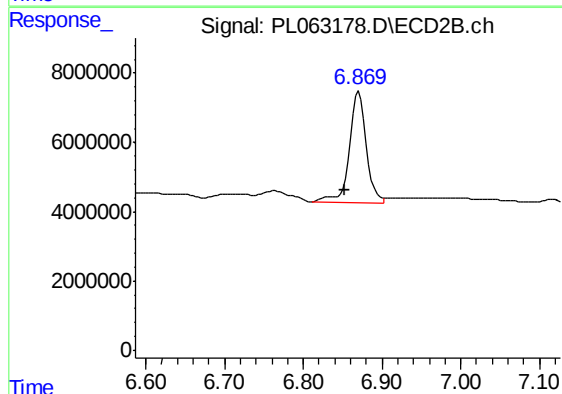


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.019 min
Response: 48318626
Conc: 14.62 ng/ml

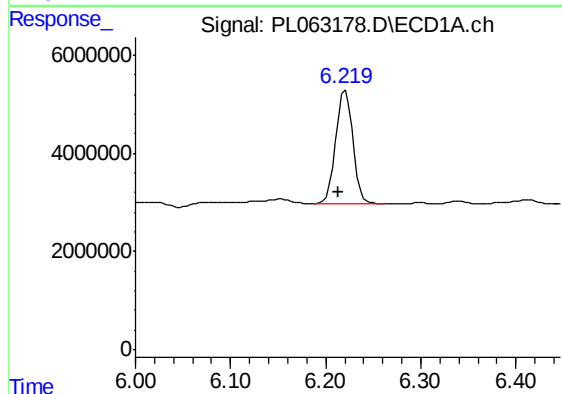


#27 Chlordane-5

R.T.: 6.221 min
Delta R.T.: 0.007 min
Response: 29419956
Conc: 505.32 ng/ml

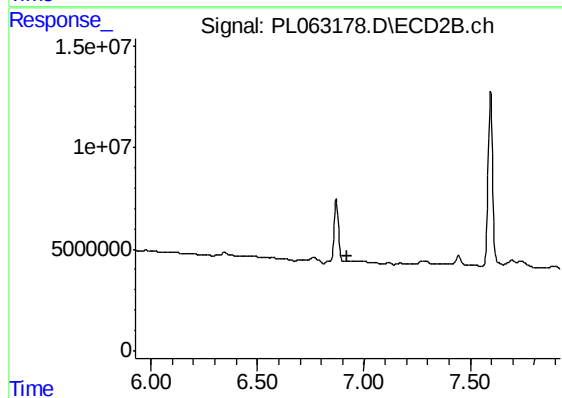

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

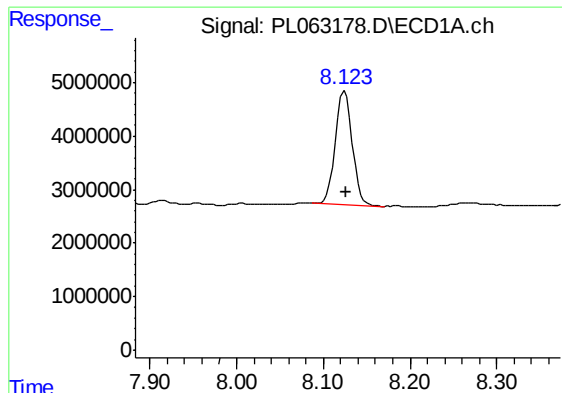

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.001 min
Response: 28913879
Conc: 15.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
RCA-EDISON-3

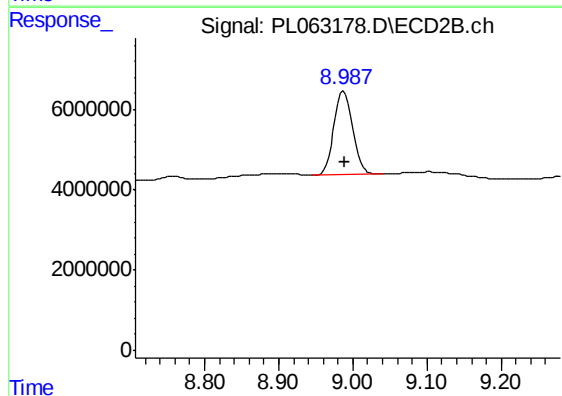

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: -0.002 min
Response: 36471334
Conc: 15.33 ng/ml