

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 17:11
 Operator : DD\AJ
 Sample : L4838-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KENS-B2-111920-6-8

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:35:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:41:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.410	3.968f	36341057	65505754	21.338	20.071m
28)	SA Decachlor...	8.125	9.008f	30725986	39563630	16.453	16.629

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 17:11
Operator : DD\AJ
Sample : L4838-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-6-8


Manual Integrations
APPROVED

Ankita
11/25/2020 5:35:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:41:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

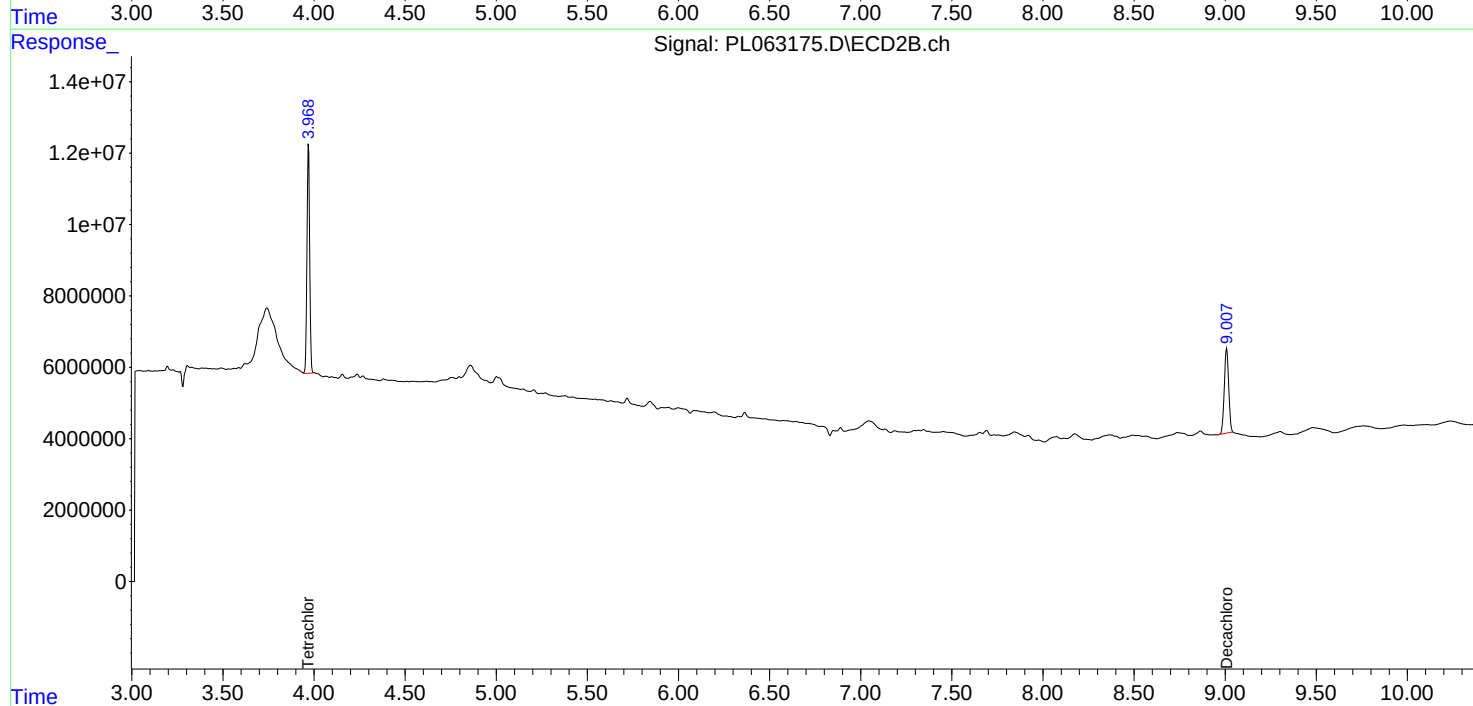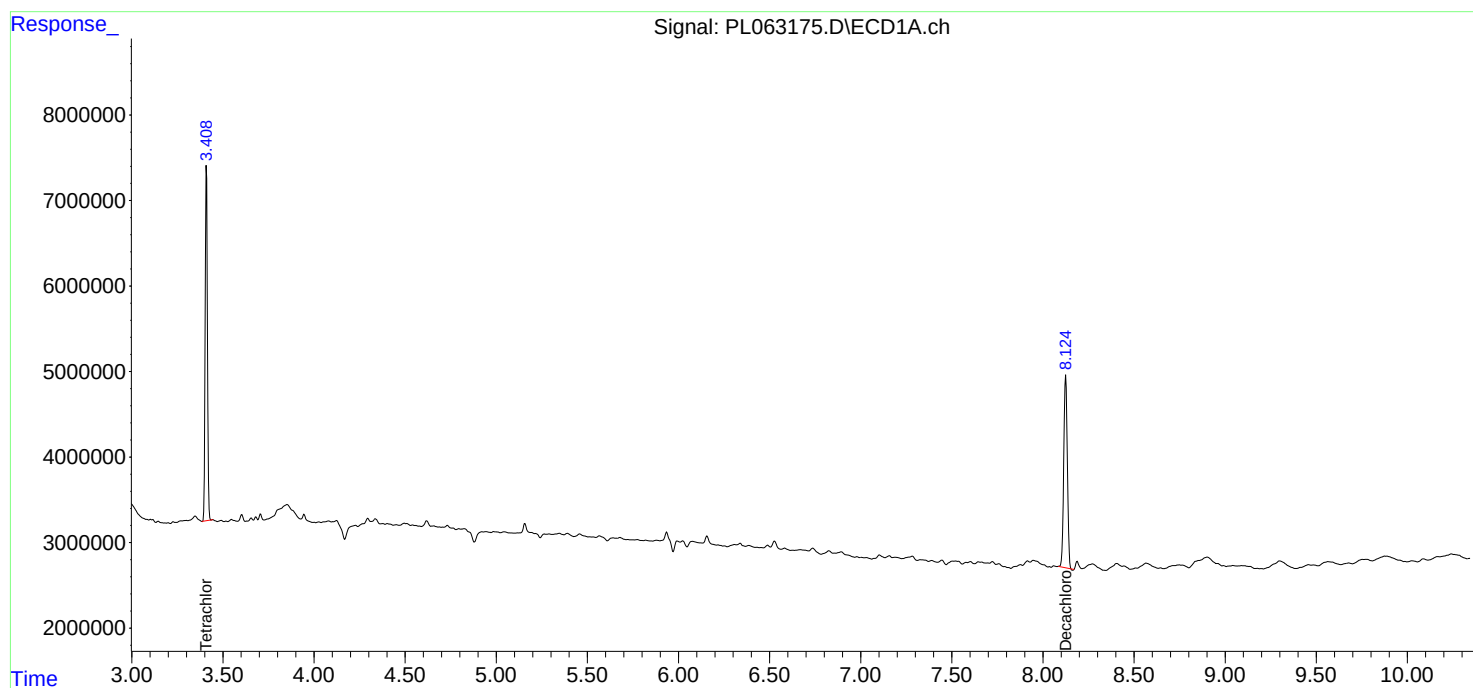

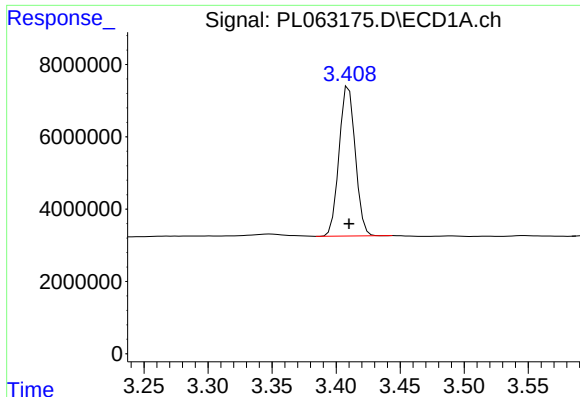


#1 Tetrachloro-m-xylene

R.T.: 3.410 min
Delta R.T.: 0.000 min
Response: 36341057
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
KENS-B2-111920-6-8


Manual Integrations
APPROVED

Ankita
11/25/2020 5:35:37 PM

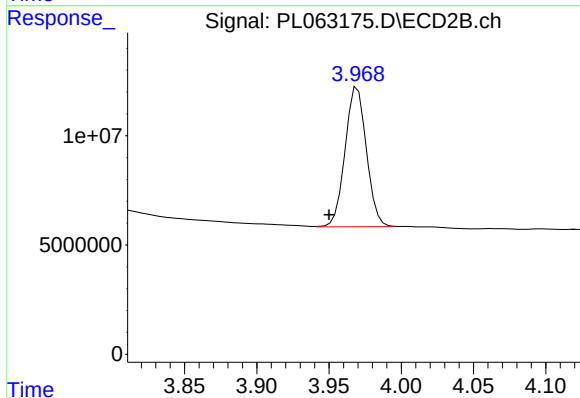


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.018 min
Response: 65505754
Conc: 20.07 ng/ml m

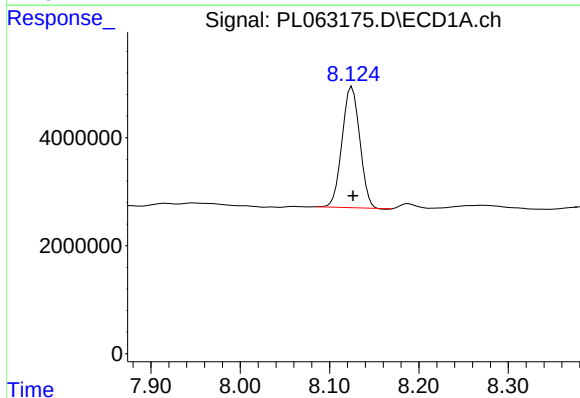

#28 Decachlorobiphenyl

R.T.: 8.125 min
Delta R.T.: -0.001 min
Response: 30725986
Conc: 16.45 ng/ml

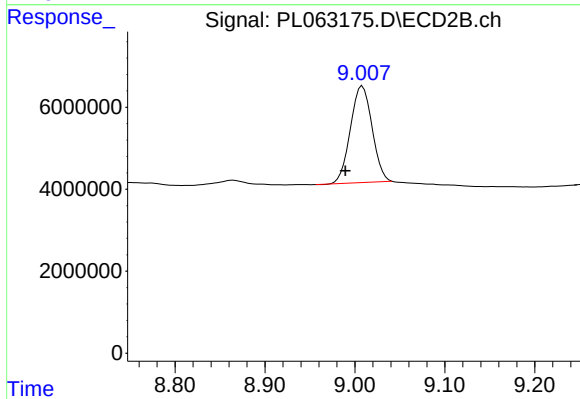

#28 Decachlorobiphenyl

R.T.: 9.008 min
Delta R.T.: 0.019 min
Response: 39563630
Conc: 16.63 ng/ml