

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
 Data File : PL063196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2020 22:10
 Operator : DD\AJ
 Sample : L4588-01 10x
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-112320

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:36:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 22:47:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 24 01:53:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.408	3.948	2517824	3859847	1.478m	1.183m
28)	SA Decachlor...	8.123	8.986	2252522	3280774	1.206m	1.379m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112420\
Data File : PL063196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2020 22:10
Operator : DD\AJ
Sample : L4588-01 10x
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HD-02-112320


Manual Integrations
APPROVED

Ankita
11/25/2020 5:36:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 22:47:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112320.M
Quant Title : GC Extractables
QLast Update : Tue Nov 24 01:53:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

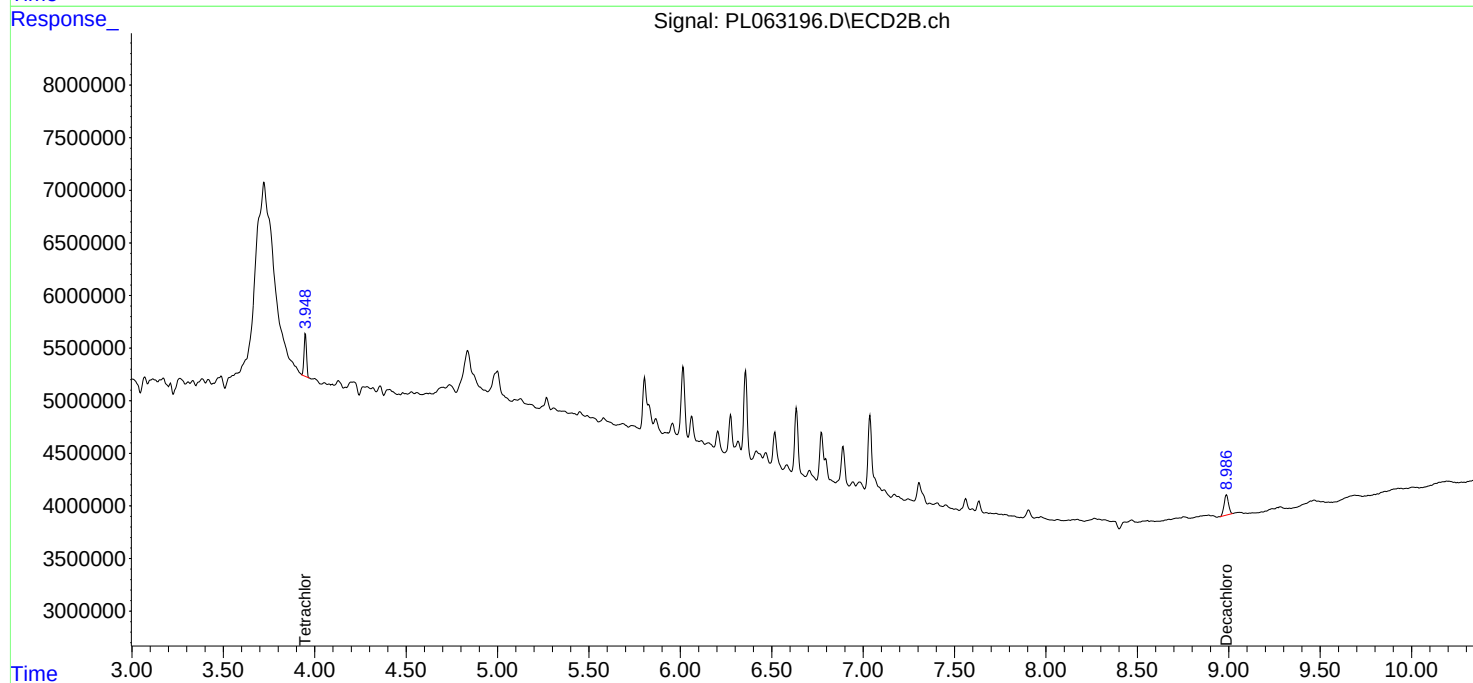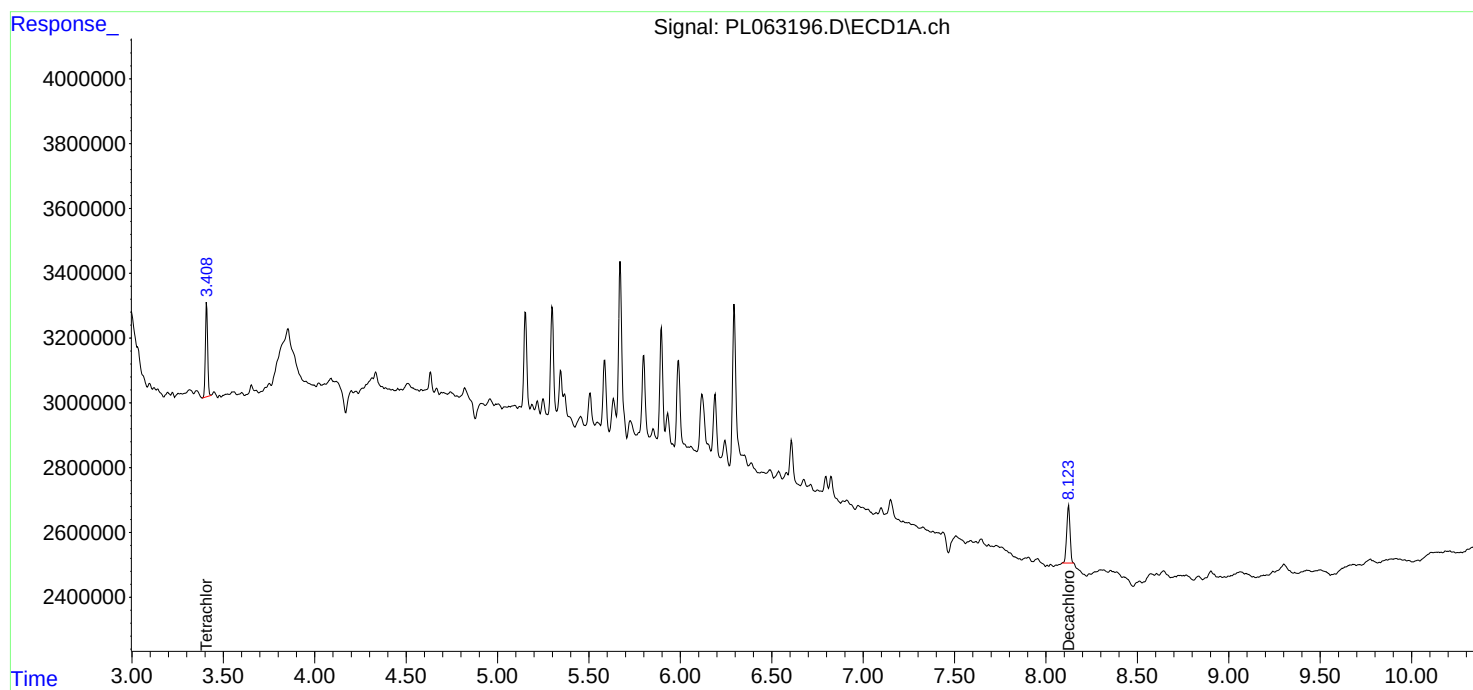

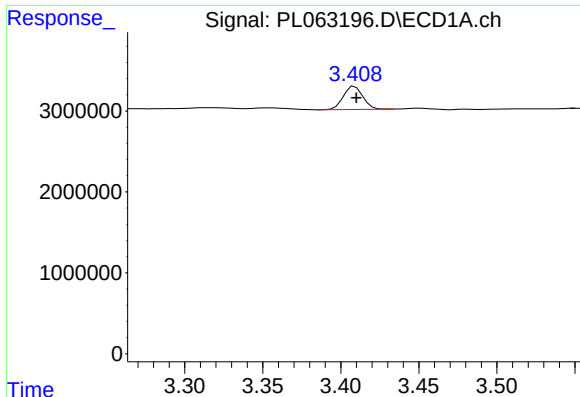


#1 Tetrachloro-m-xylene

R.T.: 3.408 min
Delta R.T.: -0.002 min
Response: 2517824
Conc: 1.48 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HD-02-112320


Manual Integrations
APPROVED

Ankita
11/25/2020 5:36:21 PM

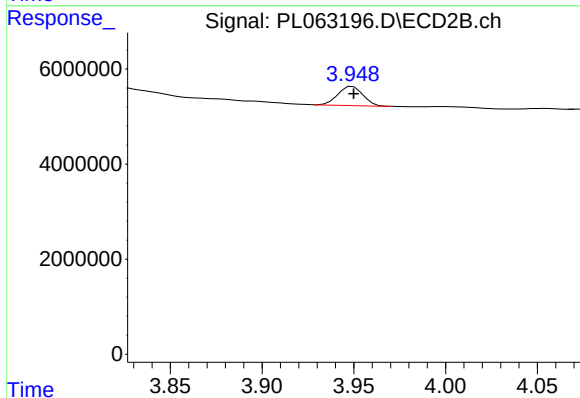


#1 Tetrachloro-m-xylene

R.T.: 3.948 min
Delta R.T.: -0.002 min
Response: 3859847
Conc: 1.18 ng/ml m

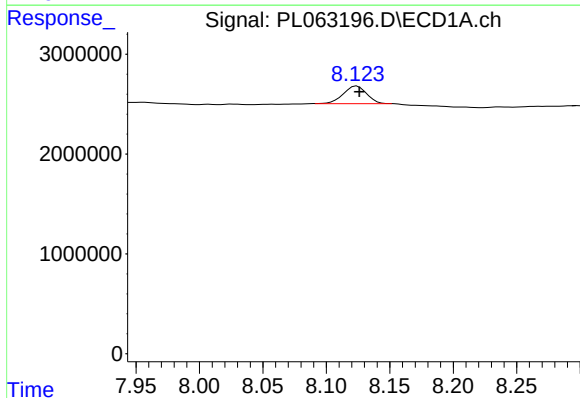

#28 Decachlorobiphenyl

R.T.: 8.123 min
Delta R.T.: -0.003 min
Response: 2252522
Conc: 1.21 ng/ml m

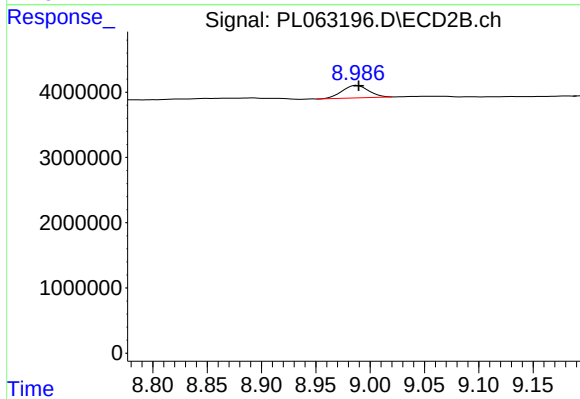

#28 Decachlorobiphenyl

R.T.: 8.986 min
Delta R.T.: -0.003 min
Response: 3280774
Conc: 1.38 ng/ml m