

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
 Data File : PL071144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 09:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 06:04:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
15) B	Endosulfa...	0.000	9.148f	0	1683443	N.D. 1.378 #
17) MA	4,4'-DDT	8.421	9.376f	428697	964794	0.779 0.765
20) A	Methoxychlor	9.007	0.000	247038	0	0.675 N.D. #
21) B	Endrin ke...	9.223	0.000	403788	0	0.565 N.D. #
22)	Mirex	0.000	10.455	0	2140072	N.D. 2.055 #
23)	Chlordane-1	5.866f	0.000	20243	0	1.187 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
Data File : PL071144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 09:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 06:04:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

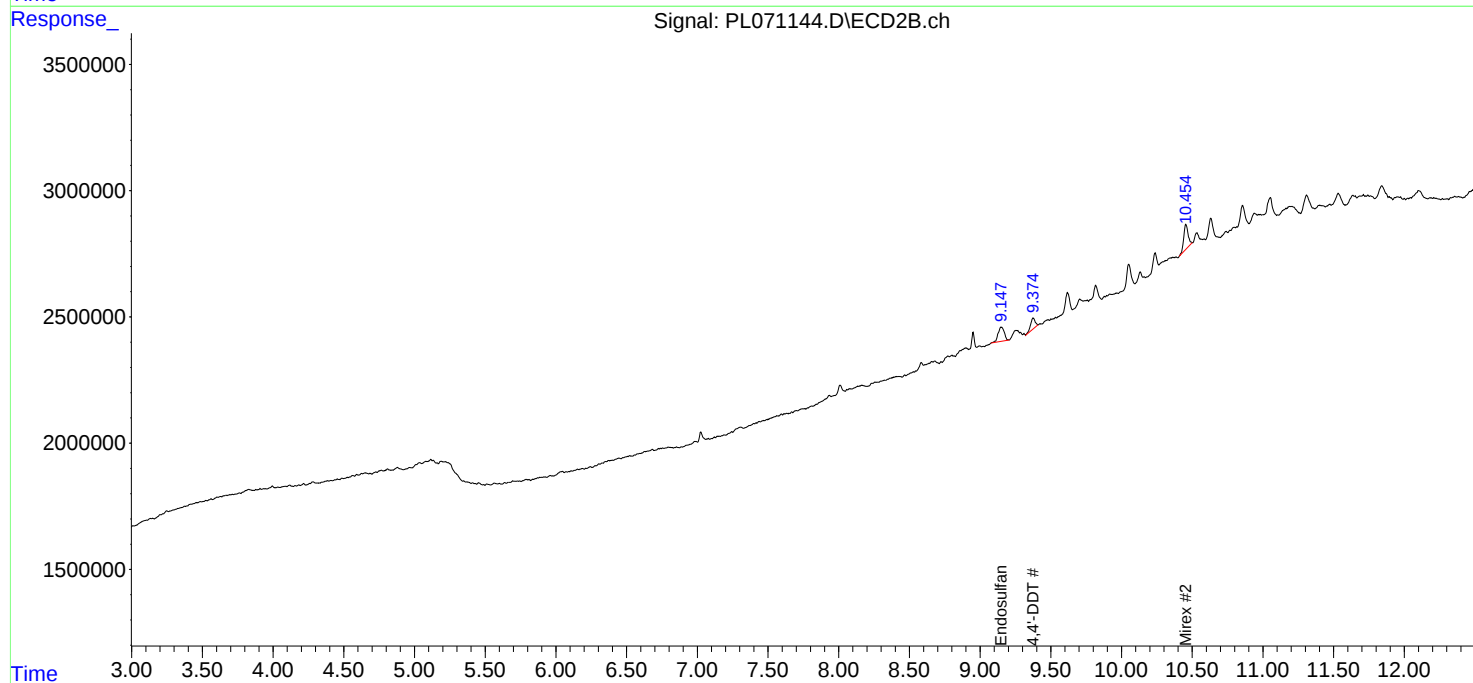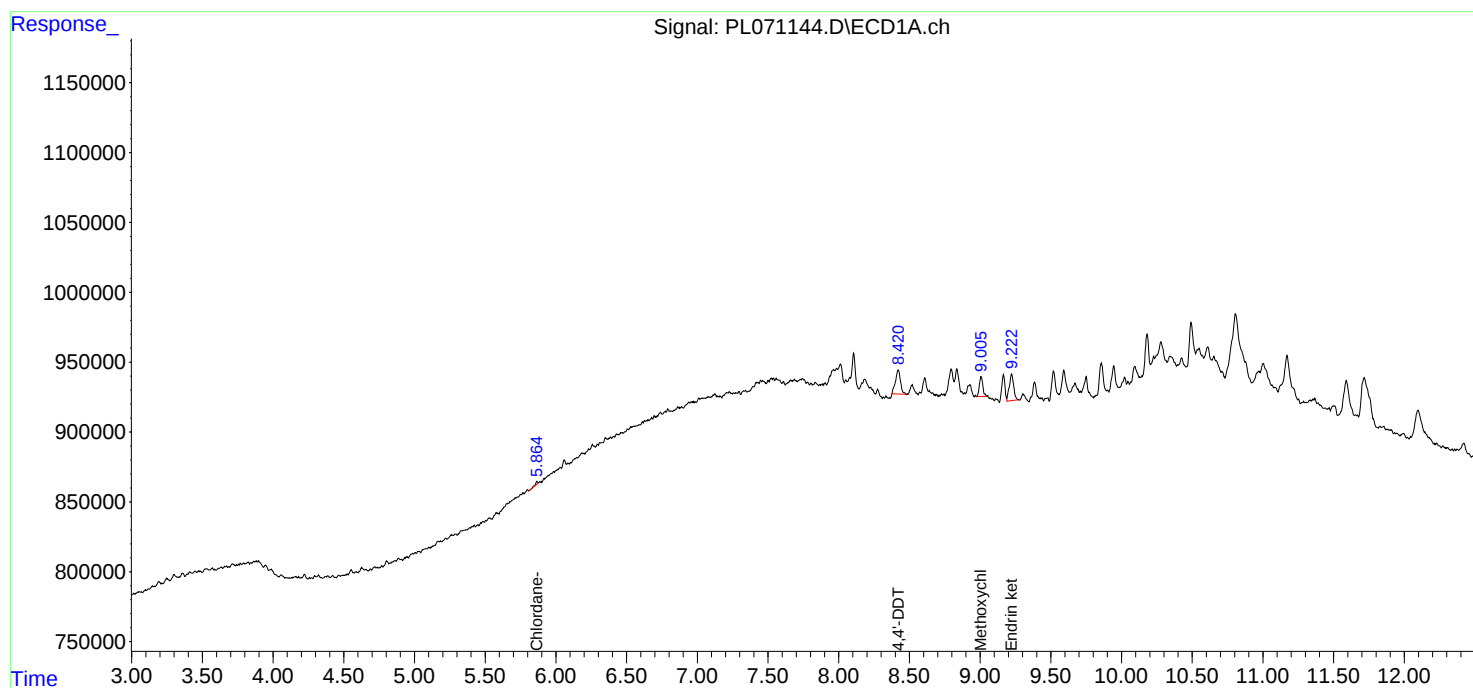


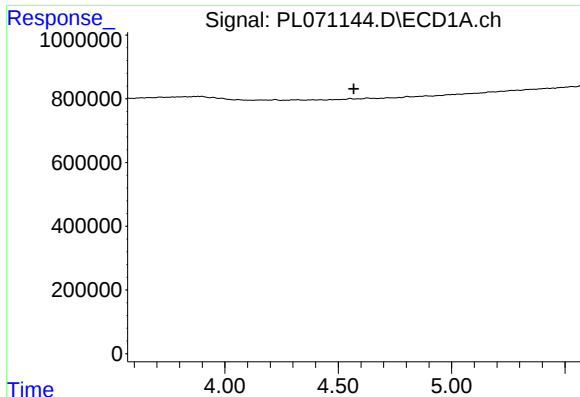

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

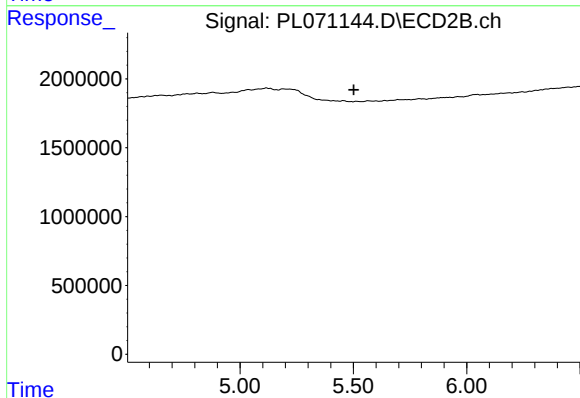

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.294 min
Response: 0
Conc: N.D.

#15 Endosulfan II


R.T.: 9.148 min
Delta R.T.: 0.022 min
Response: 1683443
Conc: 1.38 ng/ml

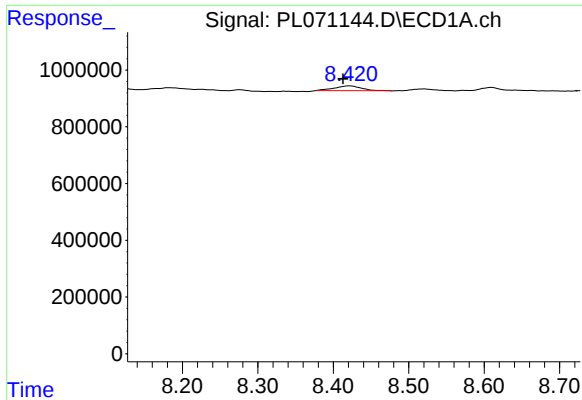

#17 4,4'-DDT


R.T.: 8.421 min
Delta R.T.: 0.008 min
Response: 428697
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

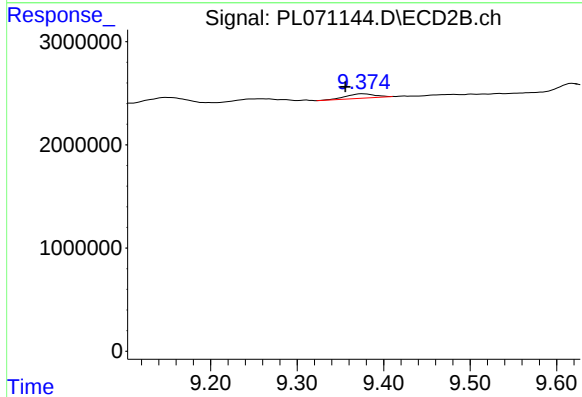


#17 4,4'-DDT

R.T.: 9.376 min
Delta R.T.: 0.021 min
Response: 964794
Conc: 0.76 ng/ml

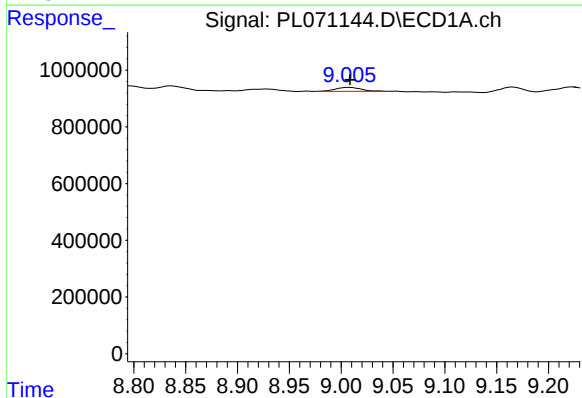


#20 Methoxychlor

R.T.: 9.007 min
Delta R.T.: -0.001 min
Response: 247038
Conc: 0.68 ng/ml

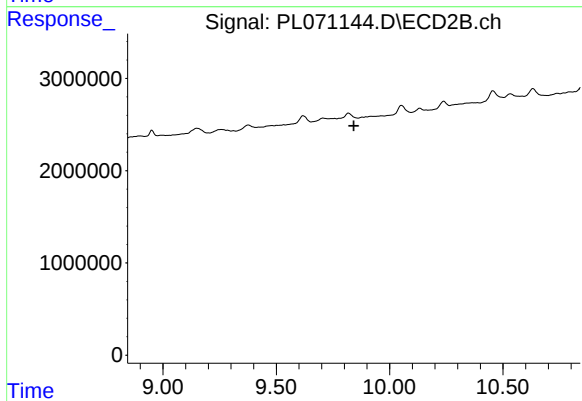

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.842 min
Response: 0
Conc: N.D.

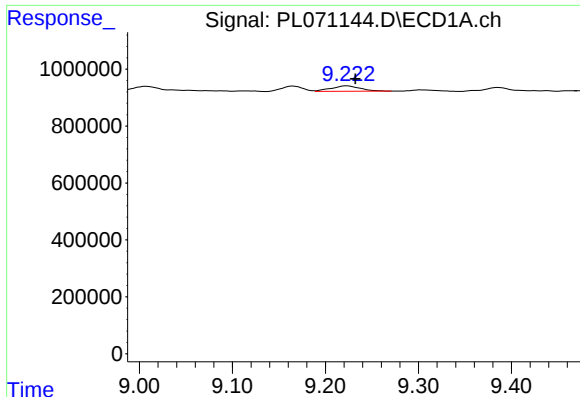

#21 Endrin ketone


R.T.: 9.223 min
Delta R.T.: -0.009 min
Response: 403788
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

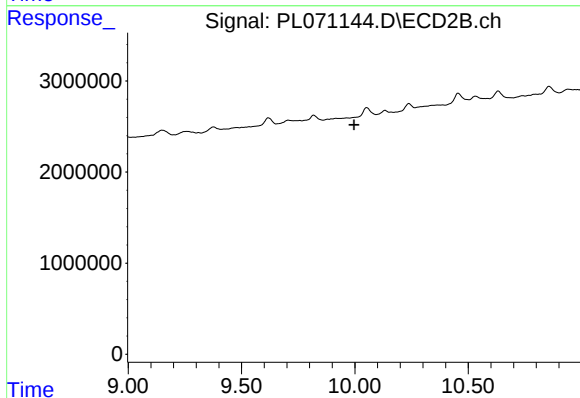


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.996 min
Response: 0
Conc: N.D.

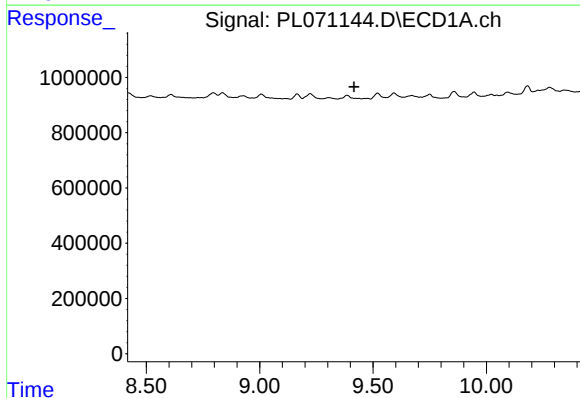


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.417 min
Response: 0
Conc: N.D.

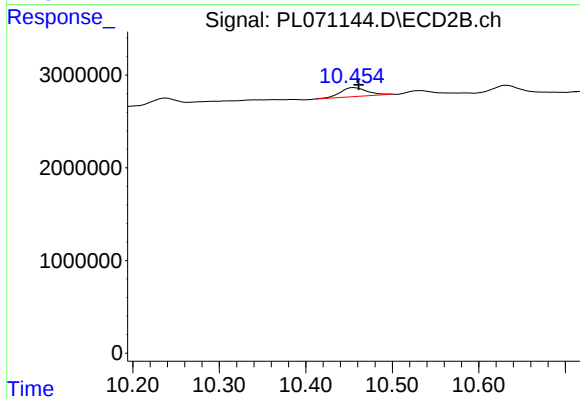

#22 Mirex


R.T.: 10.455 min
Delta R.T.: -0.006 min
Response: 2140072
Conc: 2.05 ng/ml

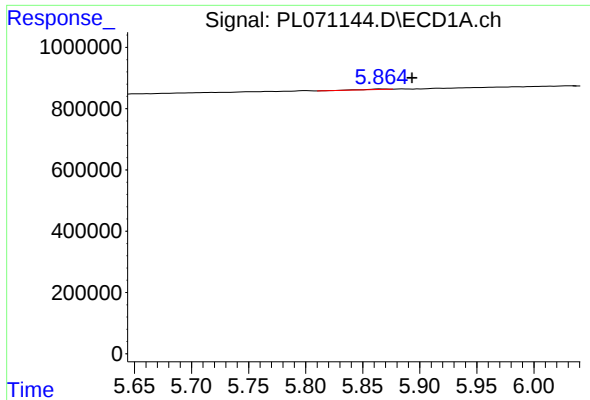

#23 Chlordane-1


R.T.: 5.866 min
Delta R.T.: -0.027 min
Response: 20243
Conc: 1.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

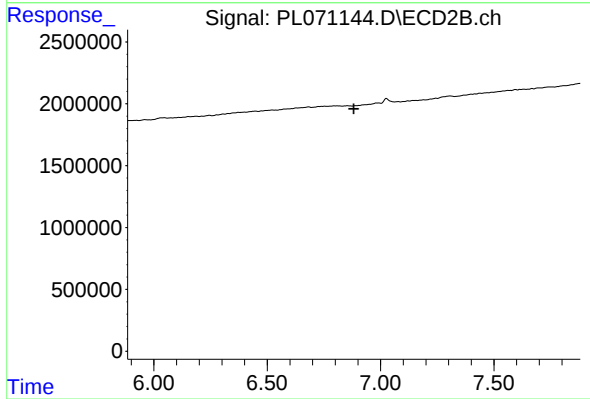


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

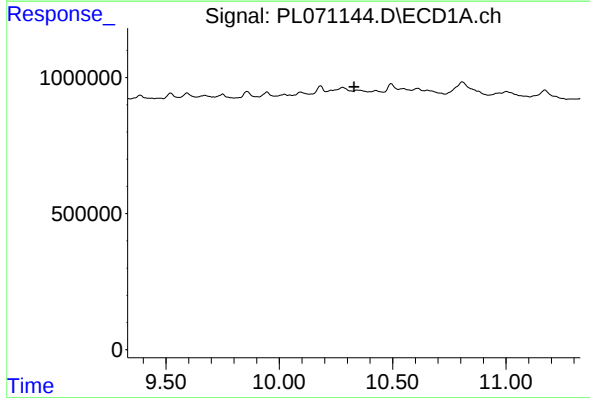

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.330 min
Response: 0
Conc: N.D.

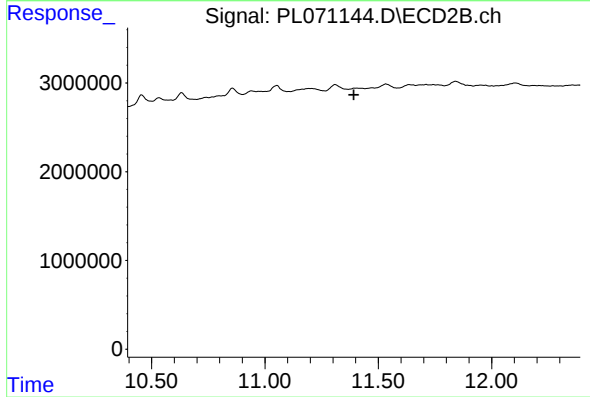

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.392 min
Response: 0
Conc: N.D.