

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
 Data File : PL071145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 09:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 06:04:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.569	5.503	9505447	23729827	19.407	18.820
28)	SA Decachlor...	10.331	11.395	13842681	23296242	20.259	17.419
Target Compounds							
2)	A alpha-BHC	5.254f	6.060f	239094	679444	0.357	0.369
20)	A Methoxychlor	9.028f	0.000	2589698	0	7.079	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
Data File : PL071145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 09:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 06:04:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

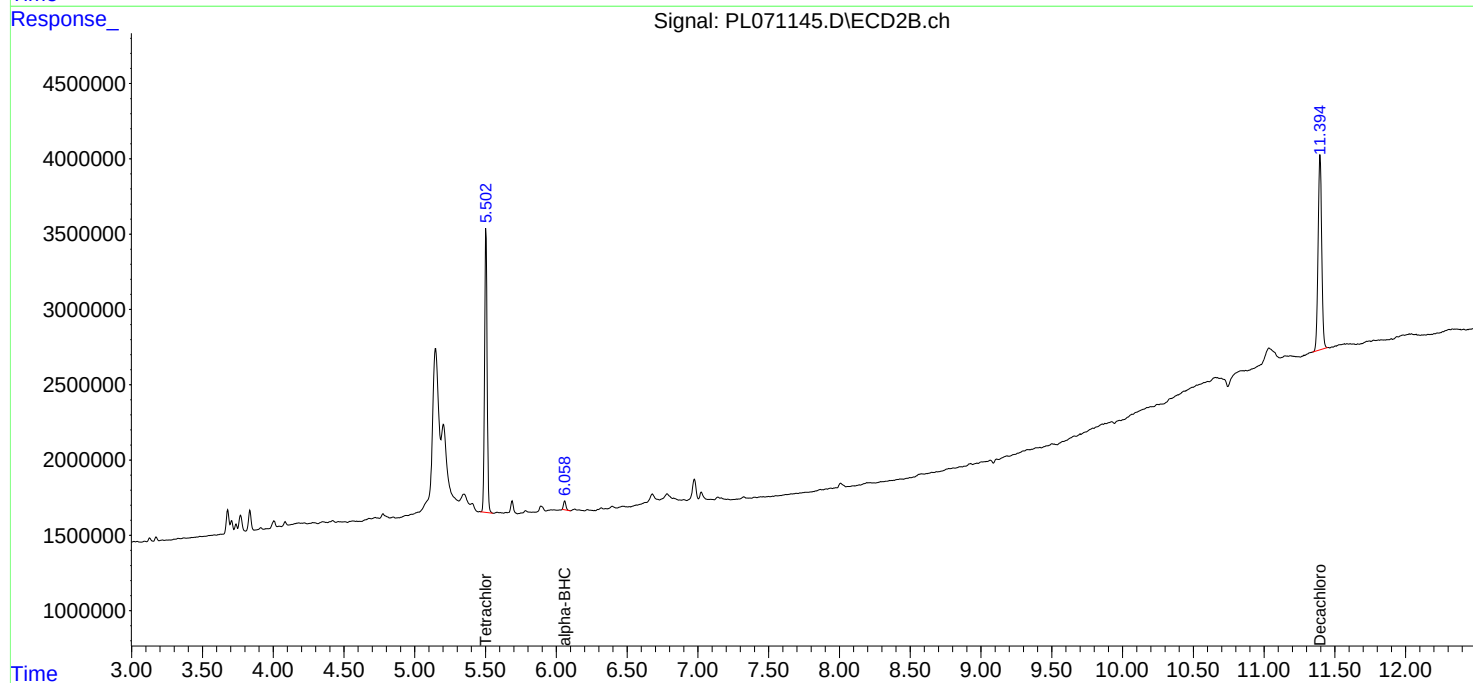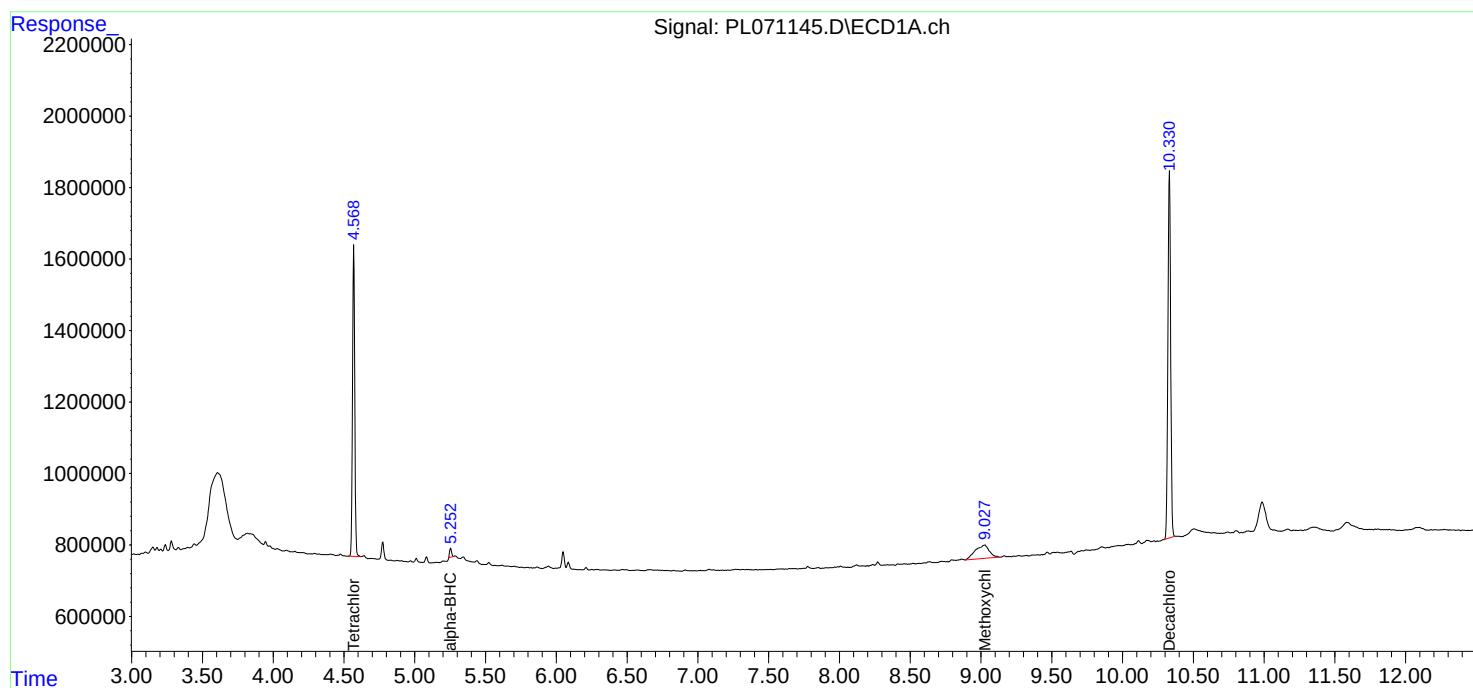


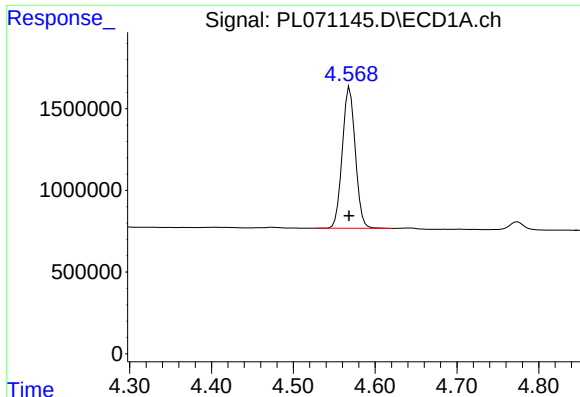

#1 Tetrachloro-m-xylene


R.T.: 4.569 min
Delta R.T.: 0.001 min
Response: 9505447
Conc: 19.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

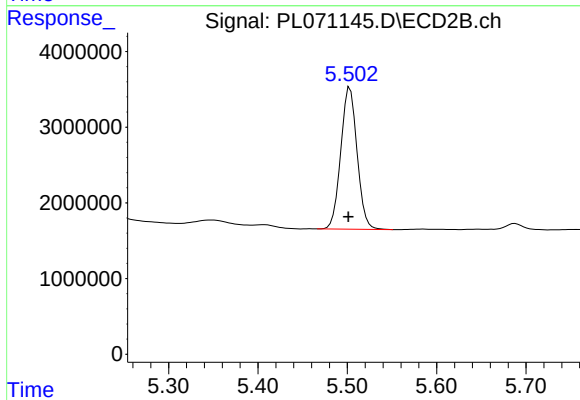


#1 Tetrachloro-m-xylene

R.T.: 5.503 min
Delta R.T.: 0.002 min
Response: 23729827
Conc: 18.82 ng/ml

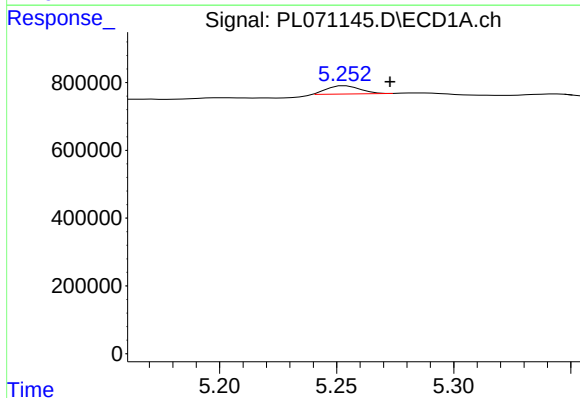


#2 alpha-BHC

R.T.: 5.254 min
Delta R.T.: -0.019 min
Response: 239094
Conc: 0.36 ng/ml

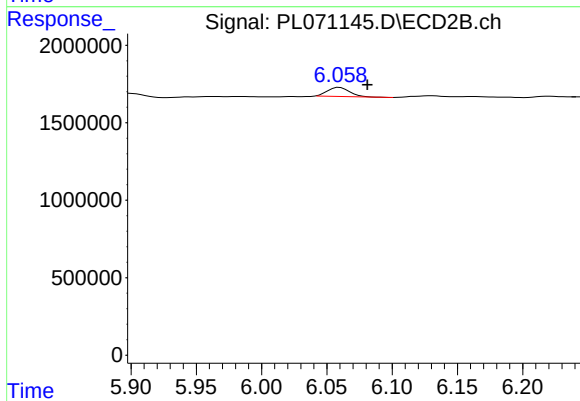

#2 alpha-BHC


R.T.: 6.060 min
Delta R.T.: -0.021 min
Response: 679444
Conc: 0.37 ng/ml

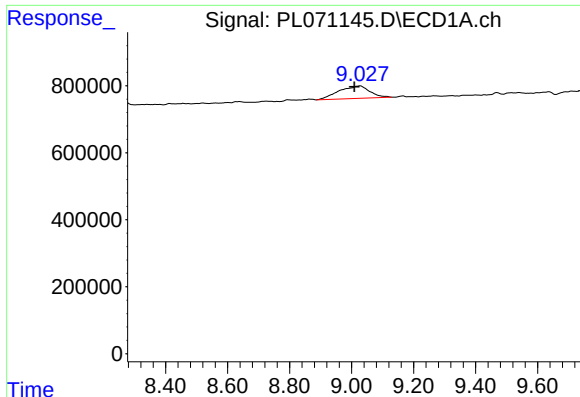

#20 Methoxychlor


R.T.: 9.028 min
Delta R.T.: 0.019 min
Response: 2589698
Conc: 7.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

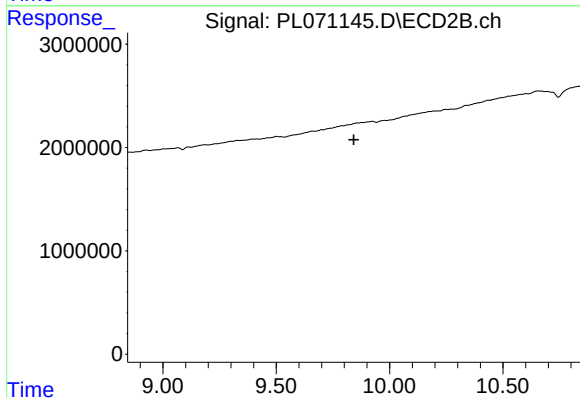


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.842 min
Response: 0
Conc: N.D.

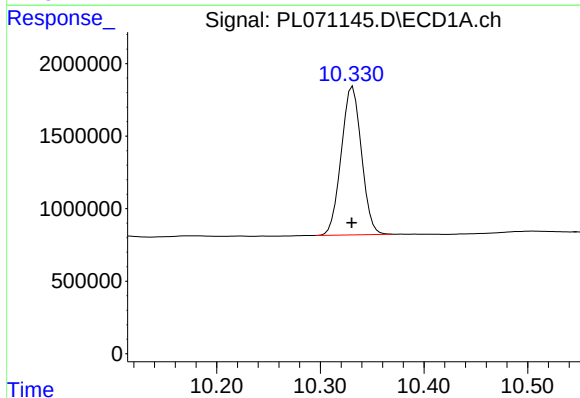

#28 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.000 min
Response: 13842681
Conc: 20.26 ng/ml

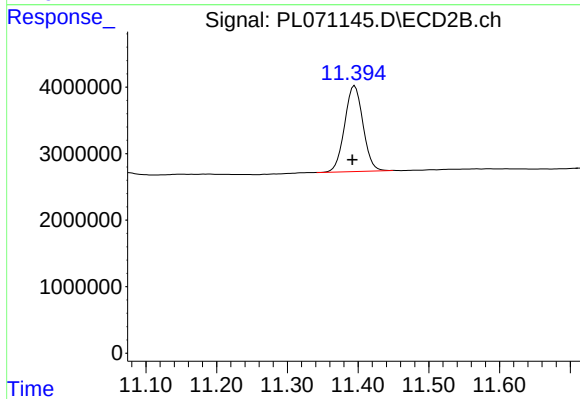

#28 Decachlorobiphenyl

R.T.: 11.395 min
Delta R.T.: 0.003 min
Response: 23296242
Conc: 17.42 ng/ml