

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
 Data File : PL071160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Nov 2021 16:50
 Operator : AR\AJ
 Sample : PB140995BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB140995BL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
 Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 05:08:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 04 19:28:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.563	5.499	9088412	24229674	18.555m	19.217
2) SA Decachlor...	10.326	11.389	14219352	26573709	20.810	19.870

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112421\
Data File : PL071160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Nov 2021 16:50
Operator : AR\AJ
Sample : PB140995BL
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB140995BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 05:08:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL110321.M
Quant Title : GC Extractables
QLast Update : Thu Nov 04 19:28:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

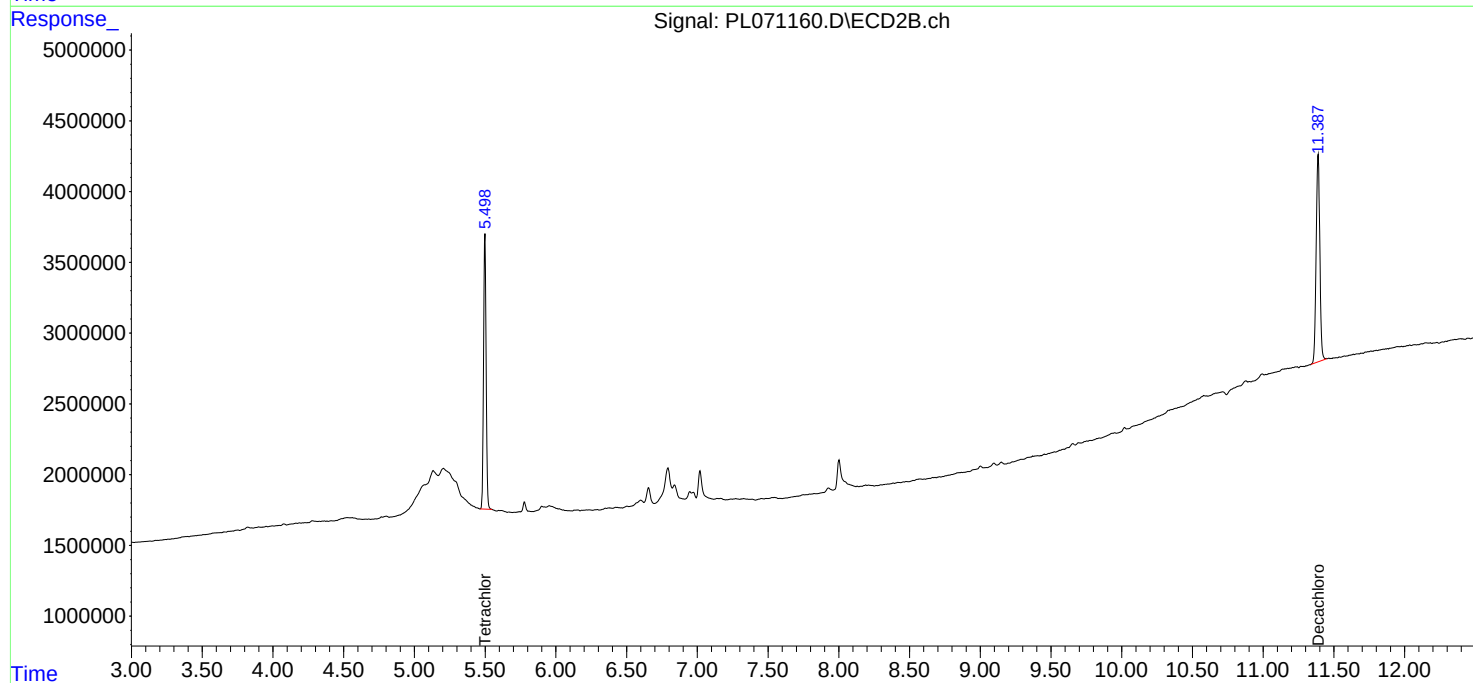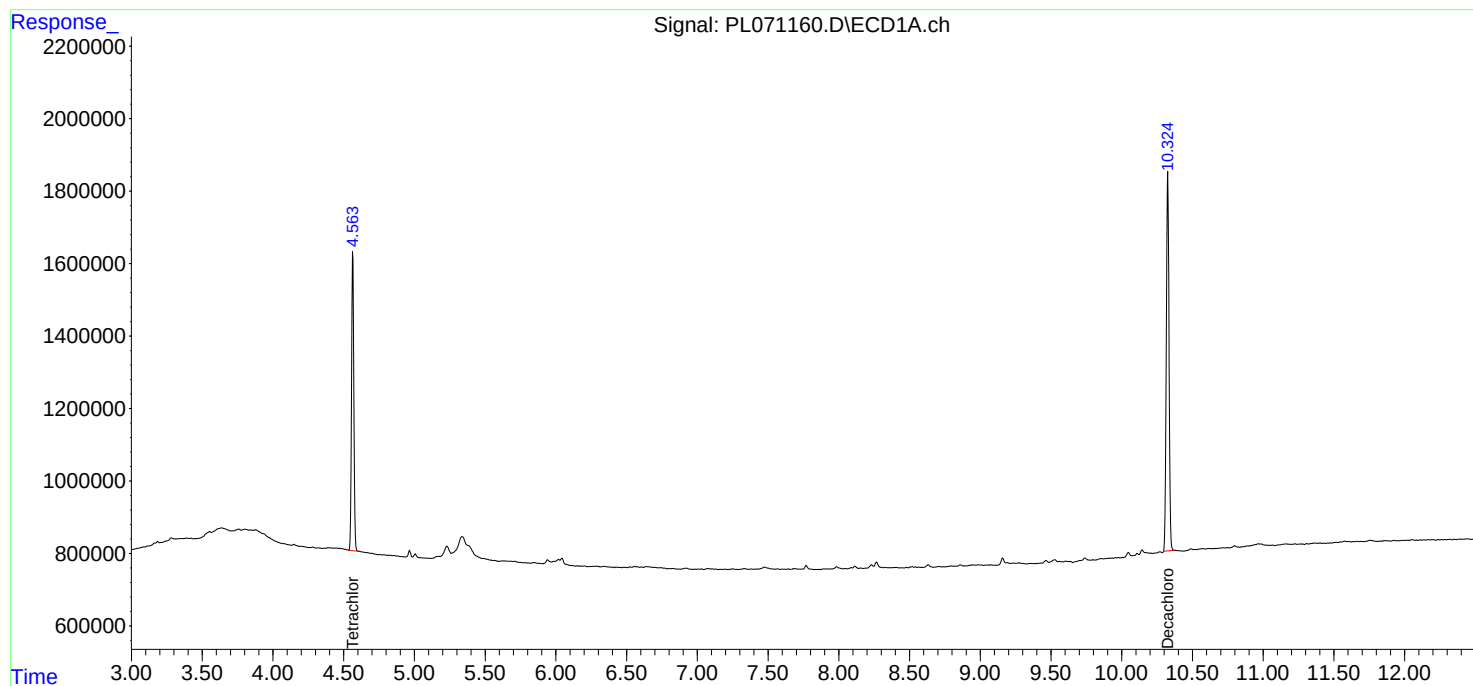

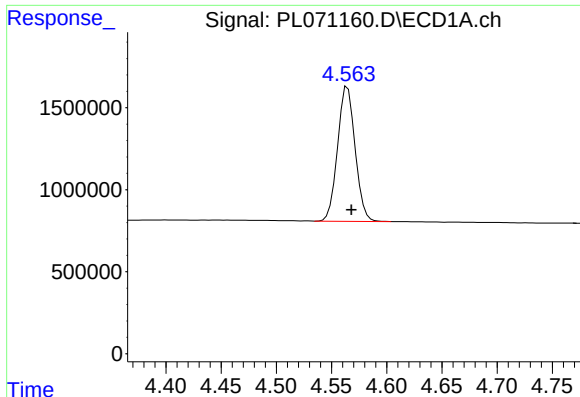


#1 Tetrachloro-m-xylene

R.T.: 4.563 min
Delta R.T.: -0.005 min
Response: 9088412
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB140995BL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/26/2021
Supervised By :mohammad ahmed 11/26/2021

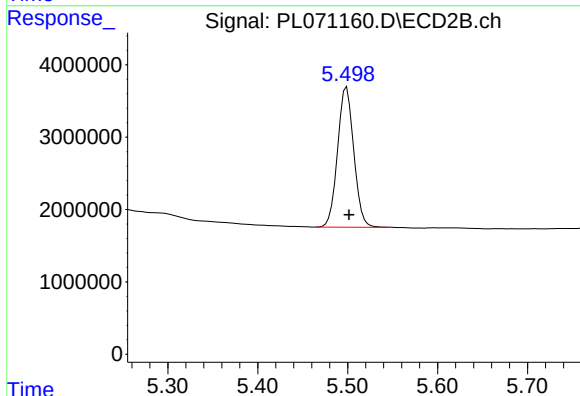


#1 Tetrachloro-m-xylene

R.T.: 5.499 min
Delta R.T.: -0.002 min
Response: 24229674
Conc: 19.22 ng/ml

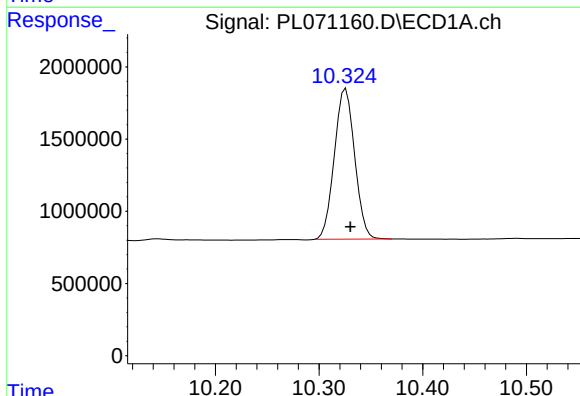

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: -0.004 min
Response: 14219352
Conc: 20.81 ng/ml

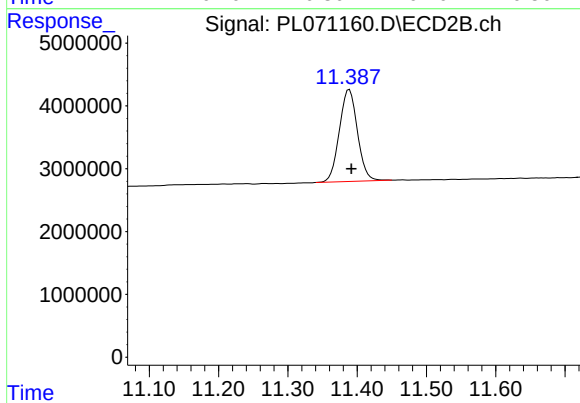

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.003 min
Response: 26573709
Conc: 19.87 ng/ml