

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112519\
 Data File : PL054586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2019 09:09
 Operator : SG\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 00:51:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 19 01:04:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.493f	0.000	15145989	0	2.356	N.D.	#
8) B	Heptachlo...	5.298f	0.000	51838255	0	4.014	N.D.	#
9) A	Endosulfan I	5.617	0.000	5441141	0	0.459	N.D.	#
10) B	gamma-Chl...	5.510	0.000	19885024	0	1.549	N.D.	#
11) B	alpha-Chl...	5.563	0.000	5627649	0	0.448	N.D.	#
22)	Mirex	7.489f	0.000	54908250	0	7.209	N.D.	#
24)	Chlordane-2	4.933	0.000	15001837	0	35.966	N.D.	#
25)	Chlordane-3	5.510	0.000	19885024	0	16.151	N.D.	#
26)	Chlordane-4	5.563	0.000	5627649	0	5.551	N.D.	#
27)	Chlordane-5	6.430f	0.000	70444644	0	190.992	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112519\
Data File : PL054586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2019 09:09
Operator : SG\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 00:51:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL111819.M
Quant Title : GC Extractables
QLast Update : Tue Nov 19 01:04:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

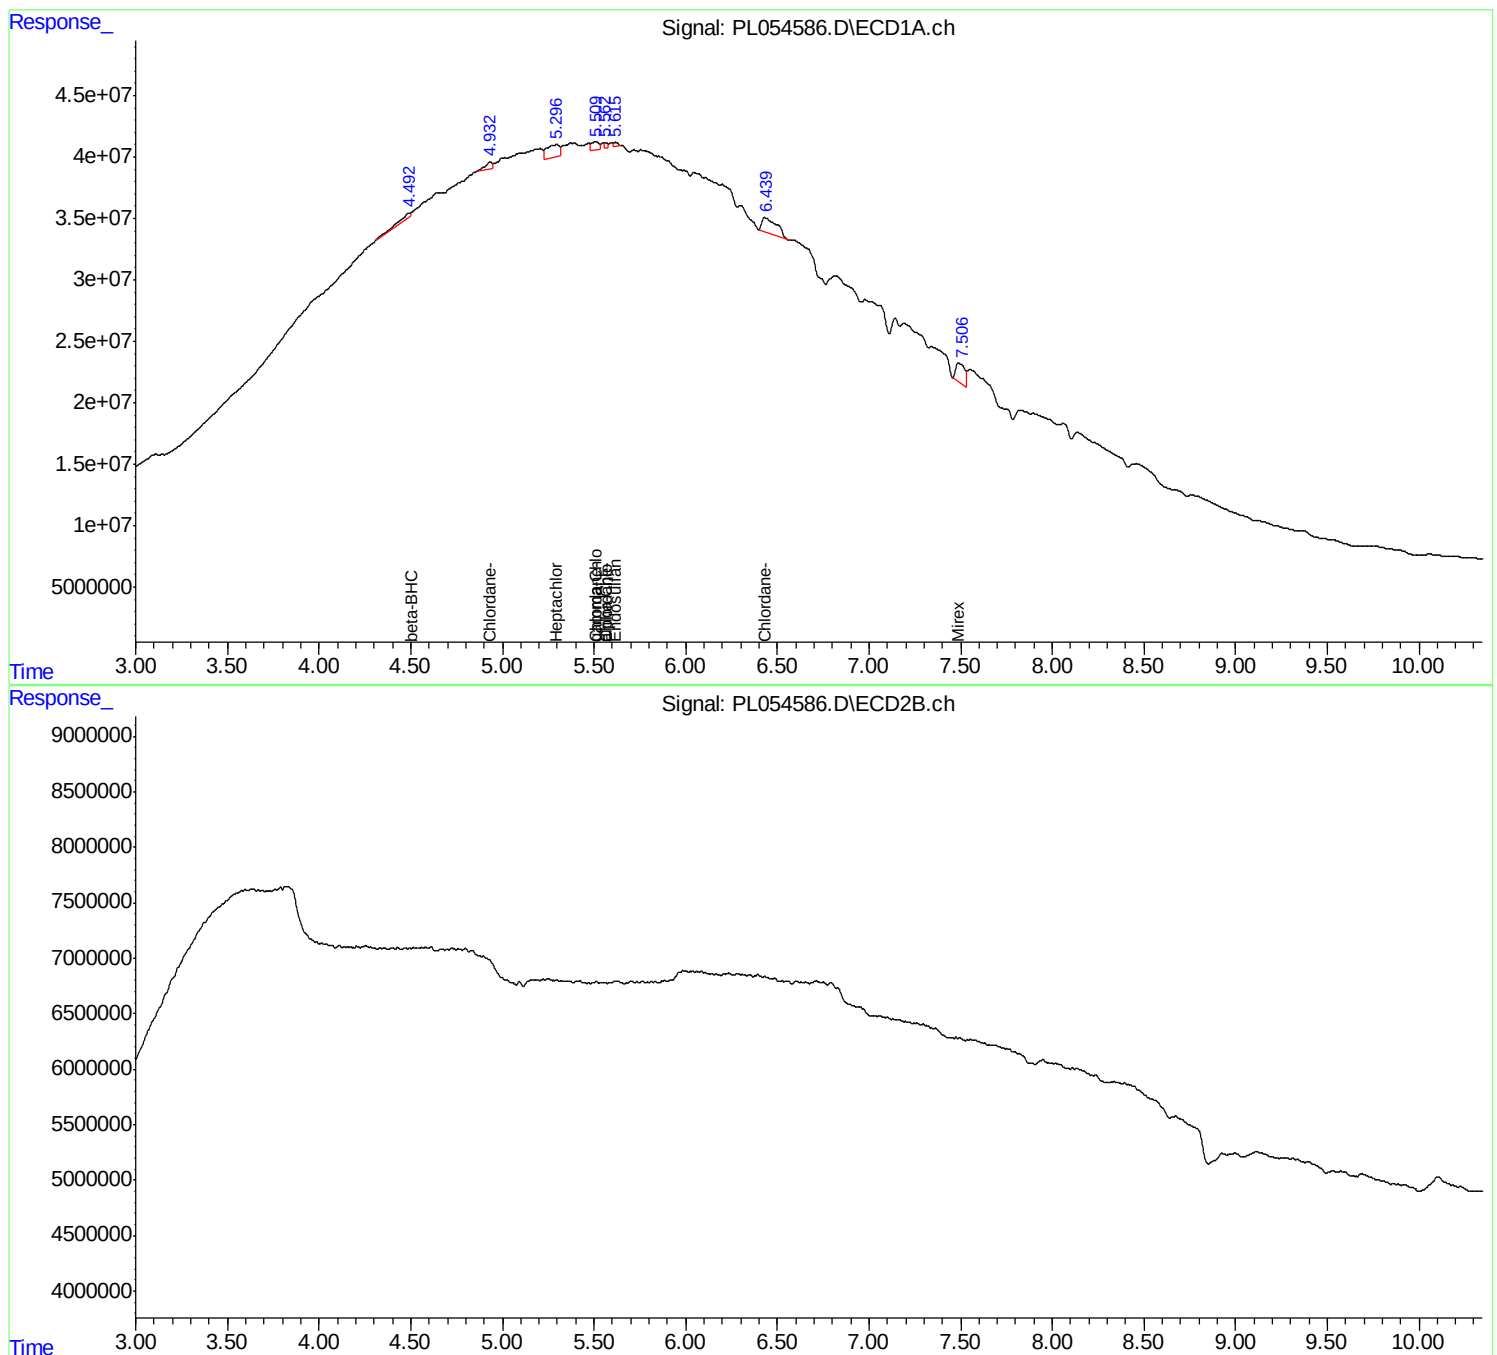


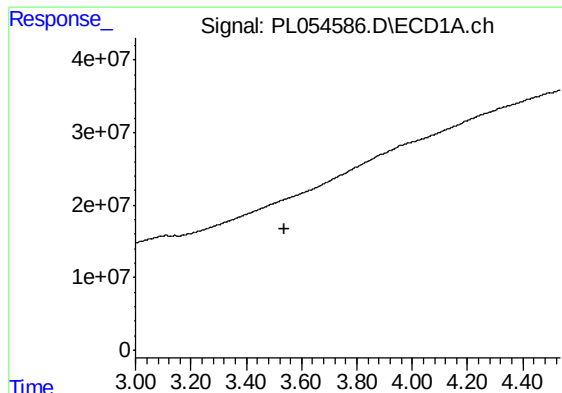

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

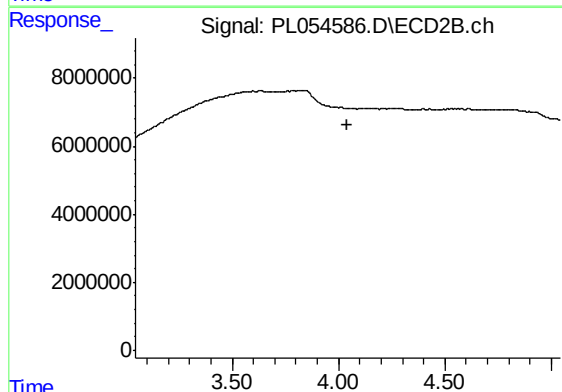


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.043 min
Response: 0
Conc: N.D.

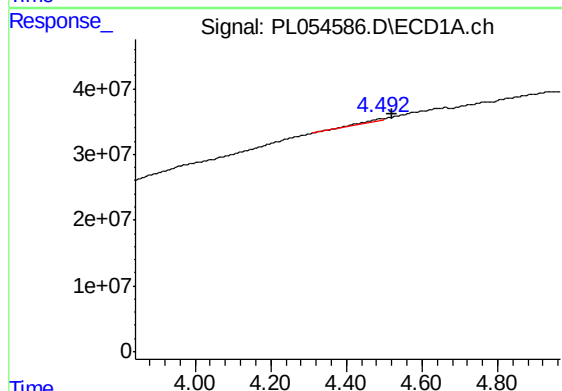


#6 beta-BHC

R.T.: 4.493 min
Delta R.T.: -0.026 min
Response: 15145989
Conc: 2.36 ng/ml

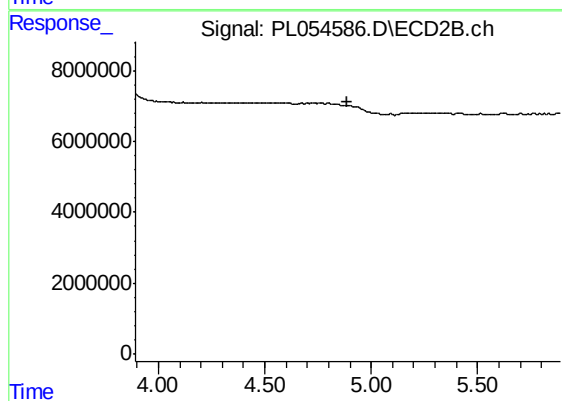

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.891 min
Response: 0
Conc: N.D.

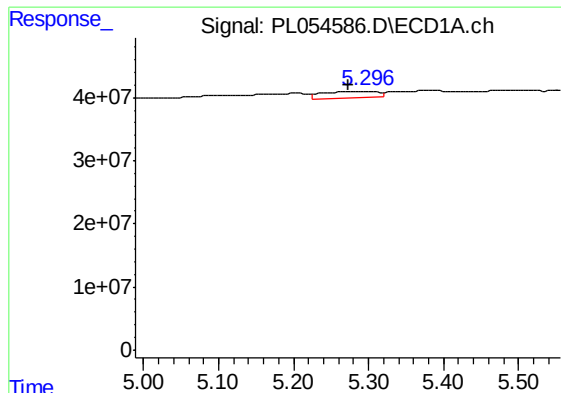

#8 Heptachlor epoxide


R.T.: 5.298 min
Delta R.T.: 0.025 min
Response: 51838255
Conc: 4.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

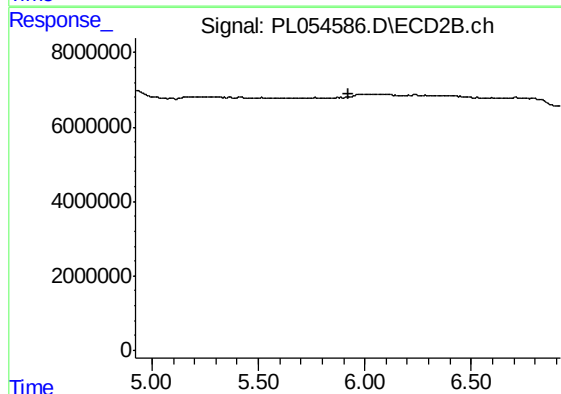


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.922 min
Response: 0
Conc: N.D.

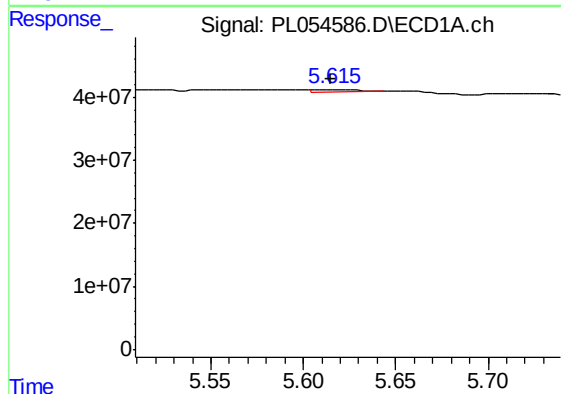


#9 Endosulfan I

R.T.: 5.617 min
Delta R.T.: 0.002 min
Response: 5441141
Conc: 0.46 ng/ml

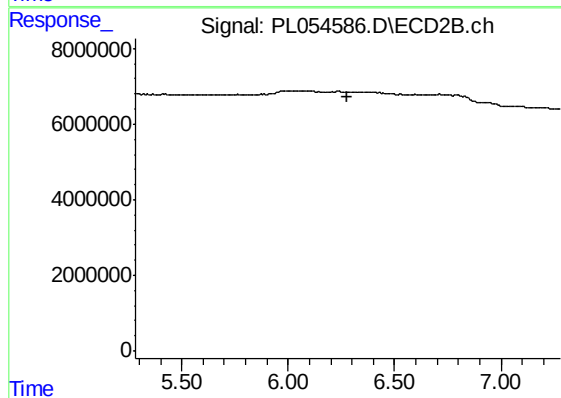

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

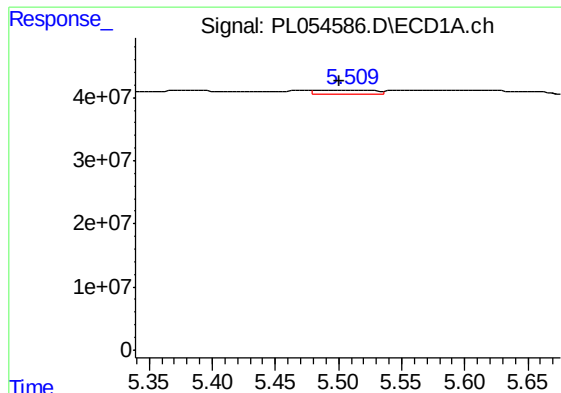

#10 gamma-Chlordane


R.T.: 5.510 min
Delta R.T.: 0.009 min
Response: 19885024
Conc: 1.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

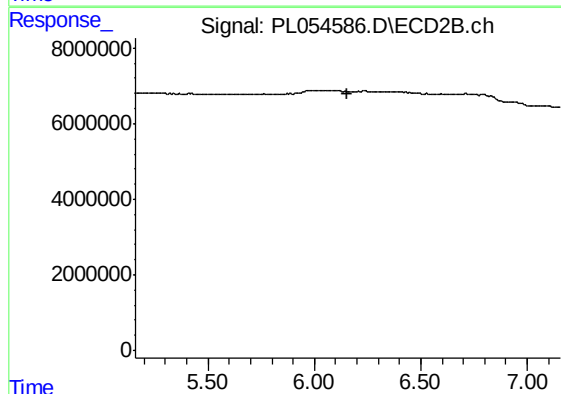


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.156 min
Response: 0
Conc: N.D.

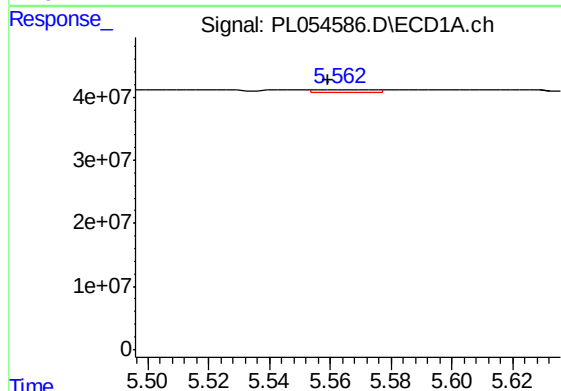


#11 alpha-Chlordane

R.T.: 5.563 min
Delta R.T.: 0.004 min
Response: 5627649
Conc: 0.45 ng/ml

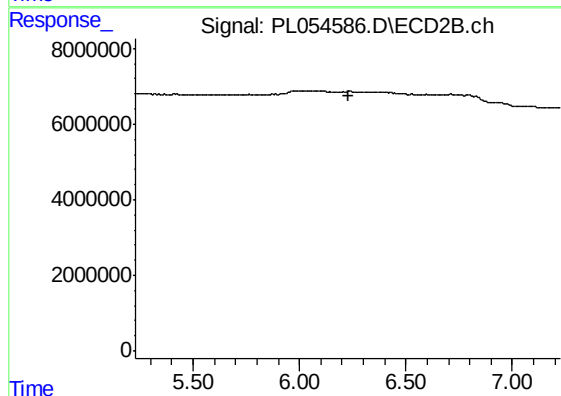

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.229 min
Response: 0
Conc: N.D.

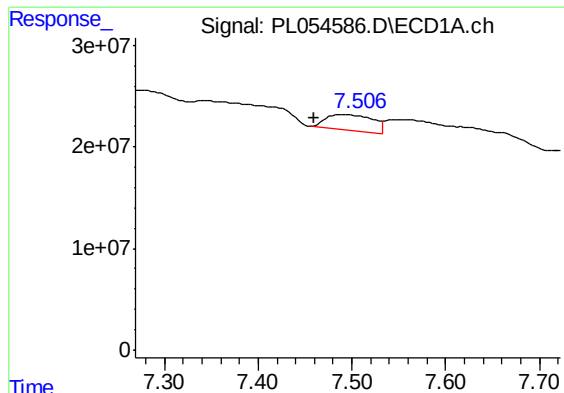

#22 Mirex


R.T.: 7.489 min
Delta R.T.: 0.029 min
Response: 54908250
Conc: 7.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

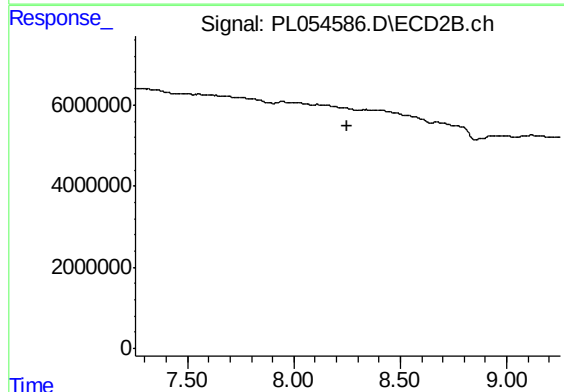


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.253 min
Response: 0
Conc: N.D.

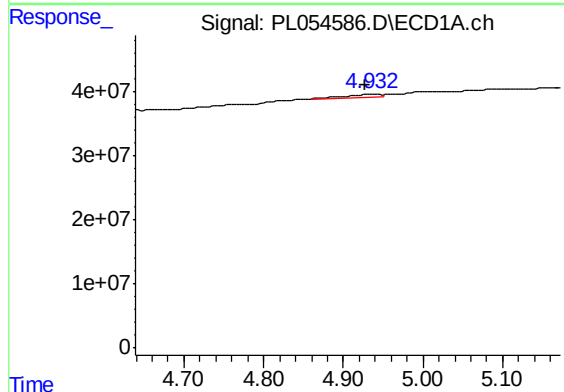


#24 Chlordane-2

R.T.: 4.933 min
Delta R.T.: 0.006 min
Response: 15001837
Conc: 35.97 ng/ml

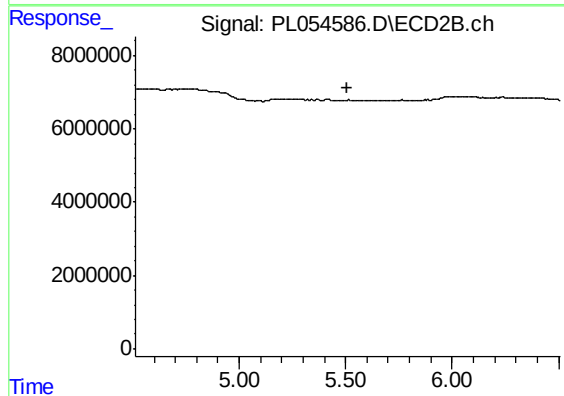

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.510 min
Response: 0
Conc: N.D.

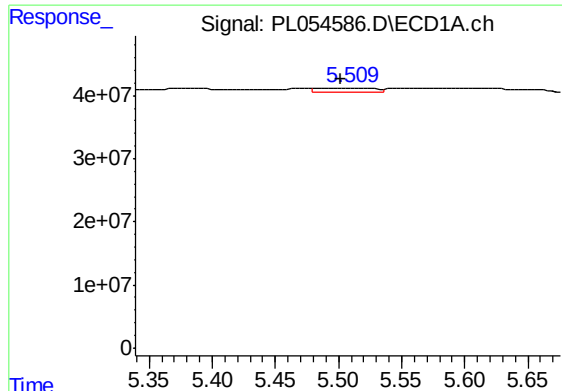

#25 Chlordane-3


R.T.: 5.510 min
Delta R.T.: 0.008 min
Response: 19885024
Conc: 16.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

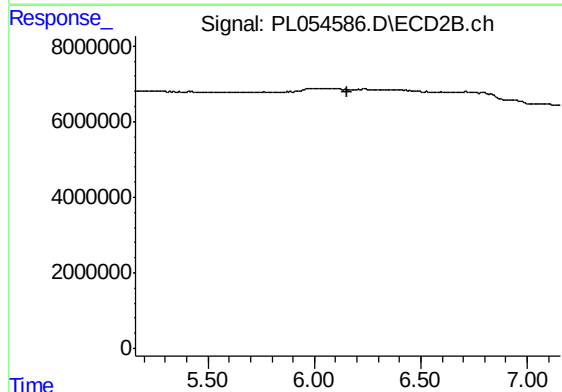


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.156 min
Response: 0
Conc: N.D.

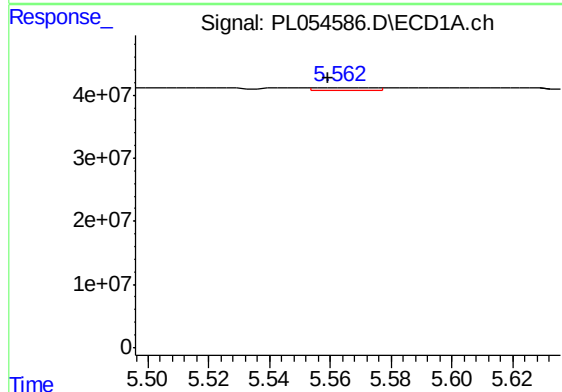


#26 Chlordane-4

R.T.: 5.563 min
Delta R.T.: 0.004 min
Response: 5627649
Conc: 5.55 ng/ml

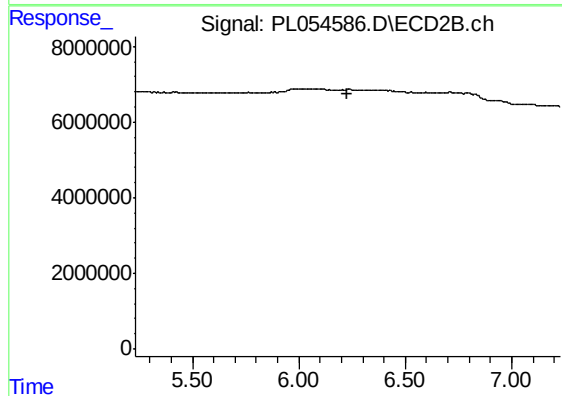

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.230 min
Response: 0
Conc: N.D.

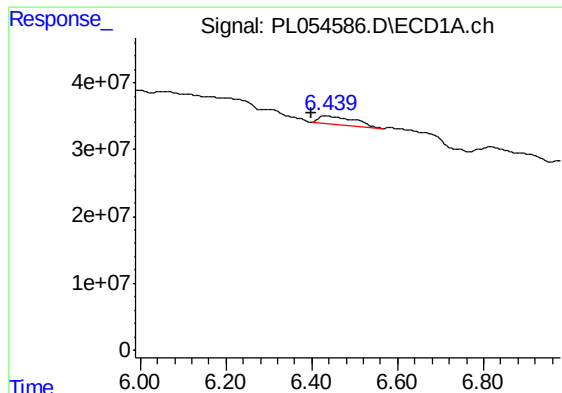

#27 Chlordane-5


R.T.: 6.430 min
Delta R.T.: 0.030 min
Response: 70444644
Conc: 190.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

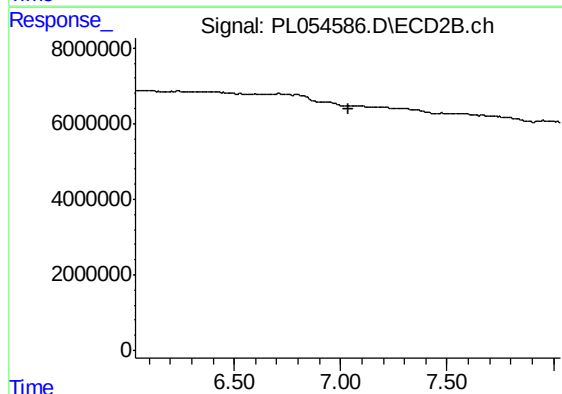


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.035 min
Response: 0
Conc: N.D.

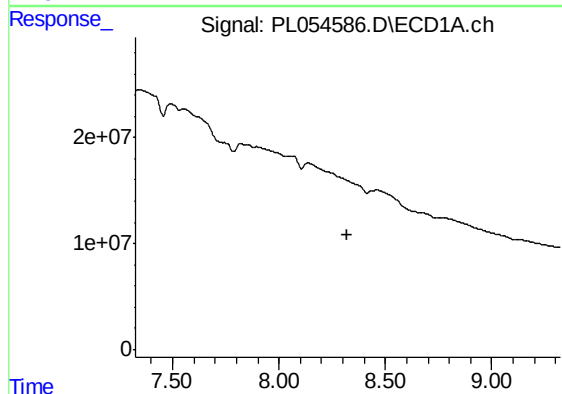

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.323 min
Response: 0
Conc: N.D.

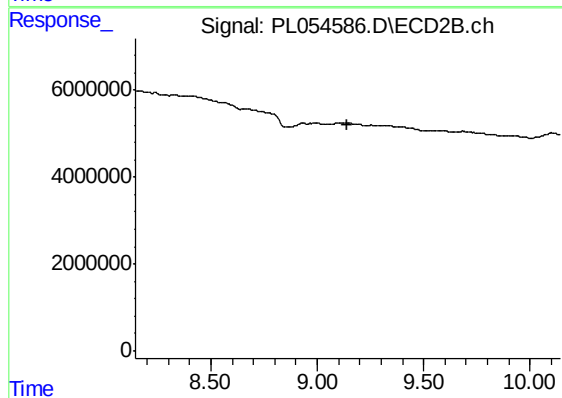

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.143 min
Response: 0
Conc: N.D.