

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
 Data File : PL093238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 12:38
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:34:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 13:29:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.773	244.3E6	357.1E6	97.301	98.777
28)	SA Decachlor...	9.053	7.912	163.1E6	277.1E6	95.756	96.606
Target Compounds							
23)	Chlordane-1	4.698	3.770	105.9E6	118.6E6	958.886	990.864
24)	Chlordane-2	5.227	4.348	105.3E6	131.7E6	948.416	972.800
25)	Chlordane-3	5.938	4.977	364.7E6	413.7E6	972.169	991.849
26)	Chlordane-4	6.020	5.041	439.7E6	393.8E6	969.294	975.160
27)	Chlordane-5	6.869	5.937	84856770	139.7E6	953.016	989.007



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
Data File : PL093238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 12:38
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:34:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 13:29:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

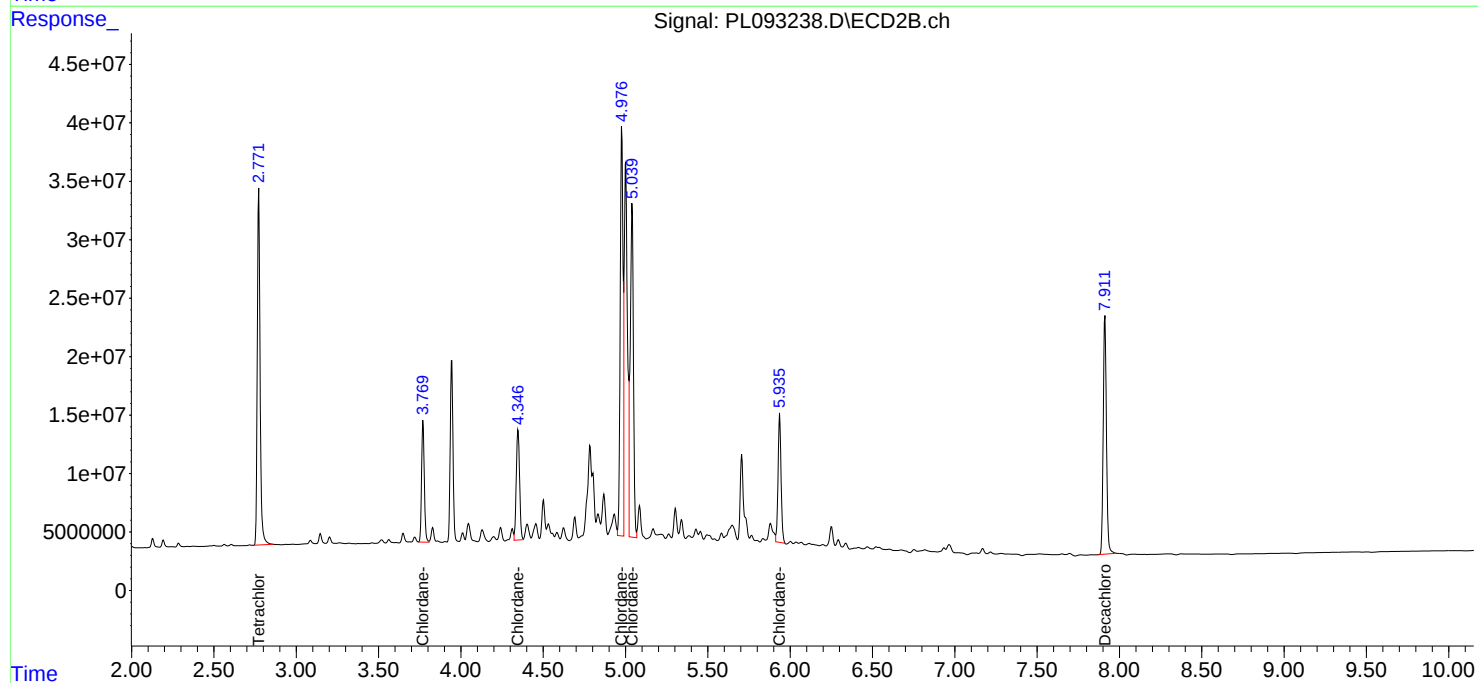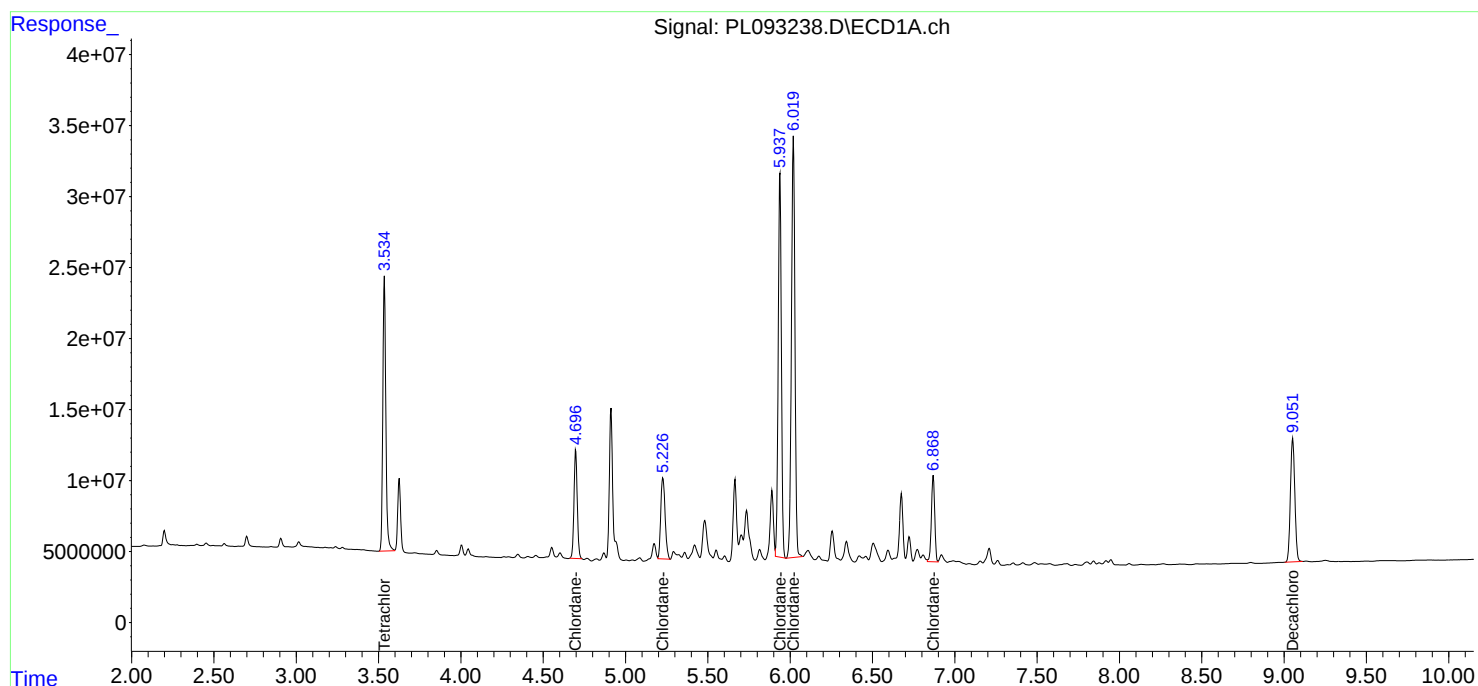


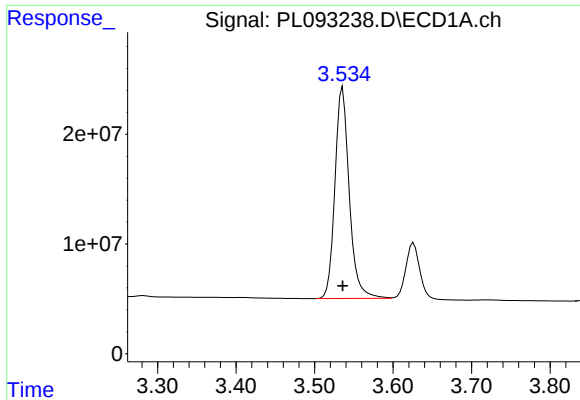

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 244332311
Conc: 97.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

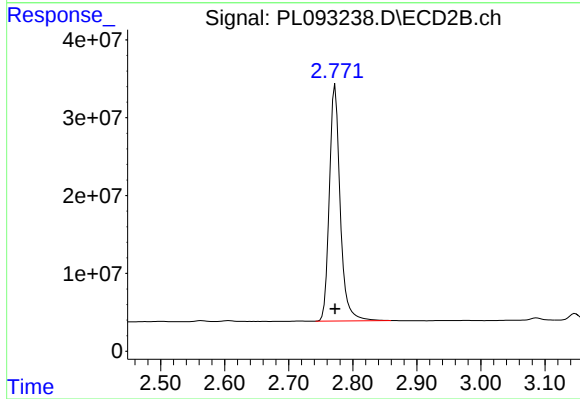


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 357112302
Conc: 98.78 ng/ml

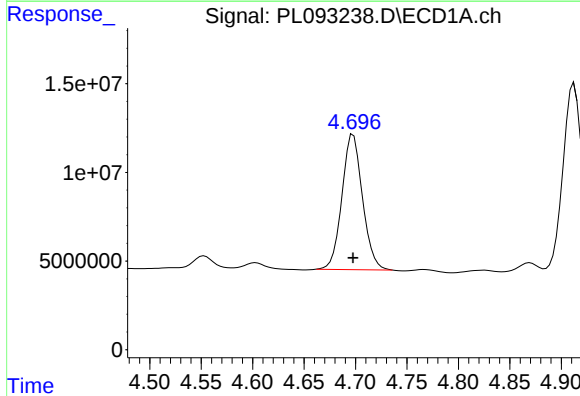


#23 Chlordane-1

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 105891892
Conc: 958.89 ng/ml

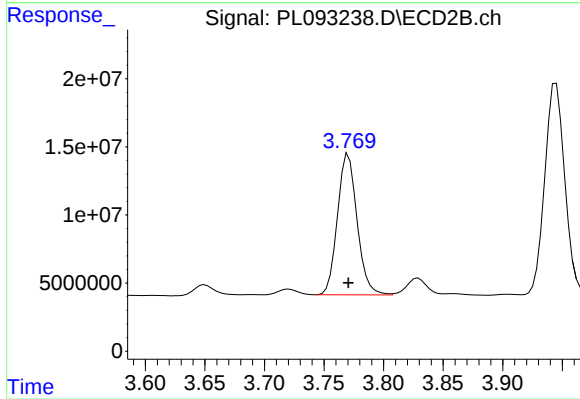

#23 Chlordane-1


R.T.: 3.770 min
Delta R.T.: 0.000 min
Response: 118573395
Conc: 990.86 ng/ml

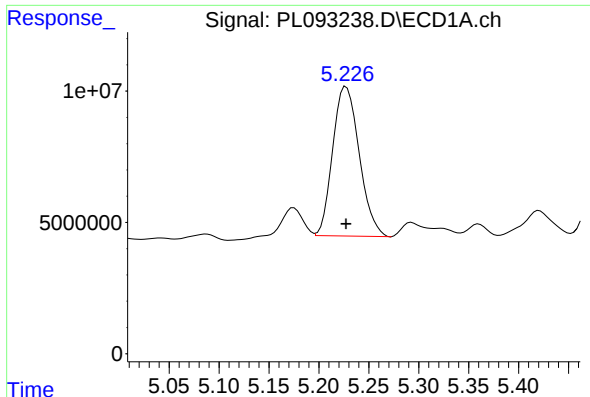

#24 Chlordane-2


R.T.: 5.227 min
Delta R.T.: 0.000 min
Response: 105315024
Conc: 948.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

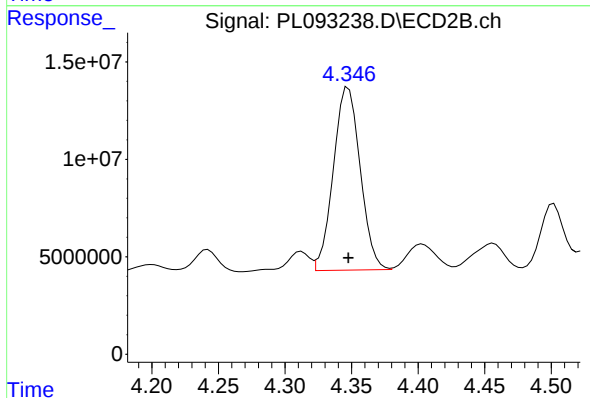


#24 Chlordane-2

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 131728774
Conc: 972.80 ng/ml

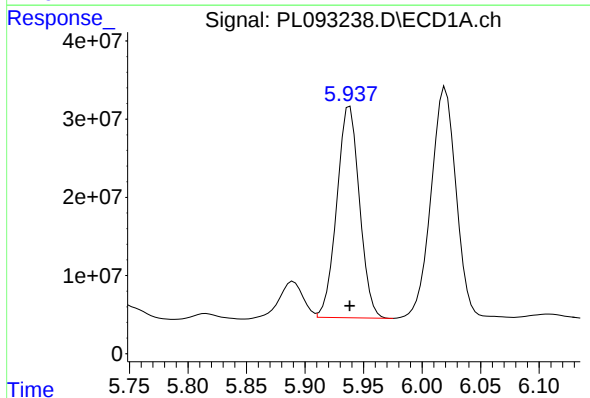


#25 Chlordane-3

R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 364706892
Conc: 972.17 ng/ml

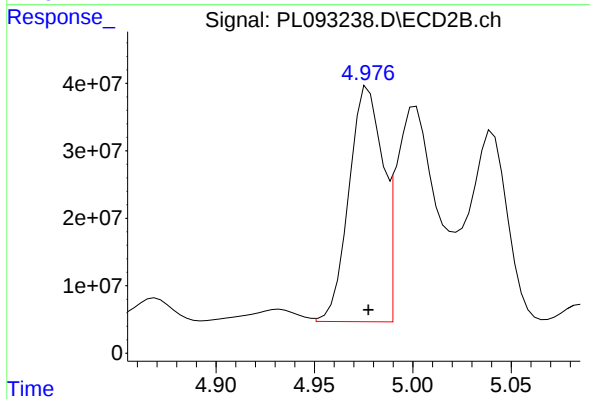

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 413713255
Conc: 991.85 ng/ml

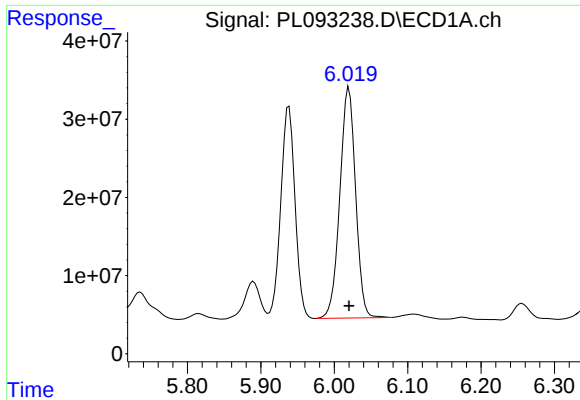

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 439703250
Conc: 969.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

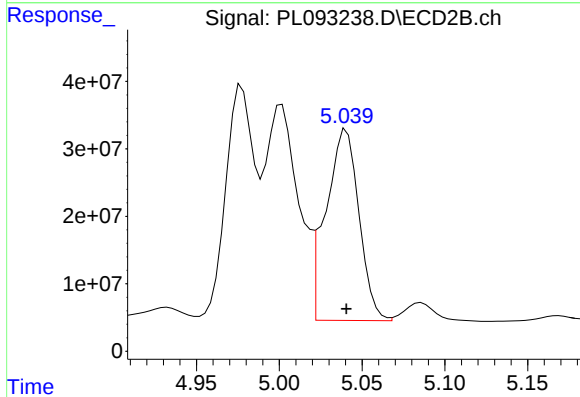


#26 Chlordane-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 393770272
Conc: 975.16 ng/ml

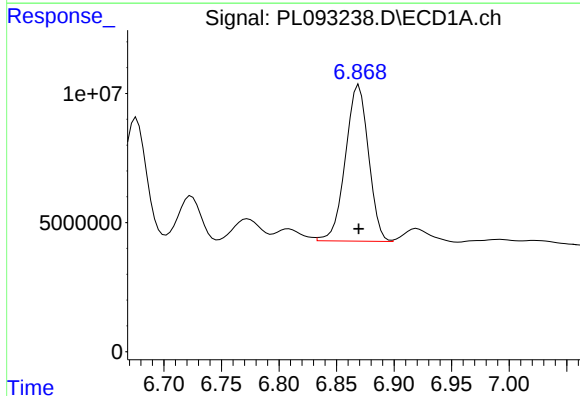


#27 Chlordane-5

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 84856770
Conc: 953.02 ng/ml

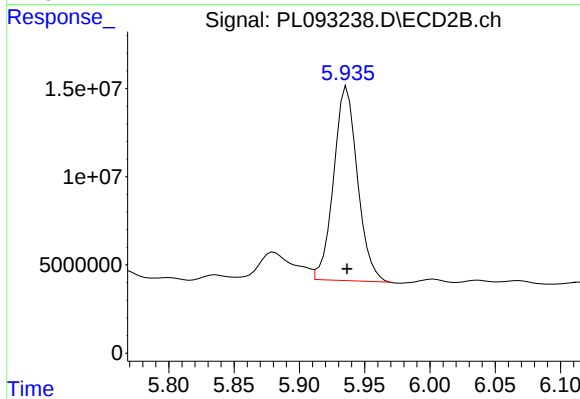

#27 Chlordane-5


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 139652556
Conc: 989.01 ng/ml

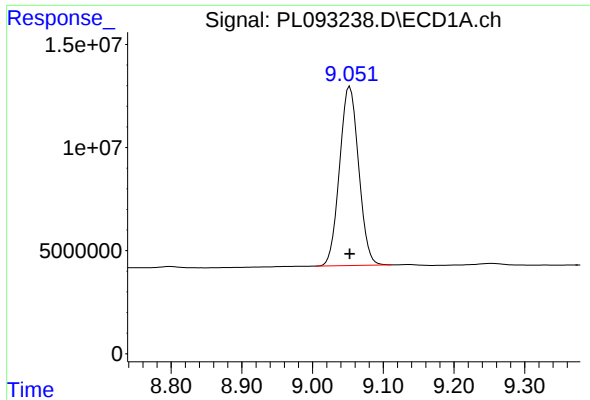

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 163074211
Conc: 95.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

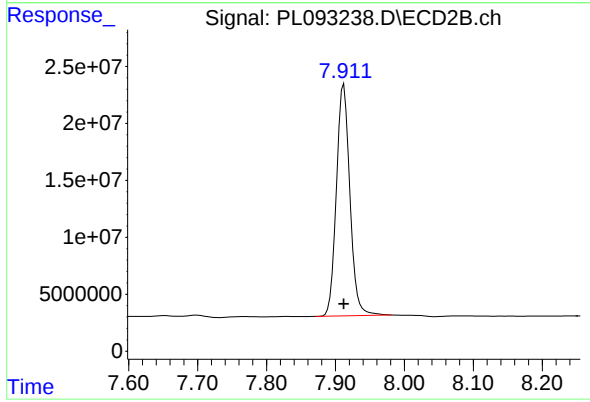

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 277117814
Conc: 96.61 ng/ml