

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
 Data File : PL093239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 12:51
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:36:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 13:29:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.772	190.2E6	276.2E6	75.489	75.930
28)	SA Decachlor...	9.053	7.912	130.1E6	217.5E6	75.940	75.554
Target Compounds							
23)	Chlordane-1	4.698	3.771	83102532	91485472	751.679	759.607
24)	Chlordane-2	5.228	4.347	83380643	102.8E6	750.590	756.189
25)	Chlordane-3	5.938	4.977	284.9E6	317.3E6	756.303	757.116
26)	Chlordane-4	6.020	5.040	343.8E6	312.6E6	755.293	765.889
27)	Chlordane-5	6.869	5.936	67442934	107.7E6	754.946	758.575



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
Data File : PL093239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 12:51
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:36:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 13:29:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

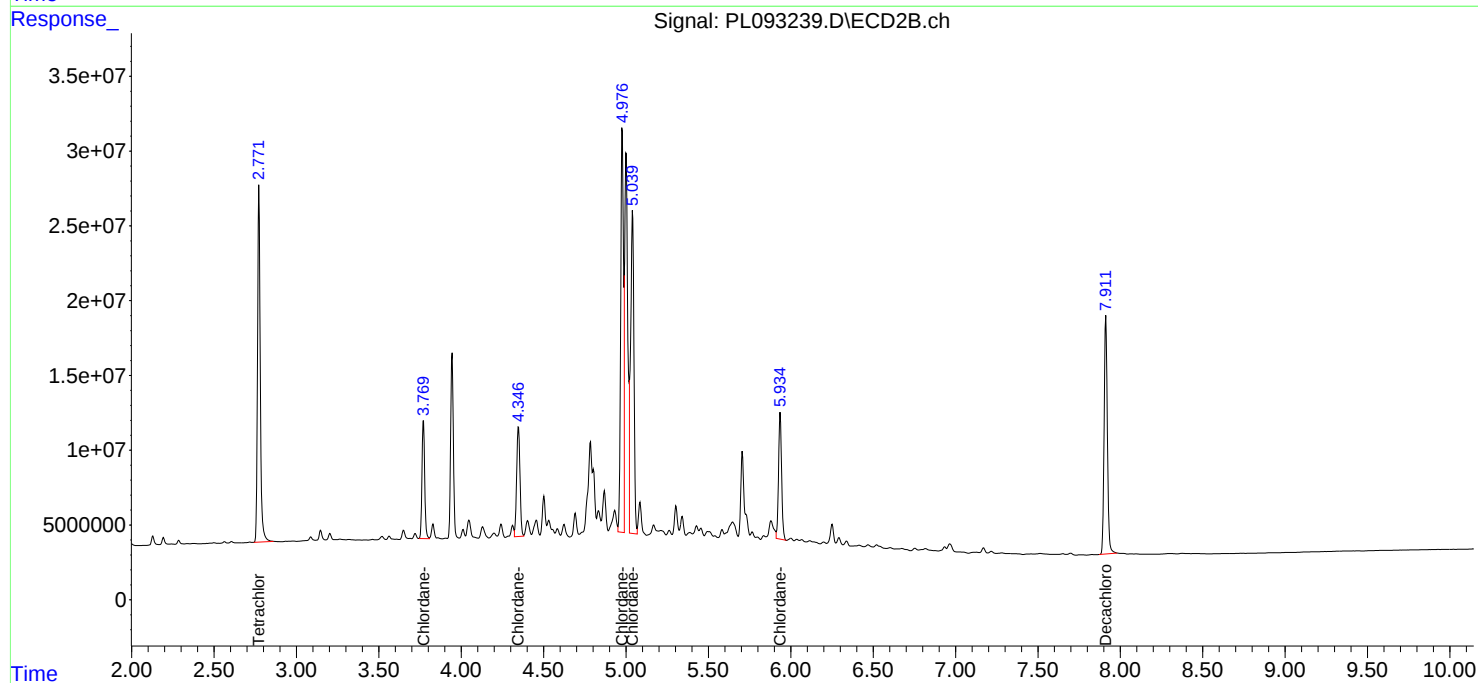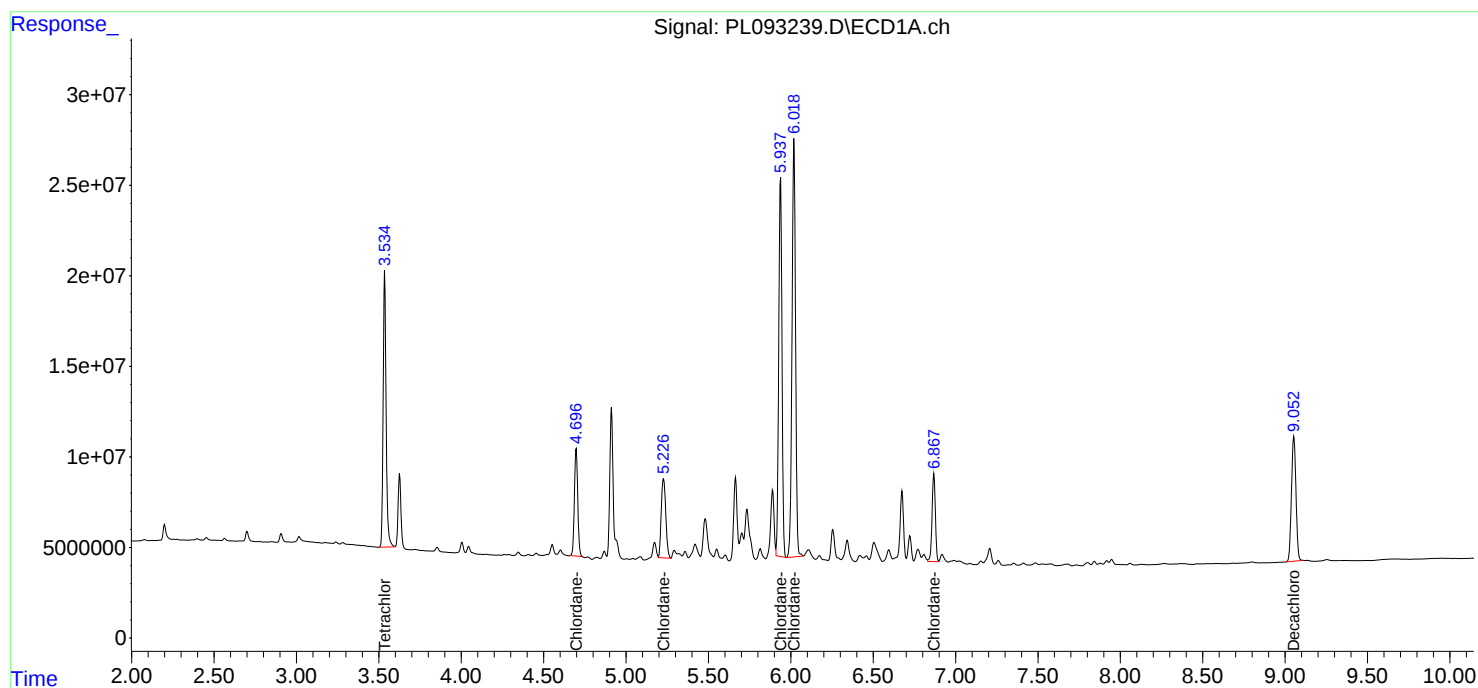


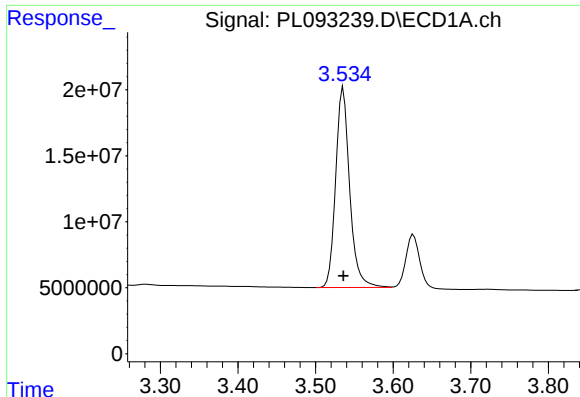

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 190179919
Conc: 75.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

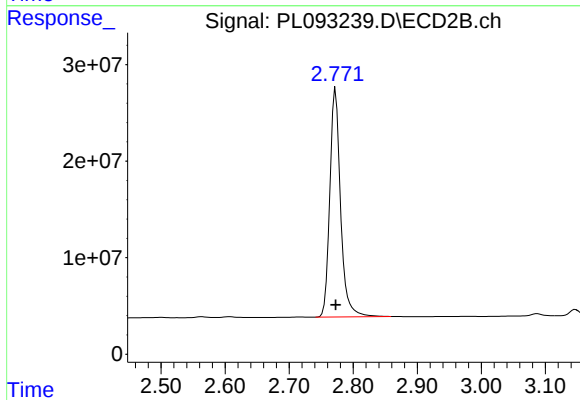


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: 0.000 min
Response: 276225194
Conc: 75.93 ng/ml

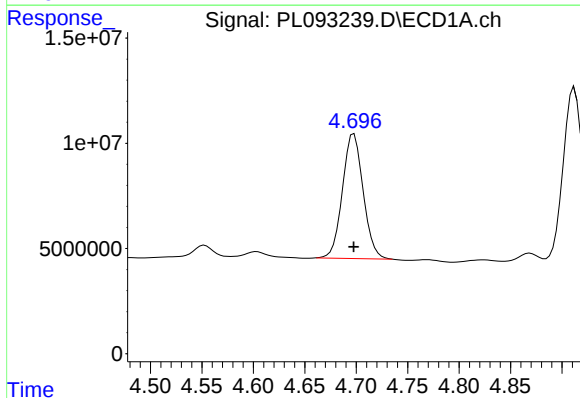


#23 Chlordane-1

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 83102532
Conc: 751.68 ng/ml

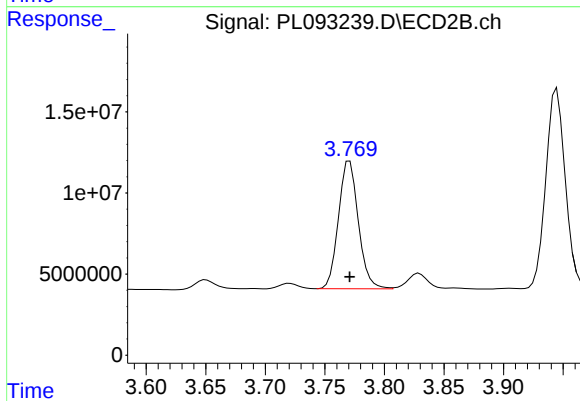

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 91485472
Conc: 759.61 ng/ml

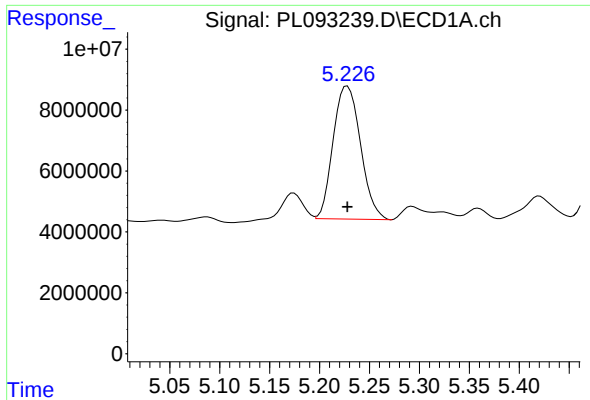

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 83380643
Conc: 750.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

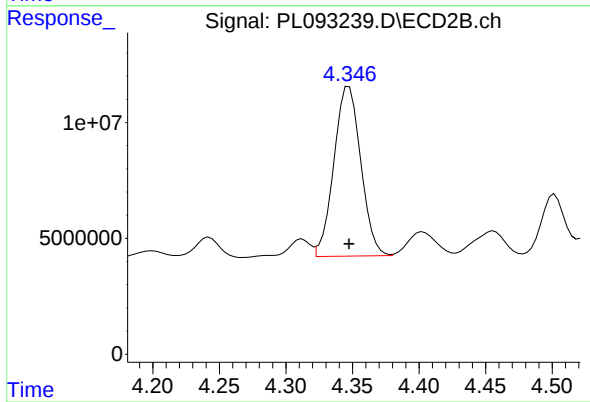


#24 Chlordane-2

R.T.: 4.347 min
Delta R.T.: 0.000 min
Response: 102821353
Conc: 756.19 ng/ml

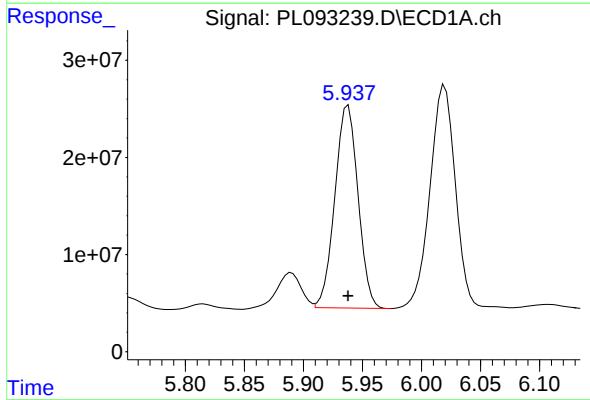


#25 Chlordane-3

R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 284922784
Conc: 756.30 ng/ml

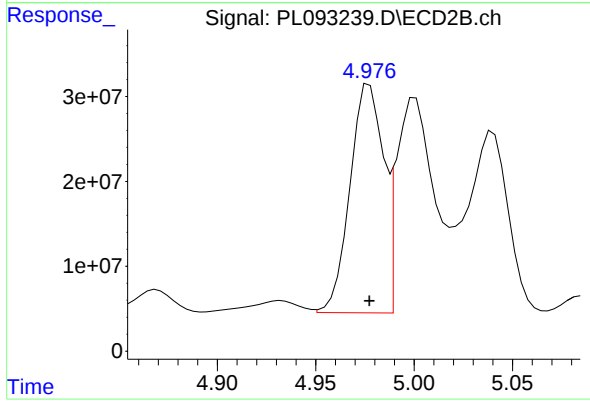

#25 Chlordane-3


R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 317308330
Conc: 757.12 ng/ml

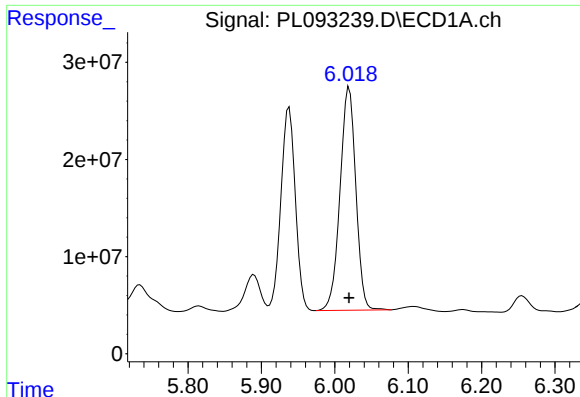

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 343838726
Conc: 755.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

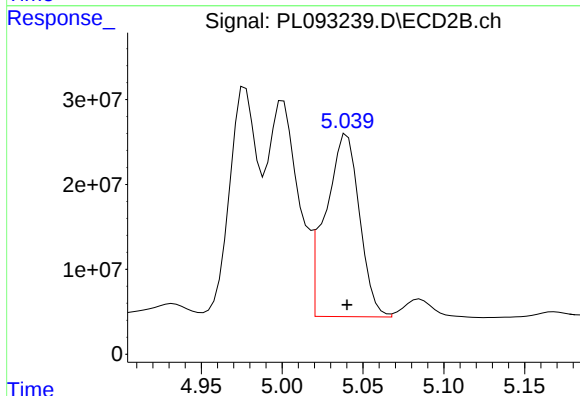


#26 Chlordane-4

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 312577071
Conc: 765.89 ng/ml

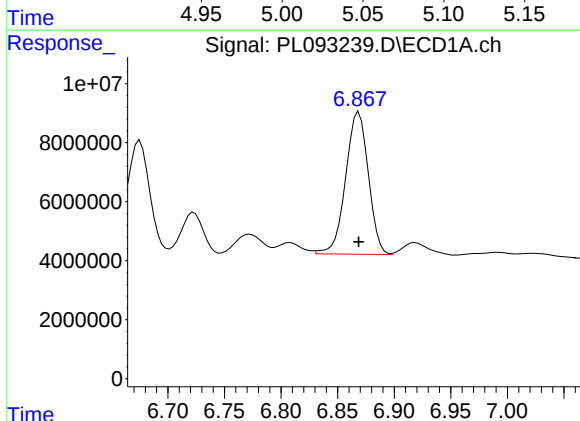


#27 Chlordane-5

R.T.: 6.869 min
Delta R.T.: 0.000 min
Response: 67442934
Conc: 754.95 ng/ml

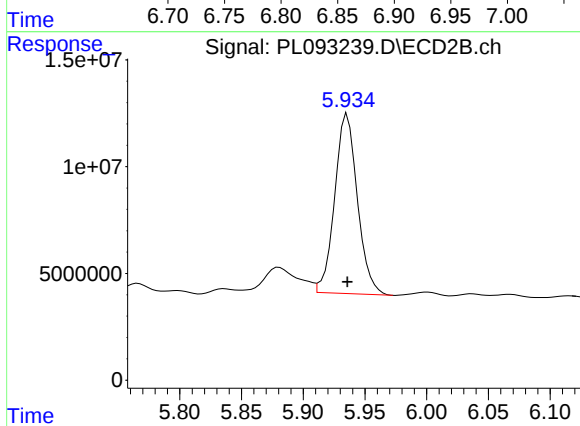

#27 Chlordane-5


R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 107730293
Conc: 758.57 ng/ml

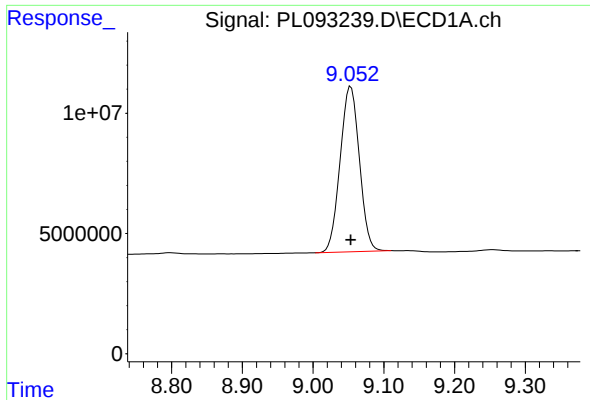

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 130143425
Conc: 75.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

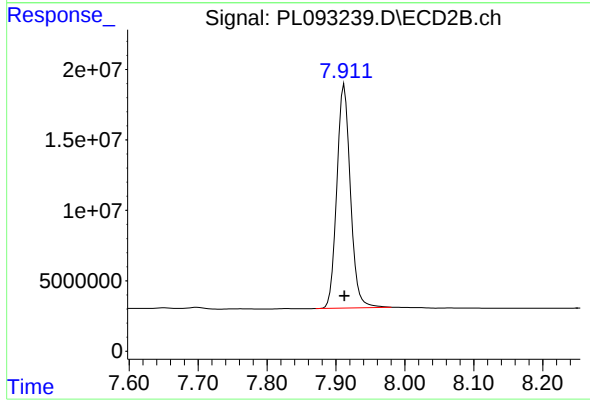

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 217531736
Conc: 75.55 ng/ml