

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
 Data File : PL093240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 13:04
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:32:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 13:29:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.773	128.9E6	183.0E6	50.000	50.000
28)	SA Decachlor...	9.054	7.913	88765425	148.3E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.698	3.771	57486281	60379931	500.000	500.000
24)	Chlordane-2	5.228	4.348	58385552	69547609	500.000	500.000
25)	Chlordane-3	5.939	4.978	192.8E6	210.3E6	500.000	500.000
26)	Chlordane-4	6.020	5.041	233.8E6	206.9E6	500.000	500.000
27)	Chlordane-5	6.870	5.936	46611842	71378576	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
Data File : PL093240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 13:04
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:32:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 13:29:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

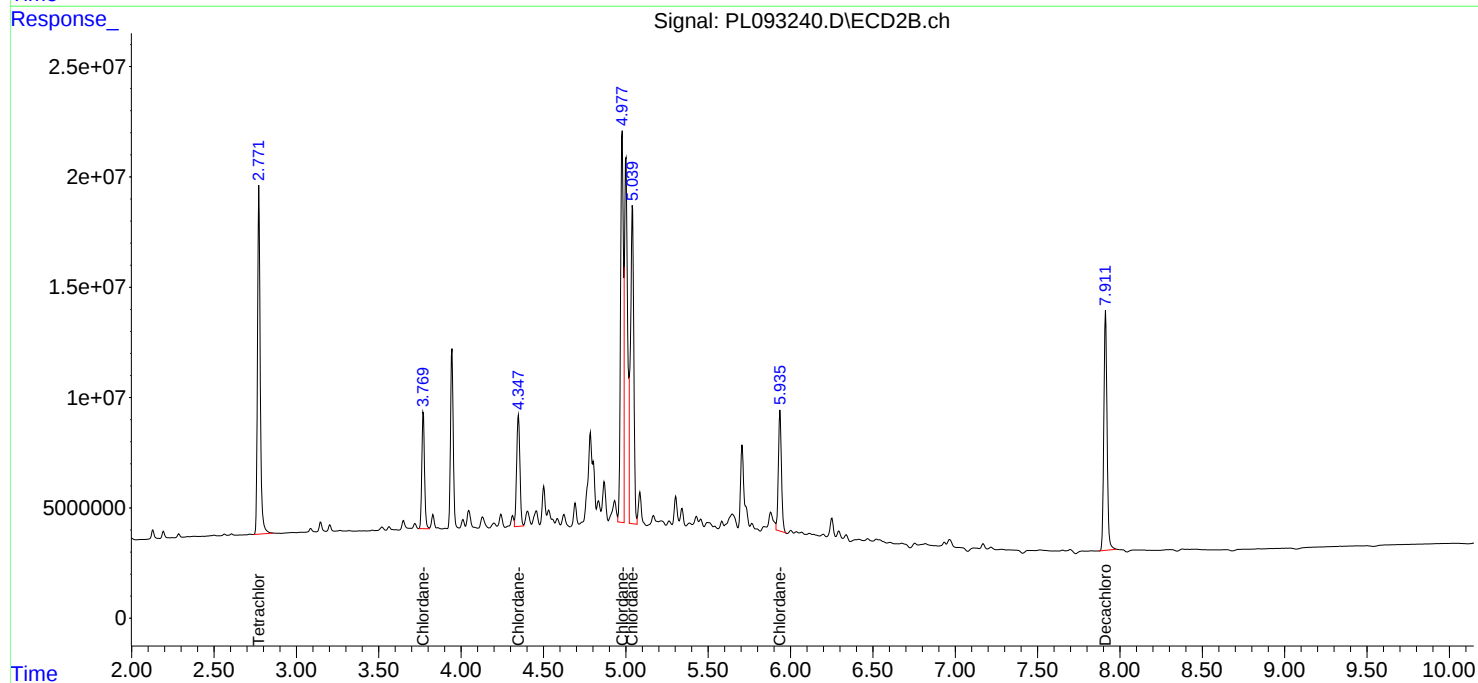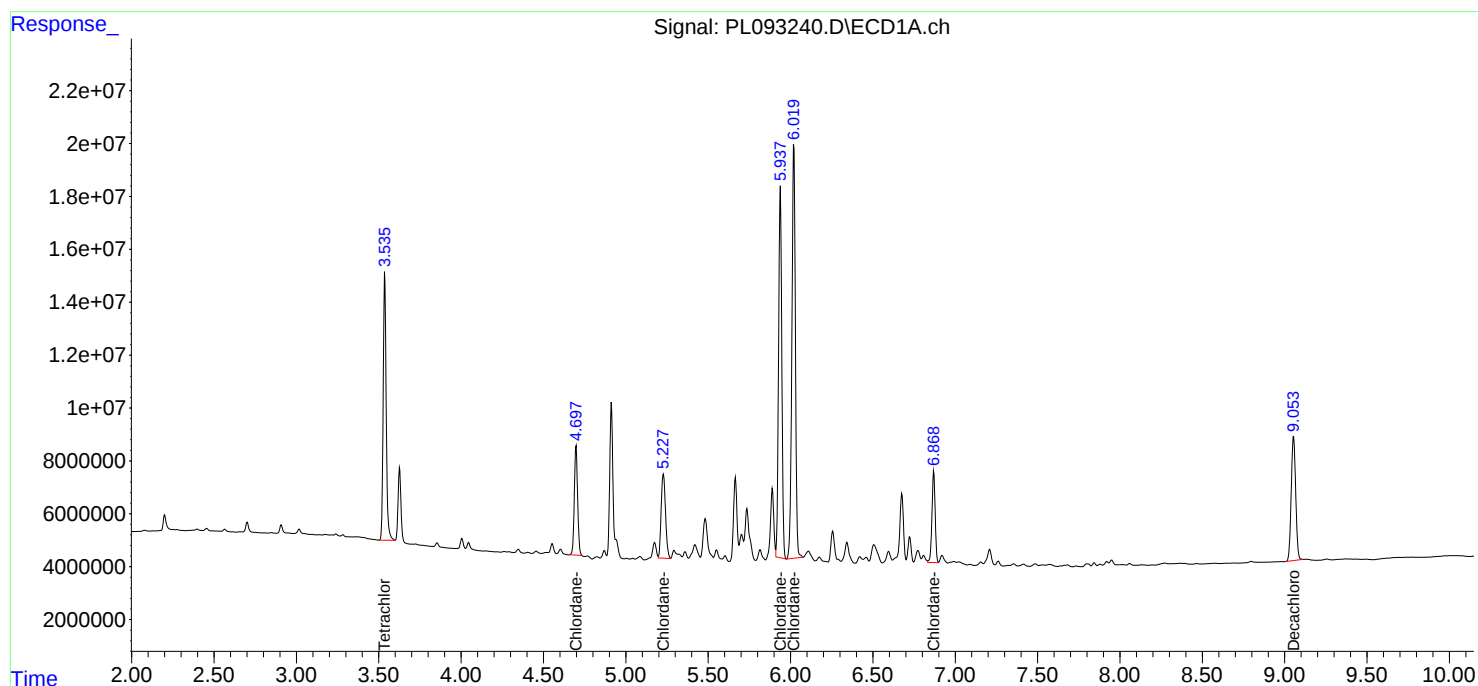


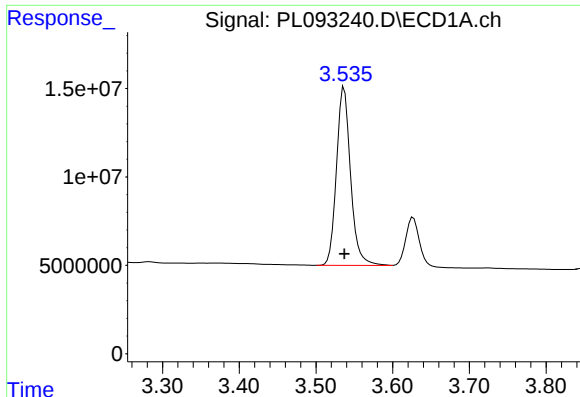

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 128943613
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

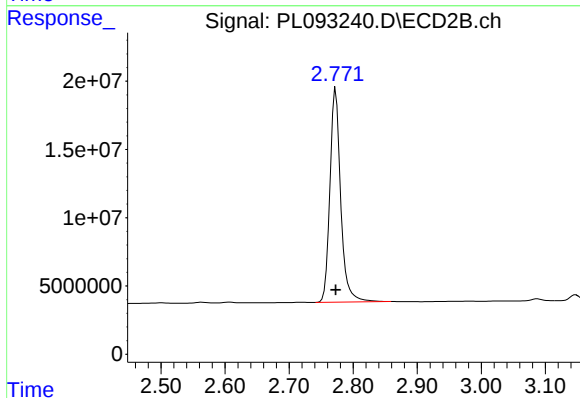


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 182978951
Conc: 50.00 ng/ml

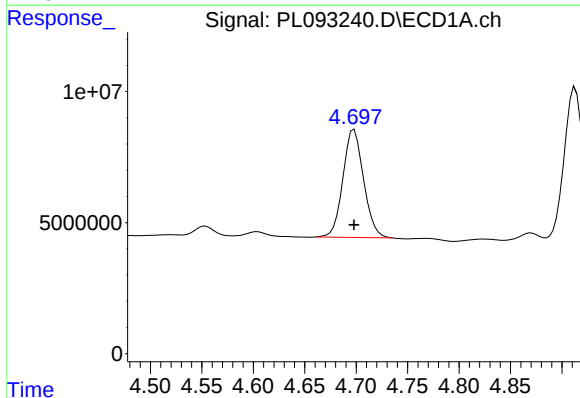


#23 Chlordane-1

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 57486281
Conc: 500.00 ng/ml

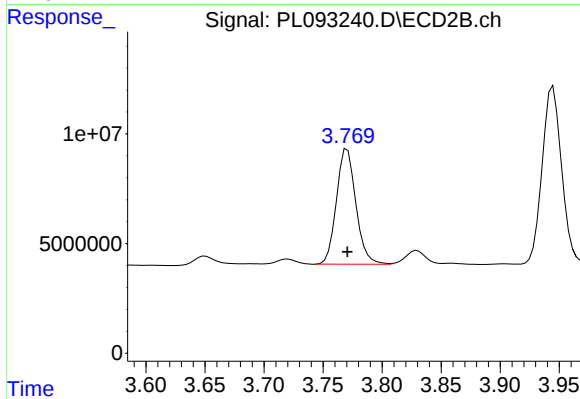

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 60379931
Conc: 500.00 ng/ml

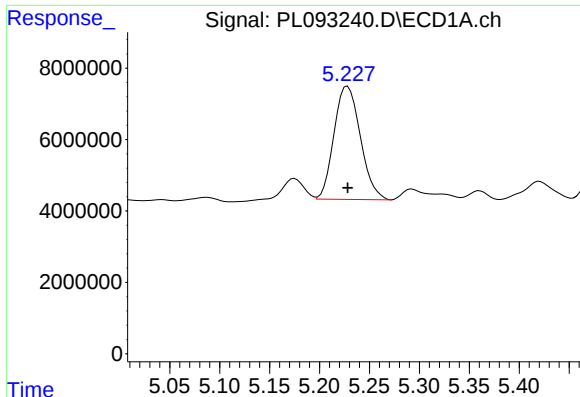

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 58385552
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

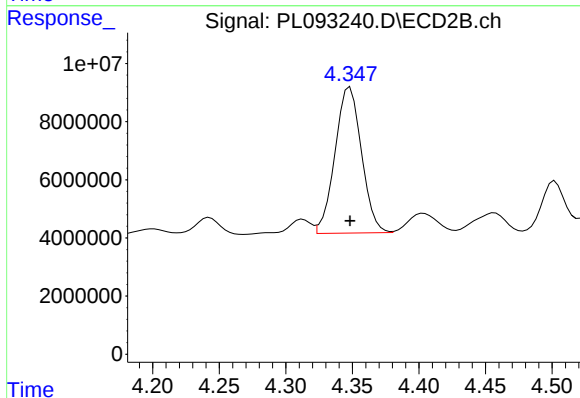


#24 Chlordane-2

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 69547609
Conc: 500.00 ng/ml

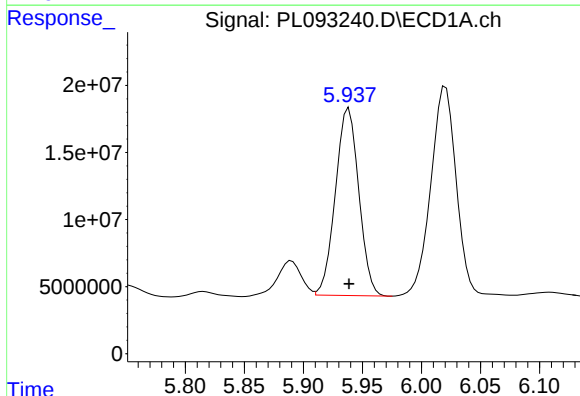


#25 Chlordane-3

R.T.: 5.939 min
Delta R.T.: 0.000 min
Response: 192794347
Conc: 500.00 ng/ml

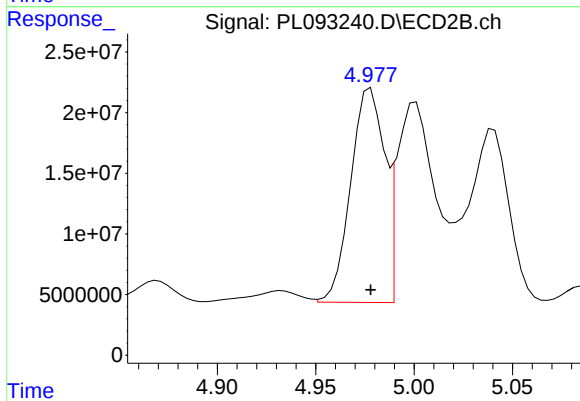

#25 Chlordane-3


R.T.: 4.978 min
Delta R.T.: 0.000 min
Response: 210256359
Conc: 500.00 ng/ml

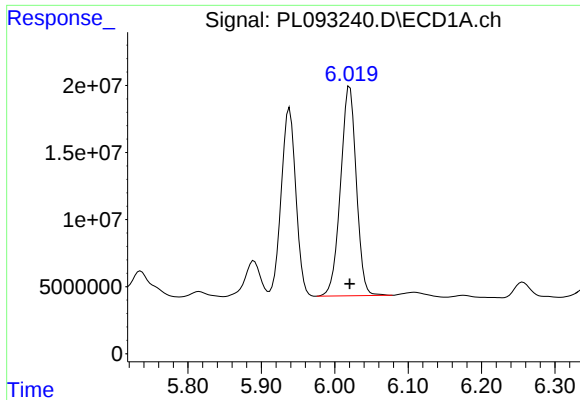

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 233780645
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

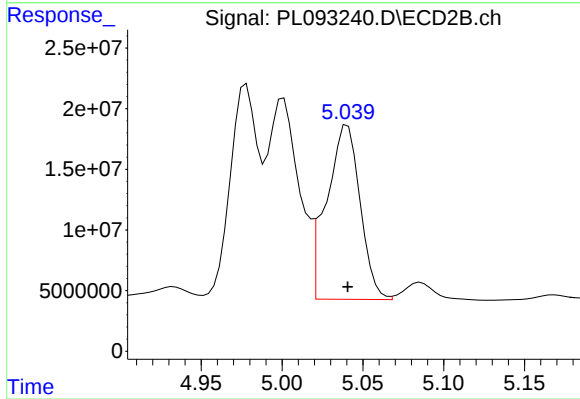


#26 Chlordane-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 206915350
Conc: 500.00 ng/ml

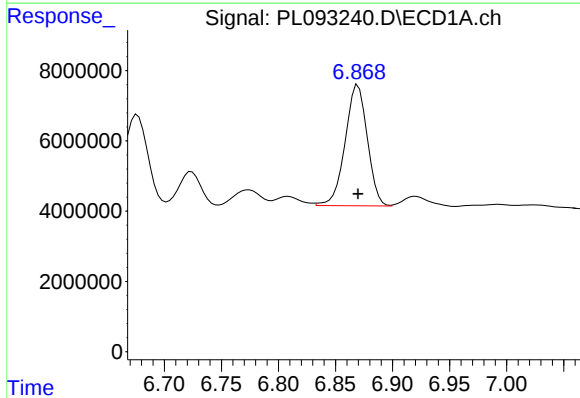


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 46611842
Conc: 500.00 ng/ml

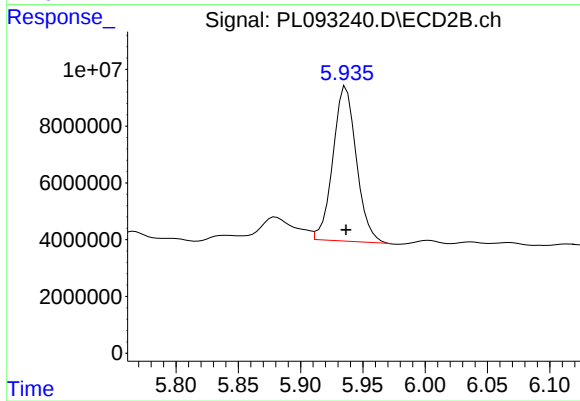

#27 Chlordane-5


R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 71378576
Conc: 500.00 ng/ml

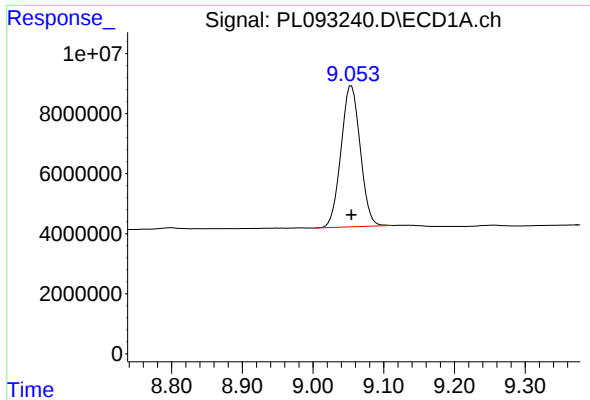

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 88765425
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

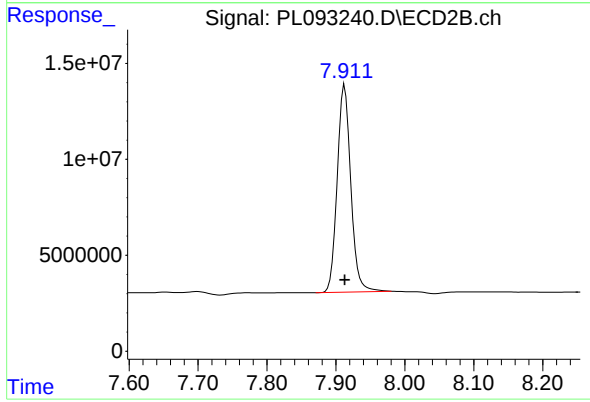

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 148294519
Conc: 50.00 ng/ml