

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
 Data File : PL093241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 13:18
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:38:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 13:29:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.773	66894295	89947271	26.147	24.793
28)	SA Decachlor...	9.054	7.914	46377204	75462098	26.515	25.896
Target Compounds							
23)	Chlordane-1	4.698	3.771	29871156	29520844	264.843	246.316
24)	Chlordane-2	5.228	4.348	30707676	34785298	269.312	254.343
25)	Chlordane-3	5.938	4.978	98817094	101.0E6	259.114	243.101
26)	Chlordane-4	6.020	5.040	121.0E6	99357582	261.693	245.055
27)	Chlordane-5	6.870	5.936	24303367	34237362	266.179	243.250



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
Data File : PL093241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 13:18
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:38:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 13:29:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

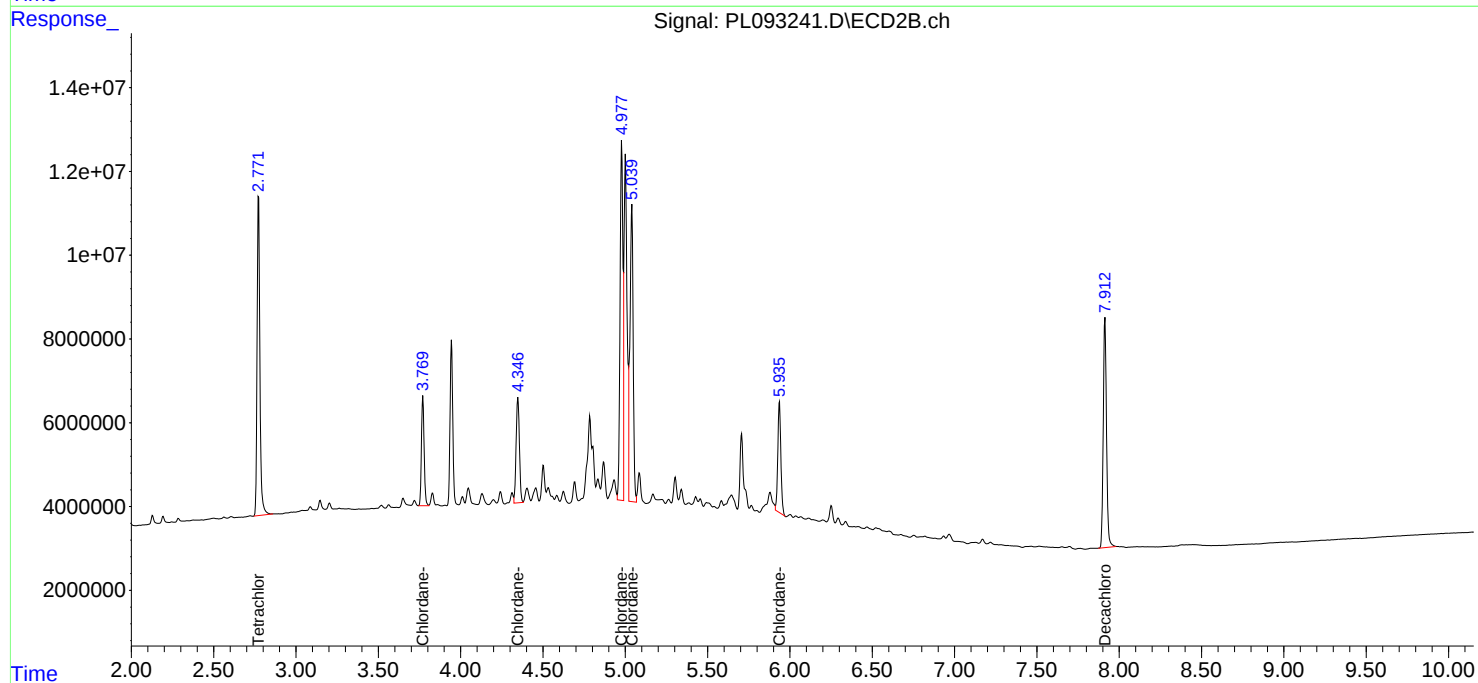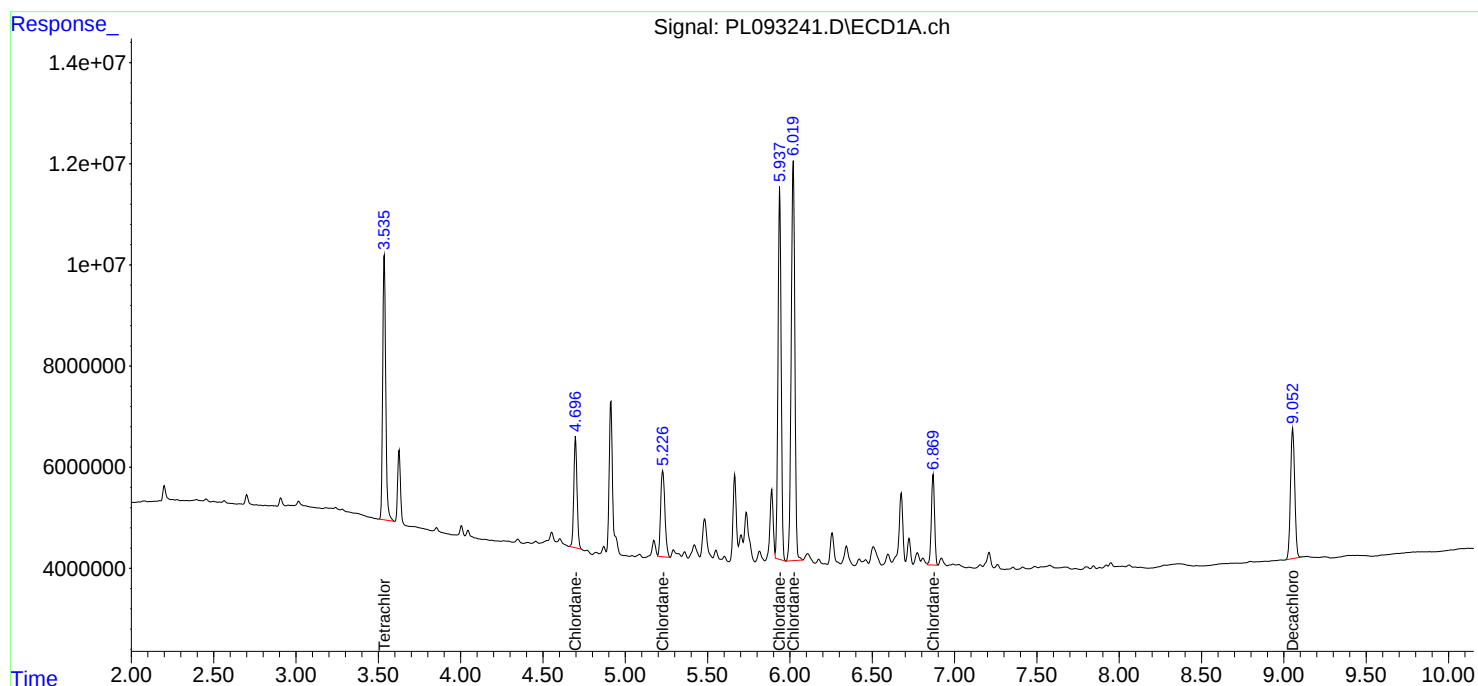


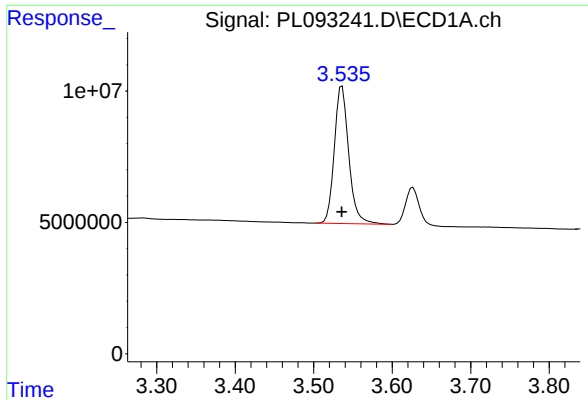

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 66894295
Conc: 26.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

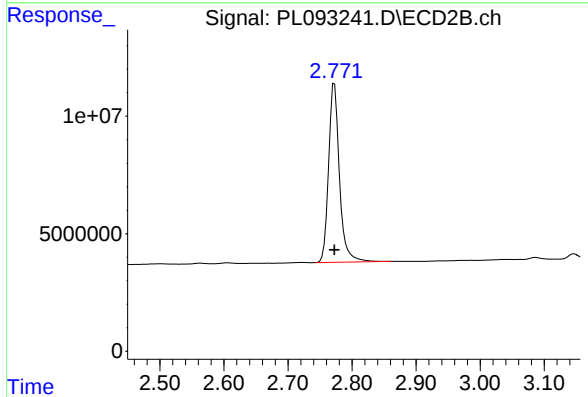


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 89947271
Conc: 24.79 ng/ml

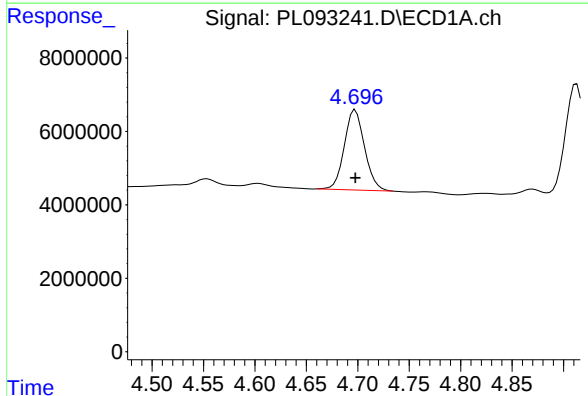


#23 Chlordane-1

R.T.: 4.698 min
Delta R.T.: 0.000 min
Response: 29871156
Conc: 264.84 ng/ml

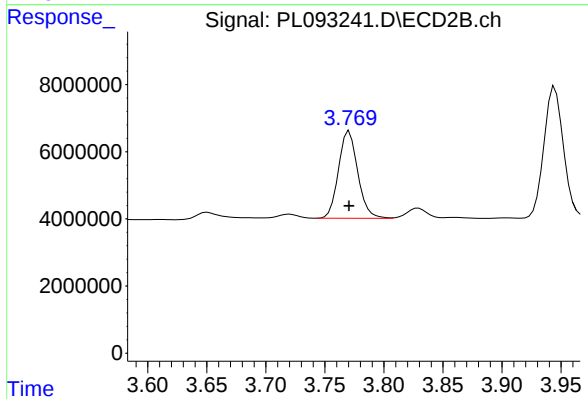

#23 Chlordane-1


R.T.: 3.771 min
Delta R.T.: 0.000 min
Response: 29520844
Conc: 246.32 ng/ml

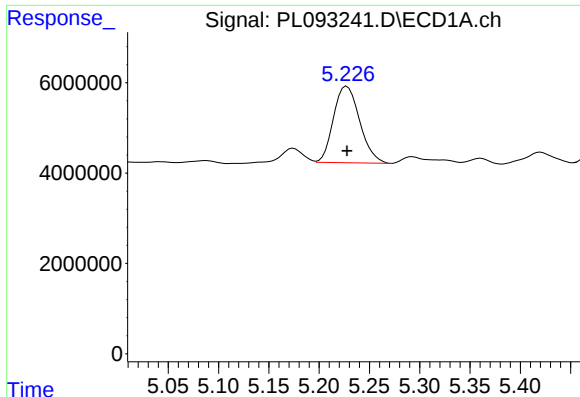

#24 Chlordane-2


R.T.: 5.228 min
Delta R.T.: 0.000 min
Response: 30707676
Conc: 269.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

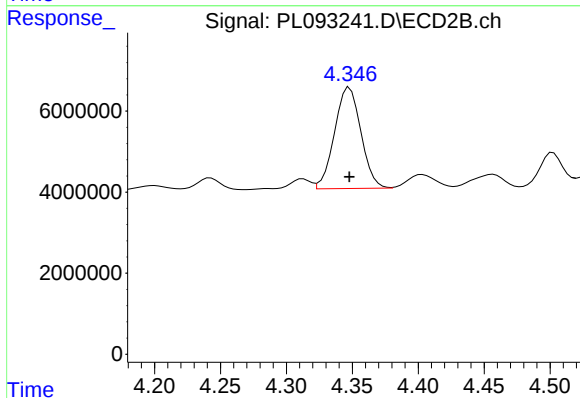


#24 Chlordane-2

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 34785298
Conc: 254.34 ng/ml

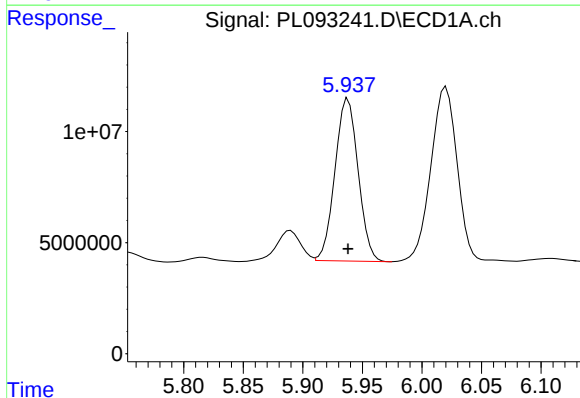


#25 Chlordane-3

R.T.: 5.938 min
Delta R.T.: 0.000 min
Response: 98817094
Conc: 259.11 ng/ml

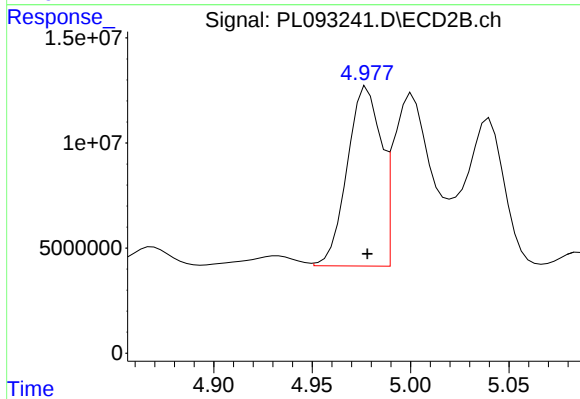

#25 Chlordane-3


R.T.: 4.978 min
Delta R.T.: 0.000 min
Response: 100955165
Conc: 243.10 ng/ml

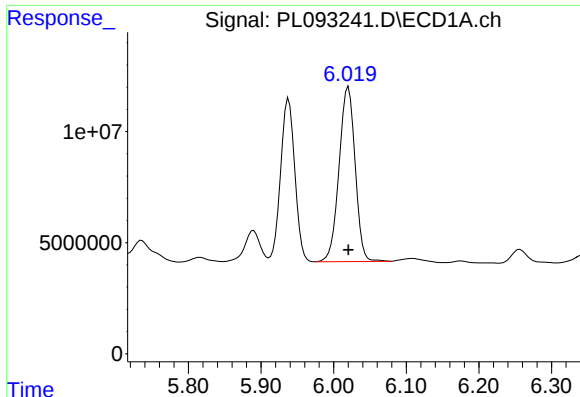

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: 0.000 min
Response: 121019649
Conc: 261.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

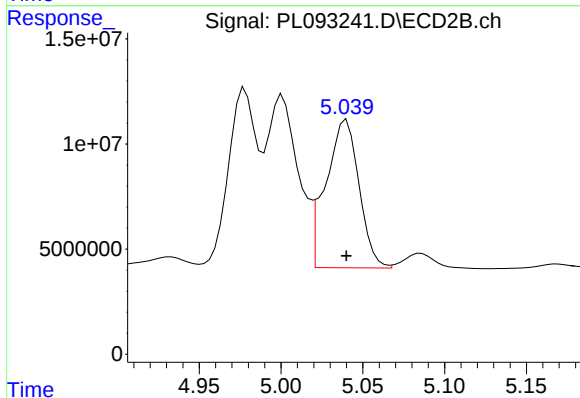


#26 Chlordane-4

R.T.: 5.040 min
Delta R.T.: 0.000 min
Response: 99357582
Conc: 245.05 ng/ml

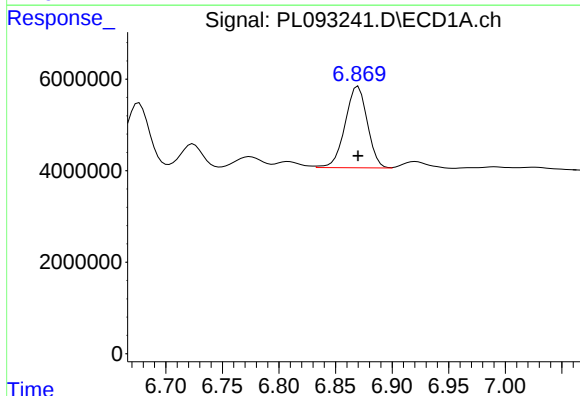


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 24303367
Conc: 266.18 ng/ml

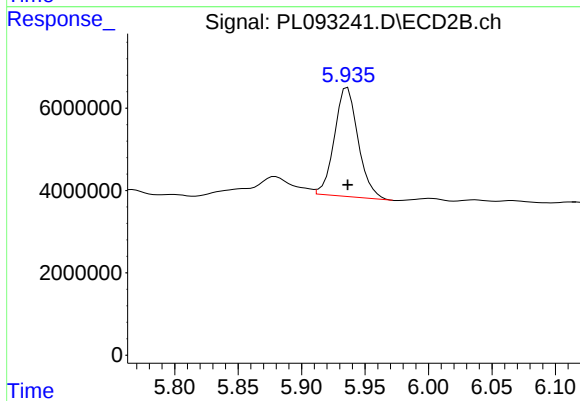

#27 Chlordane-5


R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 34237362
Conc: 243.25 ng/ml

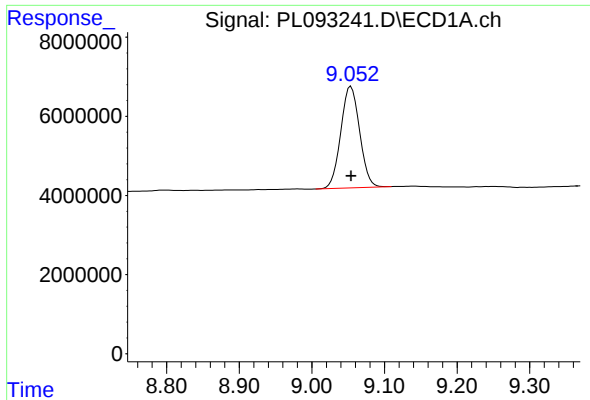

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.000 min
Response: 46377204
Conc: 26.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

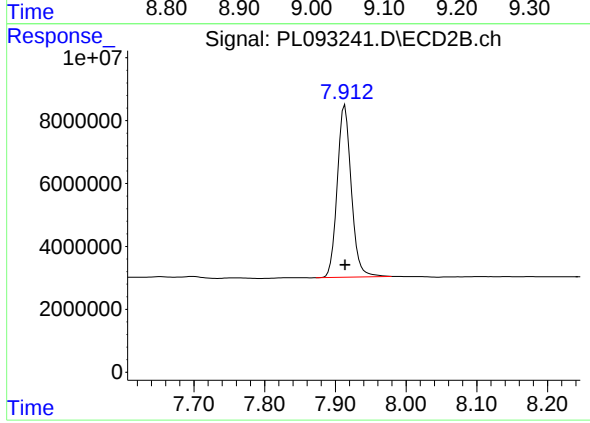

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 75462098
Conc: 25.90 ng/ml