

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
 Data File : PL093232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2024 11:18
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 14:01:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 25 13:59:47 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.773	54676032	58584410	21.038	20.313
28) SA Decachlor...	9.053	7.912	35915959	56984737	20.659	19.949
Target Compounds						
9) A Endosulfan I	6.066	5.097	26448576	32052155	10.865	9.588
10) B gamma-Chl...	5.936	4.977	28264231	37839458	10.971	10.213
12) B 4,4'-DDE	6.189	5.230	48654368	70439931	20.799	19.676
13) MA Dieldrin	6.341	5.361	51992190	69461780	20.284	18.847
19) B Endosulfa...	7.155	6.334	40004644	56150739	19.301	18.473
20) A Methoxychlor	7.498	6.610	96484728	145.9E6	92.341	95.537
21) B Endrin ke...	7.641	6.839	46046582	63046062	20.291	18.780



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112524\
Data File : PL093232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2024 11:18
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 14:01:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112524.M
Quant Title : GC Extractables
QLast Update : Mon Nov 25 13:59:47 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

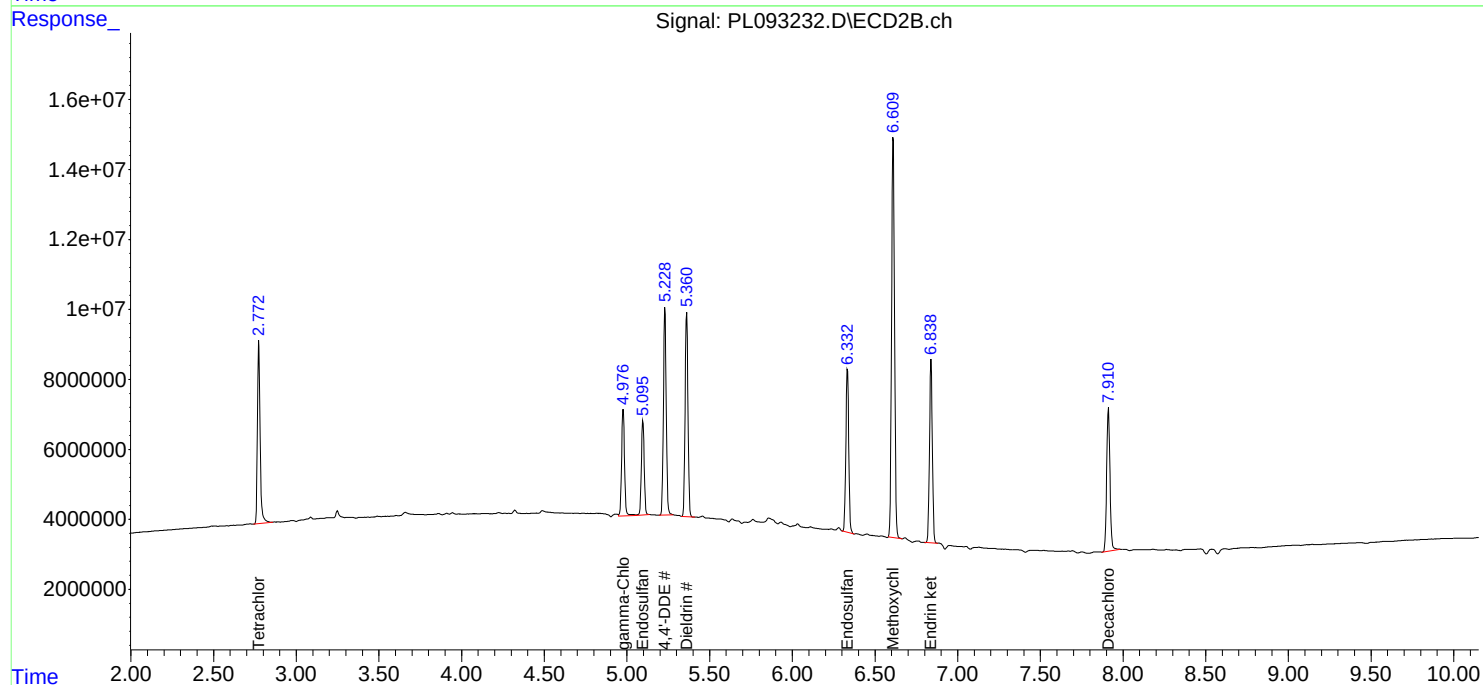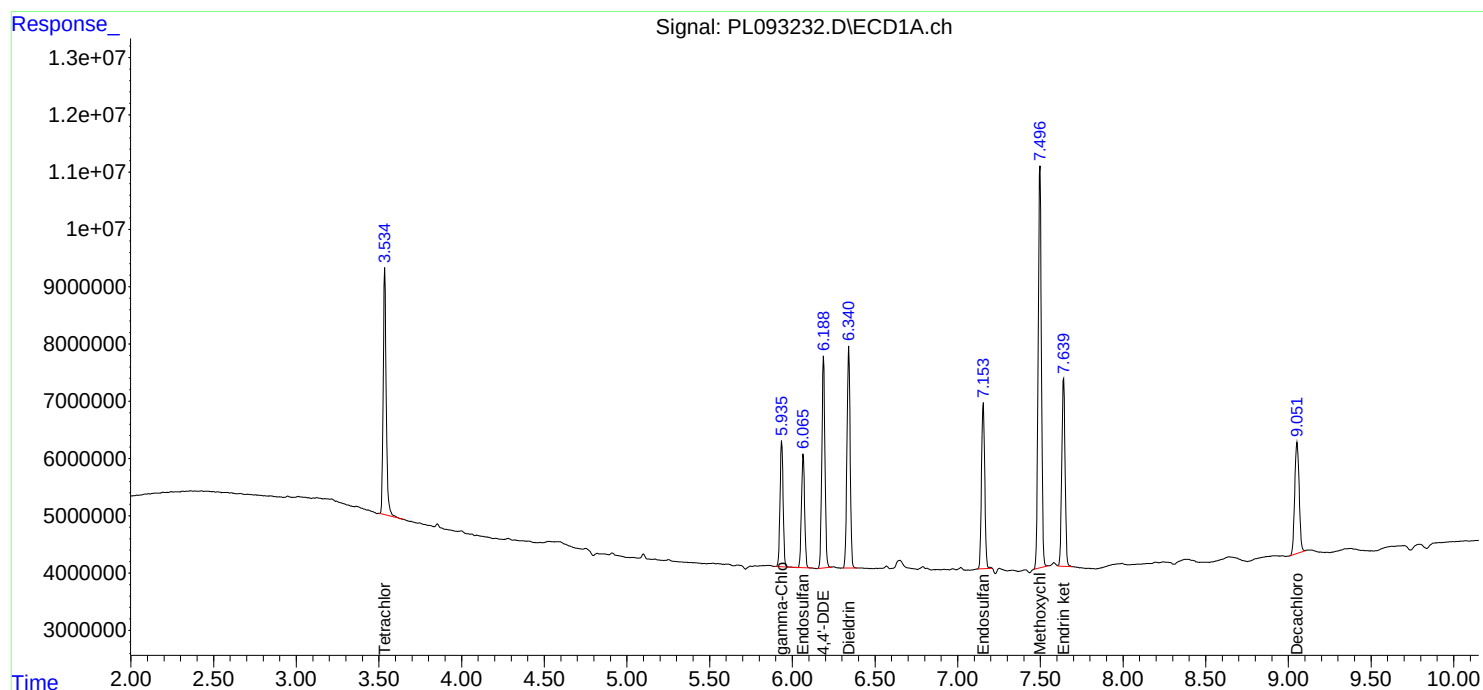


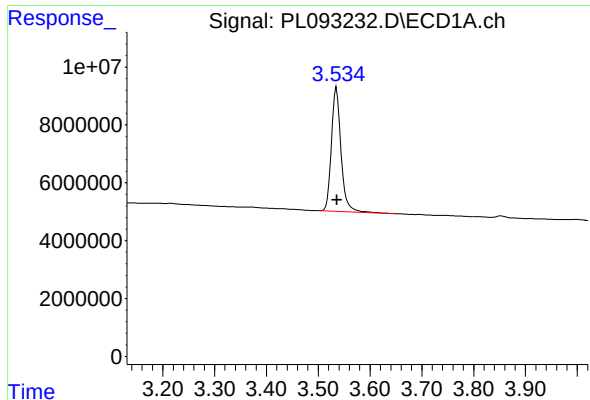

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 54676032
Conc: 21.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

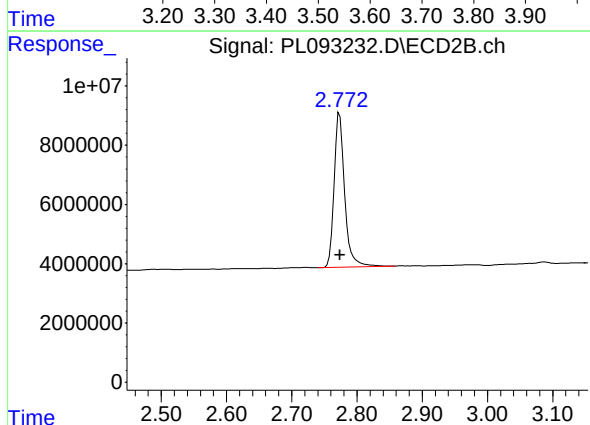


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 58584410
Conc: 20.31 ng/ml

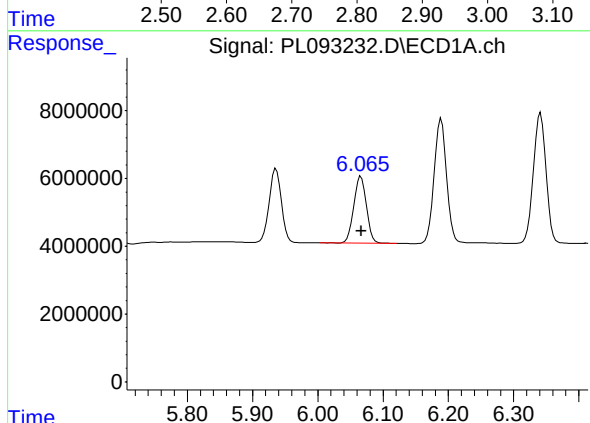


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 26448576
Conc: 10.87 ng/ml

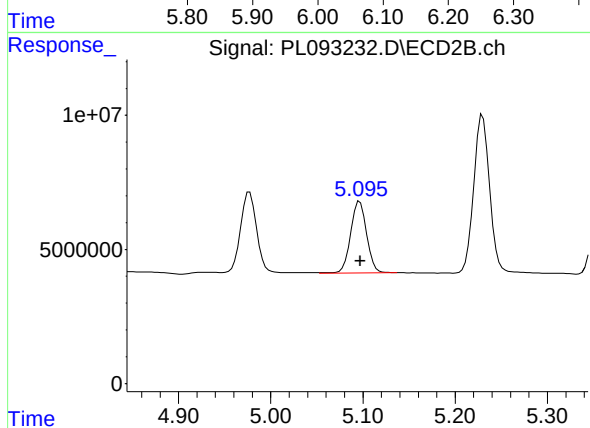

#9 Endosulfan I


R.T.: 5.097 min
Delta R.T.: 0.000 min
Response: 32052155
Conc: 9.59 ng/ml

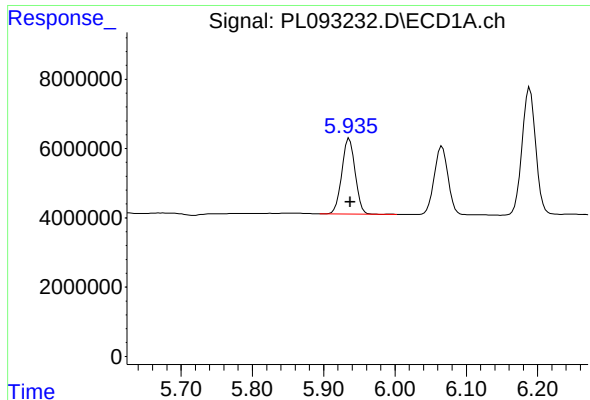

#10 gamma-Chlordane


R.T.: 5.936 min
Delta R.T.: -0.001 min
Response: 28264231
Conc: 10.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

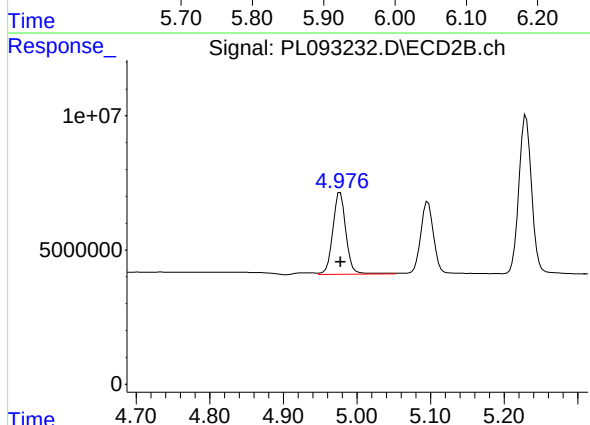


#10 gamma-Chlordane

R.T.: 4.977 min
Delta R.T.: 0.000 min
Response: 37839458
Conc: 10.21 ng/ml

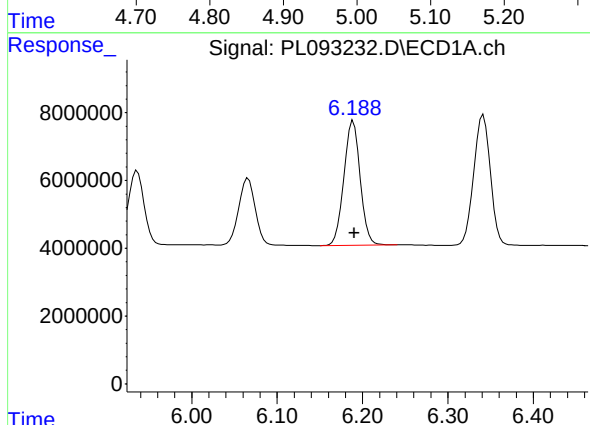


#12 4,4'-DDE

R.T.: 6.189 min
Delta R.T.: -0.001 min
Response: 48654368
Conc: 20.80 ng/ml

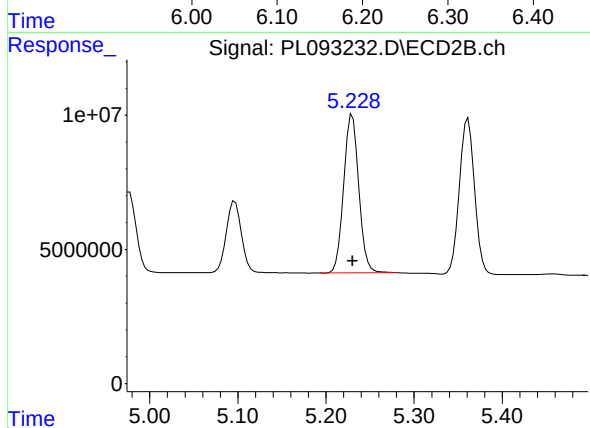

#12 4,4'-DDE


R.T.: 5.230 min
Delta R.T.: 0.000 min
Response: 70439931
Conc: 19.68 ng/ml

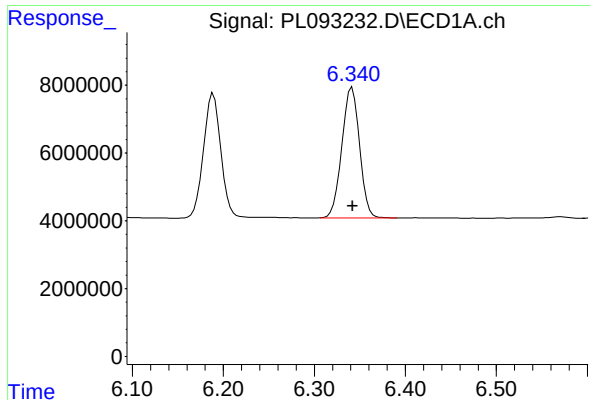

#13 Dieldrin


R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 51992190
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

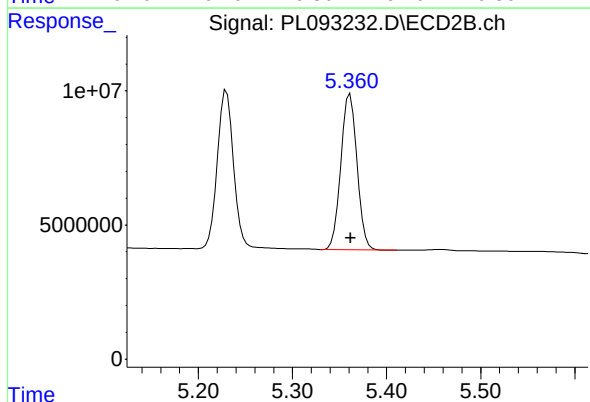


#13 Dieldrin

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 69461780
Conc: 18.85 ng/ml

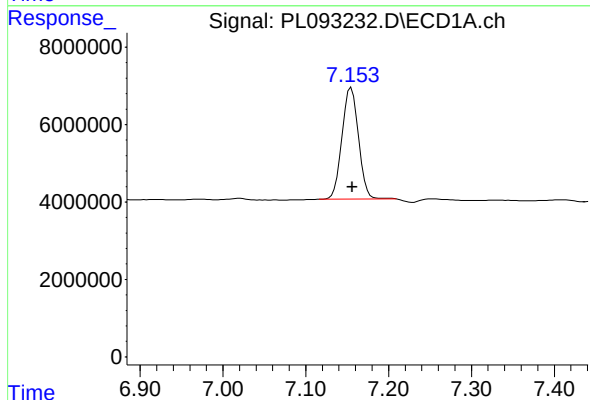


#19 Endosulfan Sulfate

R.T.: 7.155 min
Delta R.T.: -0.001 min
Response: 40004644
Conc: 19.30 ng/ml

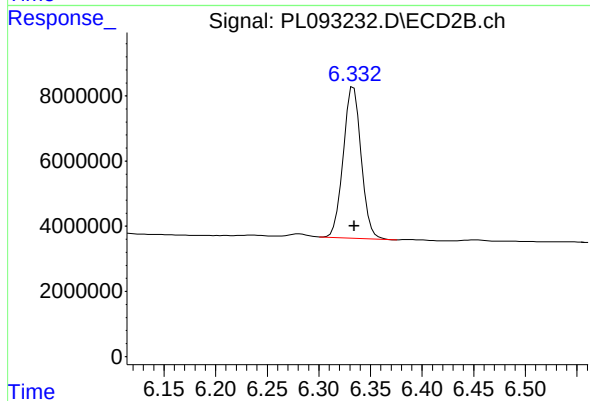

#19 Endosulfan Sulfate


R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 56150739
Conc: 18.47 ng/ml

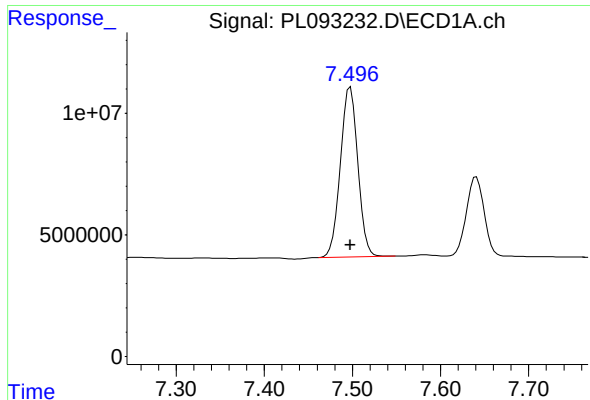

#20 Methoxychlor


R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 96484728
Conc: 92.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

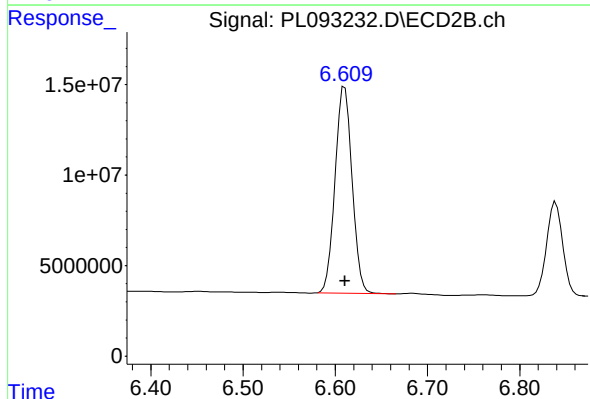


#20 Methoxychlor

R.T.: 6.610 min
Delta R.T.: 0.000 min
Response: 145879547
Conc: 95.54 ng/ml

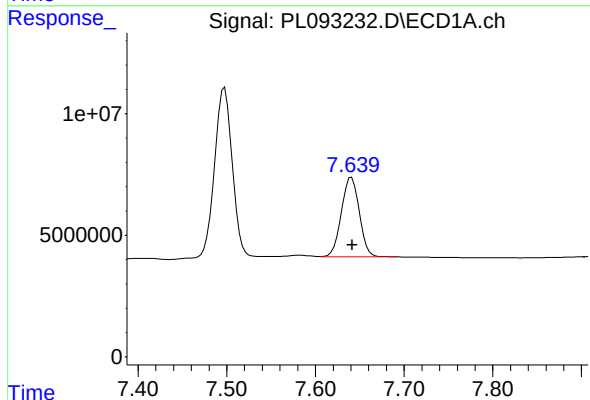


#21 Endrin ketone

R.T.: 7.641 min
Delta R.T.: 0.000 min
Response: 46046582
Conc: 20.29 ng/ml

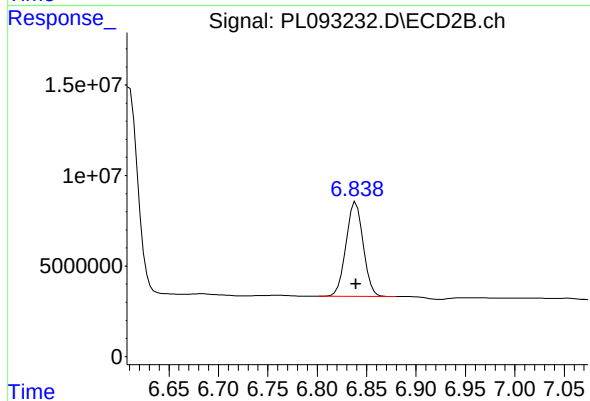

#21 Endrin ketone


R.T.: 6.839 min
Delta R.T.: 0.000 min
Response: 63046062
Conc: 18.78 ng/ml

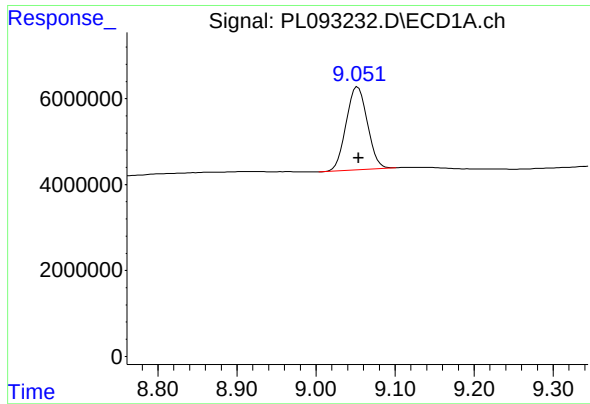

#28 Decachlorobiphenyl

R.T.: 9.053 min
Delta R.T.: -0.001 min
Response: 35915959
Conc: 20.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

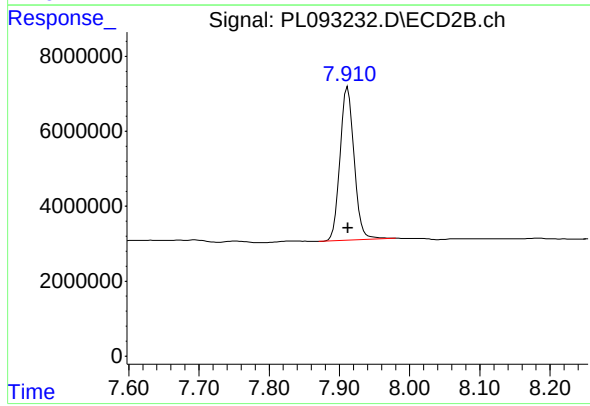

#28 Decachlorobiphenyl

R.T.: 7.912 min
Delta R.T.: 0.000 min
Response: 56984737
Conc: 19.95 ng/ml