

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
 Data File : PL097734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 10:01
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 17:59:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 25 17:56:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.623	0.000	16542968	0	2.631	N.D. #
11) B	alpha-Chl...	5.934f	5.094f	-114241	343767	N.D.	0.037
13) MA	Dieldrin	0.000	5.382f	0	59481097	N.D.	6.884 #
14) MA	Endrin	0.000	5.683	0	31284375	N.D.	4.070 #
15) B	Endosulfa...	6.716	0.000	19877608	0	3.918	N.D. #
18) B	Endrin al...	0.000	6.147	0	18462029	N.D.	3.390 #
24)	Chlordane-2	0.000	4.373	0	5452138	N.D.	18.510 #
26)	Chlordane-4	0.000	5.094	0	343767	N.D.	0.458 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
Data File : PL097734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 10:01
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 17:59:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Tue Nov 25 17:56:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

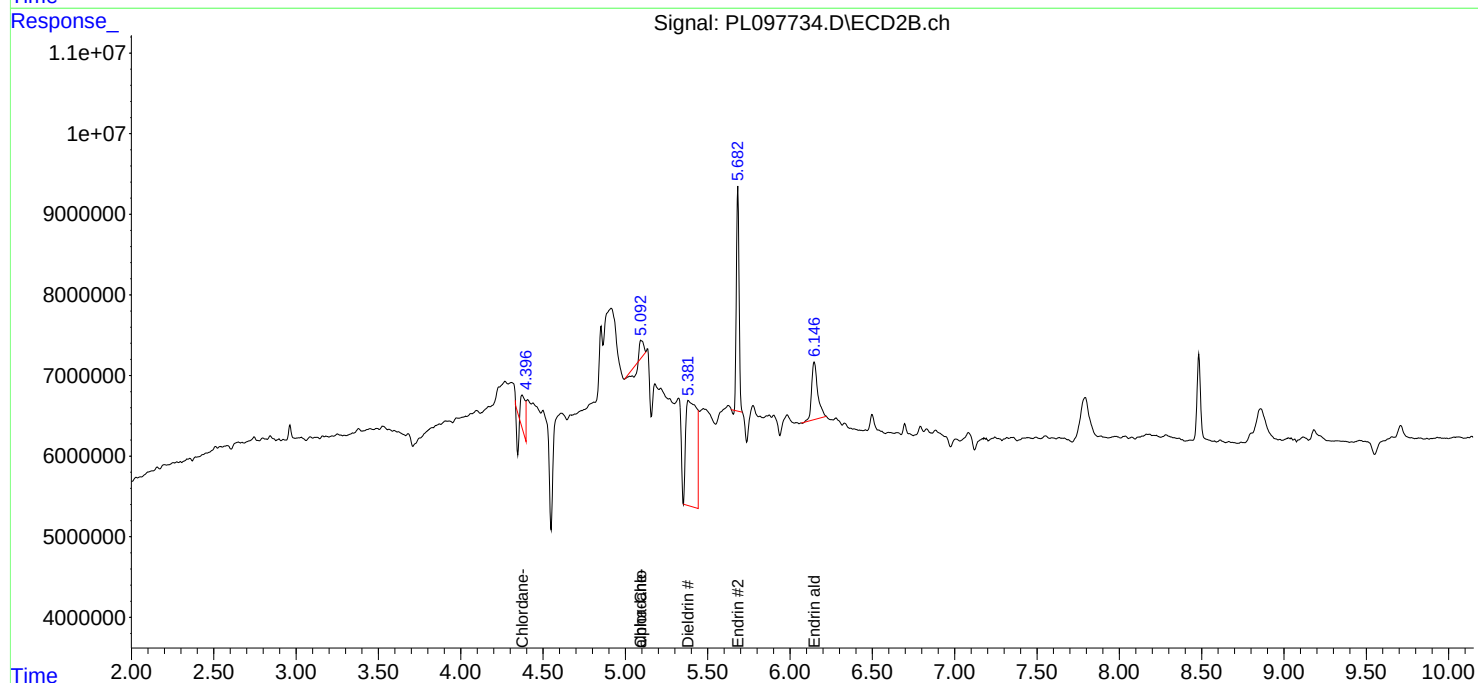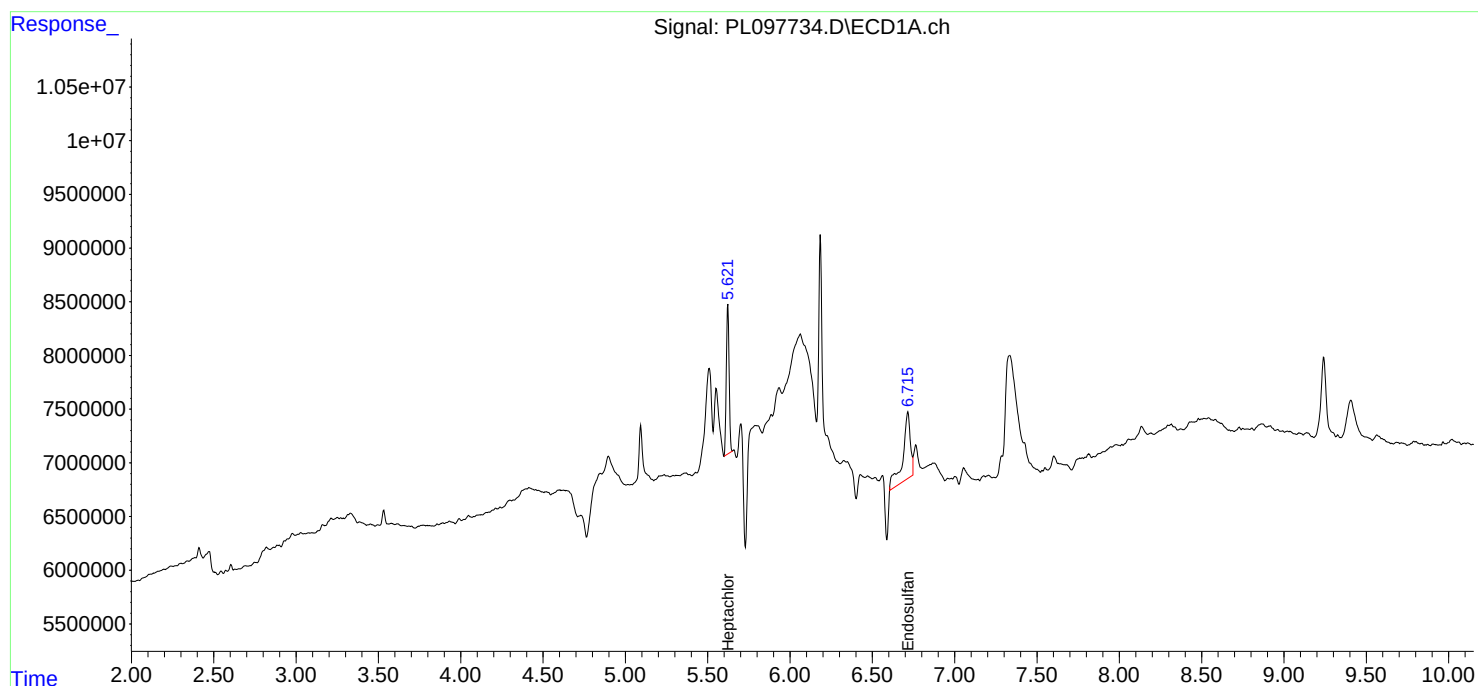


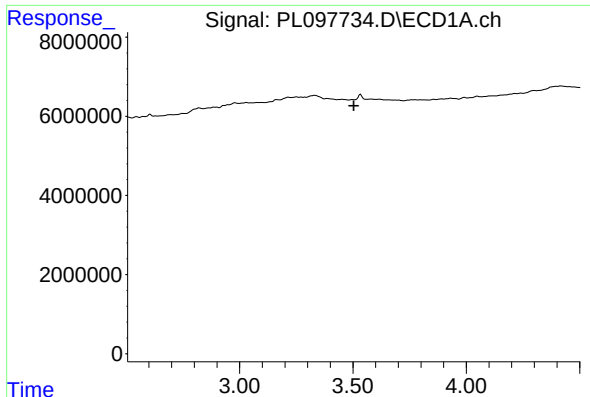

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

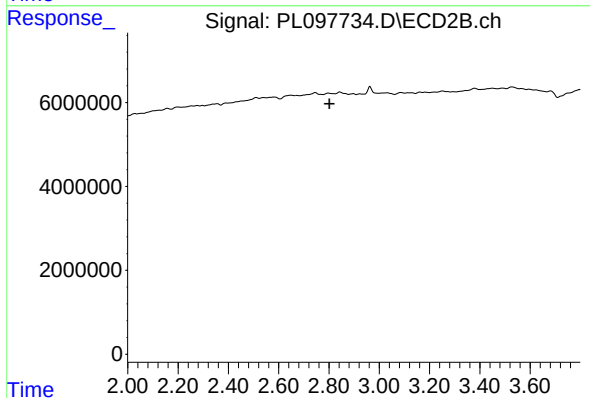


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.802 min
Response: 0
Conc: N.D.

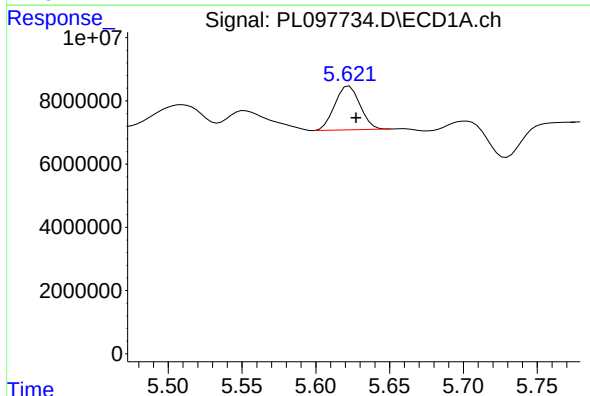


#8 Heptachlor epoxide

R.T.: 5.623 min
Delta R.T.: -0.005 min
Response: 16542968
Conc: 2.63 ng/ml

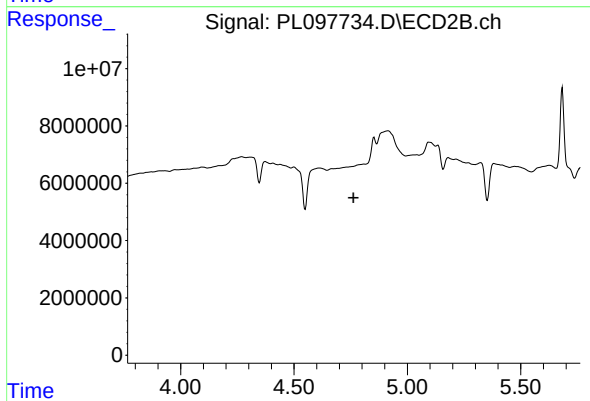

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.763 min
Response: 0
Conc: N.D.

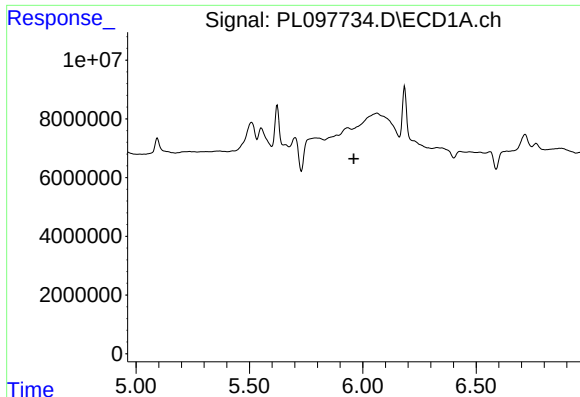

#11 alpha-Chlordane


R.T.: 5.934 min
Delta R.T.: -0.026 min
Response: -114241
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

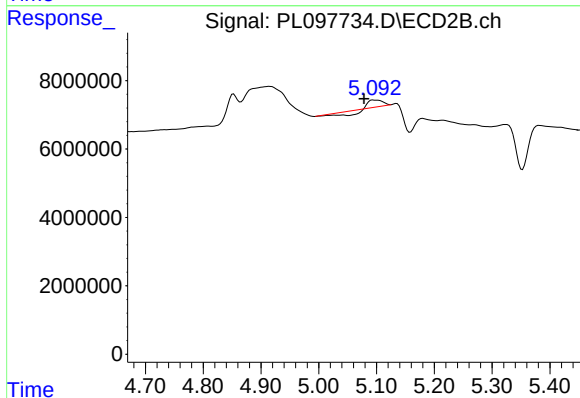


#11 alpha-Chlordane

R.T.: 5.094 min
Delta R.T.: 0.016 min
Response: 343767
Conc: 0.04 ng/ml

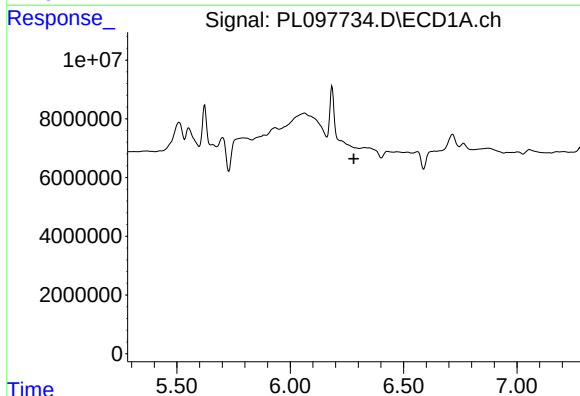


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.280 min
Response: 0
Conc: N.D.

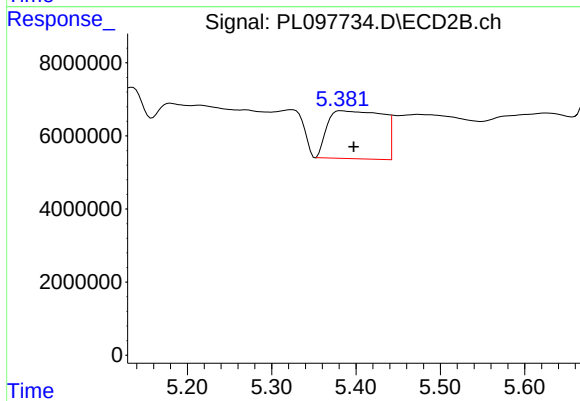

#13 Dieldrin


R.T.: 5.382 min
Delta R.T.: -0.015 min
Response: 59481097
Conc: 6.88 ng/ml

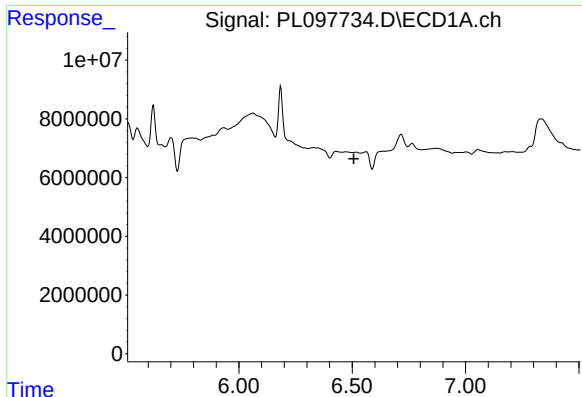

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

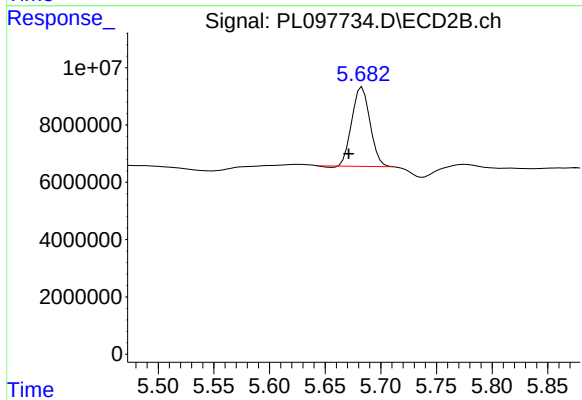


#14 Endrin

R.T.: 5.683 min
Delta R.T.: 0.012 min
Response: 31284375
Conc: 4.07 ng/ml

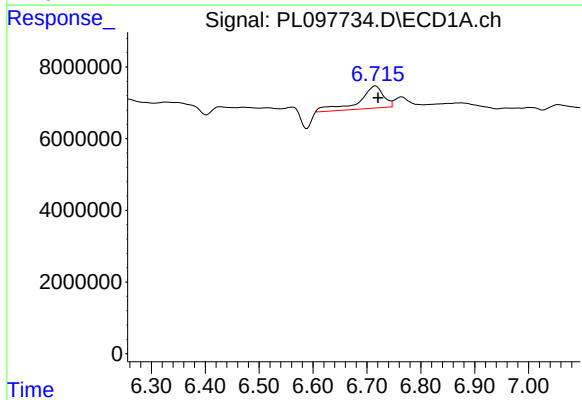


#15 Endosulfan II

R.T.: 6.716 min
Delta R.T.: -0.004 min
Response: 19877608
Conc: 3.92 ng/ml

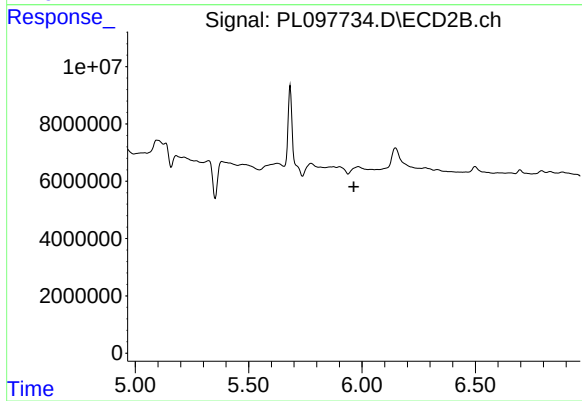

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.963 min
Response: 0
Conc: N.D.

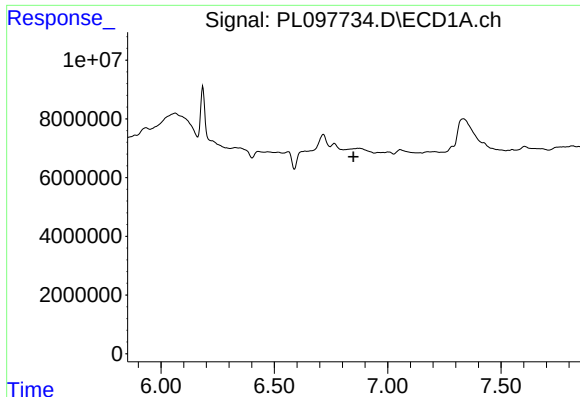

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.850 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

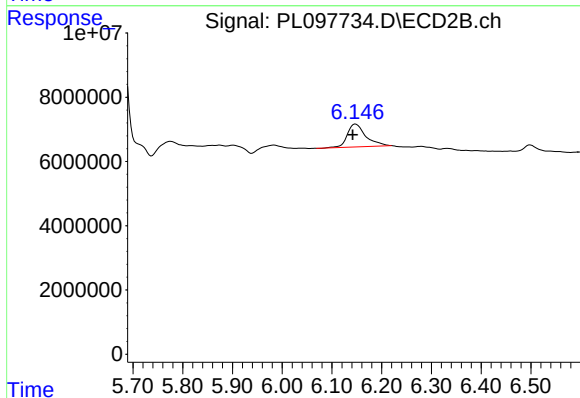


#18 Endrin aldehyde

R.T.: 6.147 min
Delta R.T.: 0.006 min
Response: 18462029
Conc: 3.39 ng/ml

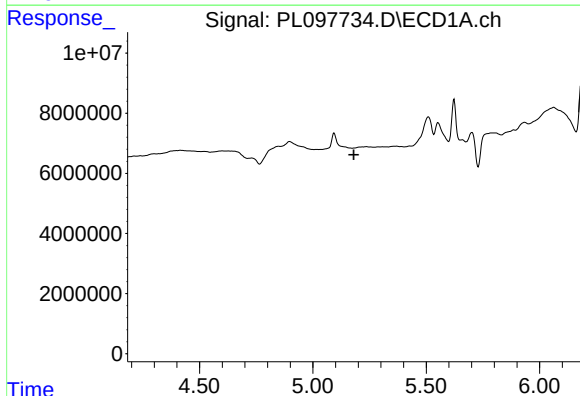


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.181 min
Response: 0
Conc: N.D.

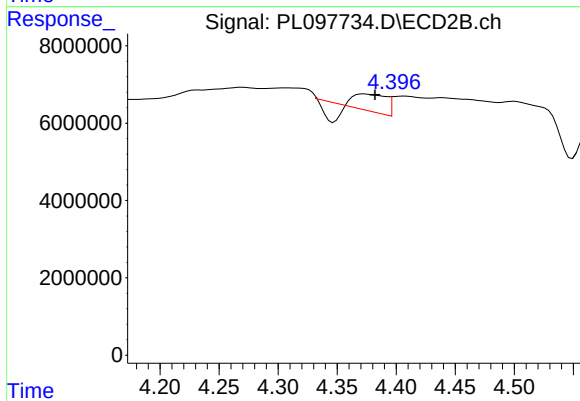

#24 Chlordane-2


R.T.: 4.373 min
Delta R.T.: -0.009 min
Response: 5452138
Conc: 18.51 ng/ml

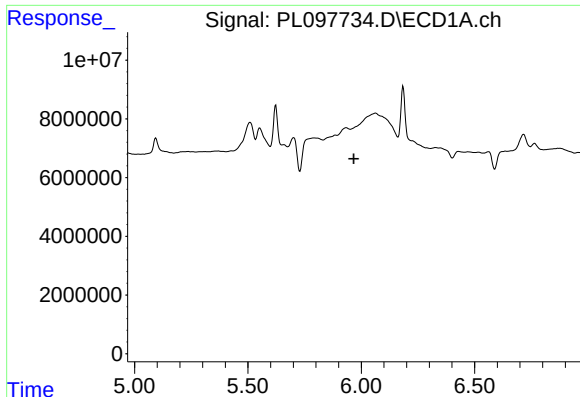

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

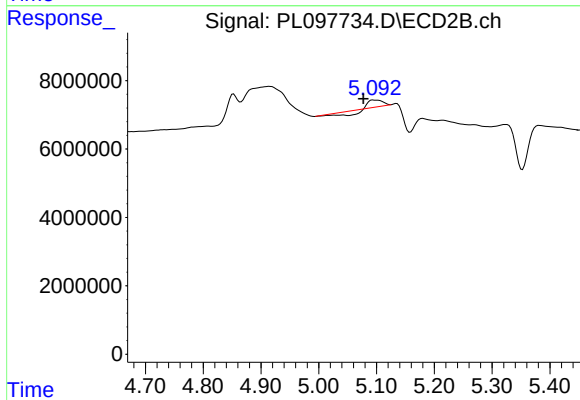


#26 Chlordane-4

R.T.: 5.094 min
Delta R.T.: 0.017 min
Response: 343767
Conc: 0.46 ng/ml

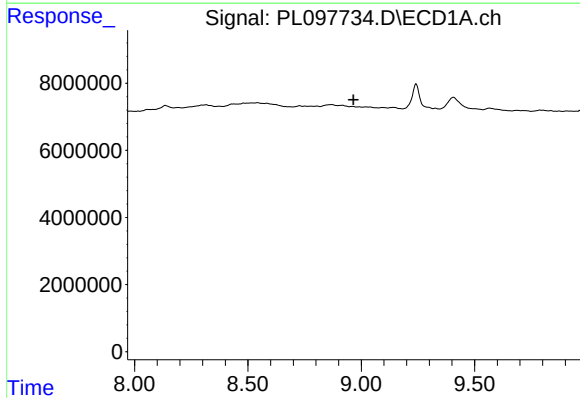

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.966 min
Response: 0
Conc: N.D.

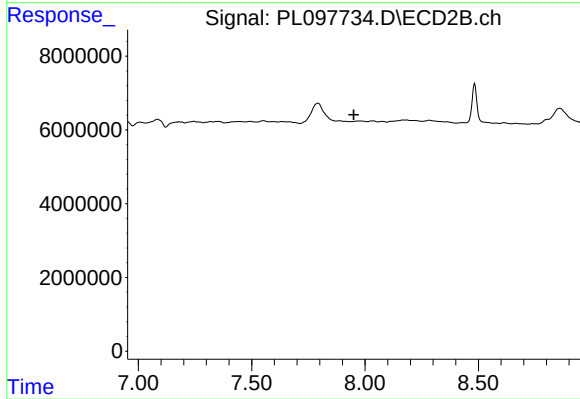

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 7.950 min
Response: 0
Conc: N.D.