

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
 Data File : PL097743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 12:35
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:26:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 25 13:23:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	2.800	371.1E6	558.1E6	99.810	101.231
28)	SA Decachlor...	8.970	7.951	229.8E6	334.6E6	98.860	98.003
Target Compounds							
23)	Chlordane-1	4.657	3.805	212.5E6	255.6E6	981.121	1006.500
24)	Chlordane-2	5.181	4.382	209.1E6	261.9E6	992.006	956.044
25)	Chlordane-3	5.884	5.014	798.2E6	847.2E6	1011.485	1015.593
26)	Chlordane-4	5.967	5.077	938.8E6	759.5E6	1005.804	999.190
27)	Chlordane-5	6.804	5.970	145.9E6	265.5E6	1011.958	1010.803



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
Data File : PL097743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 12:35
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:26:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Tue Nov 25 13:23:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

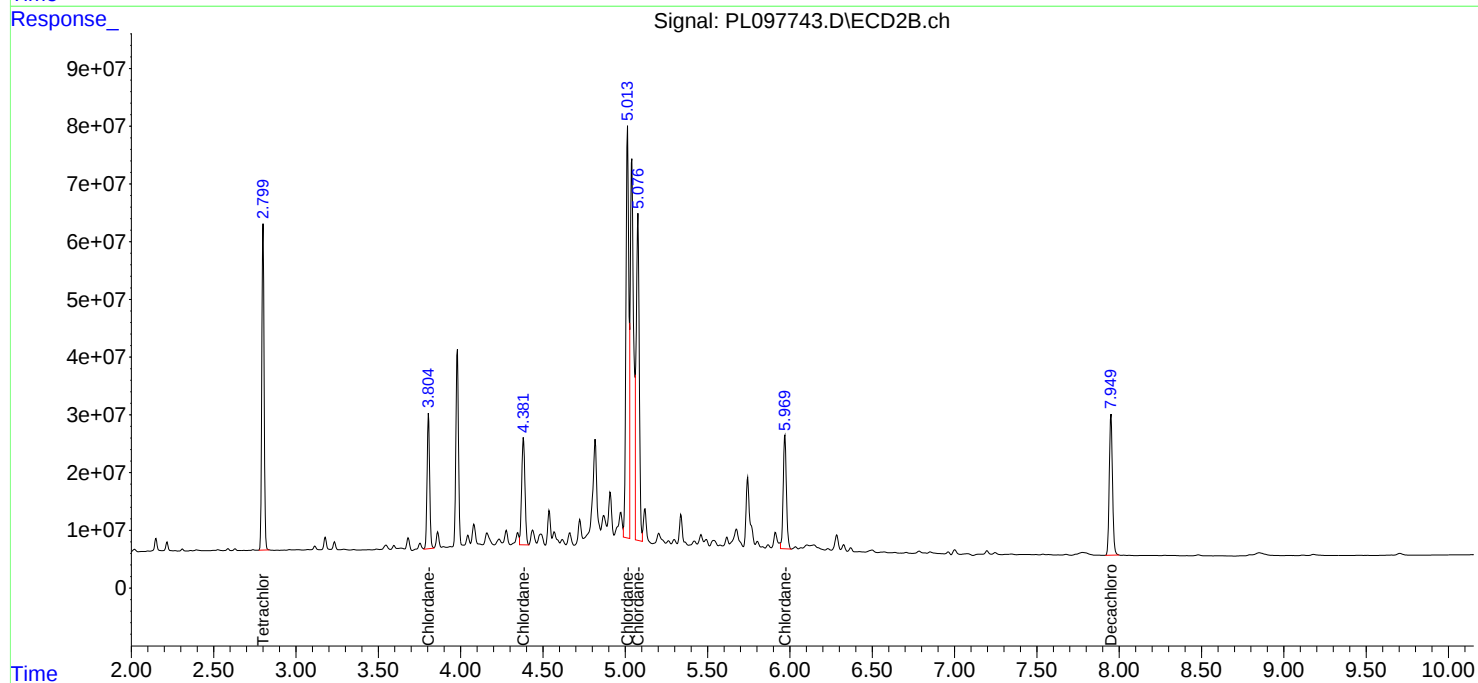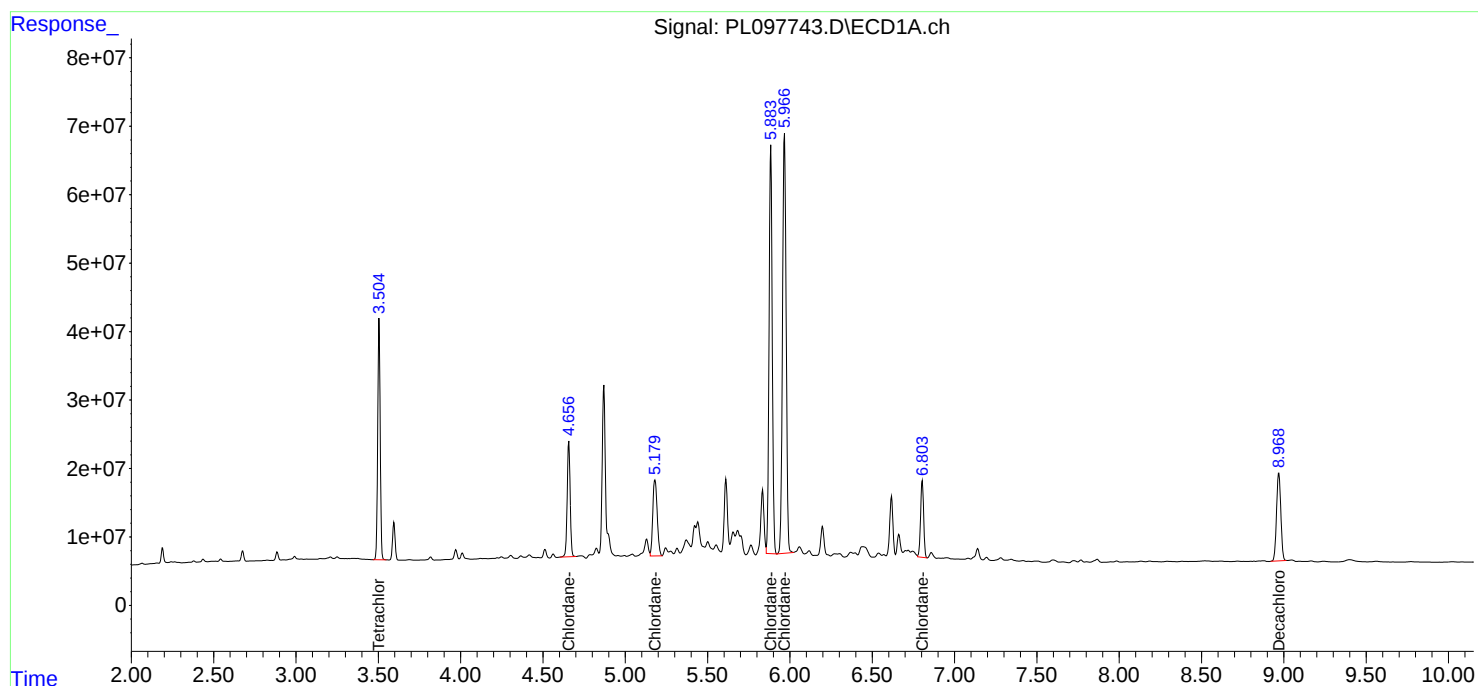


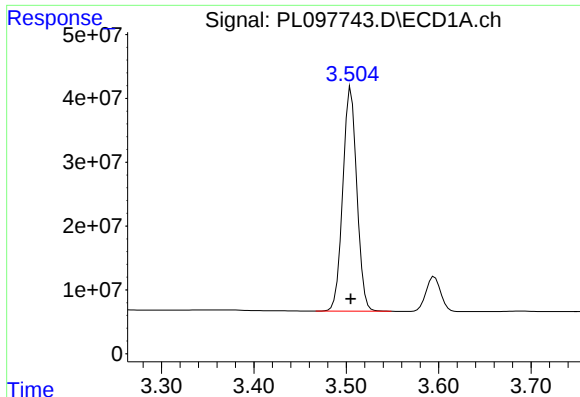

#1 Tetrachloro-m-xylene


R.T.: 3.505 min
Delta R.T.: 0.000 min
Response: 371053802
Conc: 99.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

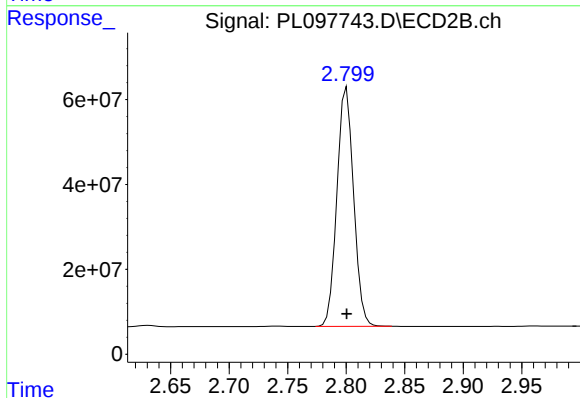


#1 Tetrachloro-m-xylene

R.T.: 2.800 min
Delta R.T.: 0.000 min
Response: 558071206
Conc: 101.23 ng/ml

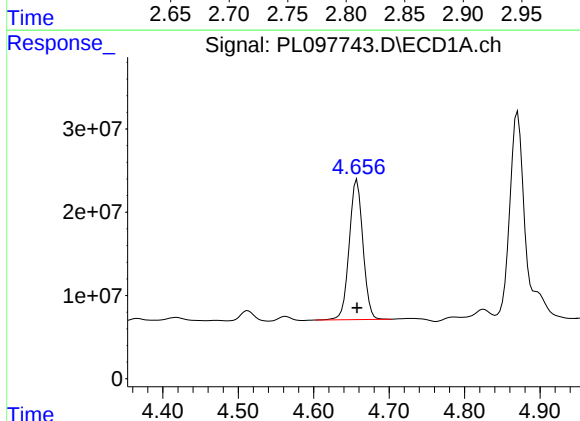


#23 Chlordane-1

R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 212499567
Conc: 981.12 ng/ml

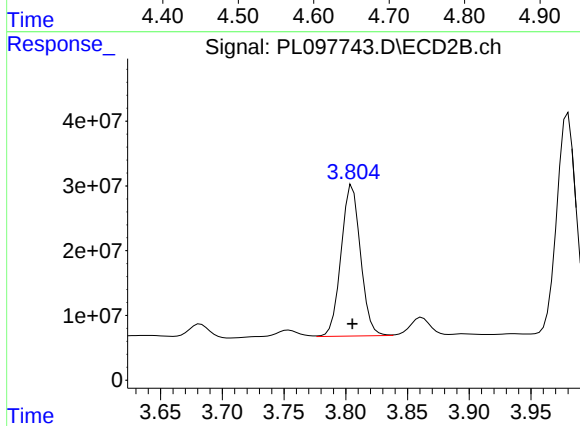

#23 Chlordane-1


R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 255644243
Conc: 1006.50 ng/ml

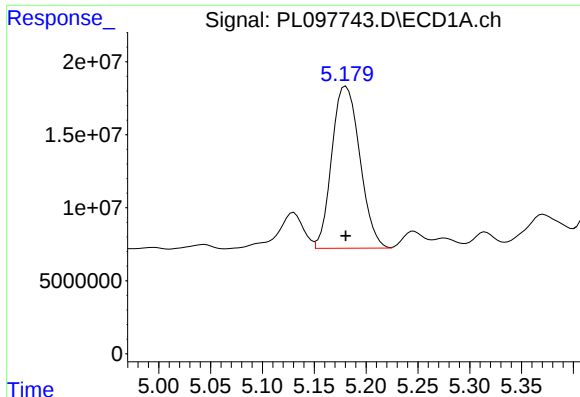

#24 Chlordane-2


R.T.: 5.181 min
Delta R.T.: 0.000 min
Response: 209066017
Conc: 992.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

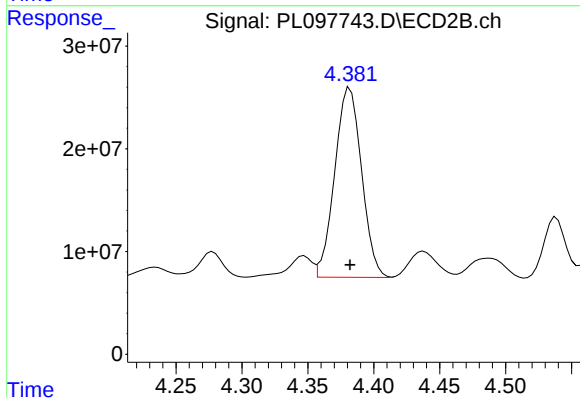


#24 Chlordane-2

R.T.: 4.382 min
Delta R.T.: 0.000 min
Response: 261871011
Conc: 956.04 ng/ml

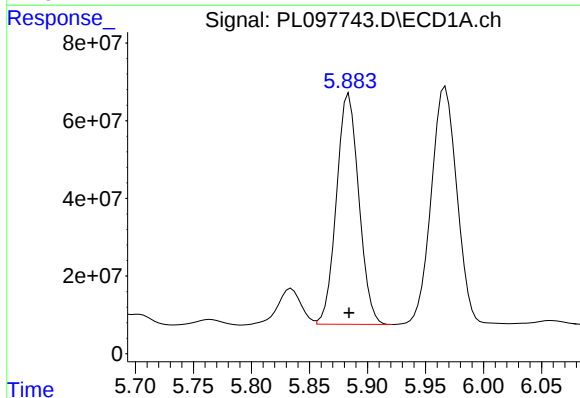


#25 Chlordane-3

R.T.: 5.884 min
Delta R.T.: 0.000 min
Response: 798179295
Conc: 1011.49 ng/ml

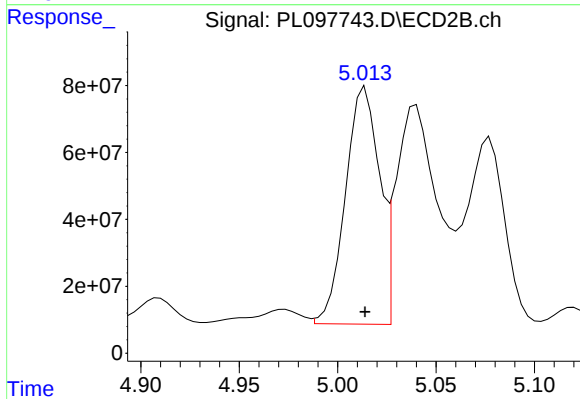

#25 Chlordane-3


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 847246899
Conc: 1015.59 ng/ml

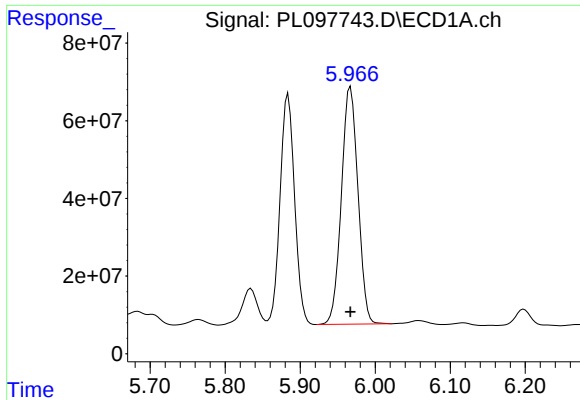

#26 Chlordane-4


R.T.: 5.967 min
Delta R.T.: 0.000 min
Response: 938827941
Conc: 1005.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

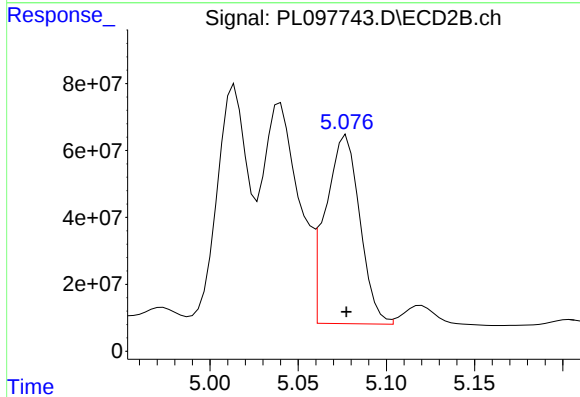


#26 Chlordane-4

R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 759515580
Conc: 999.19 ng/ml

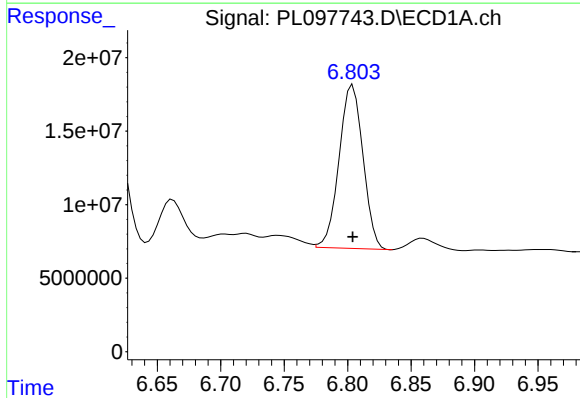


#27 Chlordane-5

R.T.: 6.804 min
Delta R.T.: 0.000 min
Response: 145911624
Conc: 1011.96 ng/ml

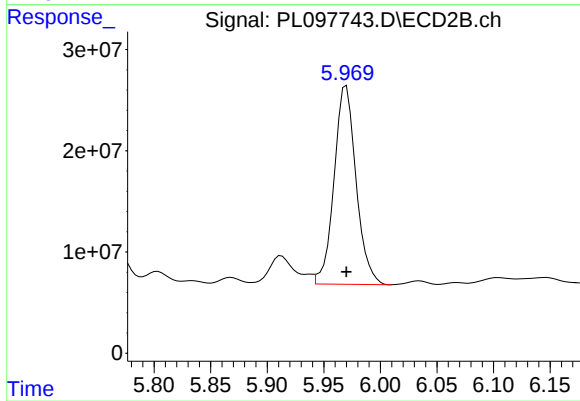

#27 Chlordane-5


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 265526759
Conc: 1010.80 ng/ml

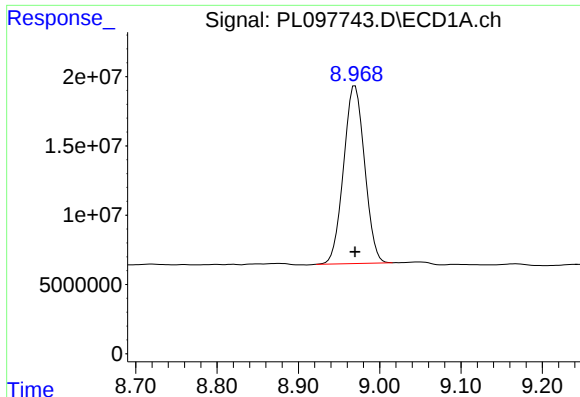

#28 Decachlorobiphenyl

R.T.: 8.970 min
Delta R.T.: 0.000 min
Response: 229773564
Conc: 98.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

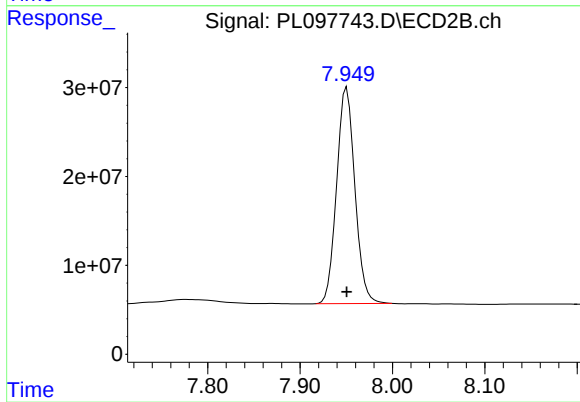

#28 Decachlorobiphenyl

R.T.: 7.951 min
Delta R.T.: 0.000 min
Response: 334569807
Conc: 98.00 ng/ml