

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
 Data File : PL097744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 12:48
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:28:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 25 13:23:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	2.802	280.1E6	412.5E6	75.235	74.882
28)	SA Decachlor...	8.966	7.949	169.9E6	257.1E6	73.723	75.200
Target Compounds							
23)	Chlordane-1	4.656	3.806	171.9E6	190.9E6	778.483	751.157
24)	Chlordane-2	5.179	4.382	161.2E6	210.5E6	760.005	762.143
25)	Chlordane-3	5.881	5.014	598.9E6	621.8E6	755.905	746.865
26)	Chlordane-4	5.965	5.078	709.8E6	571.9E6	756.941	751.604
27)	Chlordane-5	6.801	5.970	110.4E6	199.5E6	760.476	756.180



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
Data File : PL097744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 12:48
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:28:29 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Tue Nov 25 13:23:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

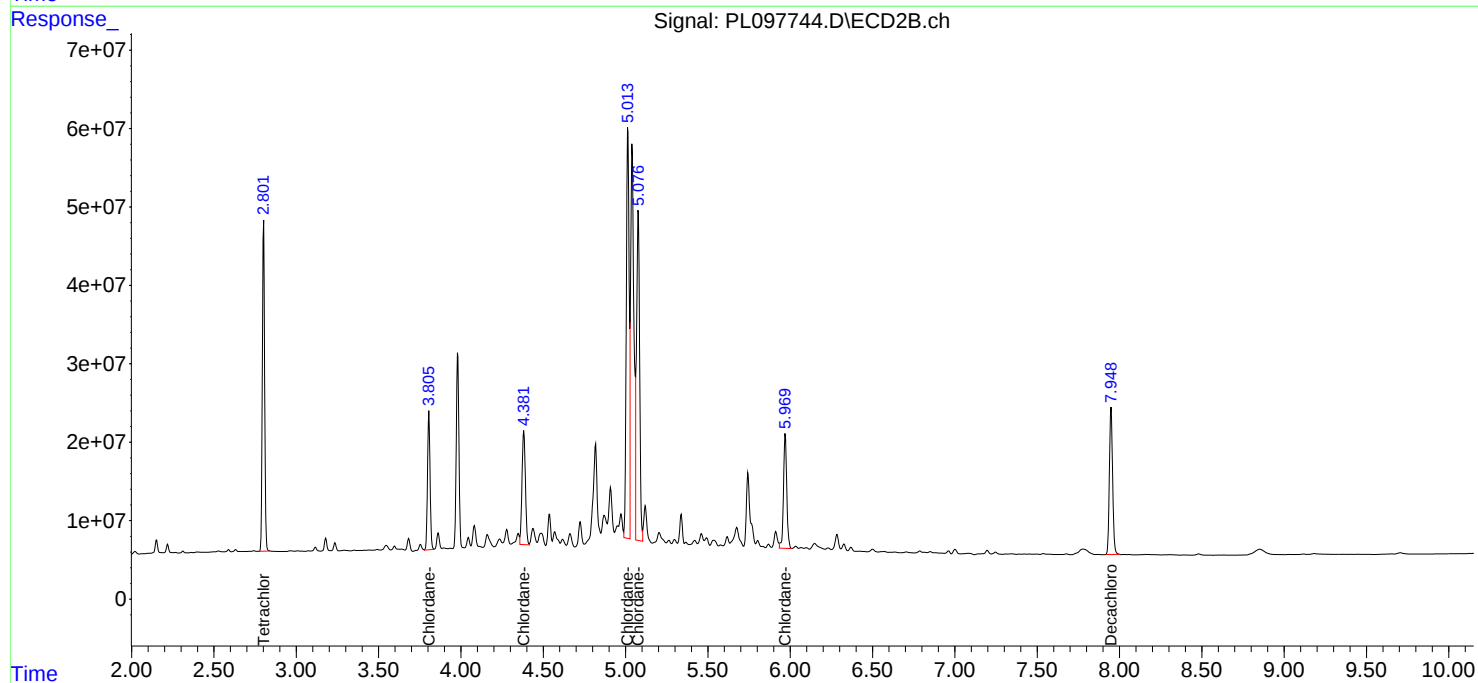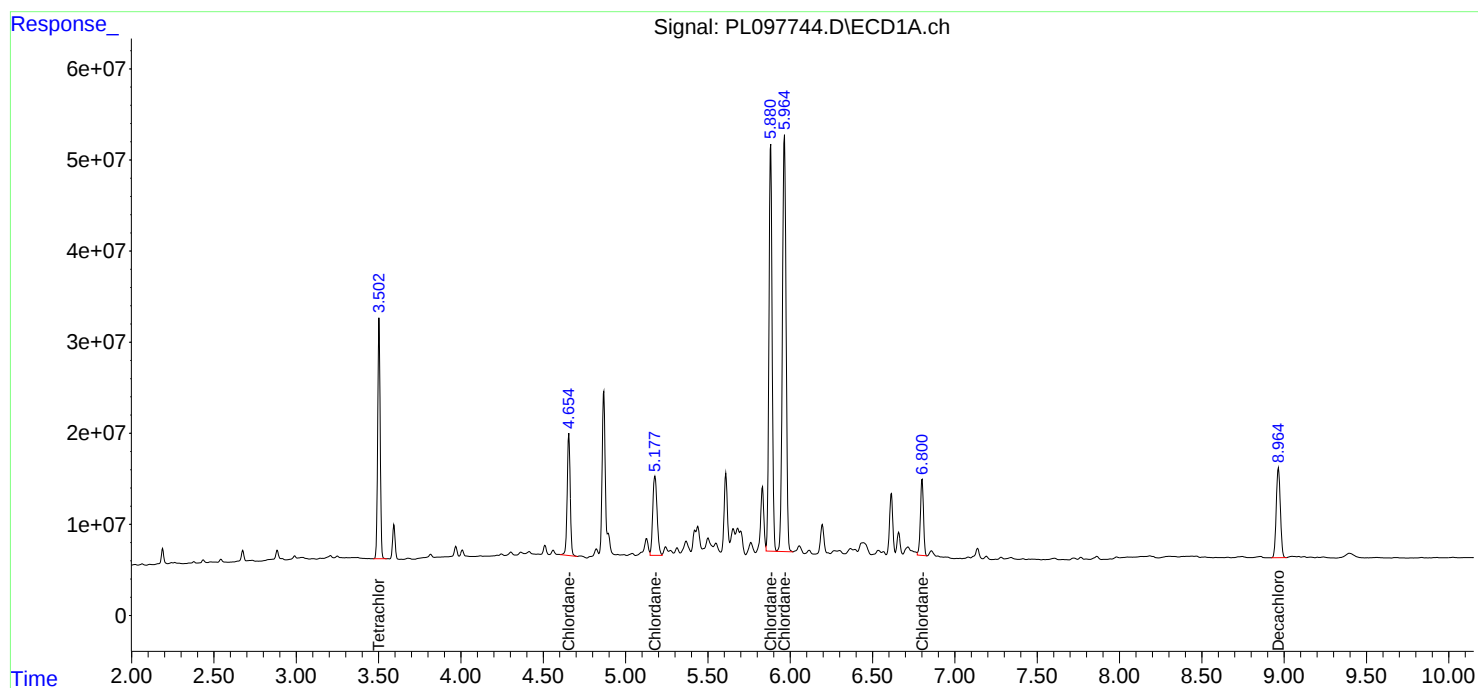


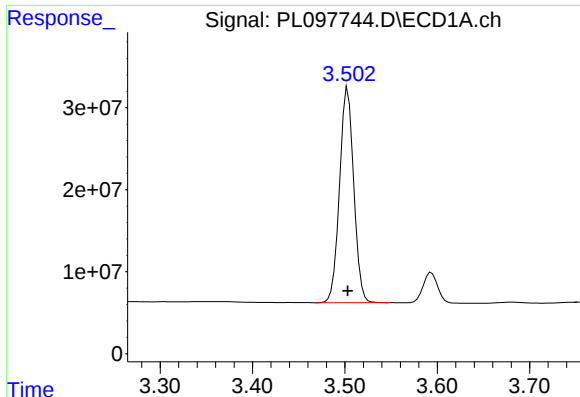

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 280132844
Conc: 75.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

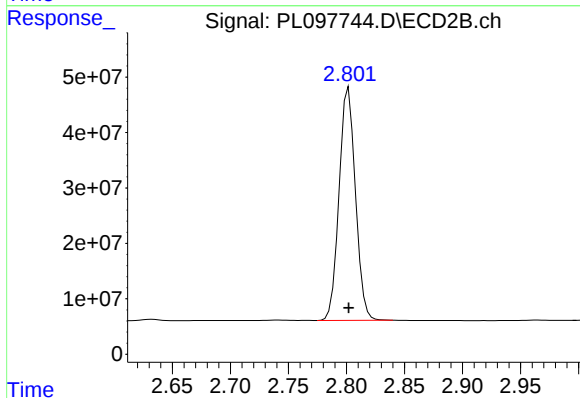


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 412484336
Conc: 74.88 ng/ml

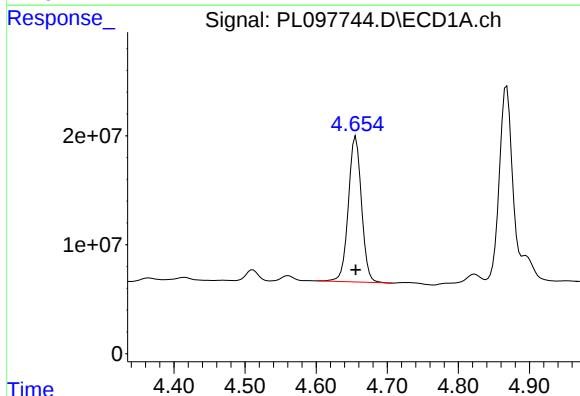


#23 Chlordane-1

R.T.: 4.656 min
Delta R.T.: 0.000 min
Response: 171874317
Conc: 778.48 ng/ml

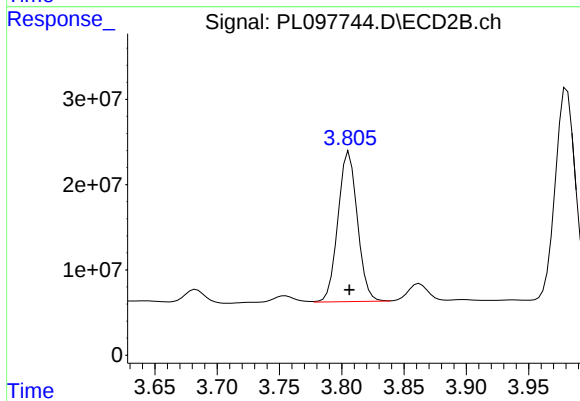

#23 Chlordane-1


R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 190936033
Conc: 751.16 ng/ml

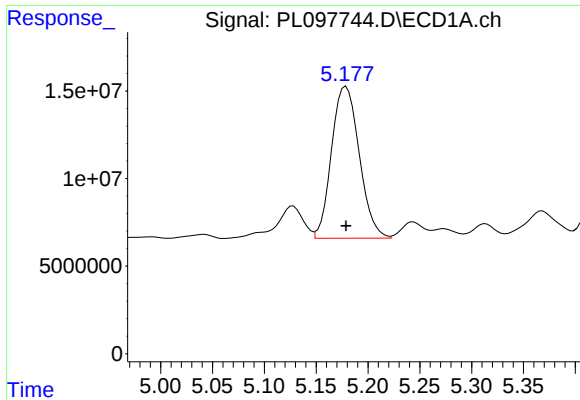

#24 Chlordane-2


R.T.: 5.179 min
Delta R.T.: 0.000 min
Response: 161247082
Conc: 760.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

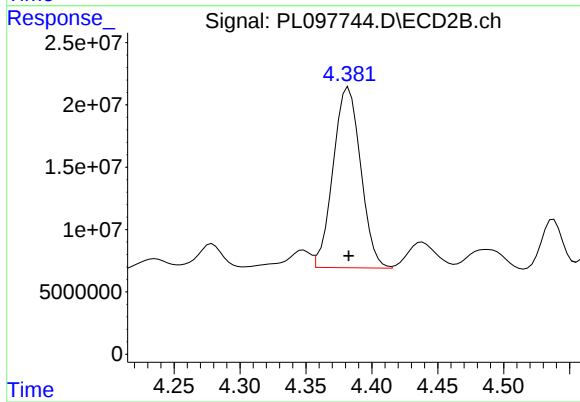


#24 Chlordane-2

R.T.: 4.382 min
Delta R.T.: 0.000 min
Response: 210463293
Conc: 762.14 ng/ml

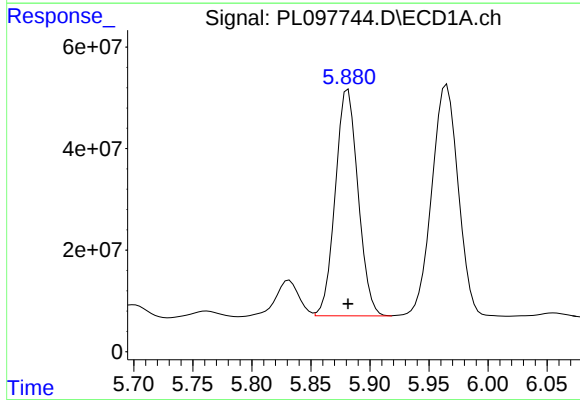


#25 Chlordane-3

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 598854292
Conc: 755.90 ng/ml

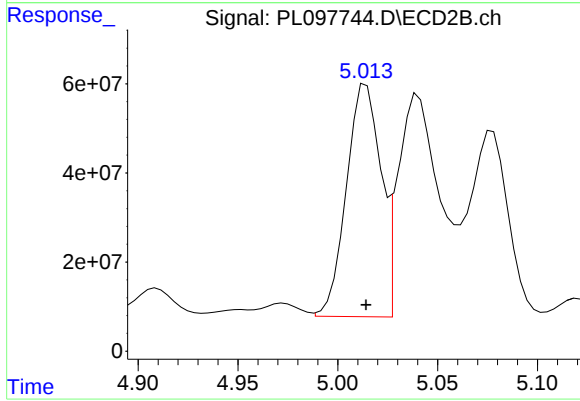

#25 Chlordane-3


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 621764619
Conc: 746.87 ng/ml

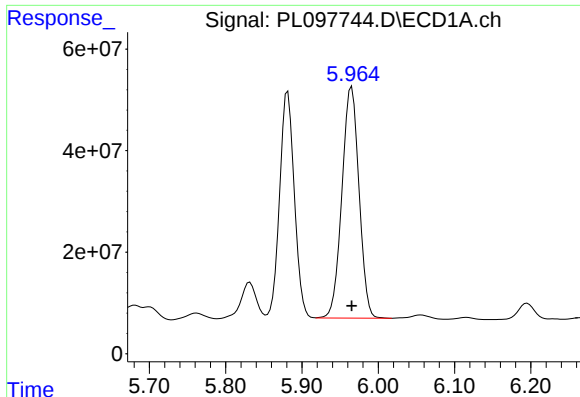

#26 Chlordane-4


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 709820958
Conc: 756.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

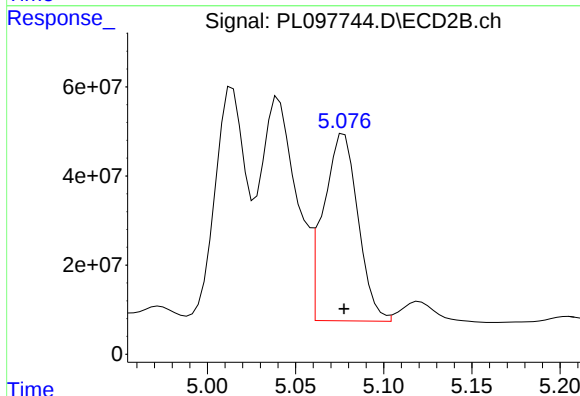


#26 Chlordane-4

R.T.: 5.078 min
Delta R.T.: 0.000 min
Response: 571930137
Conc: 751.60 ng/ml

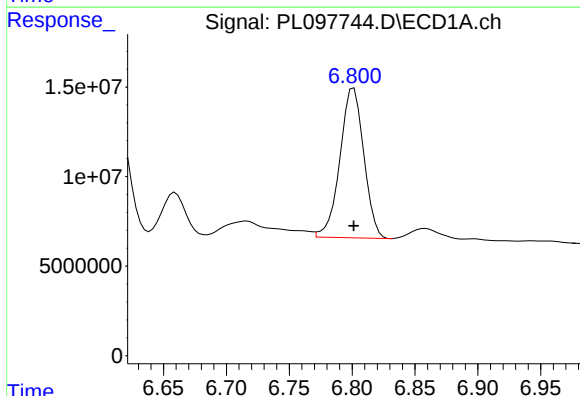


#27 Chlordane-5

R.T.: 6.801 min
Delta R.T.: 0.000 min
Response: 110422373
Conc: 760.48 ng/ml

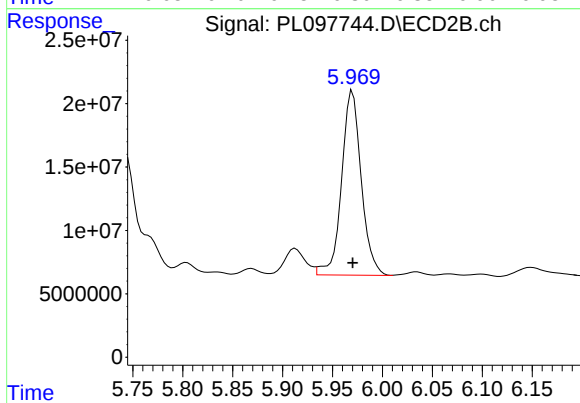

#27 Chlordane-5


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 199461702
Conc: 756.18 ng/ml

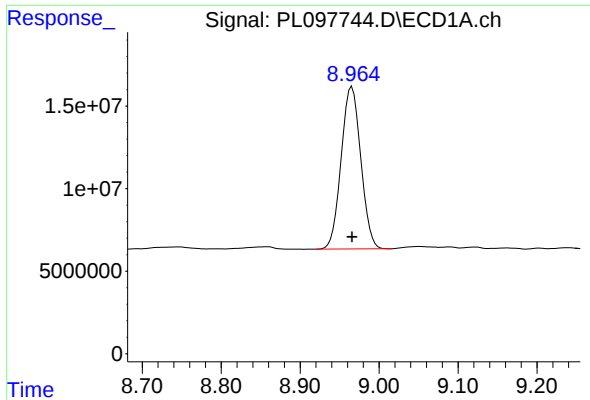

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: 0.000 min
Response: 169902465
Conc: 73.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

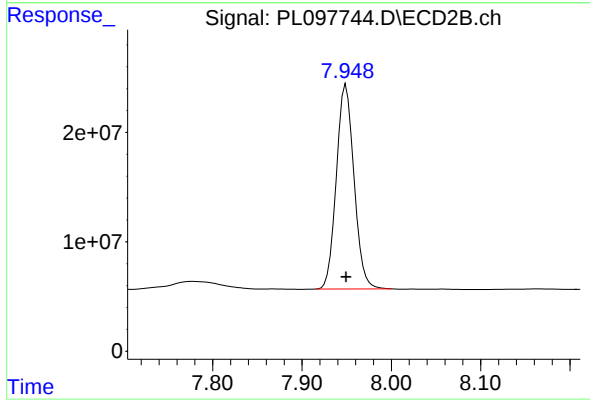

#28 Decachlorobiphenyl

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 257066123
Conc: 75.20 ng/ml