

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
 Data File : PL097745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 13:02
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:24:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 25 13:23:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	2.802	186.2E6	272.2E6	50.000	50.000
28)	SA Decachlor...	8.967	7.950	117.5E6	174.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.656	3.806	110.3E6	126.2E6	500.000	500.000
24)	Chlordane-2	5.178	4.382	106.2E6	143.0E6	500.000	500.000
25)	Chlordane-3	5.881	5.014	390.0E6	410.6E6	500.000	500.000
26)	Chlordane-4	5.965	5.078	464.0E6	380.4E6	500.000	500.000
27)	Chlordane-5	6.802	5.970	71231653	129.9E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
Data File : PL097745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 13:02
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:24:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Tue Nov 25 13:23:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

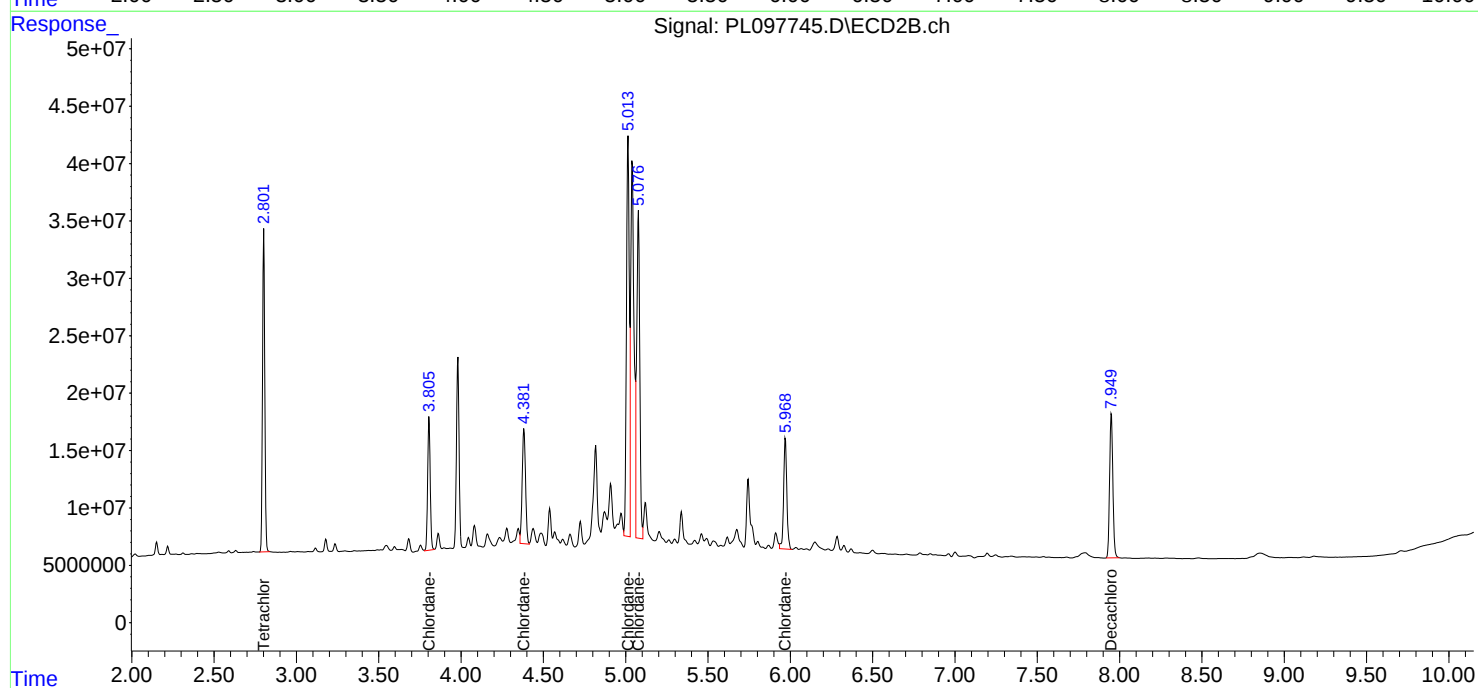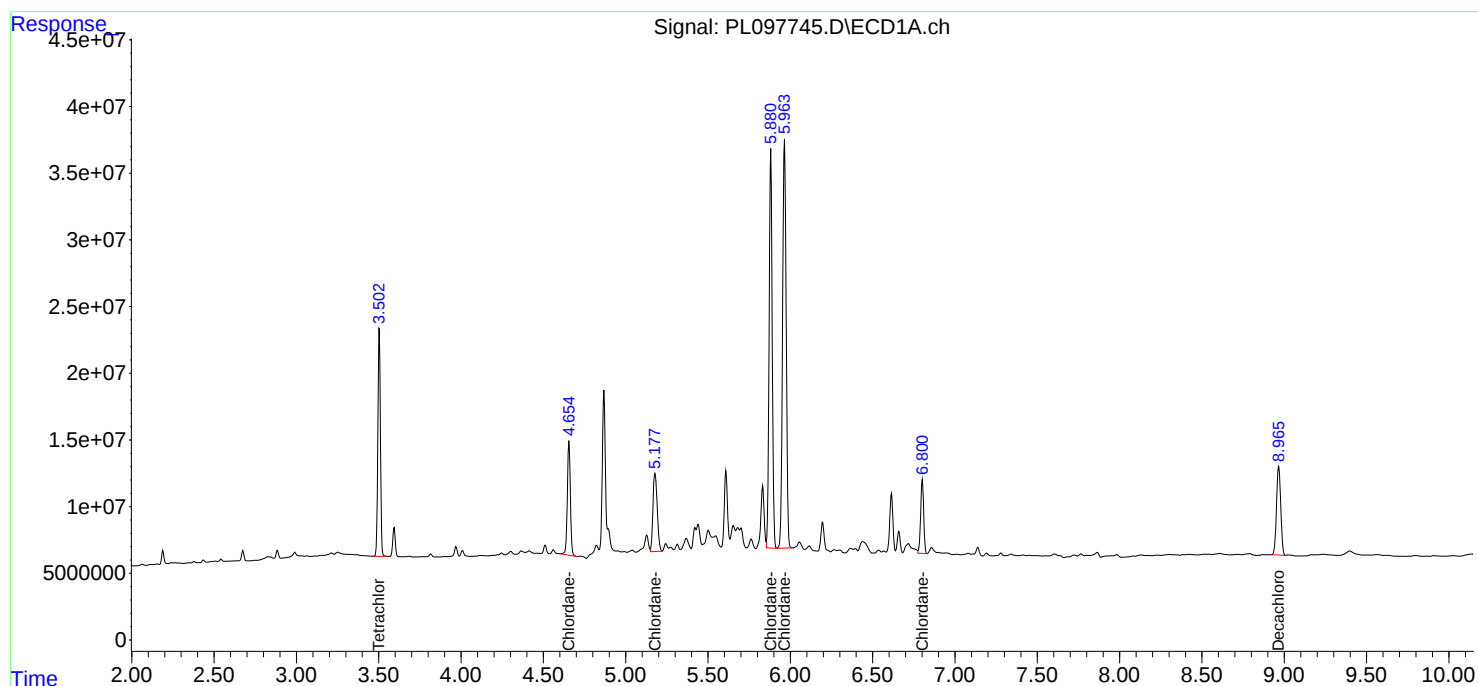


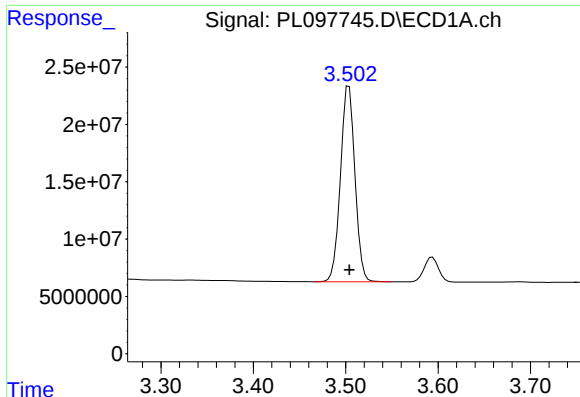

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 186233835
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

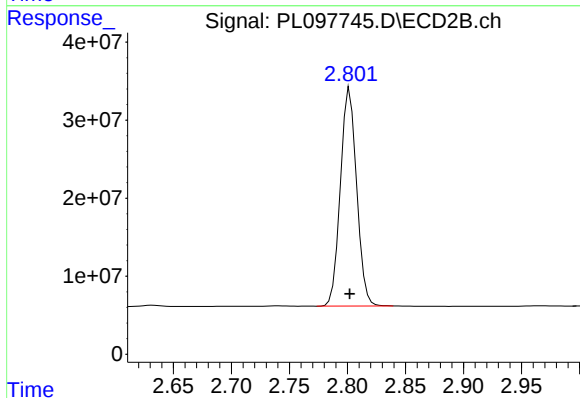


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 272246862
Conc: 50.00 ng/ml

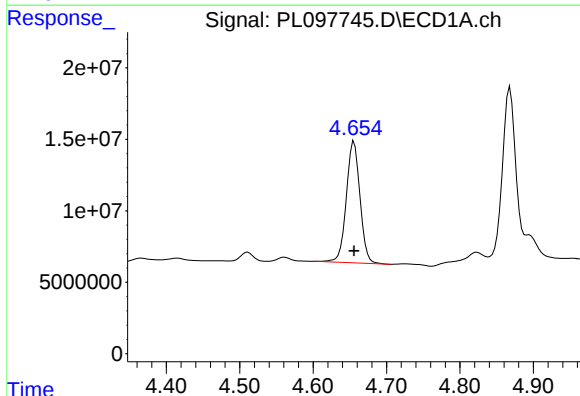


#23 Chlordane-1

R.T.: 4.656 min
Delta R.T.: 0.000 min
Response: 110338835
Conc: 500.00 ng/ml

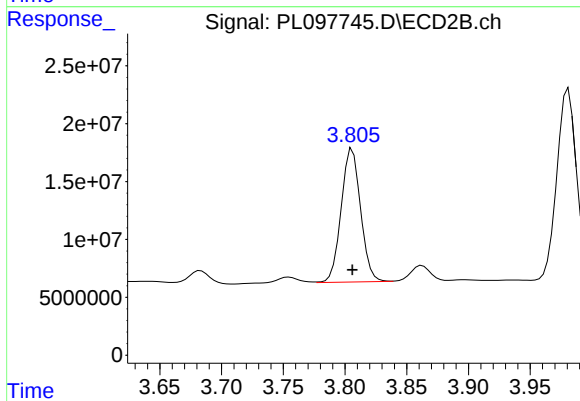

#23 Chlordane-1


R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 126171214
Conc: 500.00 ng/ml

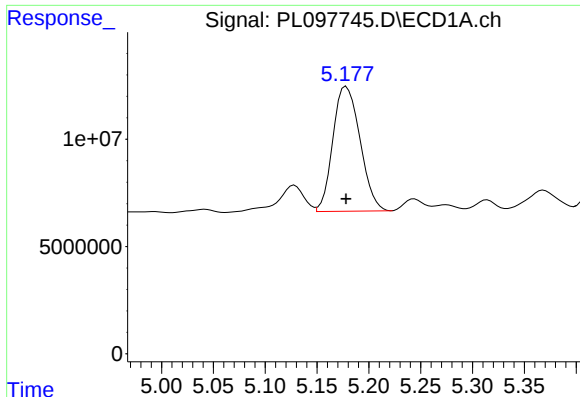

#24 Chlordane-2


R.T.: 5.178 min
Delta R.T.: 0.000 min
Response: 106217827
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

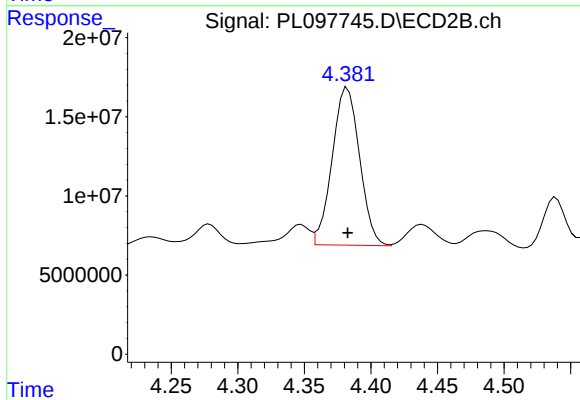


#24 Chlordane-2

R.T.: 4.382 min
Delta R.T.: 0.000 min
Response: 142975512
Conc: 500.00 ng/ml

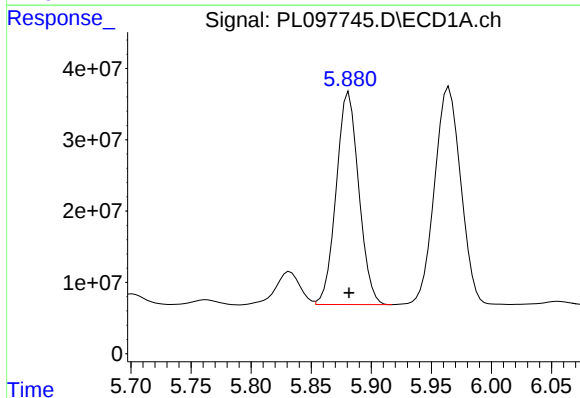


#25 Chlordane-3

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 390026541
Conc: 500.00 ng/ml

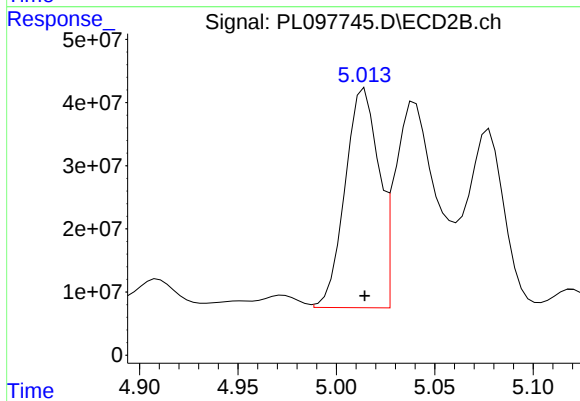

#25 Chlordane-3


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 410614997
Conc: 500.00 ng/ml

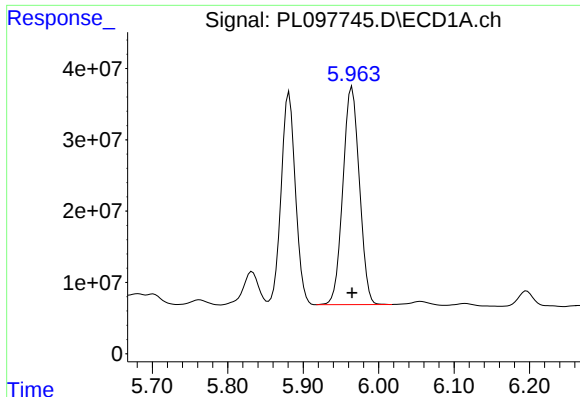

#26 Chlordane-4


R.T.: 5.965 min
Delta R.T.: 0.000 min
Response: 463996121
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

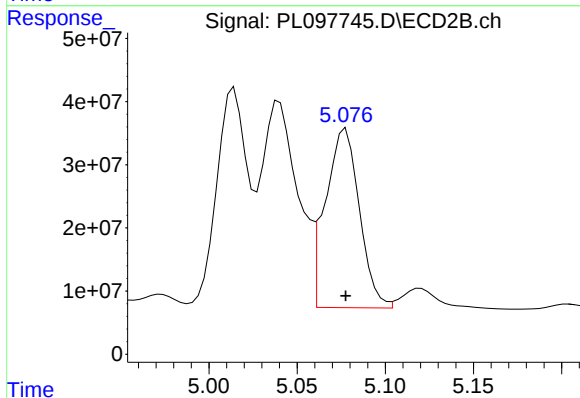


#26 Chlordane-4

R.T.: 5.078 min
Delta R.T.: 0.000 min
Response: 380373863
Conc: 500.00 ng/ml

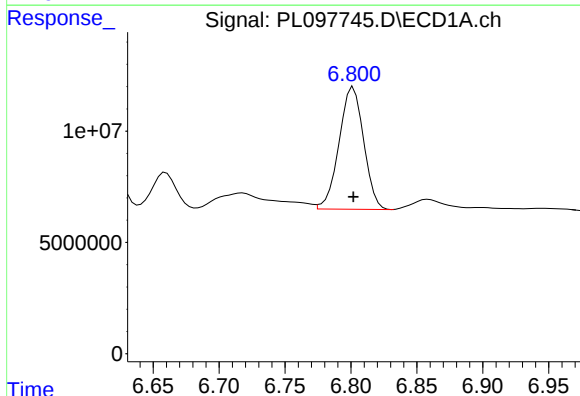


#27 Chlordane-5

R.T.: 6.802 min
Delta R.T.: 0.000 min
Response: 71231653
Conc: 500.00 ng/ml

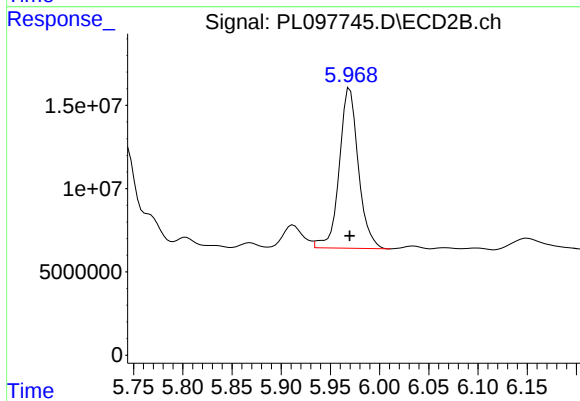

#27 Chlordane-5


R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 129925546
Conc: 500.00 ng/ml

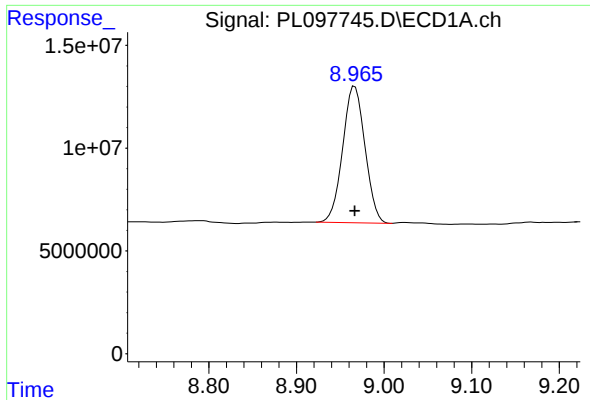

#28 Decachlorobiphenyl

R.T.: 8.967 min
Delta R.T.: 0.000 min
Response: 117536314
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

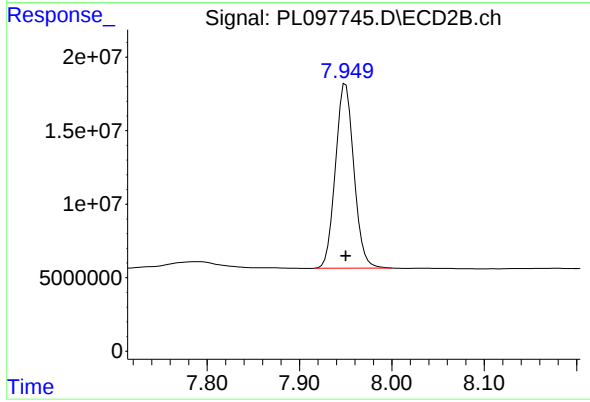

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 174103377
Conc: 50.00 ng/ml