

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
 Data File : PL097754.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2025 16:41
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL112525

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 17:54:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 25 17:53:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	2.802	190.7E6	282.5E6	50.012	51.410
28)	SA Decachlor...	8.966	7.950	119.2E6	182.7E6	50.368	48.330
Target Compounds							
23)	Chlordane-1	4.656	3.807	113.0E6	128.1E6	497.510	504.308
24)	Chlordane-2	5.179	4.383	110.4E6	144.7E6	499.659	491.128
25)	Chlordane-3	5.882	5.015	401.0E6	420.3E6	508.298	513.739
26)	Chlordane-4	5.965	5.078	478.6E6	387.8E6	503.339	516.087
27)	Chlordane-5	6.802	5.970	75958760	137.7E6	528.789	525.546



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112525\
Data File : PL097754.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2025 16:41
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL112525

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 17:54:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112525.M
Quant Title : GC Extractables
QLast Update : Tue Nov 25 17:53:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

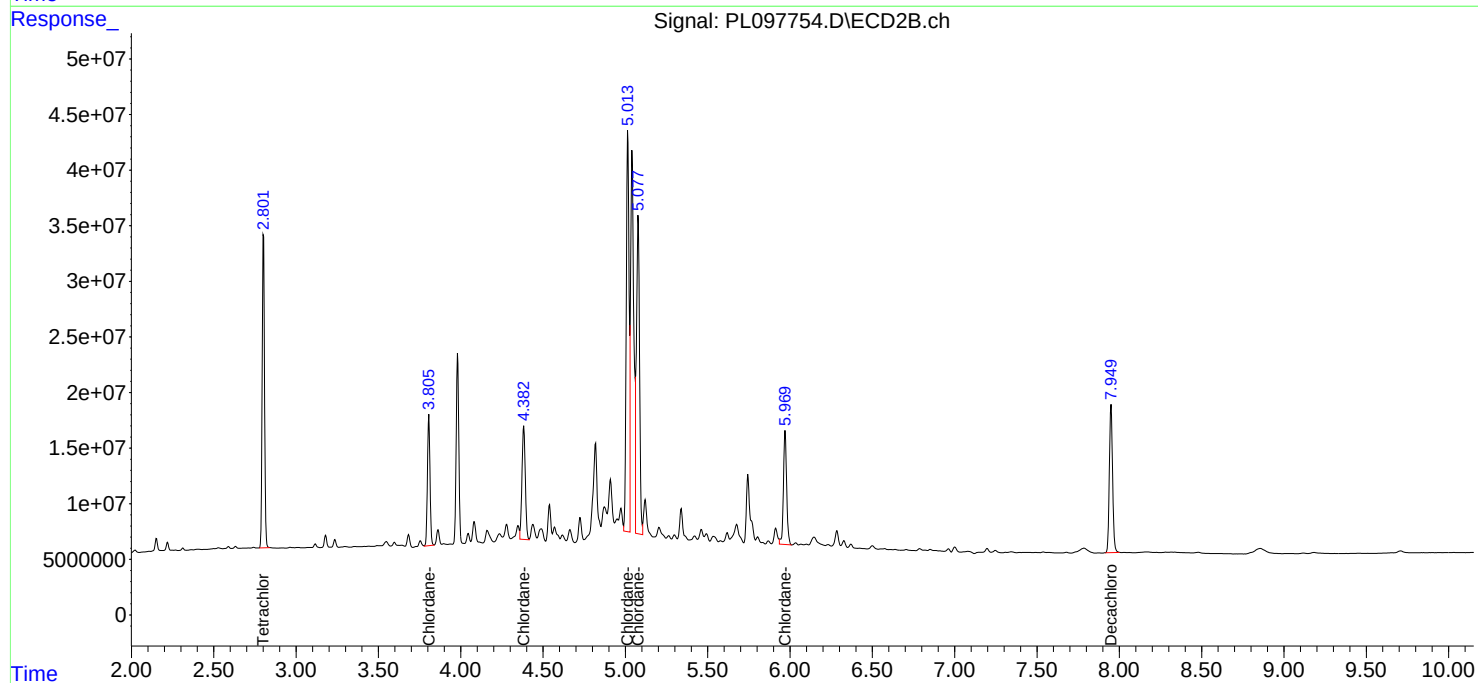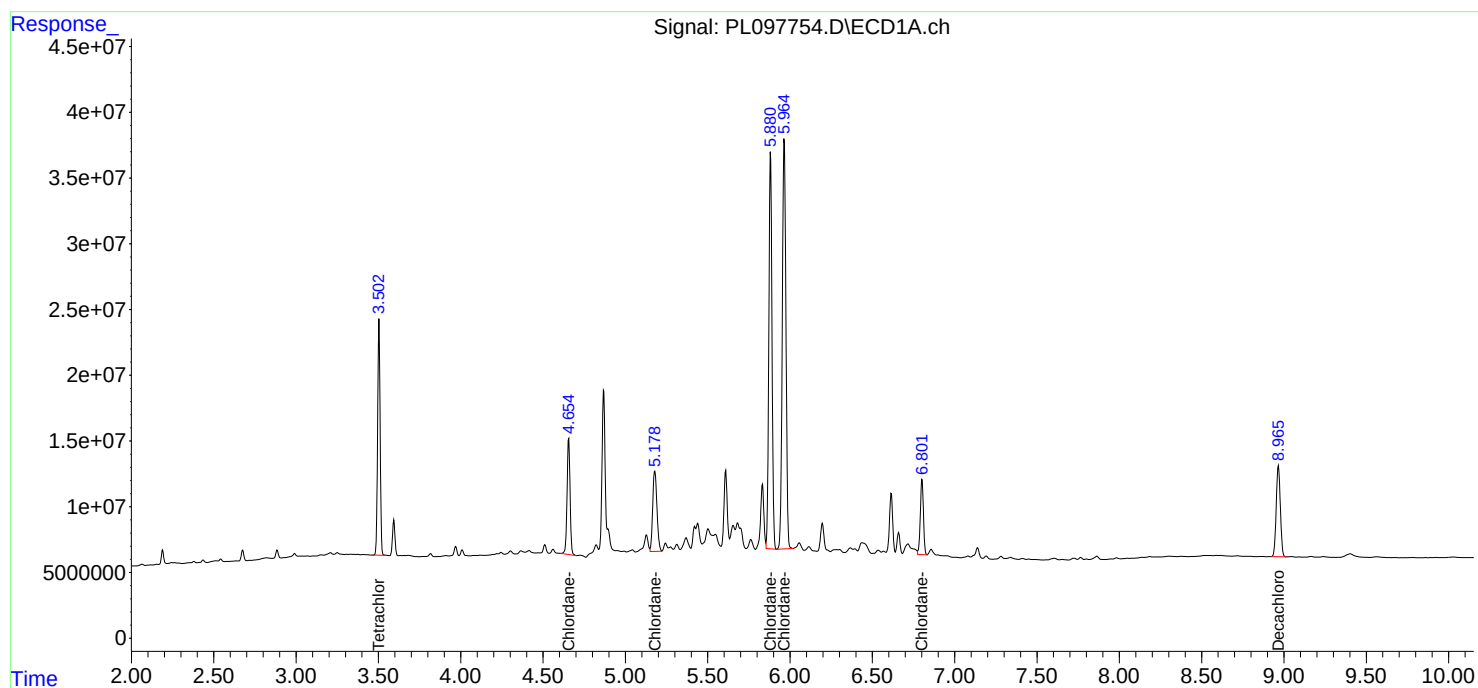


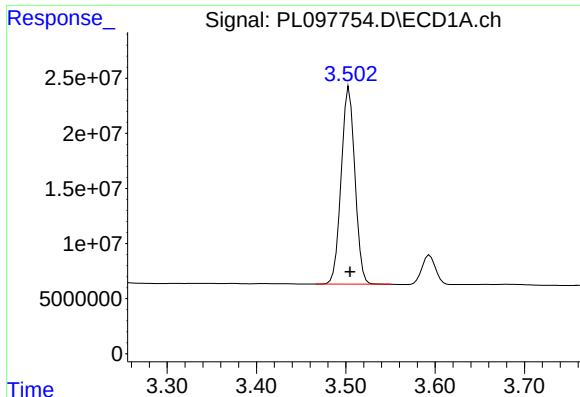

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: -0.001 min
Response: 190673001
Conc: 50.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112525

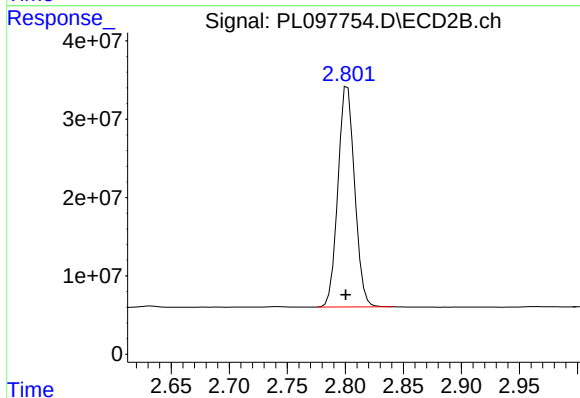


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.002 min
Response: 282455716
Conc: 51.41 ng/ml

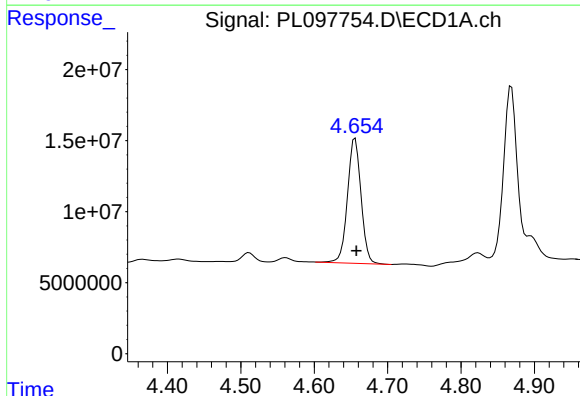


#23 Chlordane-1

R.T.: 4.656 min
Delta R.T.: -0.002 min
Response: 113020758
Conc: 497.51 ng/ml

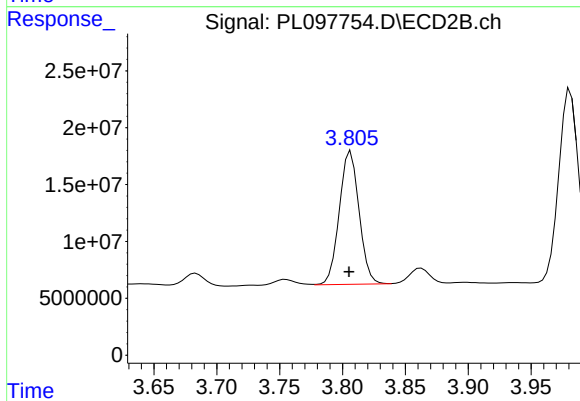

#23 Chlordane-1


R.T.: 3.807 min
Delta R.T.: 0.001 min
Response: 128147934
Conc: 504.31 ng/ml

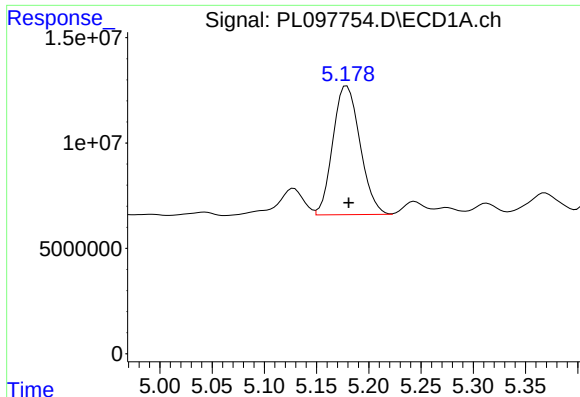

#24 Chlordane-2


R.T.: 5.179 min
Delta R.T.: -0.002 min
Response: 110415239
Conc: 499.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112525

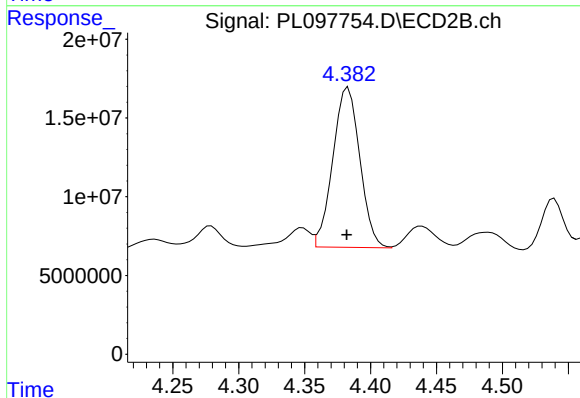


#24 Chlordane-2

R.T.: 4.383 min
Delta R.T.: 0.001 min
Response: 144661563
Conc: 491.13 ng/ml

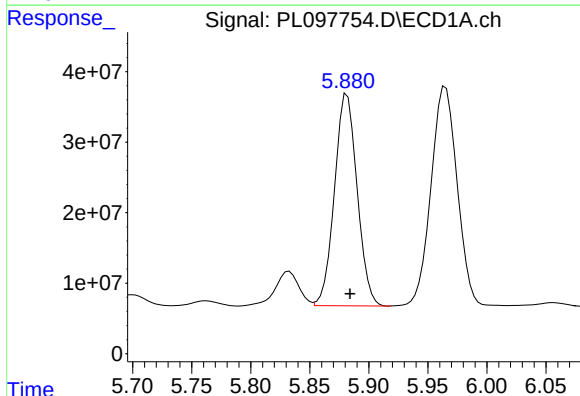


#25 Chlordane-3

R.T.: 5.882 min
Delta R.T.: -0.002 min
Response: 400974653
Conc: 508.30 ng/ml

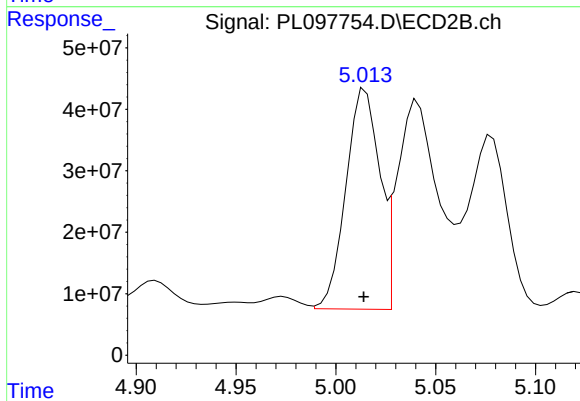

#25 Chlordane-3


R.T.: 5.015 min
Delta R.T.: 0.000 min
Response: 420260161
Conc: 513.74 ng/ml

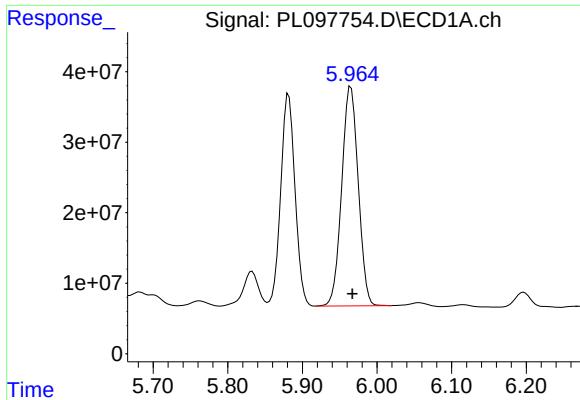

#26 Chlordane-4


R.T.: 5.965 min
Delta R.T.: -0.002 min
Response: 478606452
Conc: 503.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112525

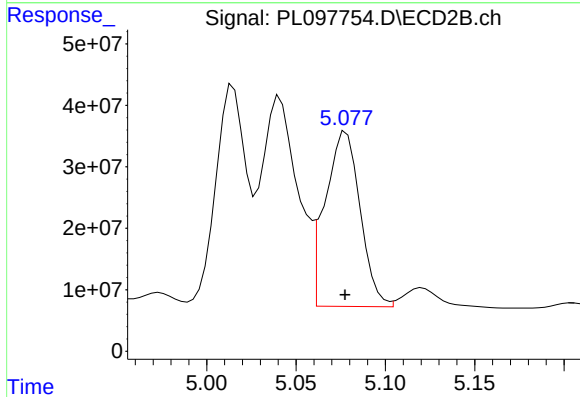


#26 Chlordane-4

R.T.: 5.078 min
Delta R.T.: 0.000 min
Response: 387770897
Conc: 516.09 ng/ml

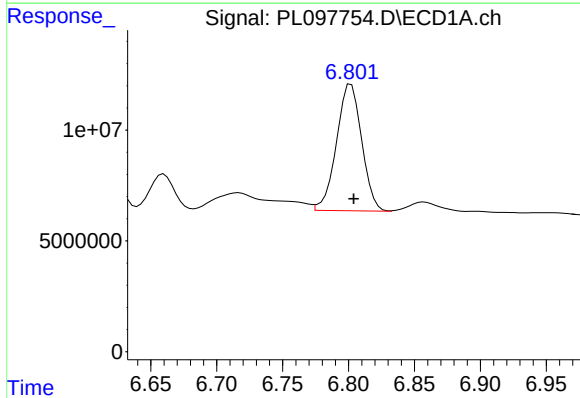


#27 Chlordane-5

R.T.: 6.802 min
Delta R.T.: -0.002 min
Response: 75958760
Conc: 528.79 ng/ml

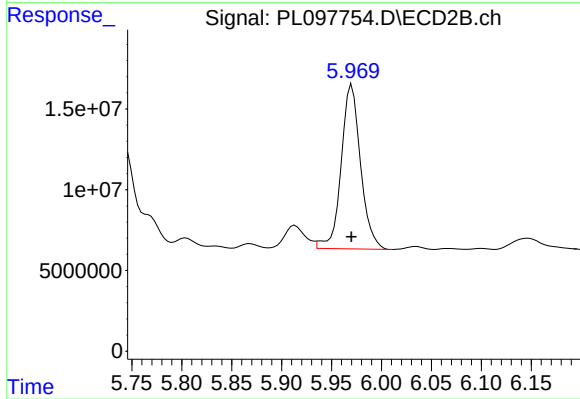

#27 Chlordane-5

R.T.: 5.970 min
Delta R.T.: 0.000 min
Response: 137692895
Conc: 525.55 ng/ml

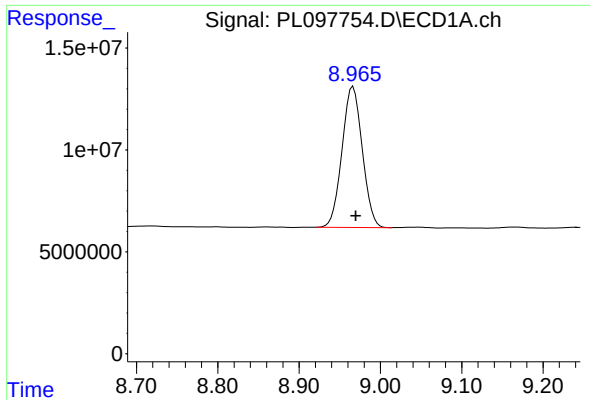

#28 Decachlorobiphenyl


R.T.: 8.966 min

Delta R.T.: -0.003 min

Response: 119162050

Conc: 50.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL112525

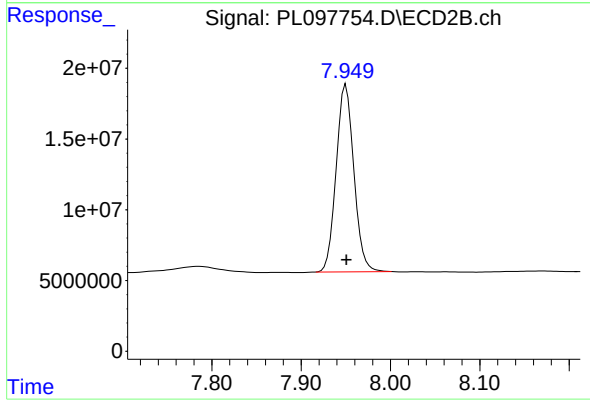

#28 Decachlorobiphenyl

R.T.: 7.950 min

Delta R.T.: 0.000 min

Response: 182682057

Conc: 48.33 ng/ml