

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
 Data File : PL042439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2018 08:19
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 10:15:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.101	129.0E6	62934423	21.928	21.882
28)	SA Decachlor...	8.207	9.233	120.4E6	52289450	19.103	21.680
Target Compounds							
5)	MB Aldrin	0.000	5.586	0	363218	N.D.	0.095 #
6)	B beta-BHC	4.403f	0.000	2512741	0	0.709	N.D. #
8)	B Heptachlo...	0.000	5.940f	0	1682181	N.D.	0.469 #
16)	A 4,4'-DDD	0.000	6.961	0	2719845	N.D.	1.033 #
19)	B Endosulfa...	6.665	0.000	14021865	0	2.247	N.D. #
20)	A Methoxychlor	6.883f	0.000	857911	0	0.272	N.D. #
23)	Chlordane-1	4.403	0.000	2512741	0	9.089	N.D. #
24)	Chlordane-2	0.000	5.586	0	363218	N.D.	2.605 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
Data File : PL042439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2018 08:19
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 10:15:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

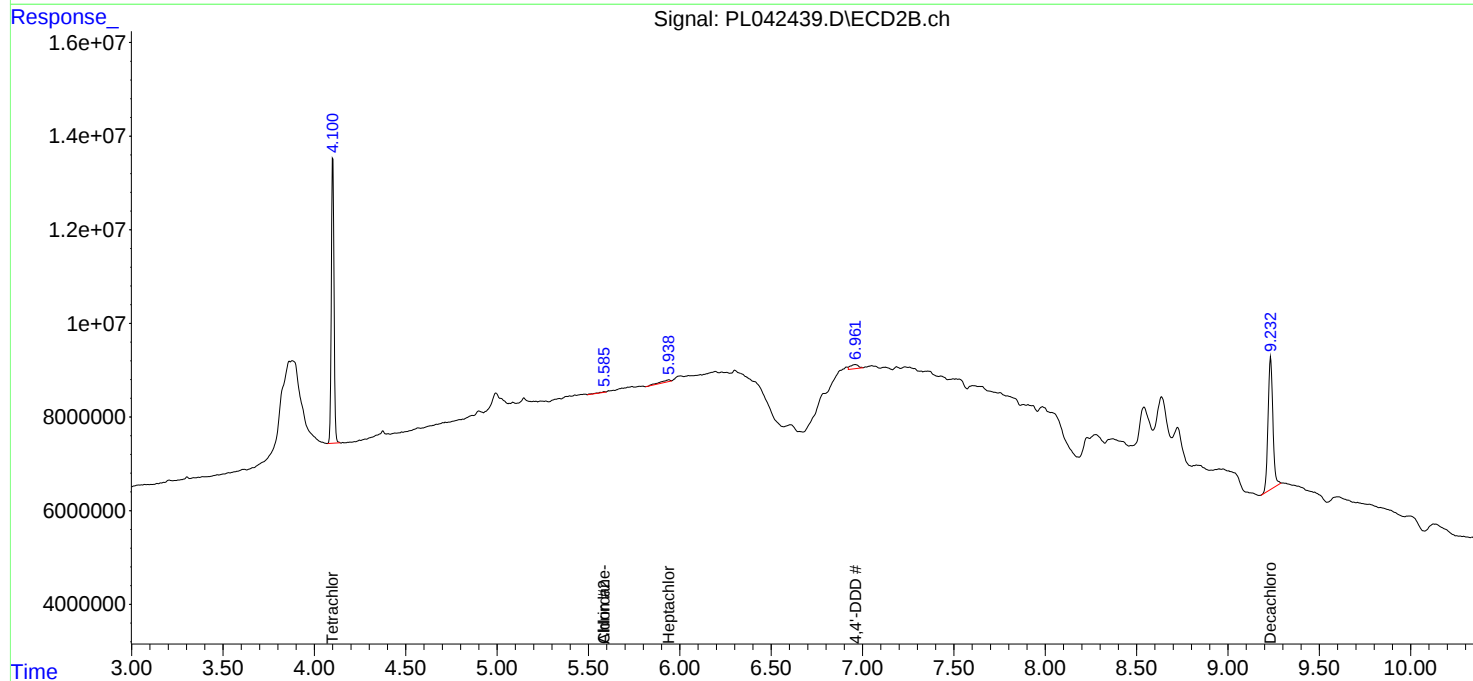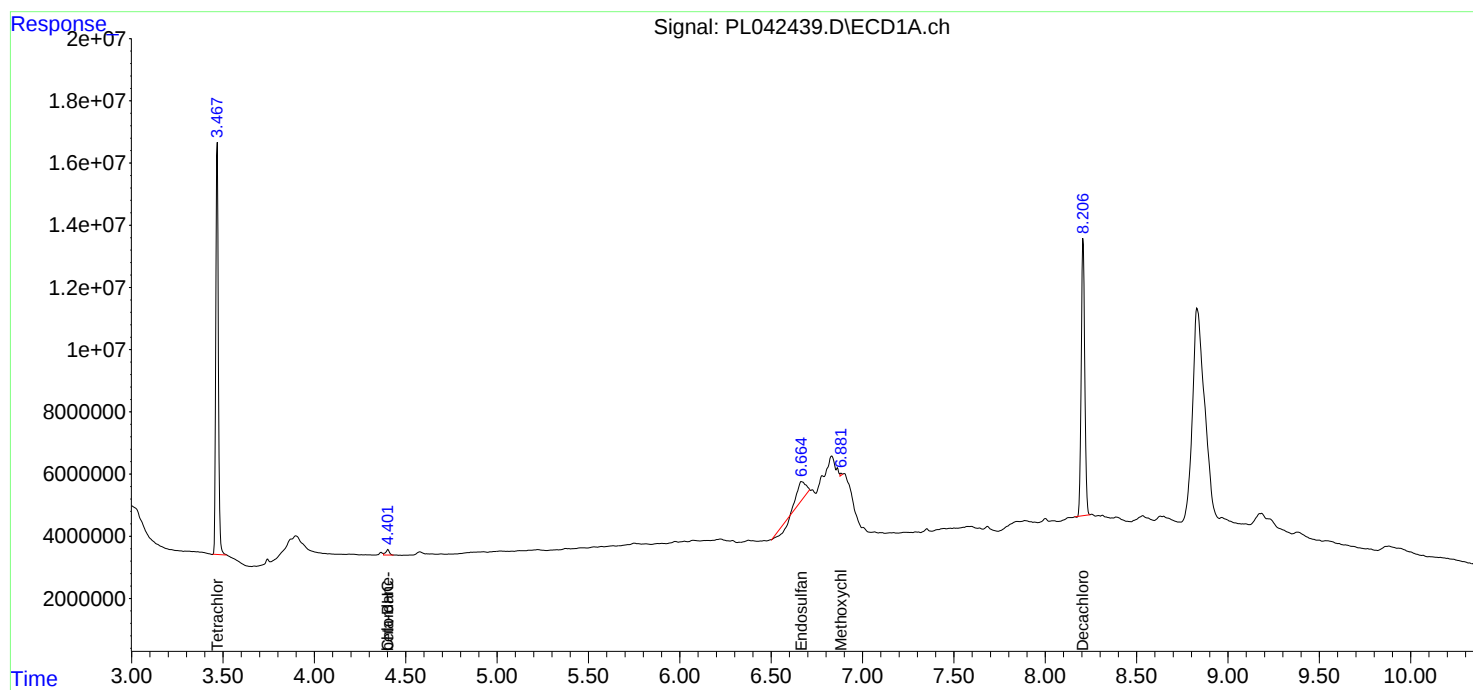


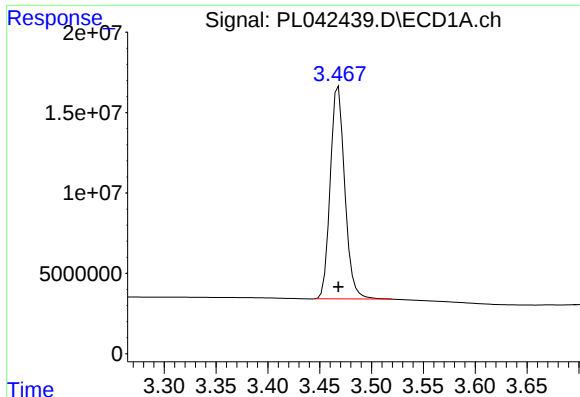

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 129013361
Conc: 21.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

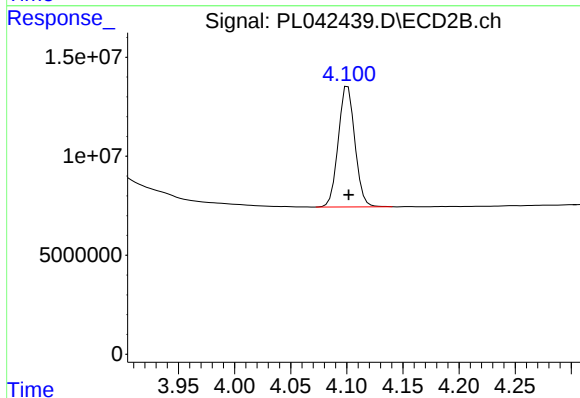


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 62934423
Conc: 21.88 ng/ml

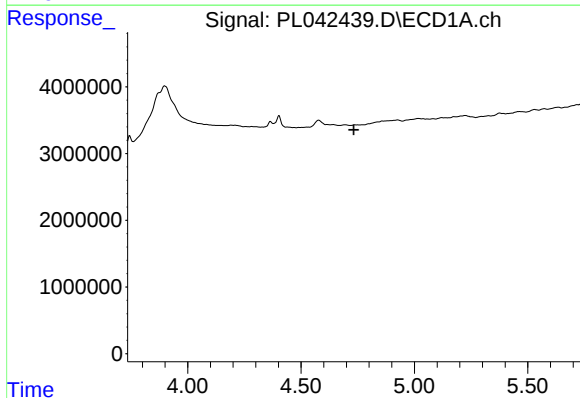


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.733 min
Response: 0
Conc: N.D.

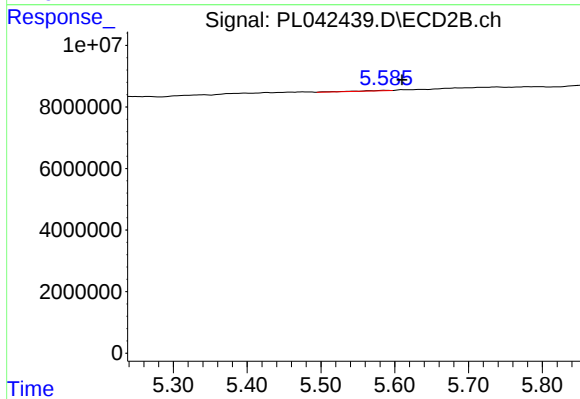

#5 Aldrin


R.T.: 5.586 min
Delta R.T.: -0.024 min
Response: 363218
Conc: 0.09 ng/ml

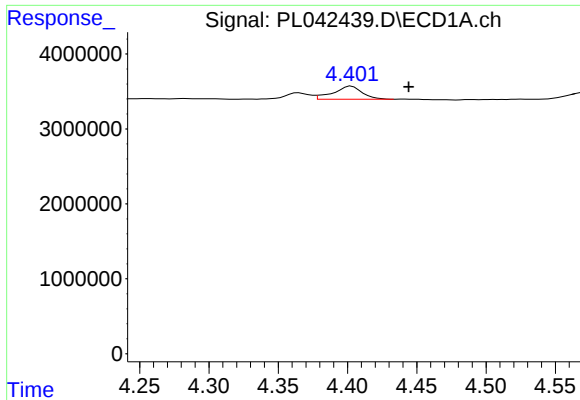

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: -0.041 min
Response: 2512741
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

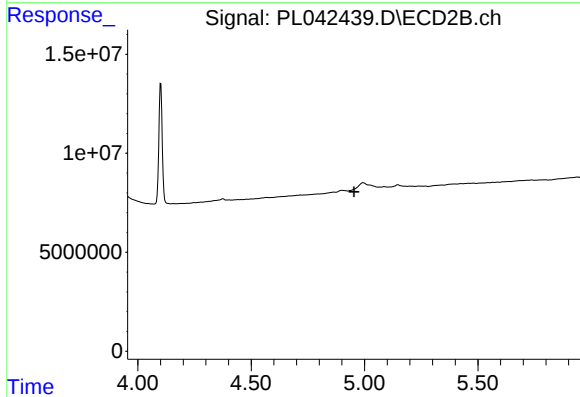


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

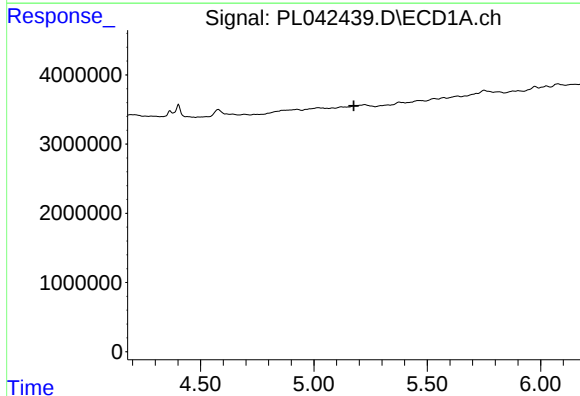


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

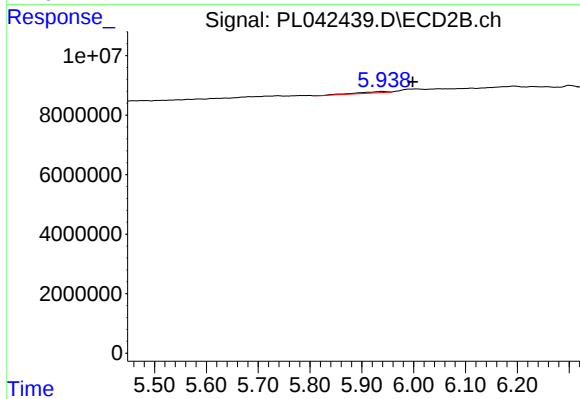

#8 Heptachlor epoxide


R.T.: 5.940 min
Delta R.T.: -0.059 min
Response: 1682181
Conc: 0.47 ng/ml

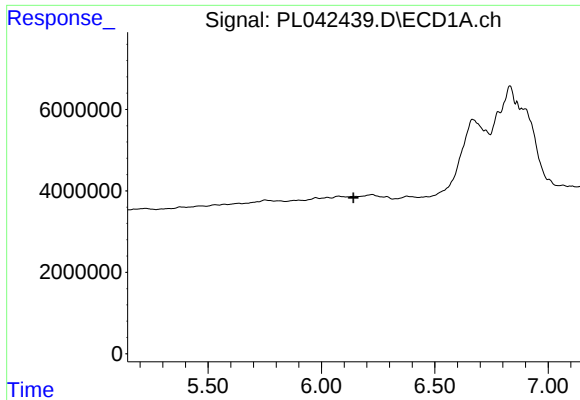

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

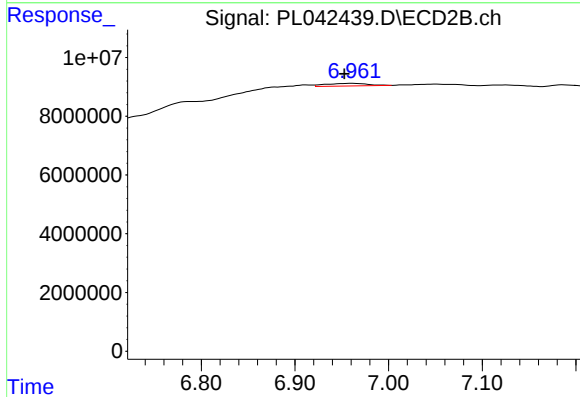


#16 4,4'-DDD

R.T.: 6.961 min
Delta R.T.: 0.009 min
Response: 2719845
Conc: 1.03 ng/ml

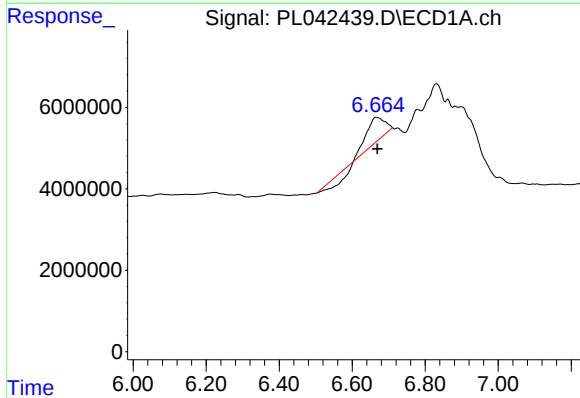


#19 Endosulfan Sulfate

R.T.: 6.665 min
Delta R.T.: -0.003 min
Response: 14021865
Conc: 2.25 ng/ml

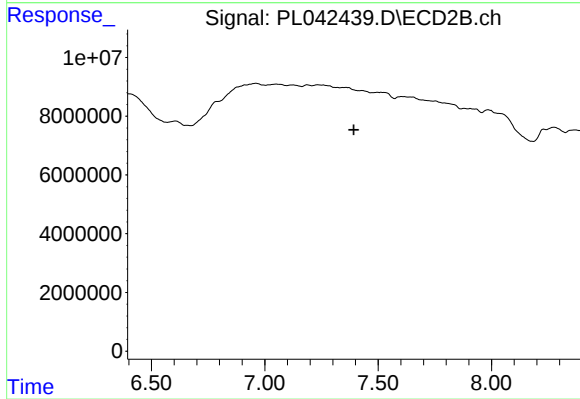

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.392 min
Response: 0
Conc: N.D.

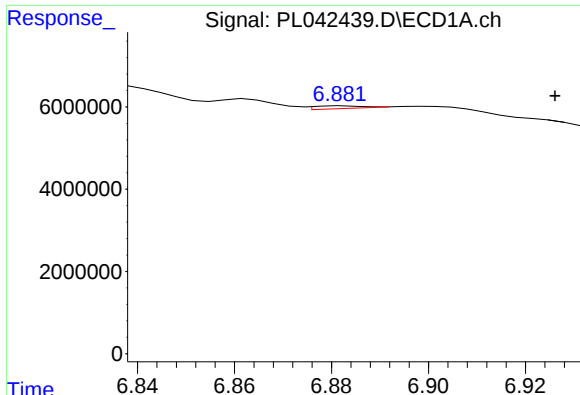

#20 Methoxychlor


R.T.: 6.883 min
Delta R.T.: -0.043 min
Response: 857911
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

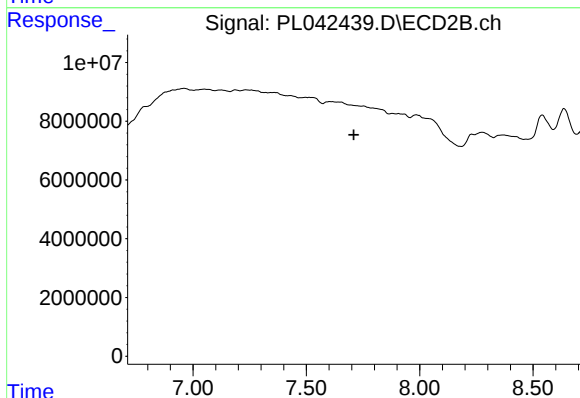


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

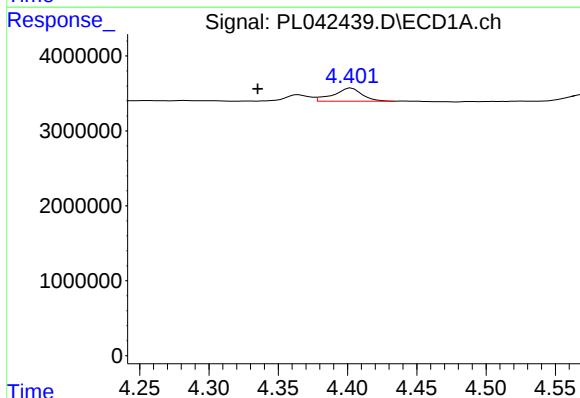


#23 Chlordane-1

R.T.: 4.403 min
Delta R.T.: 0.068 min
Response: 2512741
Conc: 9.09 ng/ml

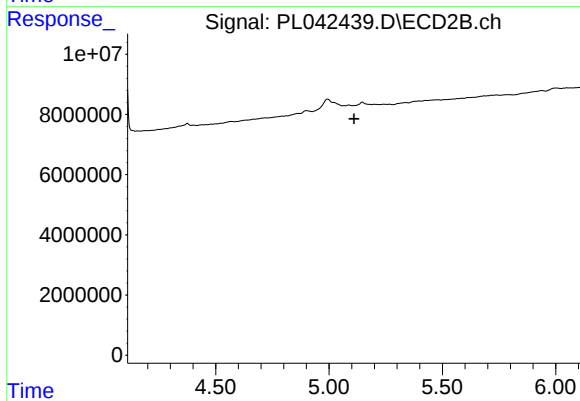

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

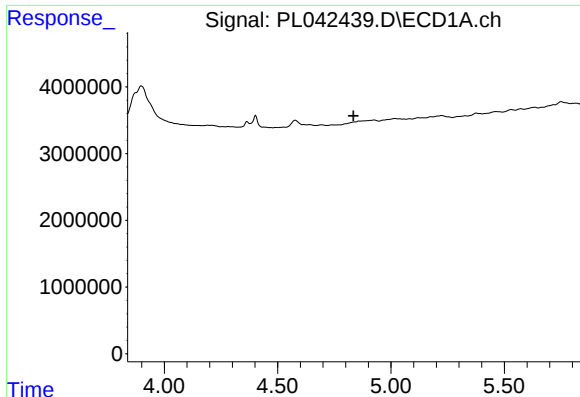

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.835 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

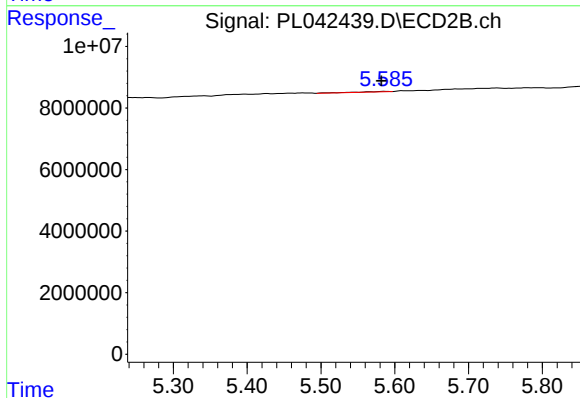


#24 Chlordane-2

R.T.: 5.586 min
Delta R.T.: 0.005 min
Response: 363218
Conc: 2.60 ng/ml

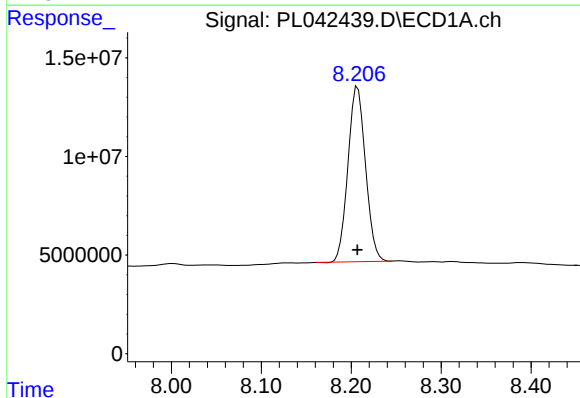

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 120391001
Conc: 19.10 ng/ml

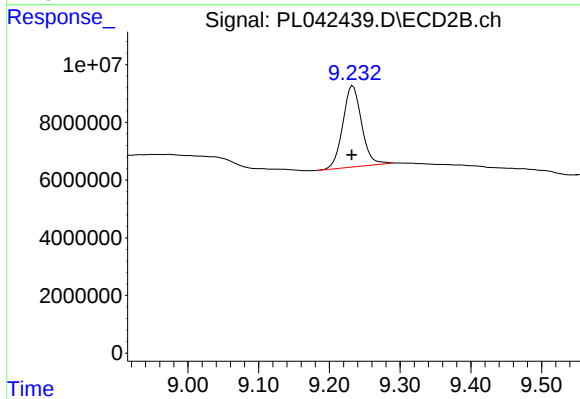

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 52289450
Conc: 21.68 ng/ml