

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
 Data File : PL042450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2018 13:42
 Operator : AJ\SJ
 Sample : PB115045BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:31:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.101	95606459	47523736	16.250	16.523
28)	SA Decachlor...	8.218	9.239	99153808	40138426	15.733	16.642
Target Compounds							
6)	B beta-BHC	4.412f	0.000	2711301	0	0.765	N.D. #
8)	B Heptachlo...	0.000	5.994	0	3297185	N.D.	0.920 #
9)	A Endosulfan I	0.000	6.313f	0	5128233	N.D.	1.624 #
10)	B gamma-Chl...	5.375	6.173f	1160852	3893083	0.152	1.144 #
11)	B alpha-Chl...	0.000	6.313	0	5128233	N.D.	1.534 #
14)	MA Endrin	6.044	6.870	622360	1029445	0.095	0.374 #
25)	Chlordane-3	5.375	6.173	1160852	3893083	1.324	8.284 #
26)	Chlordane-4	0.000	6.313	0	5128233	N.D.	9.373 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
Data File : PL042450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2018 13:42
Operator : AJ\SJ
Sample : PB115045BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:31:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

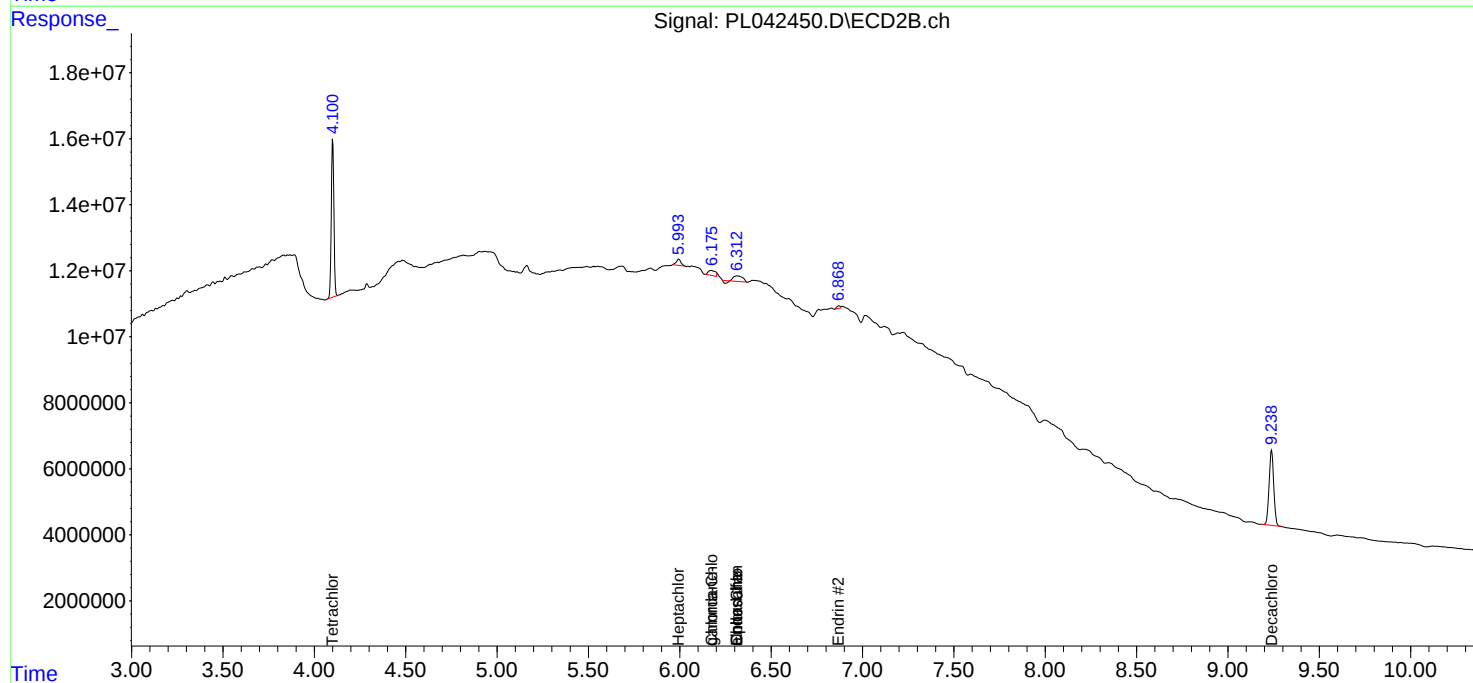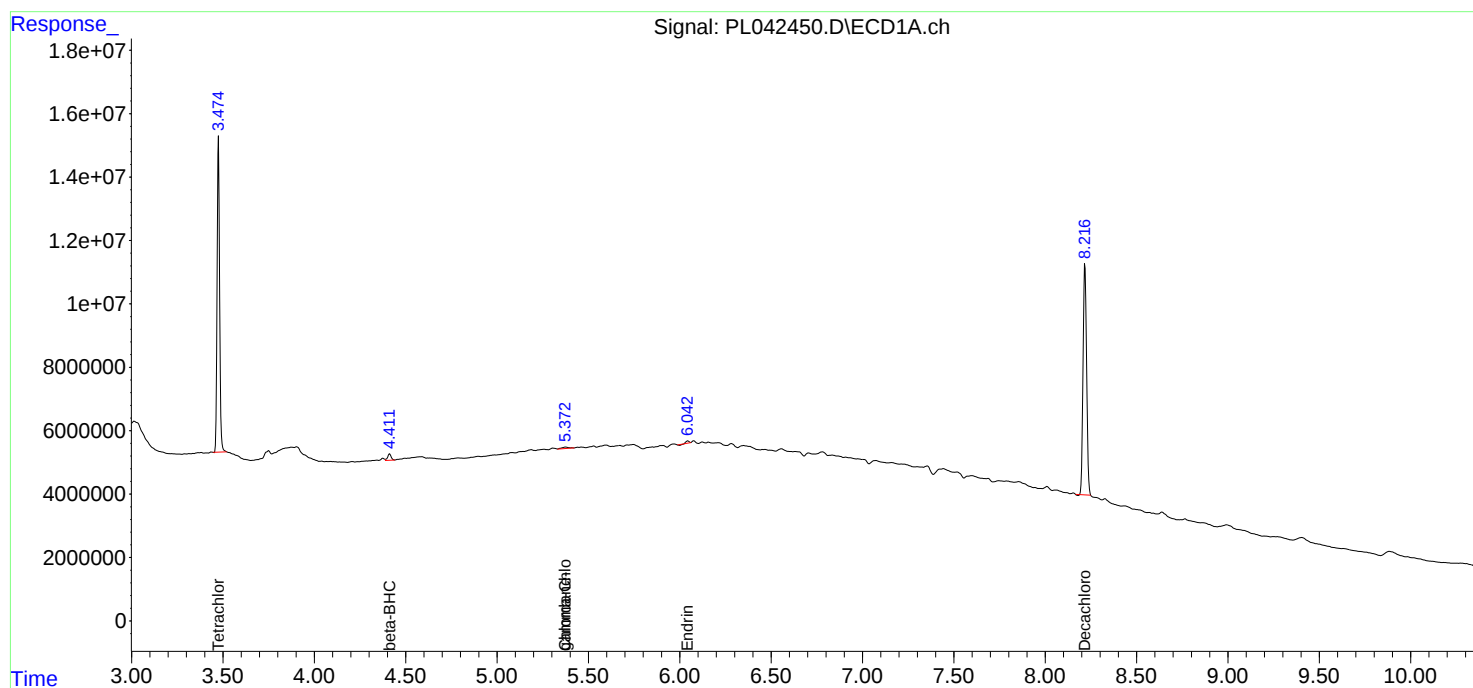


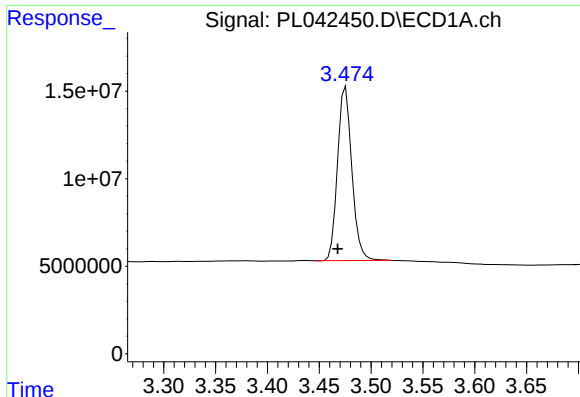

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.008 min
Response: 95606459
Conc: 16.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

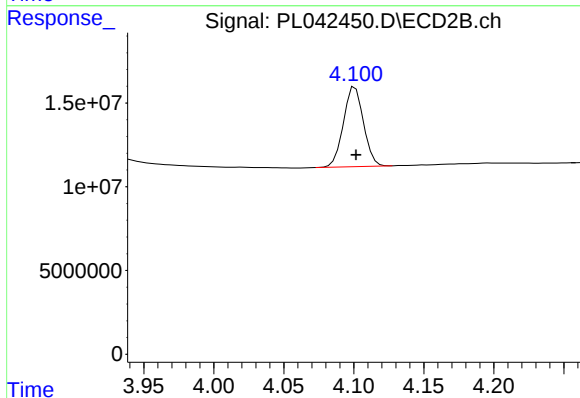


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 47523736
Conc: 16.52 ng/ml

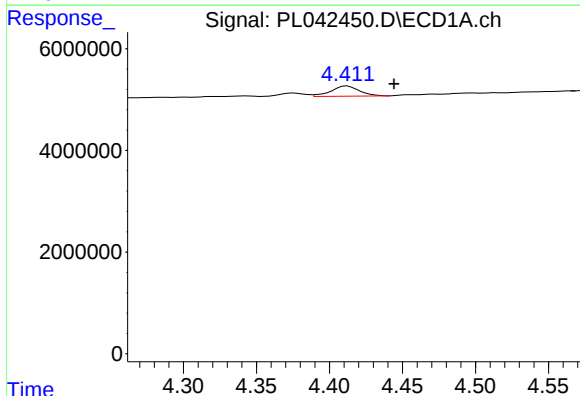


#6 beta-BHC

R.T.: 4.412 min
Delta R.T.: -0.032 min
Response: 2711301
Conc: 0.77 ng/ml

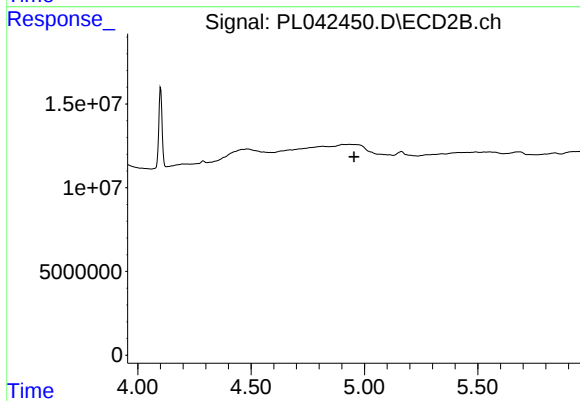

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

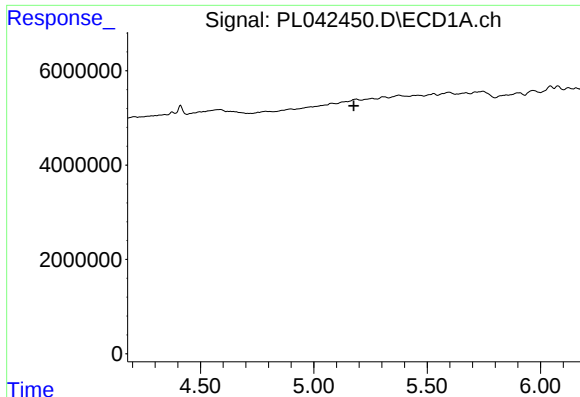

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

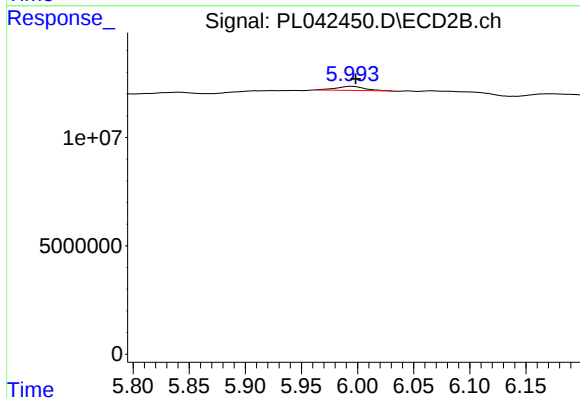


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.004 min
Response: 3297185
Conc: 0.92 ng/ml

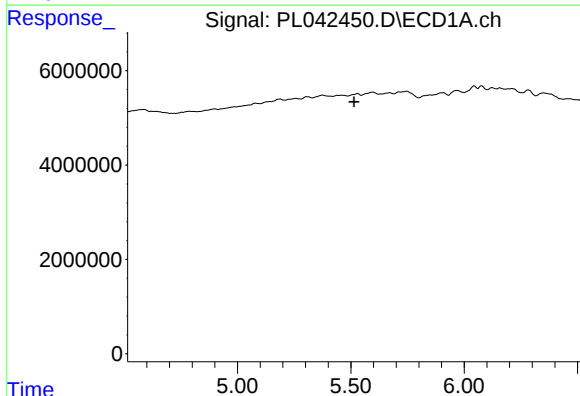


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

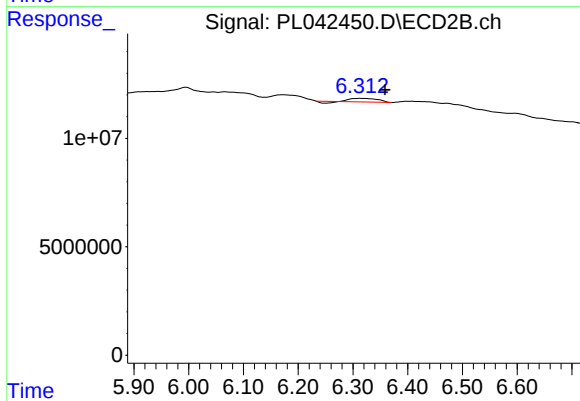

#9 Endosulfan I


R.T.: 6.313 min
Delta R.T.: -0.046 min
Response: 5128233
Conc: 1.62 ng/ml

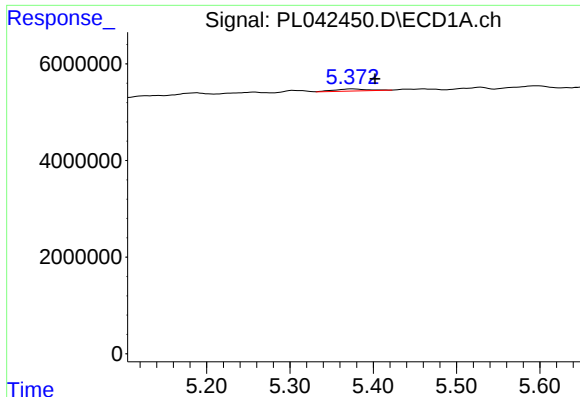

#10 gamma-Chlordane


R.T.: 5.375 min
Delta R.T.: -0.027 min
Response: 1160852
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

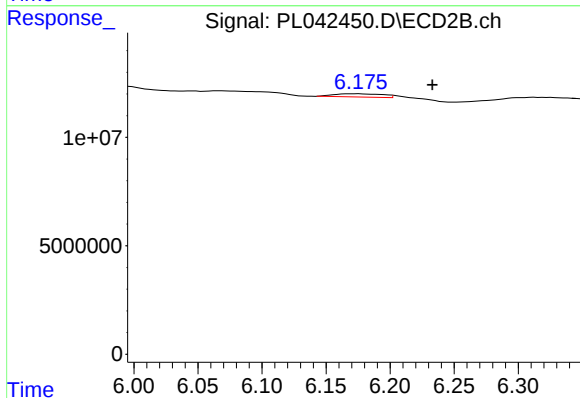


#10 gamma-Chlordane

R.T.: 6.173 min
Delta R.T.: -0.060 min
Response: 3893083
Conc: 1.14 ng/ml

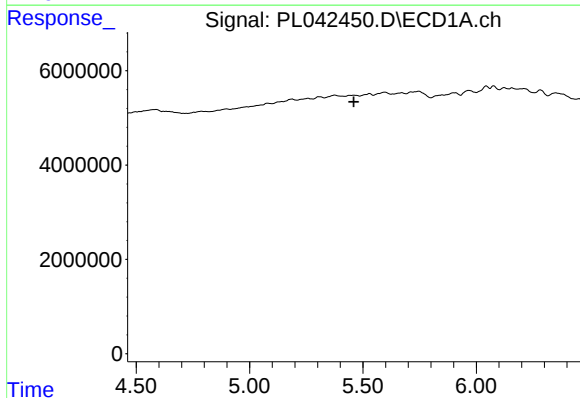


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

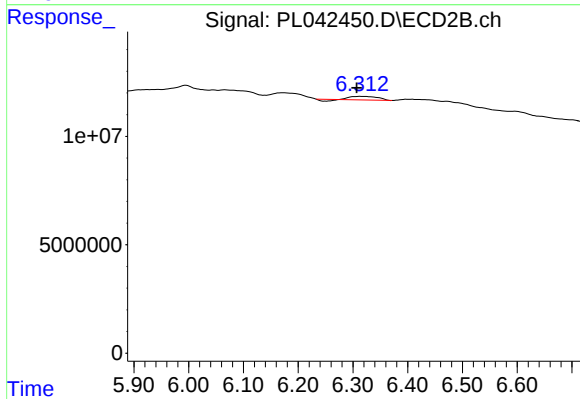

#11 alpha-Chlordane


R.T.: 6.313 min
Delta R.T.: 0.006 min
Response: 5128233
Conc: 1.53 ng/ml

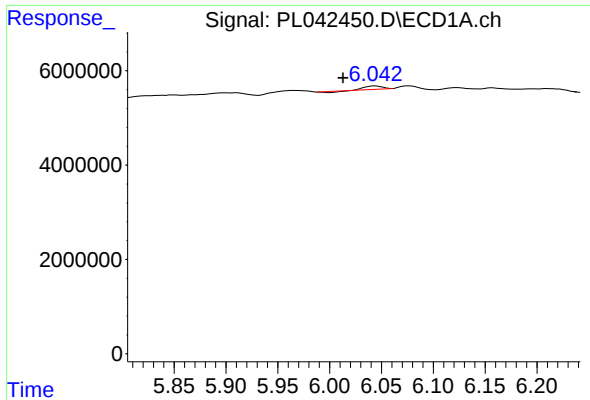

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.031 min
Response: 622360
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

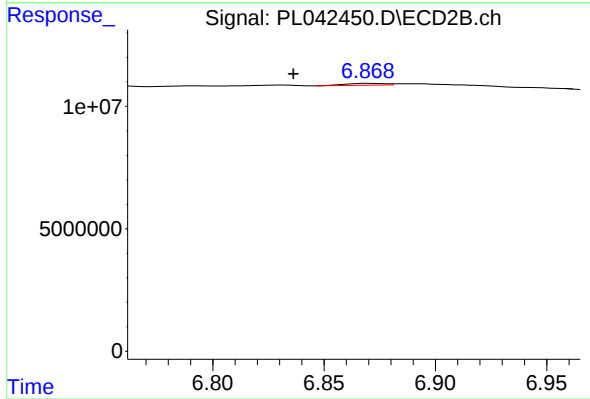


#14 Endrin

R.T.: 6.870 min
Delta R.T.: 0.034 min
Response: 1029445
Conc: 0.37 ng/ml

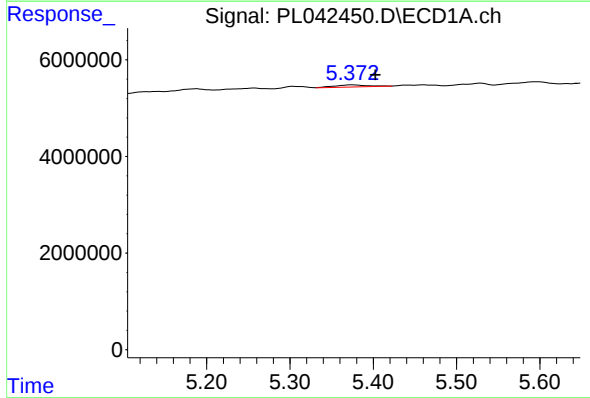


#25 Chlordane-3

R.T.: 5.375 min
Delta R.T.: -0.027 min
Response: 1160852
Conc: 1.32 ng/ml

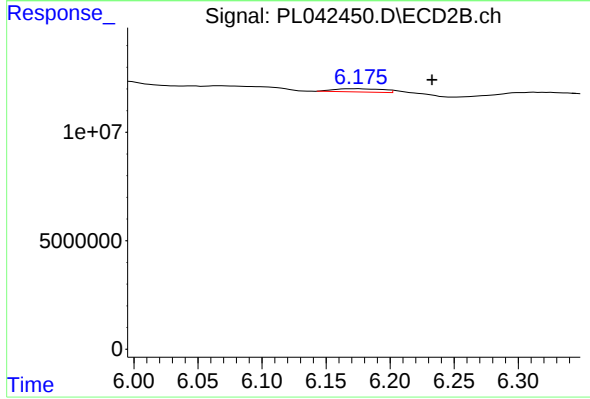

#25 Chlordane-3


R.T.: 6.173 min
Delta R.T.: -0.060 min
Response: 3893083
Conc: 8.28 ng/ml

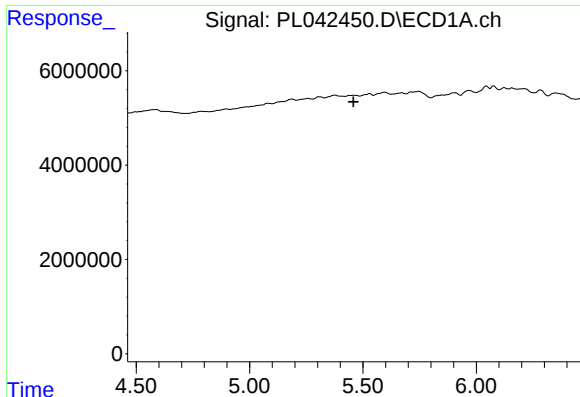

#26 Chlorodane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

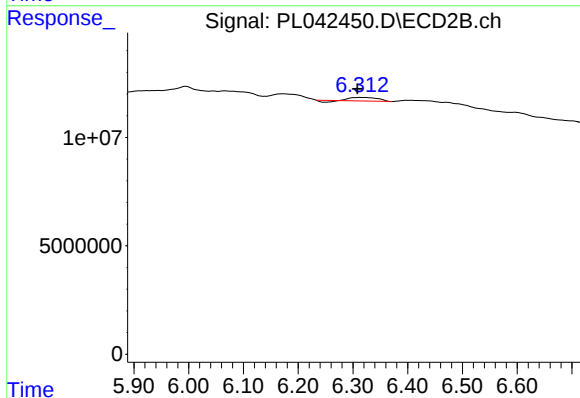


#26 Chlorodane-4

R.T.: 6.313 min
Delta R.T.: 0.005 min
Response: 5128233
Conc: 9.37 ng/ml

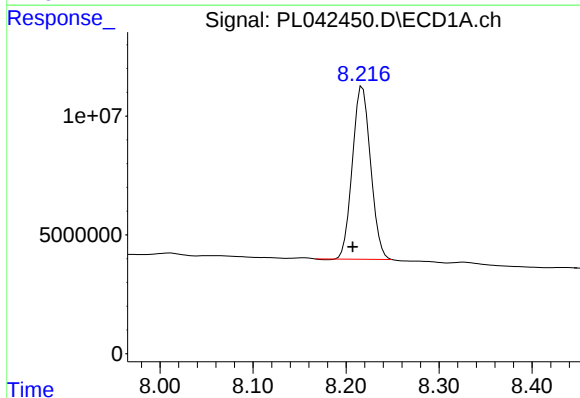

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: 0.011 min
Response: 99153808
Conc: 15.73 ng/ml

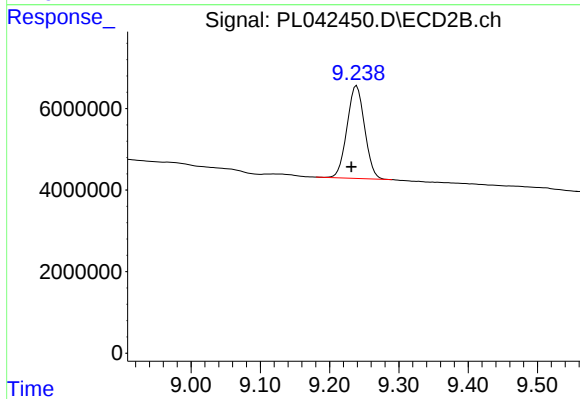

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.008 min
Response: 40138426
Conc: 16.64 ng/ml