

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
 Data File : PL042467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2018 18:41
 Operator : AJ\SJ
 Sample : J6028-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

mohammad
 11/28/2018 2:40:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:37:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.103	107.6E6	55006534	18.284	19.125
28)	SA Decachlor...	8.210	9.239	82286765	33776042	13.057	14.004
Target Compounds							
10)	B gamma-Chl...	5.403	6.234	24237666	19657105	3.179	5.774m#
11)	B alpha-Chl...	5.459	6.310	29346531	15170007	3.909m	4.537

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
Data File : PL042467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2018 18:41
Operator : AJ\SJ
Sample : J6028-08
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-3


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:37:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

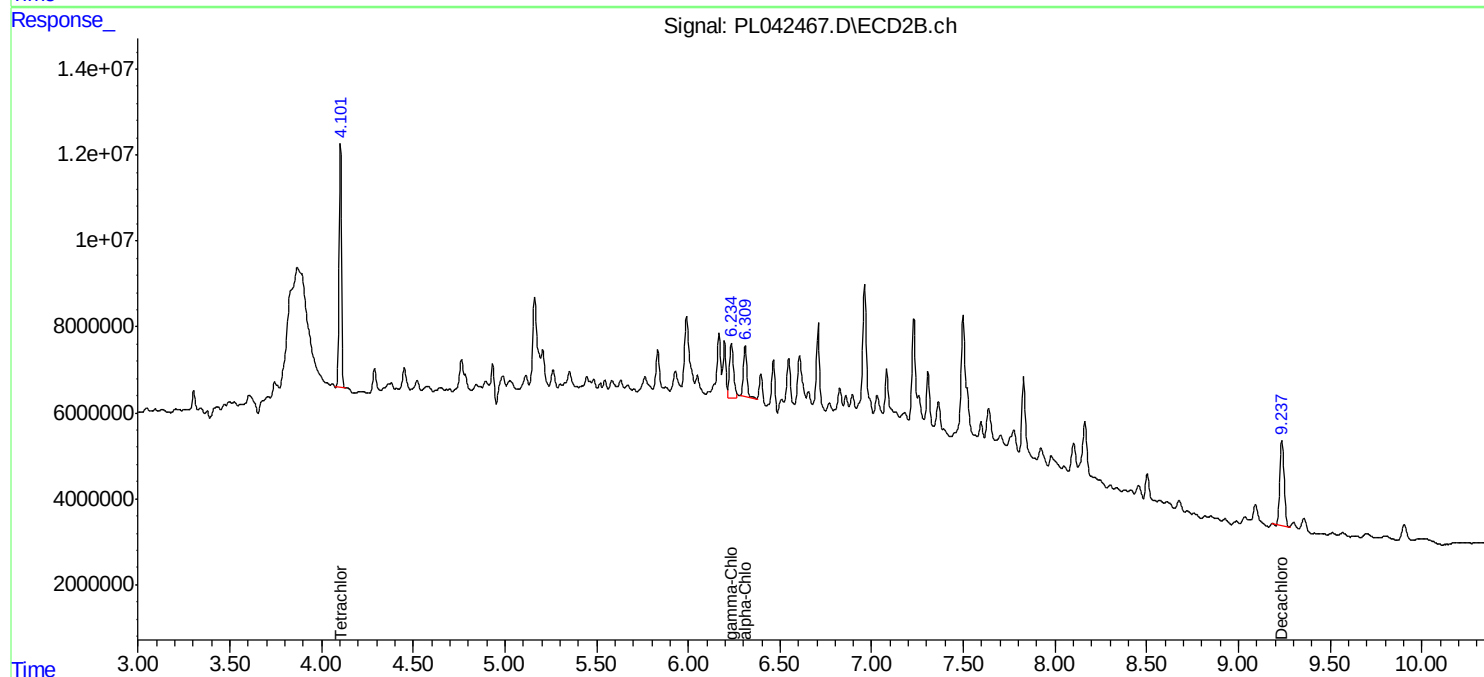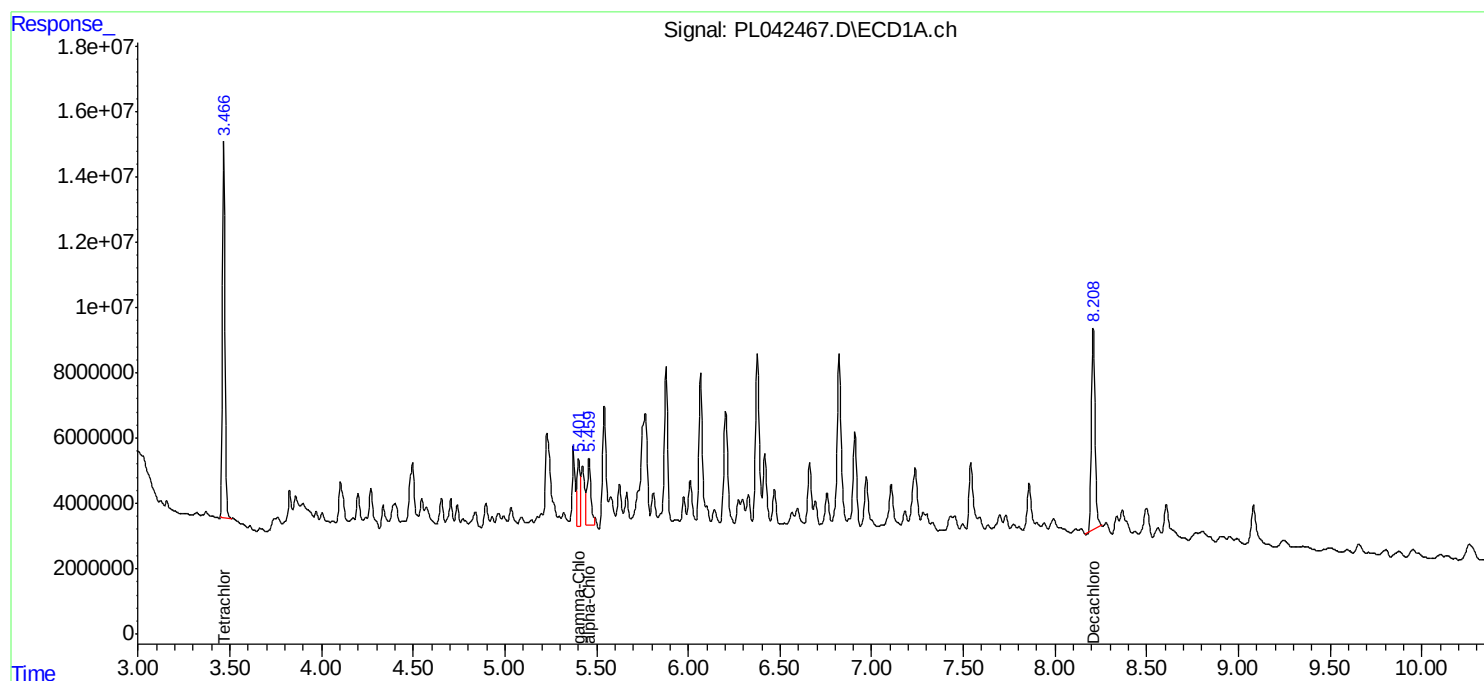

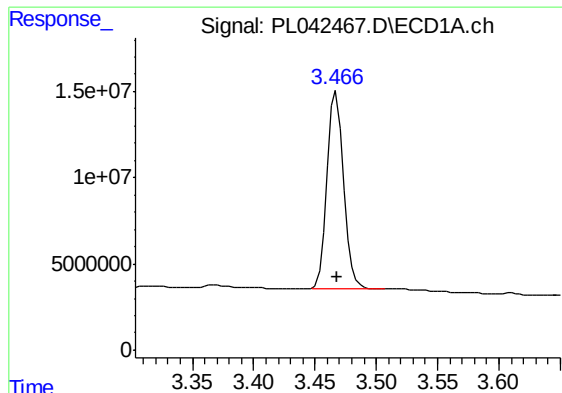


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 107574951
Conc: 18.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:00 PM

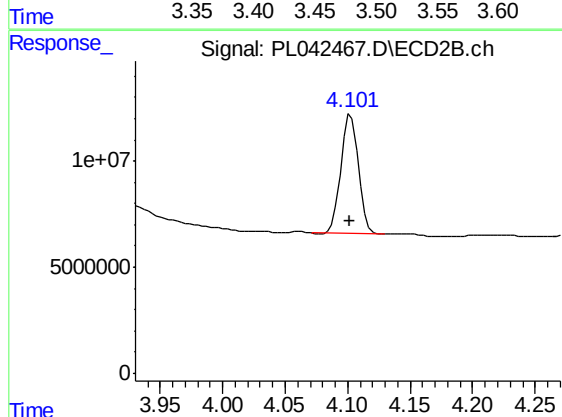


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 55006534
Conc: 19.13 ng/ml

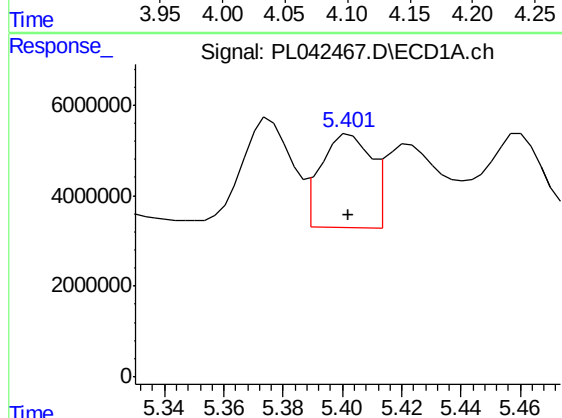


#10 gamma-Chlordane

R.T.: 5.403 min
Delta R.T.: 0.000 min
Response: 24237666
Conc: 3.18 ng/ml

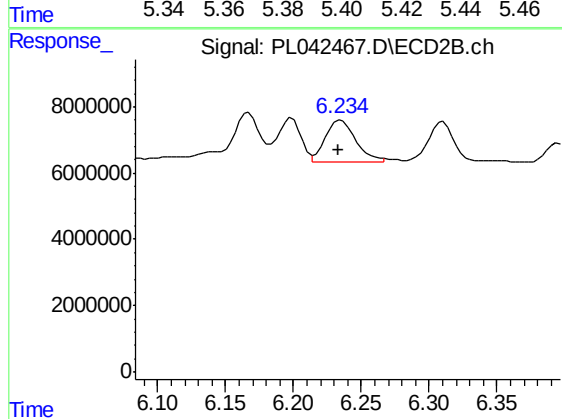

#10 gamma-Chlordane

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 19657105
Conc: 5.77 ng/ml m

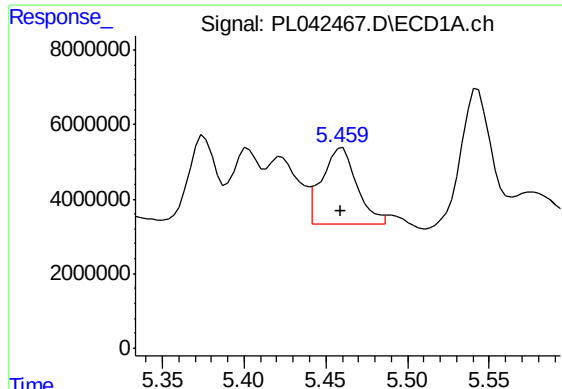


#11 alpha-Chlordane

R.T.: 5.459 min
Delta R.T.: 0.000 min
Response: 29346531
Conc: 3.91 ng/ml m

Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:00 PM

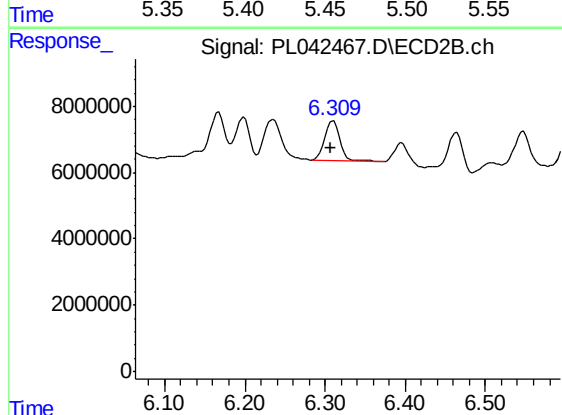


#11 alpha-Chlordane

R.T.: 6.310 min
Delta R.T.: 0.004 min
Response: 15170007
Conc: 4.54 ng/ml

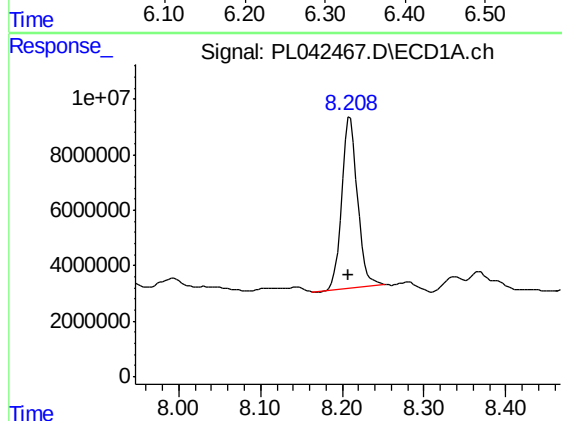

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.003 min
Response: 82286765
Conc: 13.06 ng/ml

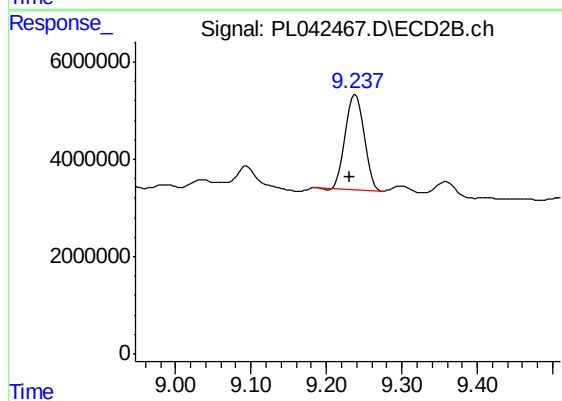

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 33776042
Conc: 14.00 ng/ml