

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
 Data File : PL042475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2018 20:34
 Operator : AJ\SJ
 Sample : J6030-03MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DTW-03MS

Manual Integrations
 APPROVED

mohammad
 11/28/2018 2:40:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:39:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.471	4.100	347.4E6	124.9E6	59.053m	43.412m#
28)	SA Decachlor...	8.211	9.238	54078750	18228933	8.581	7.558

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
Data File : PL042475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2018 20:34
Operator : AJ\SJ
Sample : J6030-03MS
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DTW-03MS


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:39:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

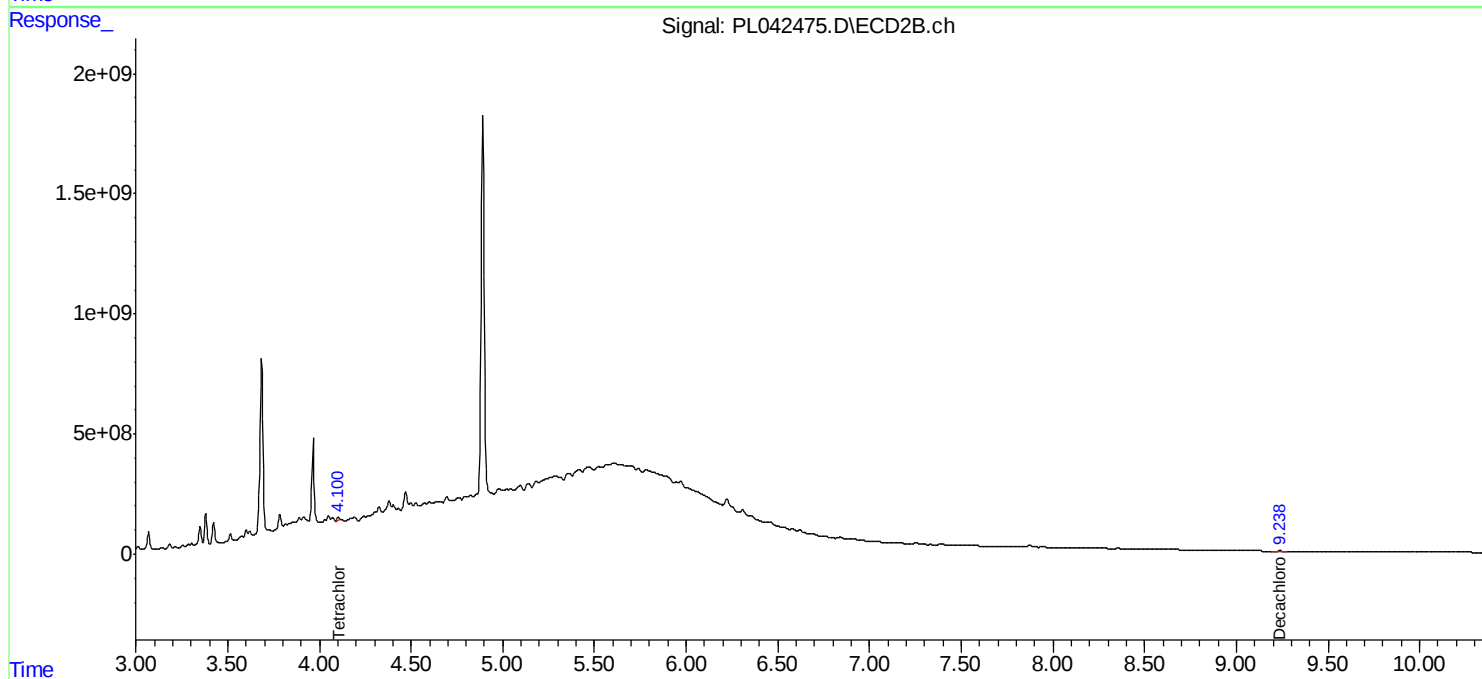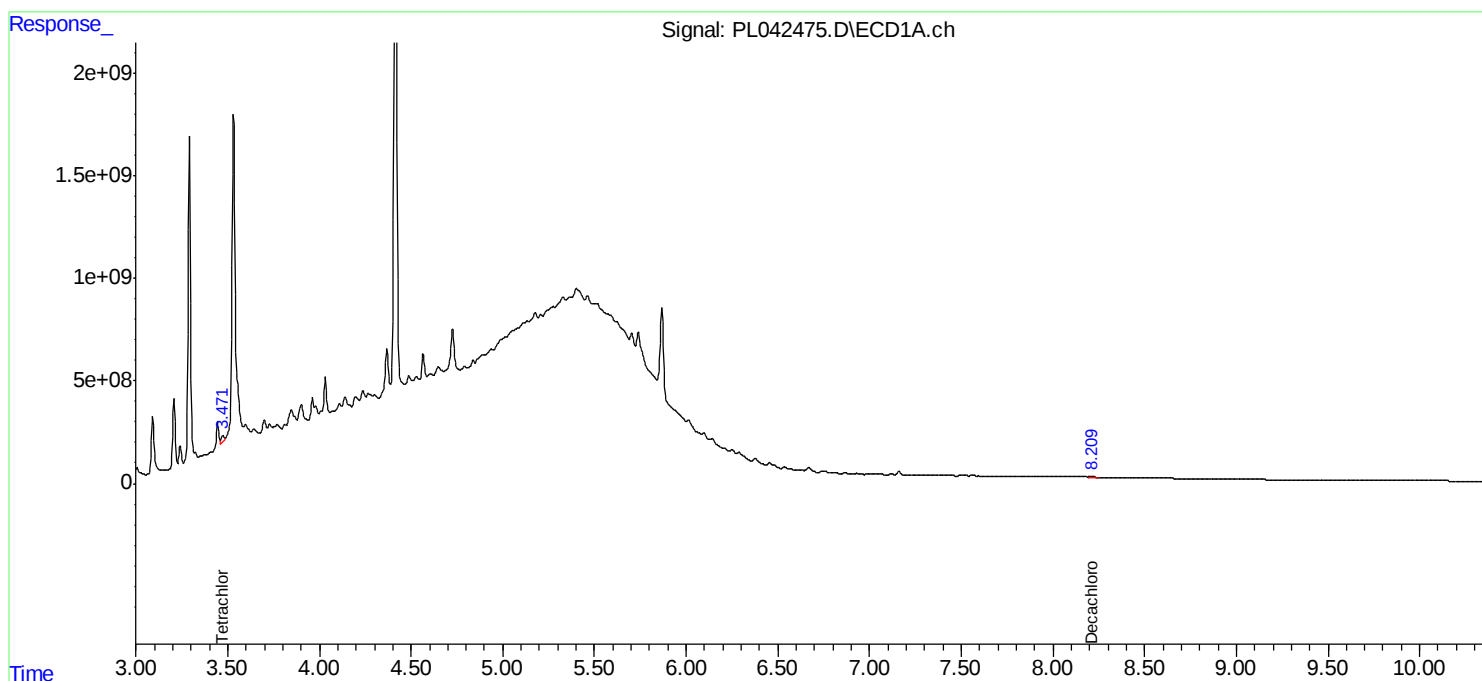

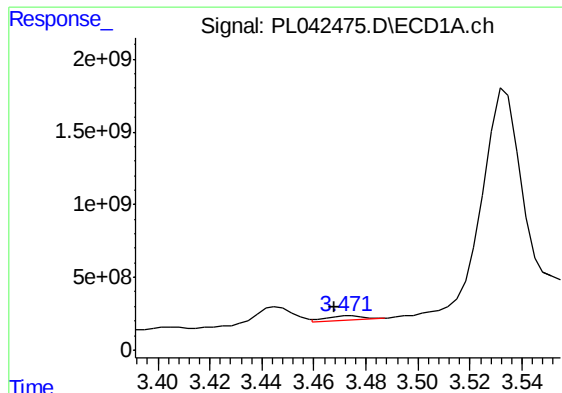


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.003 min
Response: 347437687
Conc: 59.05 ng/ml m

Instrument :
ECD_L
ClientSampleId :
DTW-03MS


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:22 PM

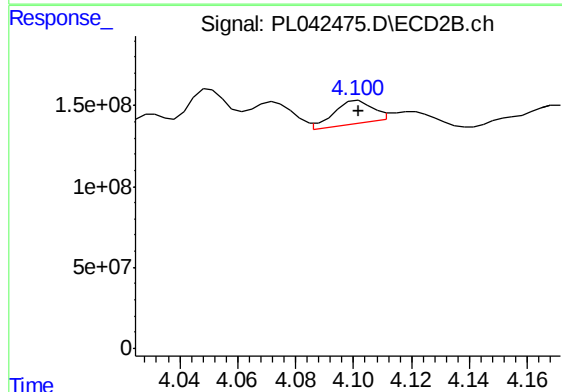


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.001 min
Response: 124857713
Conc: 43.41 ng/ml m

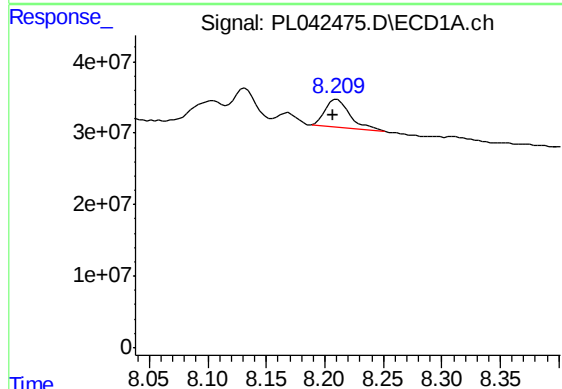

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: 0.004 min
Response: 54078750
Conc: 8.58 ng/ml

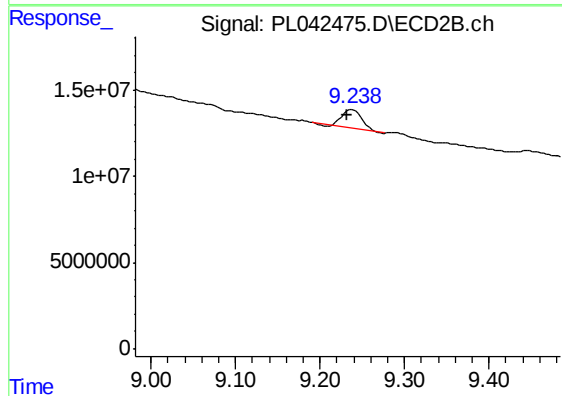

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.006 min
Response: 18228933
Conc: 7.56 ng/ml