

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
 Data File : PL042476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2018 20:48
 Operator : AJ\SJ
 Sample : J6030-04MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DTW-03MSD

Manual Integrations
 APPROVED

mohammad
 11/28/2018 2:40:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 00:39:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.472	4.100	206.3E6	44751552	35.072m	15.560m#
28)	SA Decachlor...	8.209	9.239	37328129	13894197	5.923m	5.761m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112618\
Data File : PL042476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2018 20:48
Operator : AJ\SJ
Sample : J6030-04MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
DTW-03MSD


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 00:39:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

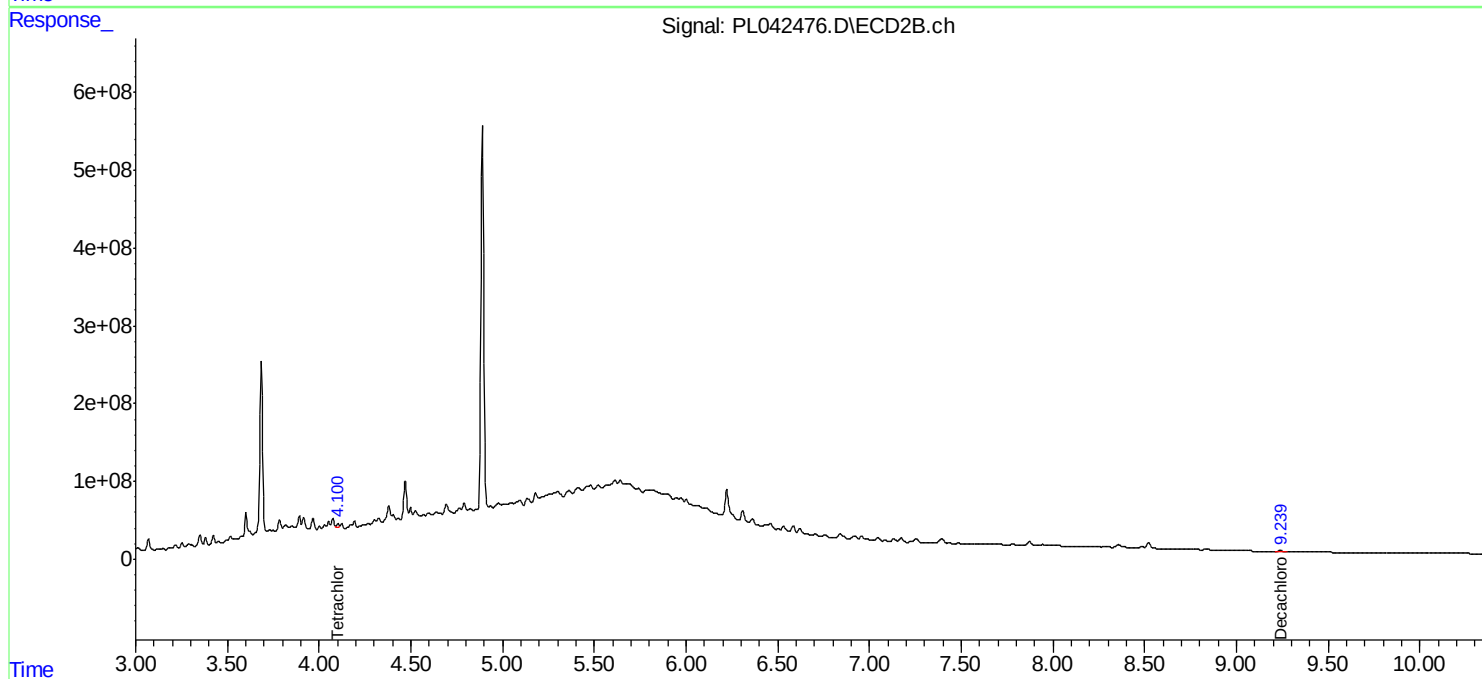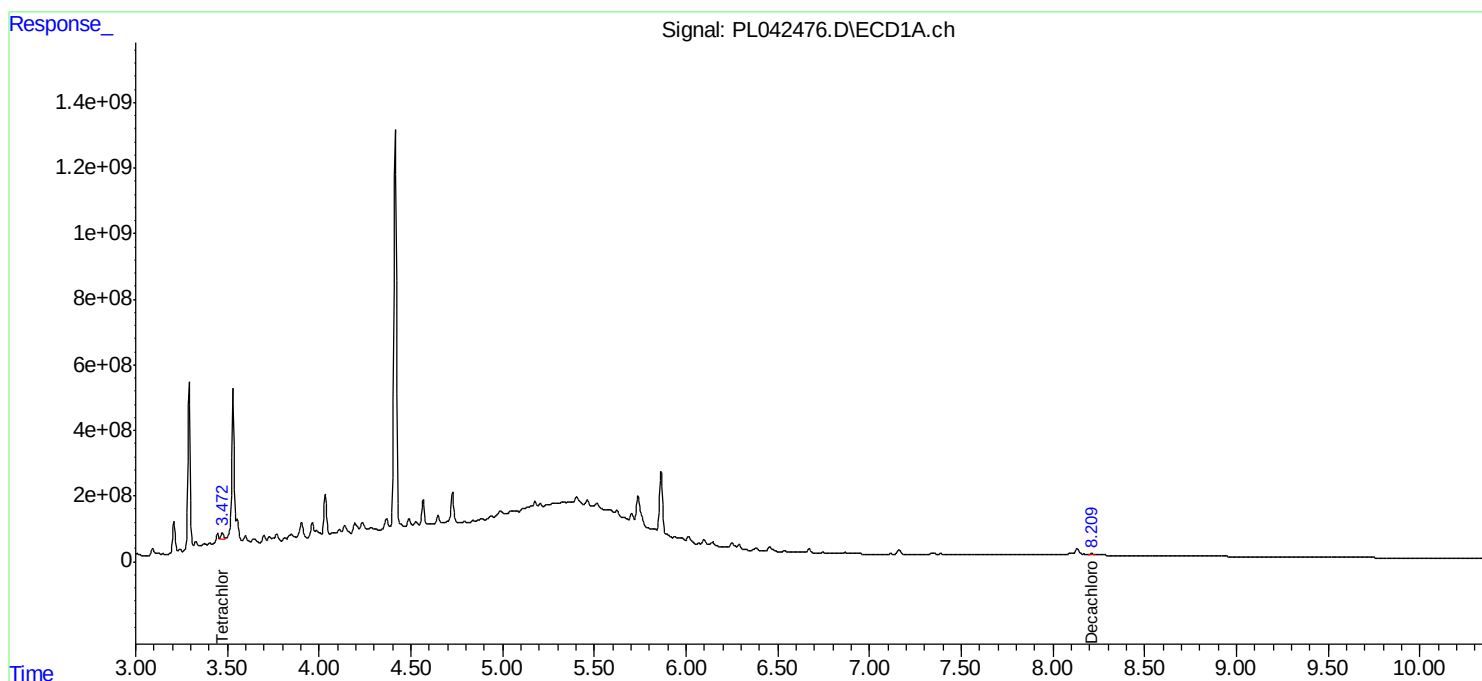

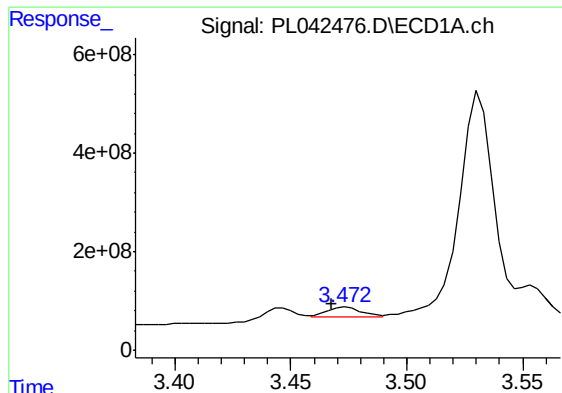


#1 Tetrachloro-m-xylene

R.T.: 3.472 min
Delta R.T.: 0.004 min
Response: 206343592
Conc: 35.07 ng/ml m

Instrument :
ECD_L
ClientSampleId :
DTW-03MSD


Manual Integrations
APPROVED

mohammad
11/28/2018 2:40:25 PM

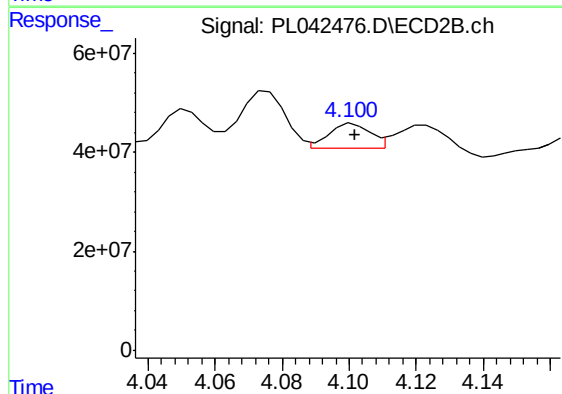


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.002 min
Response: 44751552
Conc: 15.56 ng/ml m

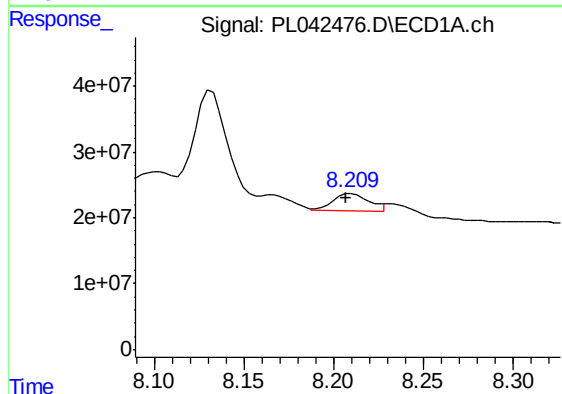

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 37328129
Conc: 5.92 ng/ml m

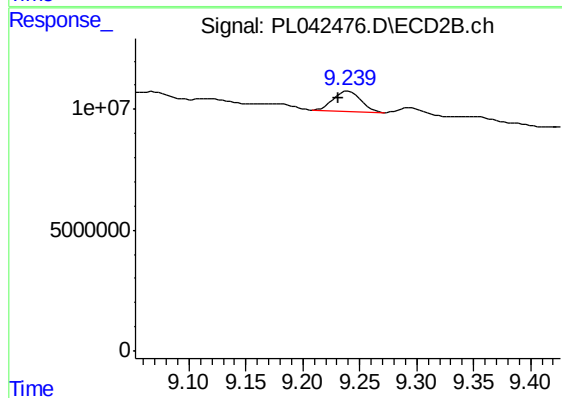

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 13894197
Conc: 5.76 ng/ml m