

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 12:35
 Operator : SG\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 01:17:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:17:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	4.051	650.2E6	115.6E6	50.000	50.000
28)	SA Decachlor...	8.319	9.151	444.9E6	110.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.420	5.049	197.3E6	39856751	500.000	500.000
24)	Chlordane-2	4.924	5.517	217.1E6	44812014	500.000	500.000
25)	Chlordane-3	5.499	6.164	642.1E6	155.2E6	500.000	500.000
26)	Chlordane-4	5.556	6.239	528.1E6	188.1E6	500.000	500.000
27)	Chlordane-5	6.397	7.045	188.3E6	33708736	500.000	500.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 12:35
Operator : SG\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 01:17:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:17:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

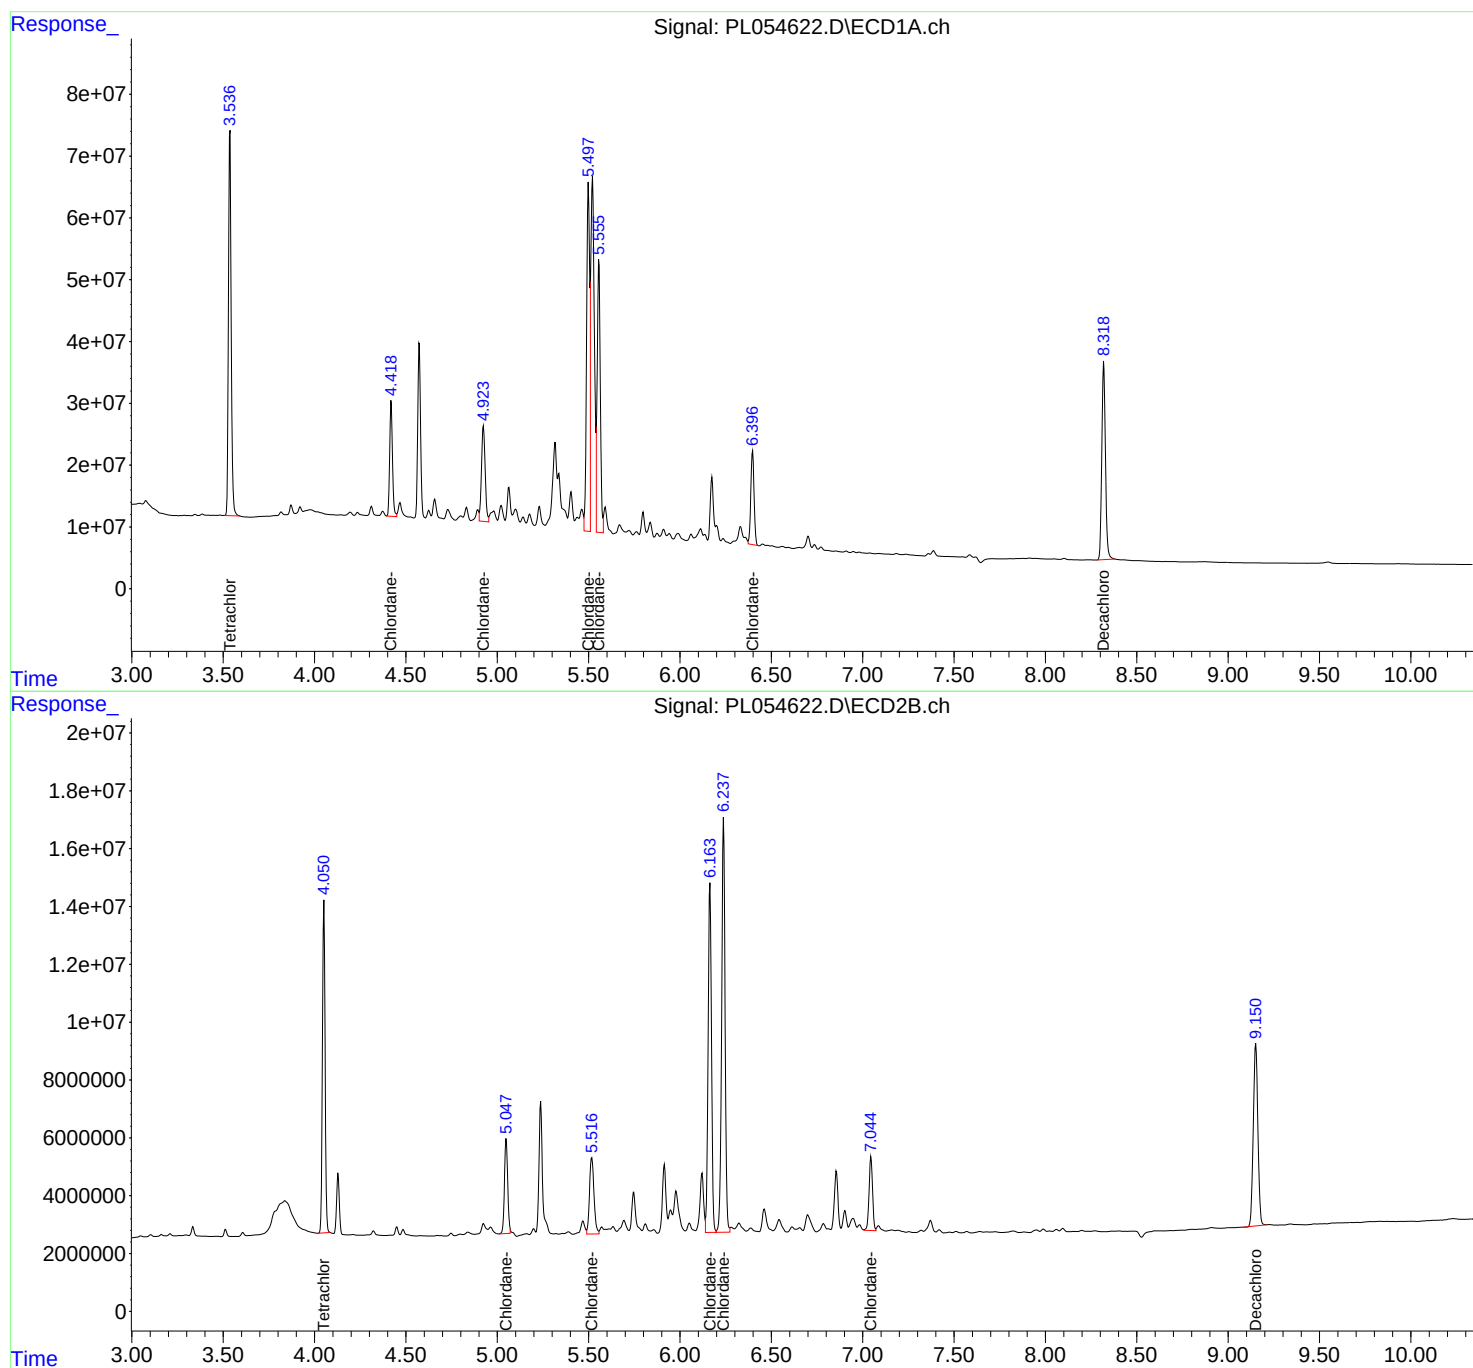


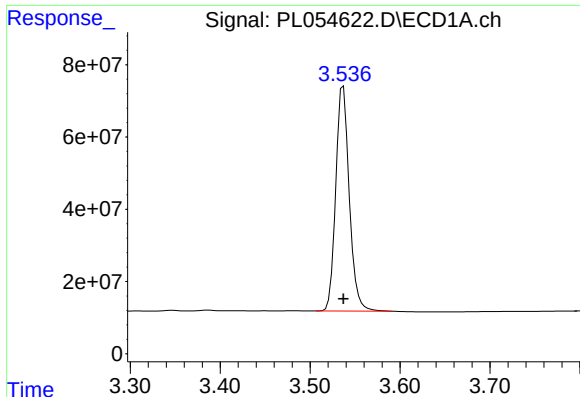

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 650230622
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

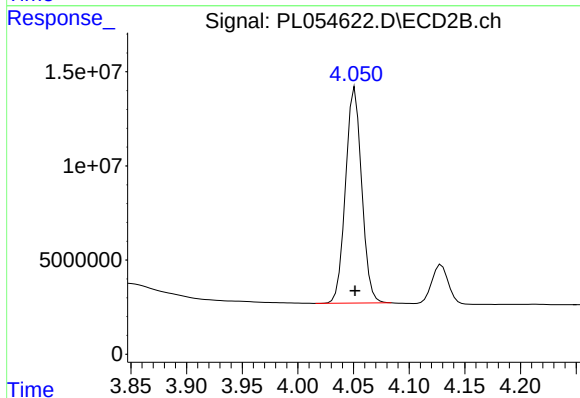


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 115628656
Conc: 50.00 ng/ml

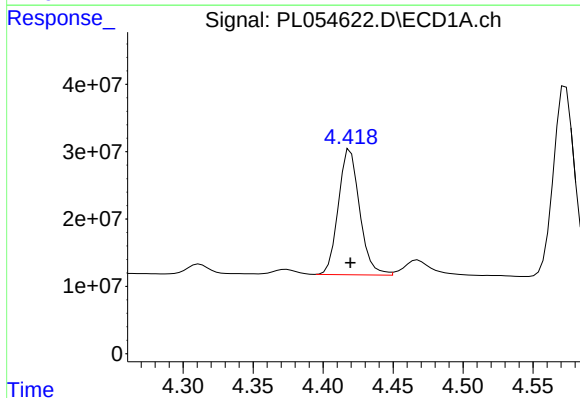


#23 Chlordane-1

R.T.: 4.420 min
Delta R.T.: 0.000 min
Response: 197317980
Conc: 500.00 ng/ml

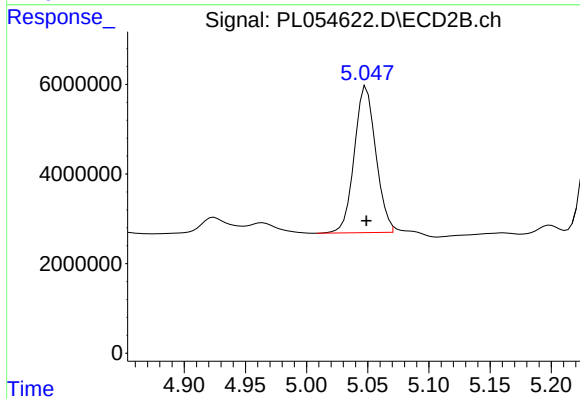

#23 Chlordane-1


R.T.: 5.049 min
Delta R.T.: 0.000 min
Response: 39856751
Conc: 500.00 ng/ml

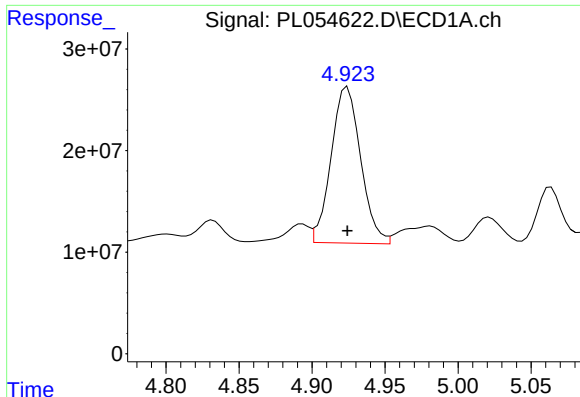

#24 Chlordane-2


R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 217128514
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

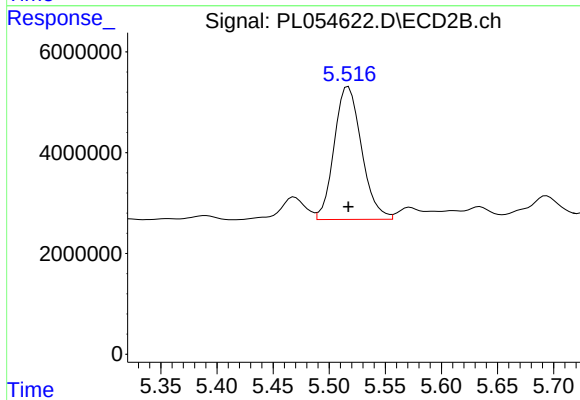


#24 Chlordane-2

R.T.: 5.517 min
Delta R.T.: 0.000 min
Response: 44812014
Conc: 500.00 ng/ml

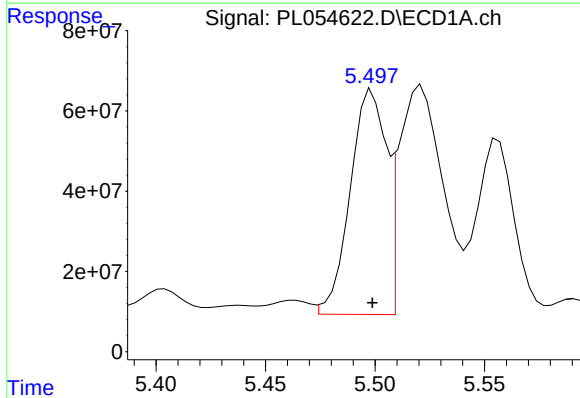


#25 Chlordane-3

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 642065246
Conc: 500.00 ng/ml

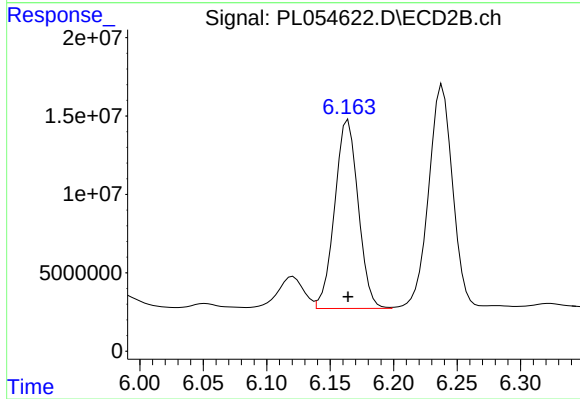

#25 Chlordane-3


R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 155200479
Conc: 500.00 ng/ml

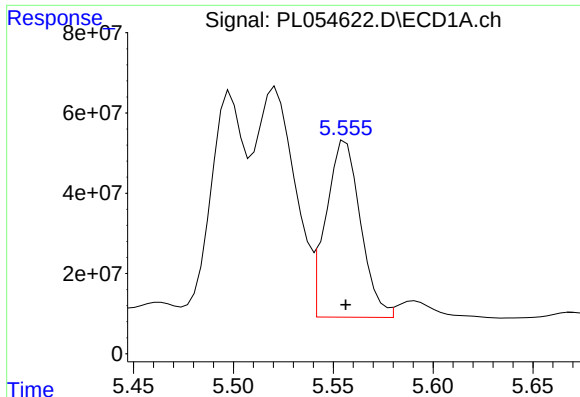

#26 Chlordane-4


R.T.: 5.556 min
Delta R.T.: 0.000 min
Response: 528144756
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

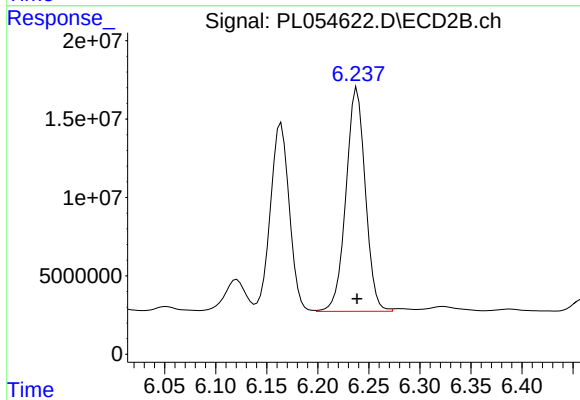


#26 Chlordane-4

R.T.: 6.239 min
Delta R.T.: 0.000 min
Response: 188144543
Conc: 500.00 ng/ml

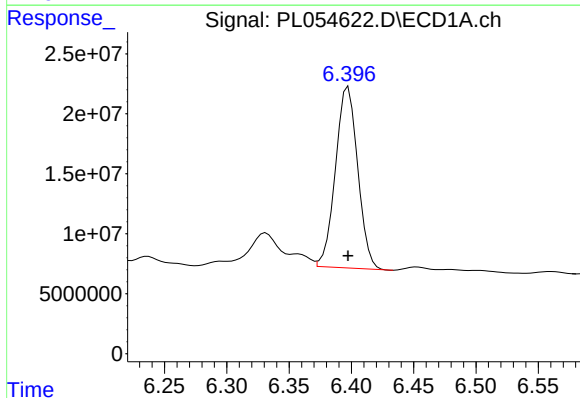


#27 Chlordane-5

R.T.: 6.397 min
Delta R.T.: 0.000 min
Response: 188250899
Conc: 500.00 ng/ml

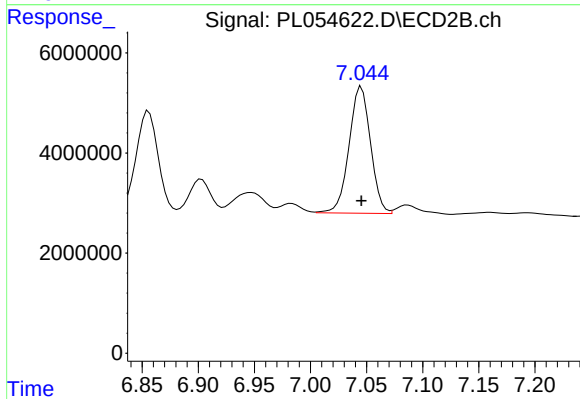

#27 Chlordane-5


R.T.: 7.045 min
Delta R.T.: 0.000 min
Response: 33708736
Conc: 500.00 ng/ml

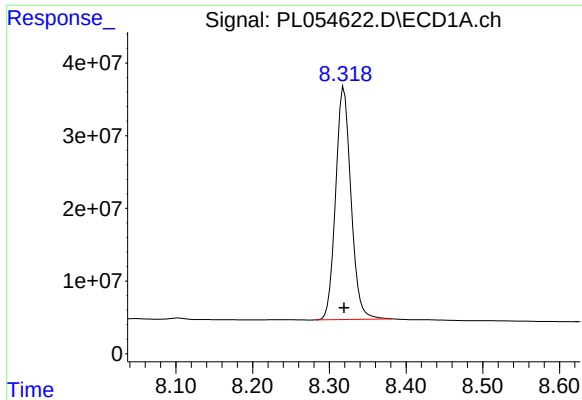

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 444927670
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

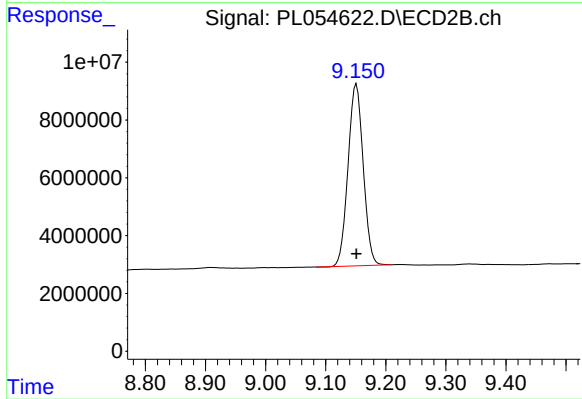

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 110024593
Conc: 50.00 ng/ml