

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 23:27
 Operator : SG\AJ
 Sample : K5672-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-112219

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 02:50:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.052	221.6E6	53339631	19.047	20.903
28)	SA Decachlor...	8.320	9.151	189.8E6	52962708	19.822	22.091
Target Compounds							
7)	B delta-BHC	4.738	5.143f	9732763	1805333	0.599	0.677
8)	B Heptachlo...	5.269	5.923	61802540	8058052	4.086	3.226
9)	A Endosulfan I	5.615	0.000	198.5E6	0	14.557	N.D. #
10)	B gamma-Chl...	0.000	6.151	0	5672038	N.D.	2.153 #
12)	B 4,4'-DDE	5.745f	0.000	7097565	0	0.533	N.D. #
14)	MA Endrin	6.115	6.758	25646740	-1354764	2.014	N.D. #
23)	Chlordane-1	4.421	0.000	7250819	0	18.373	N.D. #
25)	Chlordane-3	0.000	6.151	0	5672038	N.D.	18.273 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 23:27
Operator : SG\AJ
Sample : K5672-05
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 02:50:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

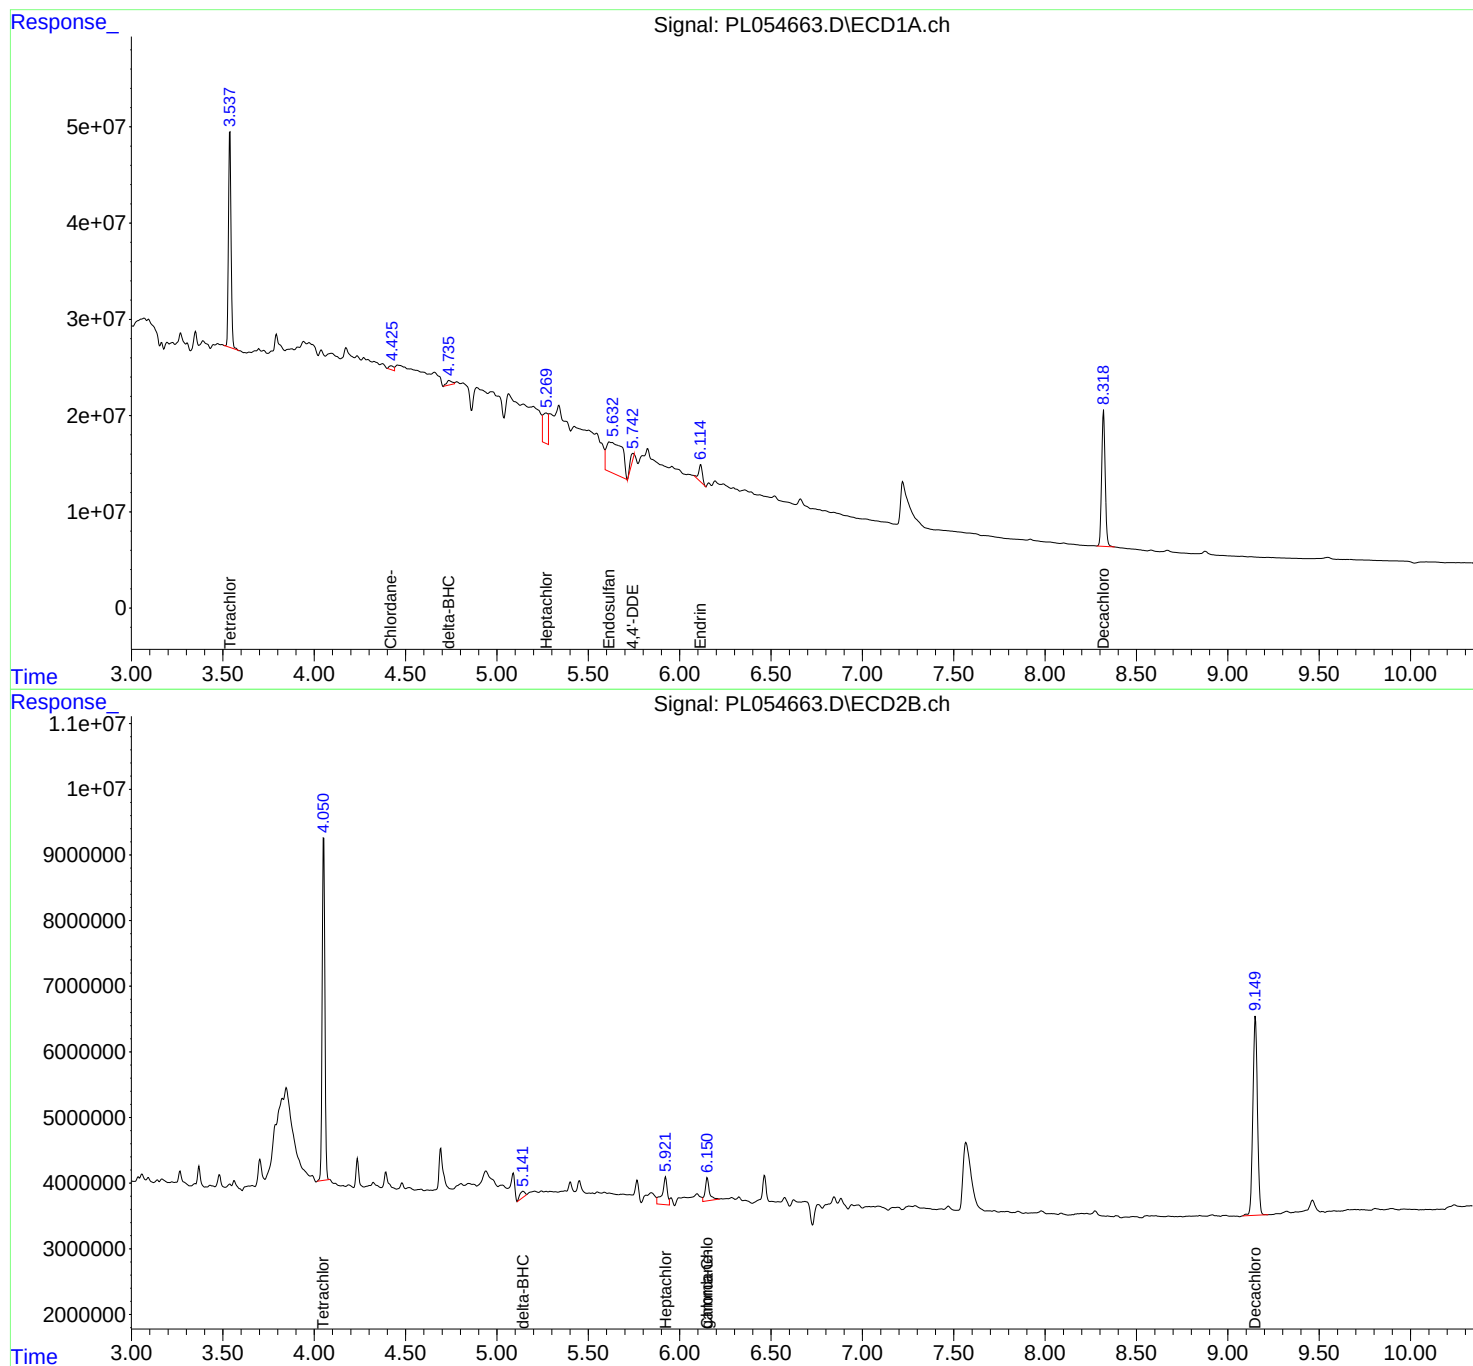


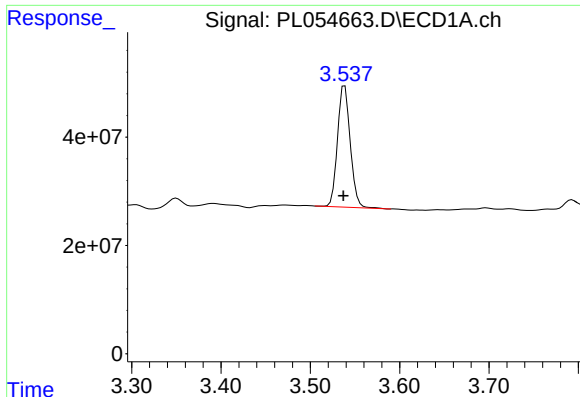

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.002 min
Response: 221591238
Conc: 19.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

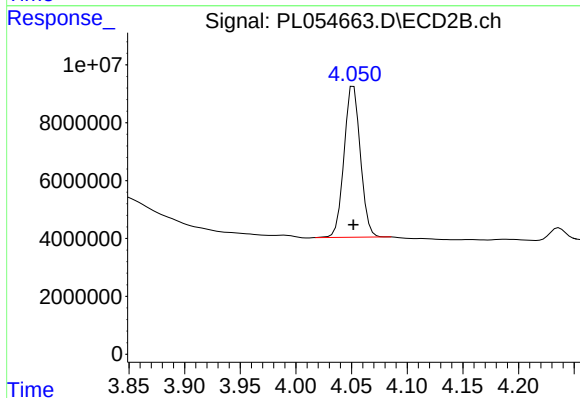


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 53339631
Conc: 20.90 ng/ml

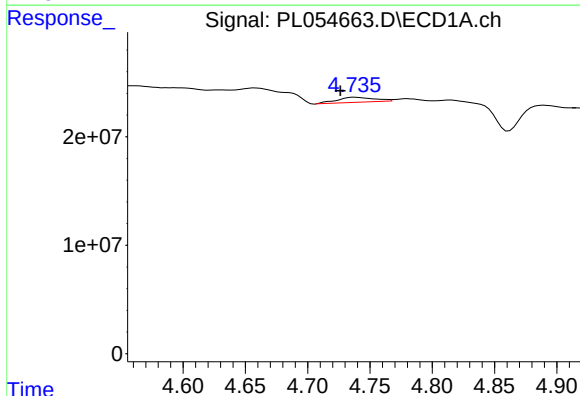


#7 delta-BHC

R.T.: 4.738 min
Delta R.T.: 0.011 min
Response: 9732763
Conc: 0.60 ng/ml

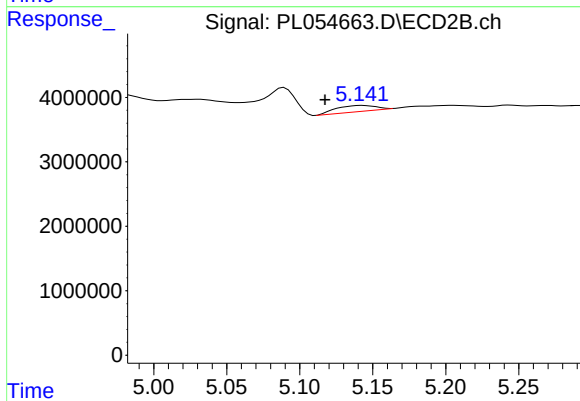

#7 delta-BHC


R.T.: 5.143 min
Delta R.T.: 0.025 min
Response: 1805333
Conc: 0.68 ng/ml

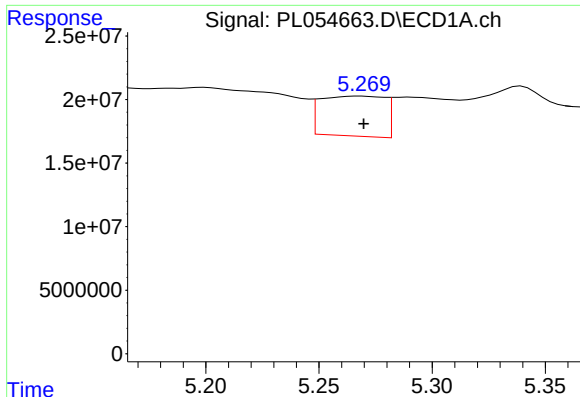

#8 Heptachlor epoxide


R.T.: 5.269 min
Delta R.T.: -0.001 min
Response: 61802540
Conc: 4.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

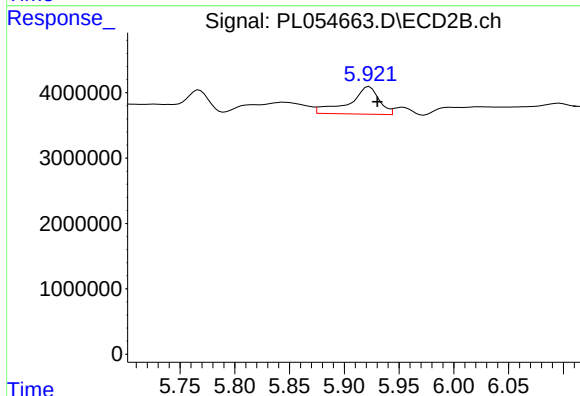


#8 Heptachlor epoxide

R.T.: 5.923 min
Delta R.T.: -0.008 min
Response: 8058052
Conc: 3.23 ng/ml

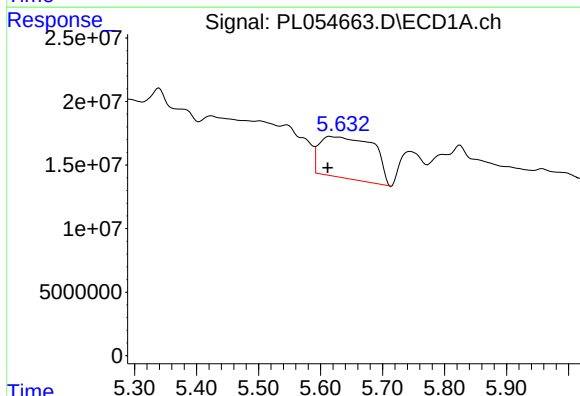


#9 Endosulfan I

R.T.: 5.615 min
Delta R.T.: 0.003 min
Response: 198505294
Conc: 14.56 ng/ml

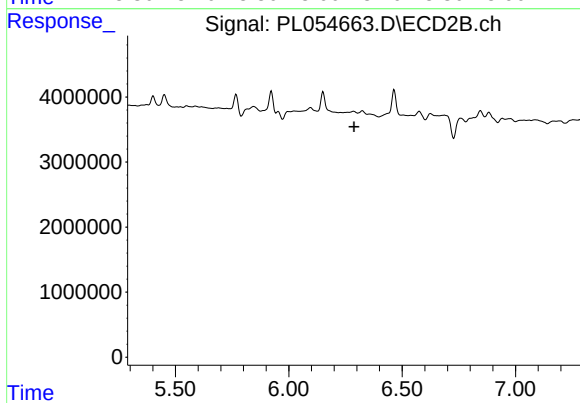

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

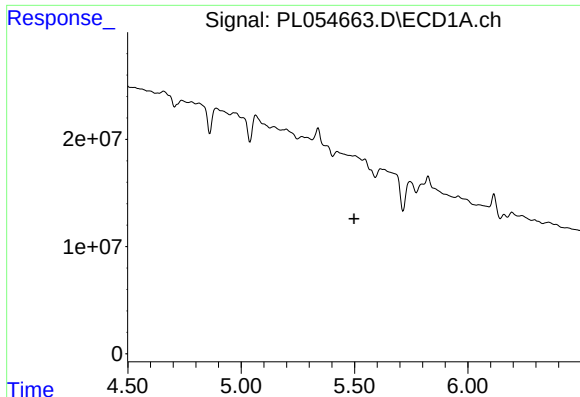

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

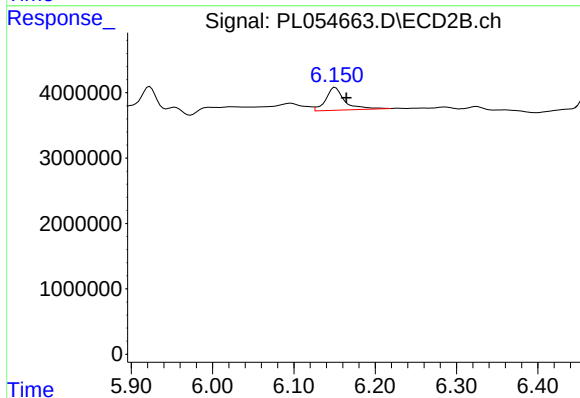


#10 gamma-Chlordane

R.T.: 6.151 min
Delta R.T.: -0.014 min
Response: 5672038
Conc: 2.15 ng/ml

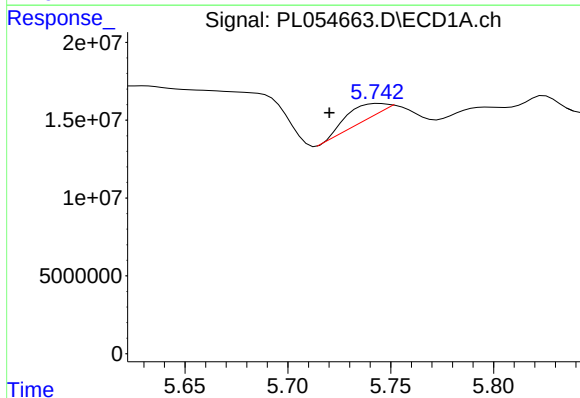


#12 4,4'-DDE

R.T.: 5.745 min
Delta R.T.: 0.024 min
Response: 7097565
Conc: 0.53 ng/ml

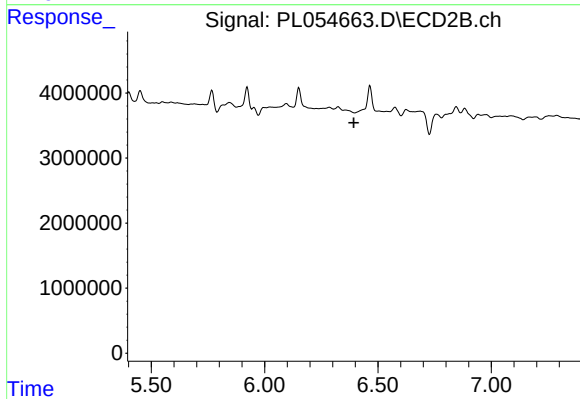

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.394 min
Response: 0
Conc: N.D.

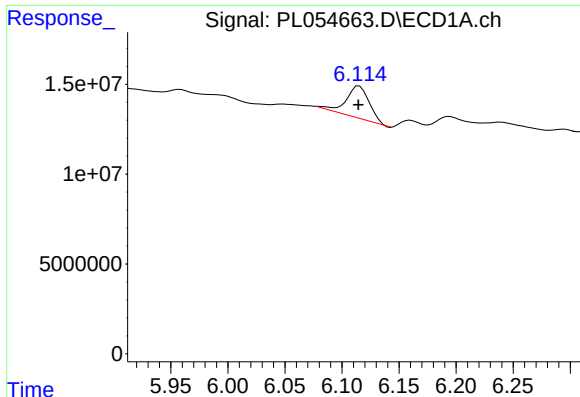

#14 Endrin


R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 25646740
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

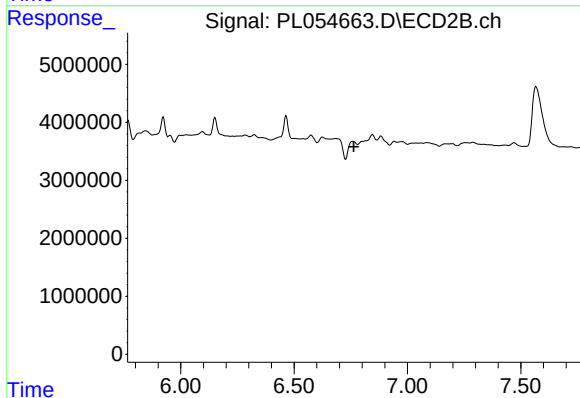


#14 Endrin

R.T.: 6.758 min
Delta R.T.: -0.006 min
Response: -1354764
Conc: N.D.

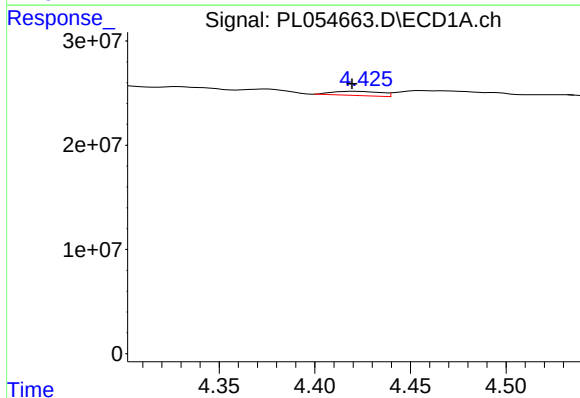


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.001 min
Response: 7250819
Conc: 18.37 ng/ml

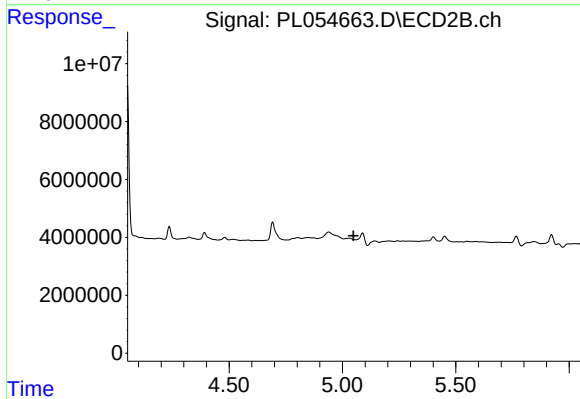

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.049 min
Response: 0
Conc: N.D.

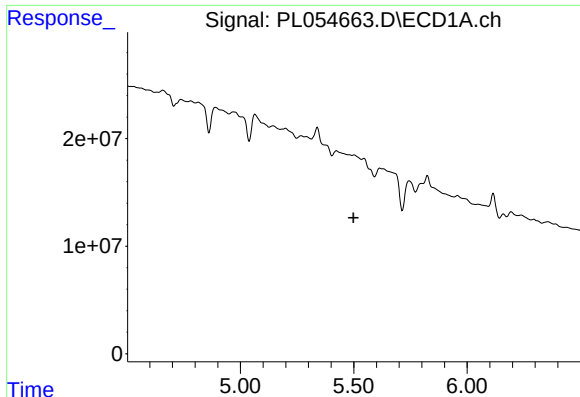

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-112219

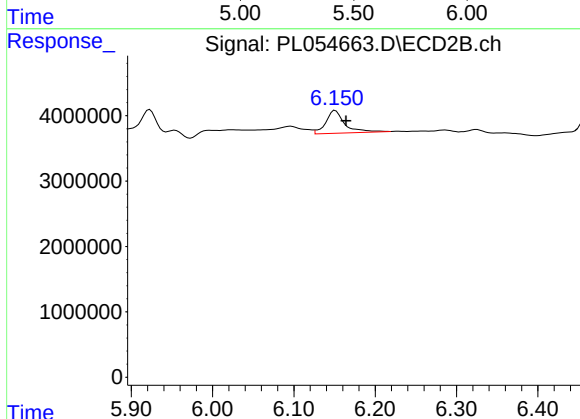


#25 Chlordane-3

R.T.: 6.151 min
Delta R.T.: -0.013 min
Response: 5672038
Conc: 18.27 ng/ml

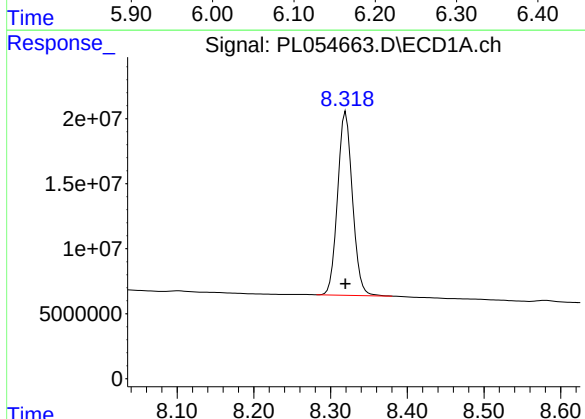

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 189819384
Conc: 19.82 ng/ml

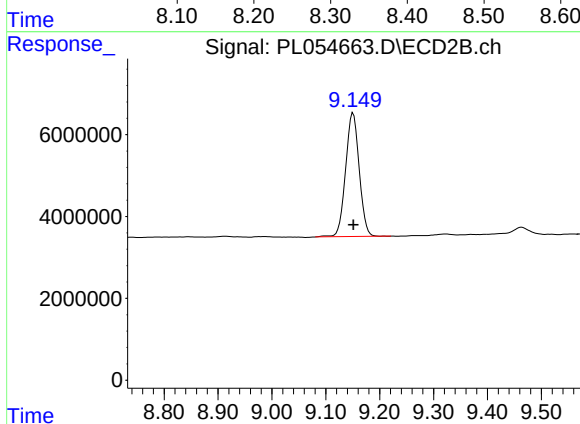

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 52962708
Conc: 22.09 ng/ml