

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 01:06
 Operator : SG\AJ
 Sample : K6008-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CALVTANK-1-20191121

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 02:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.051	212.1E6	49972230	18.231	19.583
28)	SA Decachlor...	8.320	9.149	164.4E6	43464737	17.164	18.130
Target Compounds							
5)	MB Aldrin	4.828	0.000	16360844	0	1.004	N.D. #
6)	B beta-BHC	4.495f	0.000	9168077	0	1.236	N.D. #
7)	B delta-BHC	0.000	5.145f	0	3788656	N.D.	1.421 #
8)	B Heptachlo...	0.000	5.919	0	4044948	N.D.	1.619 #
9)	A Endosulfan I	5.622	0.000	56092182	0	4.113	N.D. #
12)	B 4,4'-DDE	5.743f	0.000	7046865	0	0.530	N.D. #
14)	MA Endrin	6.114	6.759	26305945	-233680	2.066	N.D. #
15)	B Endosulfa...	0.000	6.967	0	3909394	N.D.	1.663 #
23)	Chlordane-1	4.391f	5.038	10296662	2198537	26.092	27.580
27)	Chlordane-5	0.000	7.025f	0	384149	N.D.	5.698 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 01:06
Operator : SG\AJ
Sample : K6008-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 02:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

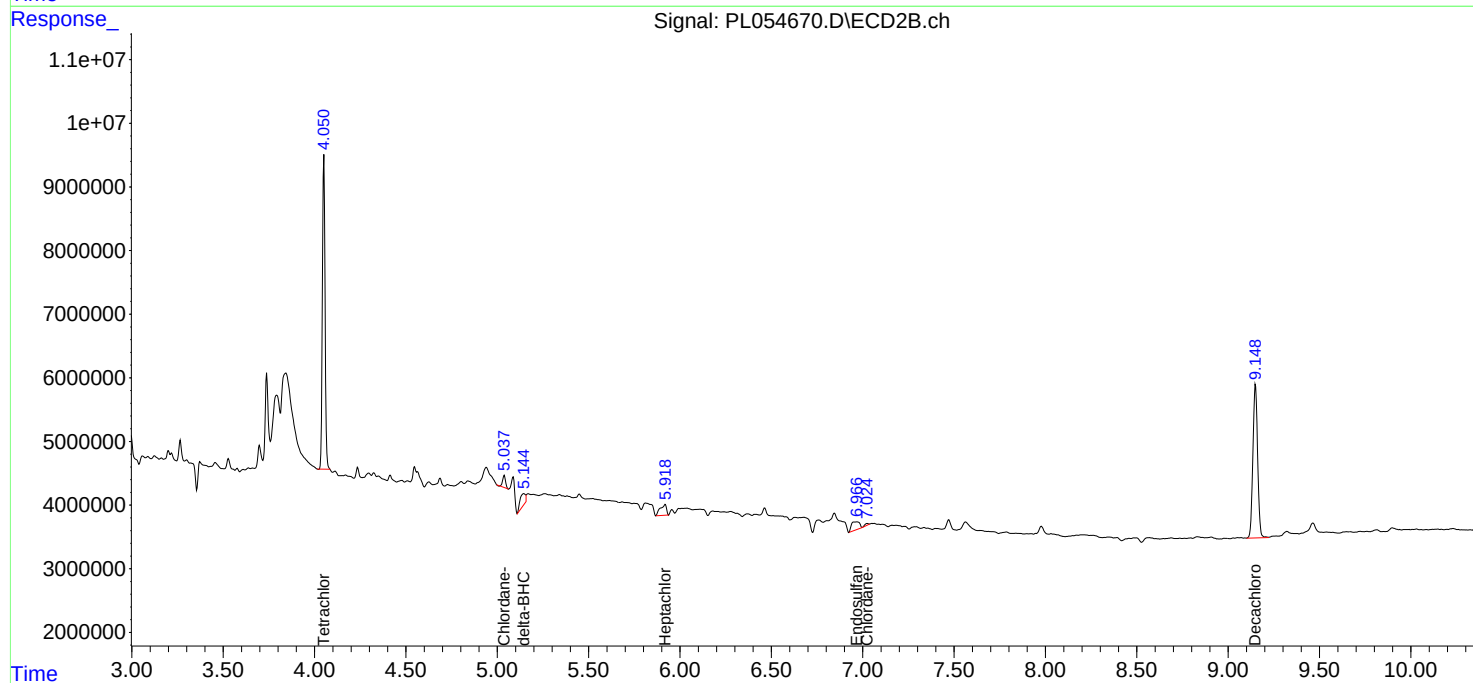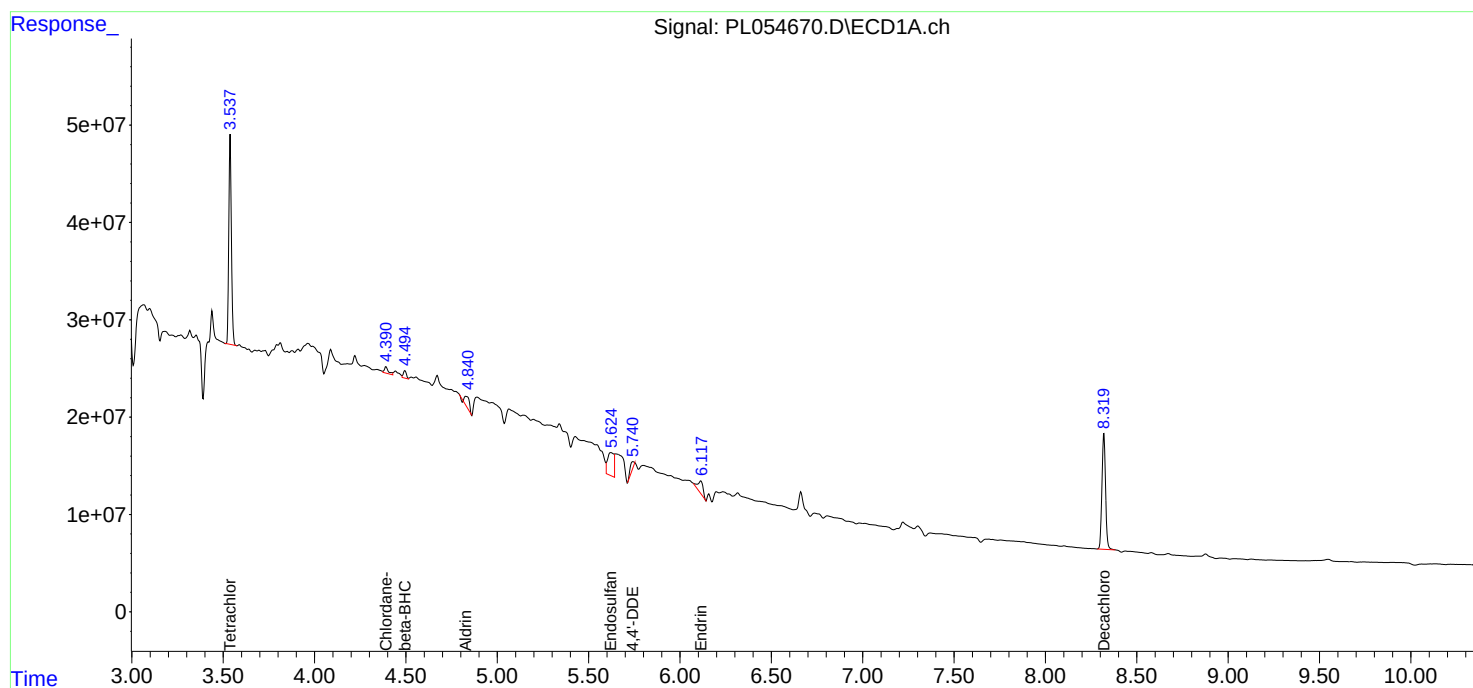


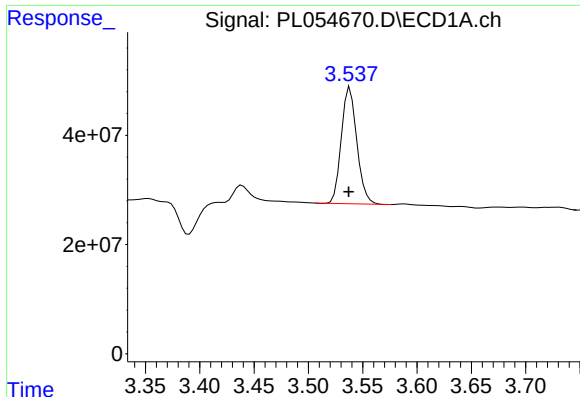

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.001 min
Response: 212103505
Conc: 18.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

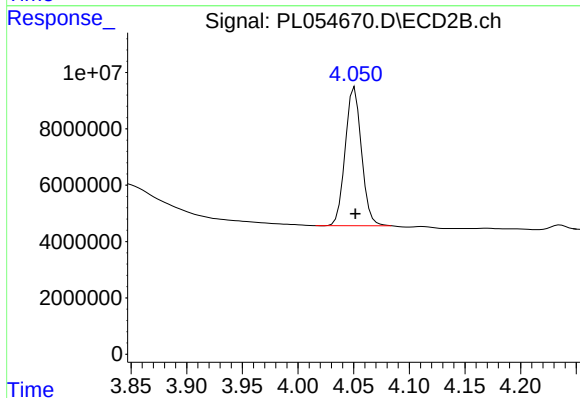


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 49972230
Conc: 19.58 ng/ml

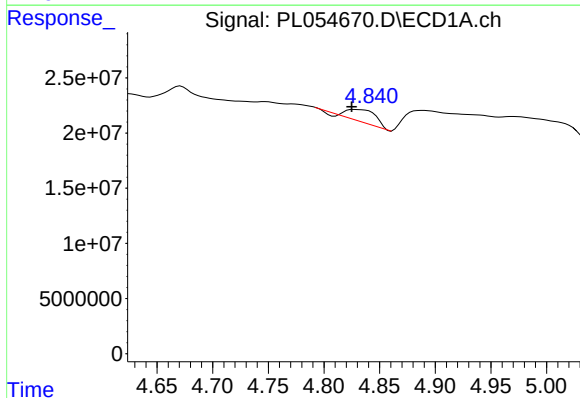


#5 Aldrin

R.T.: 4.828 min
Delta R.T.: 0.003 min
Response: 16360844
Conc: 1.00 ng/ml

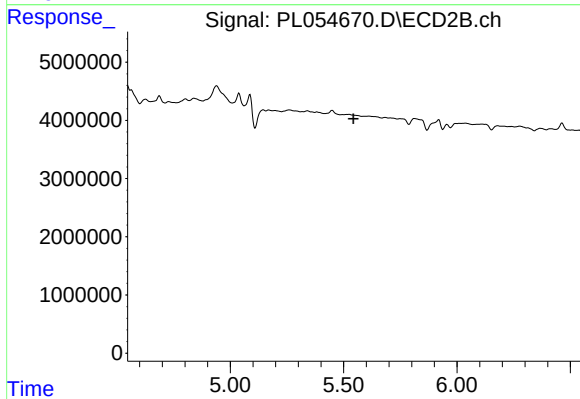

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.544 min
Response: 0
Conc: N.D.

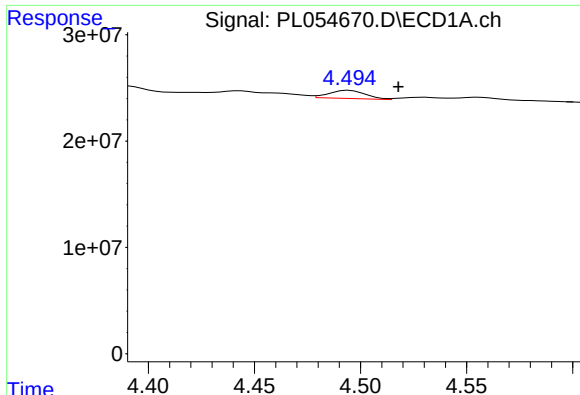

#6 beta-BHC


R.T.: 4.495 min
Delta R.T.: -0.023 min
Response: 9168077
Conc: 1.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

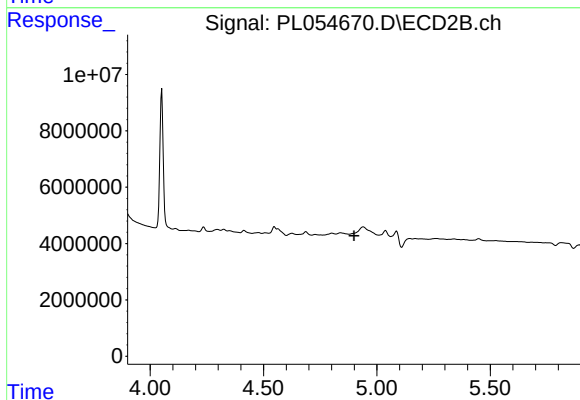


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.899 min
Response: 0
Conc: N.D.

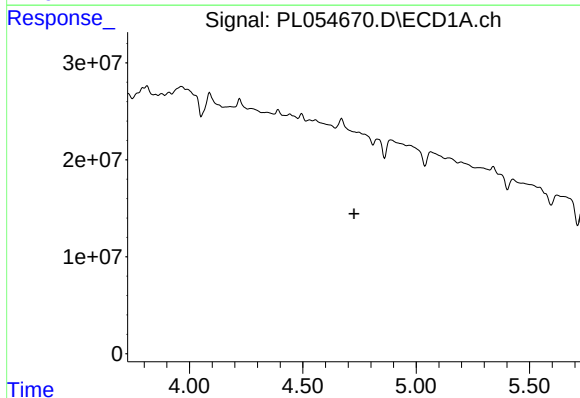


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

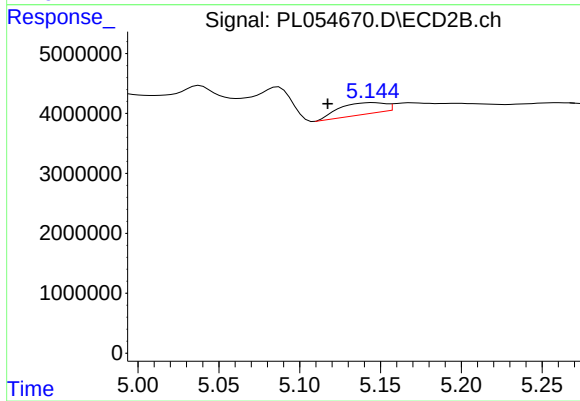

#7 delta-BHC


R.T.: 5.145 min
Delta R.T.: 0.028 min
Response: 3788656
Conc: 1.42 ng/ml

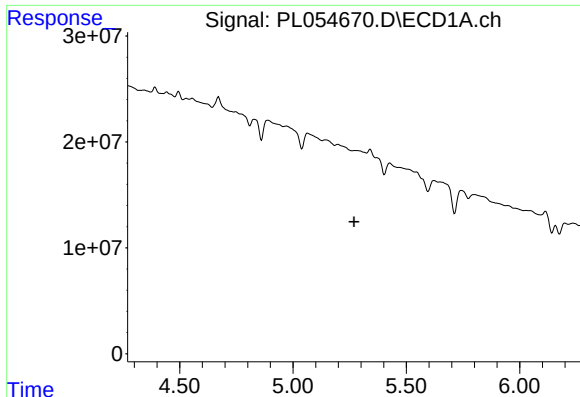

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

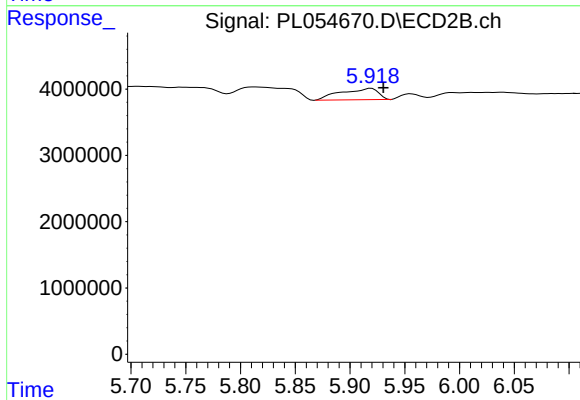


#8 Heptachlor epoxide

R.T.: 5.919 min
Delta R.T.: -0.011 min
Response: 4044948
Conc: 1.62 ng/ml

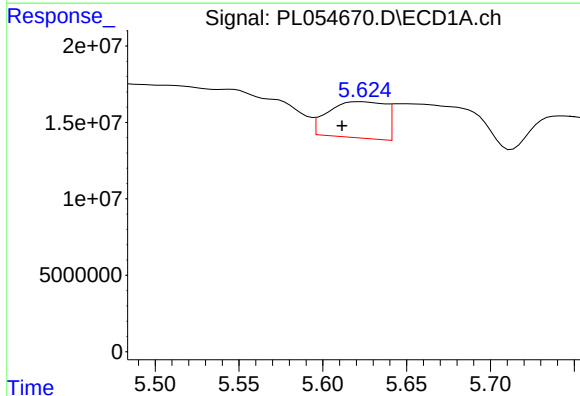


#9 Endosulfan I

R.T.: 5.622 min
Delta R.T.: 0.010 min
Response: 56092182
Conc: 4.11 ng/ml

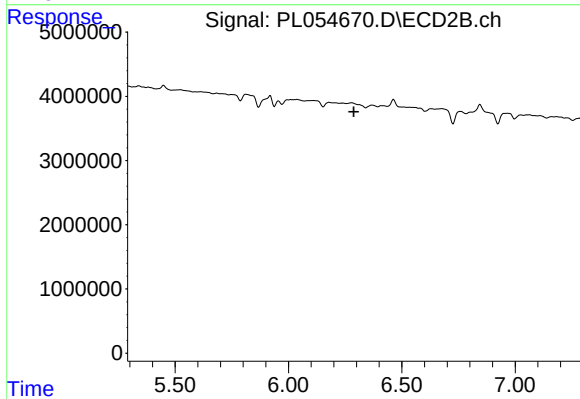

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.288 min
Response: 0
Conc: N.D.

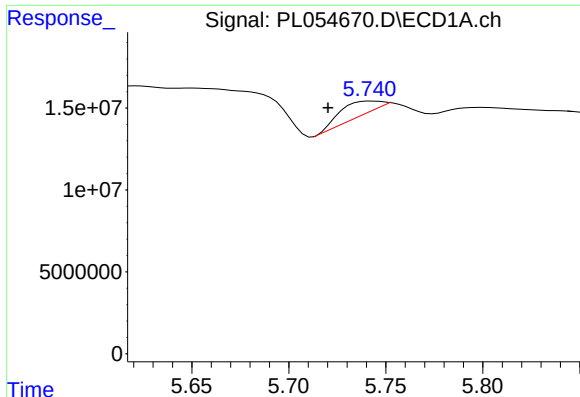

#12 4,4'-DDE

R.T.: 5.743 min
Delta R.T.: 0.023 min
Response: 7046865
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

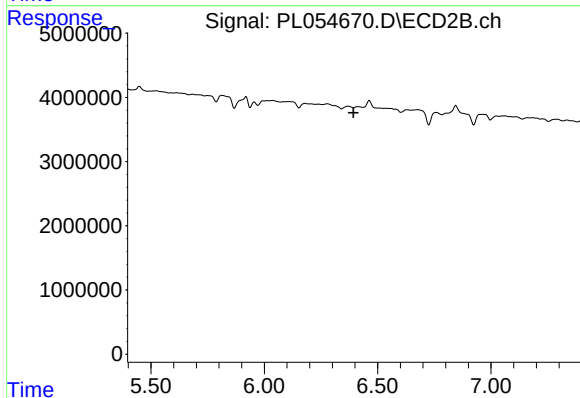


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.394 min
Response: 0
Conc: N.D.


#14 Endrin

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 26305945
Conc: 2.07 ng/ml

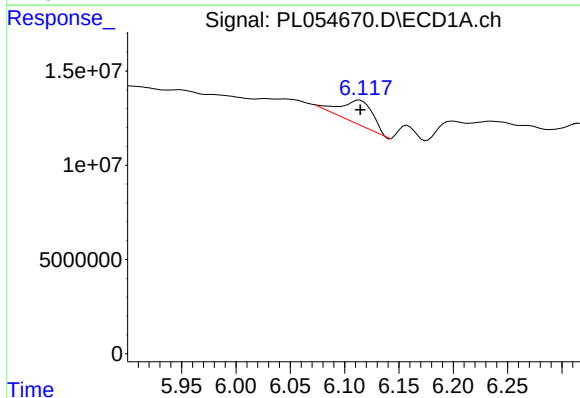

#14 Endrin


R.T.: 6.759 min
Delta R.T.: -0.005 min
Response: -233680
Conc: N.D.

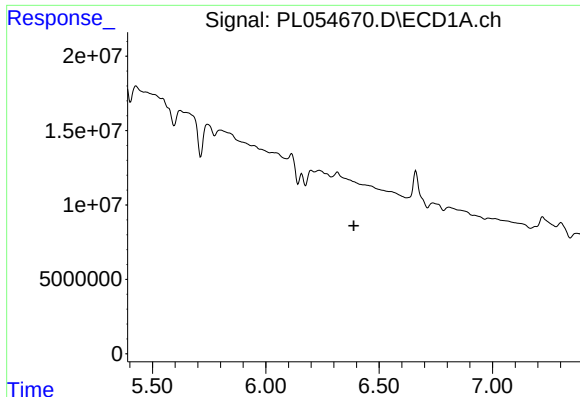

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

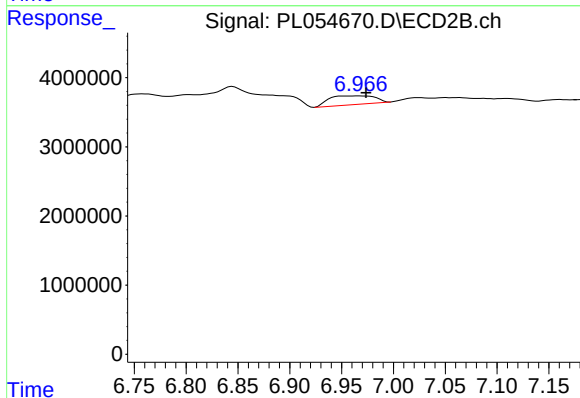


#15 Endosulfan II

R.T.: 6.967 min
Delta R.T.: -0.006 min
Response: 3909394
Conc: 1.66 ng/ml

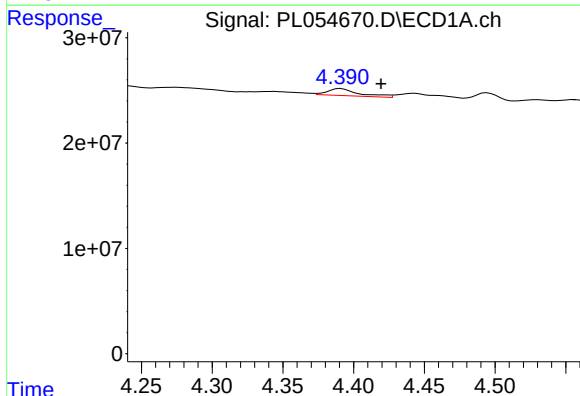


#23 Chlordane-1

R.T.: 4.391 min
Delta R.T.: -0.029 min
Response: 10296662
Conc: 26.09 ng/ml

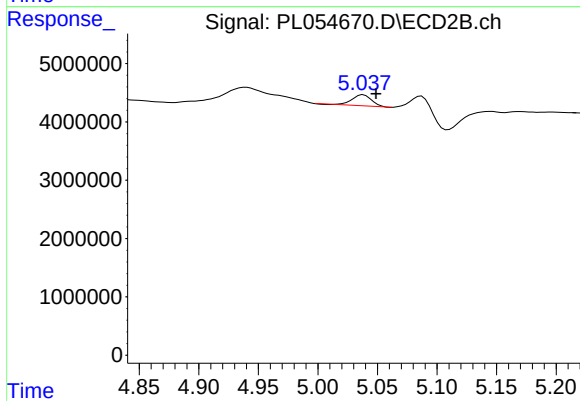

#23 Chlordane-1


R.T.: 5.038 min
Delta R.T.: -0.011 min
Response: 2198537
Conc: 27.58 ng/ml

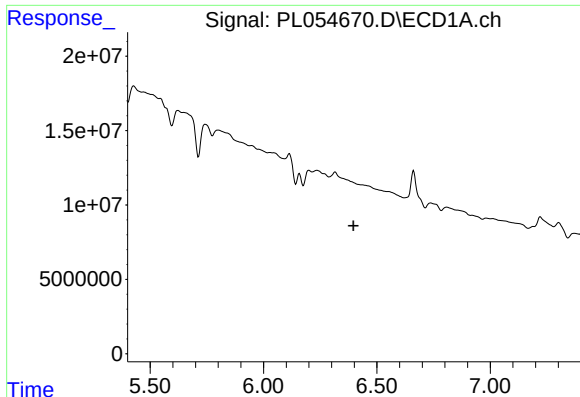

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CALVTANK-1-20191121

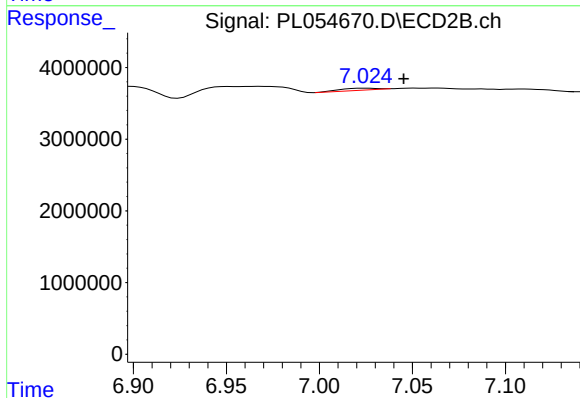


#27 Chlordane-5

R.T.: 7.025 min
Delta R.T.: -0.020 min
Response: 384149
Conc: 5.70 ng/ml

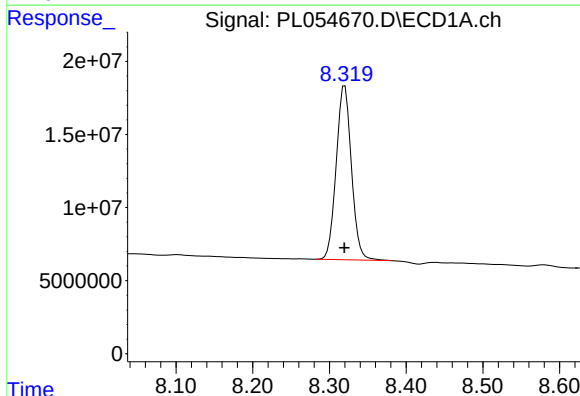

#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 164367425
Conc: 17.16 ng/ml

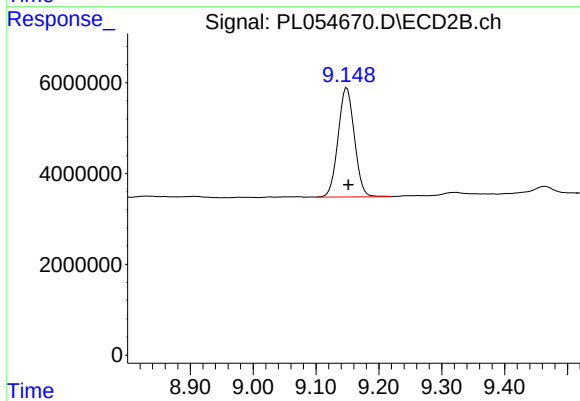

#28 Decachlorobiphenyl

R.T.: 9.149 min
Delta R.T.: -0.002 min
Response: 43464737
Conc: 18.13 ng/ml