

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 02:30
 Operator : SG\AJ
 Sample : K6024-07
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TWP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 06:18:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	4.051	91505967	22304068	7.865	8.740
28)	SA Decachlor...	8.319	9.150	71355013	19892026	7.451	8.297
Target Compounds							
2)	A alpha-BHC	3.971	0.000	20756457	0	1.093	N.D. #
3)	MA gamma-BHC...	4.268	0.000	17511256	0	1.027	N.D. #
8)	B Heptachlo...	0.000	5.909f	0	2751828	N.D.	1.102 #
10)	B gamma-Chl...	5.473f	0.000	61264034	0	4.040	N.D. #
15)	B Endosulfa...	0.000	6.955f	0	5360797	N.D.	2.280 #
18)	B Endrin al...	0.000	7.104	0	414440	N.D.	0.211 #
22)	Mirex	7.479f	0.000	2999031	0	0.369	N.D. #
25)	Chlordane-3	5.473f	0.000	61264034	0	47.709	N.D. #
27)	Chlordane-5	0.000	7.018f	0	809490	N.D.	12.007 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 02:30
Operator : SG\AJ
Sample : K6024-07
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TWP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 06:18:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

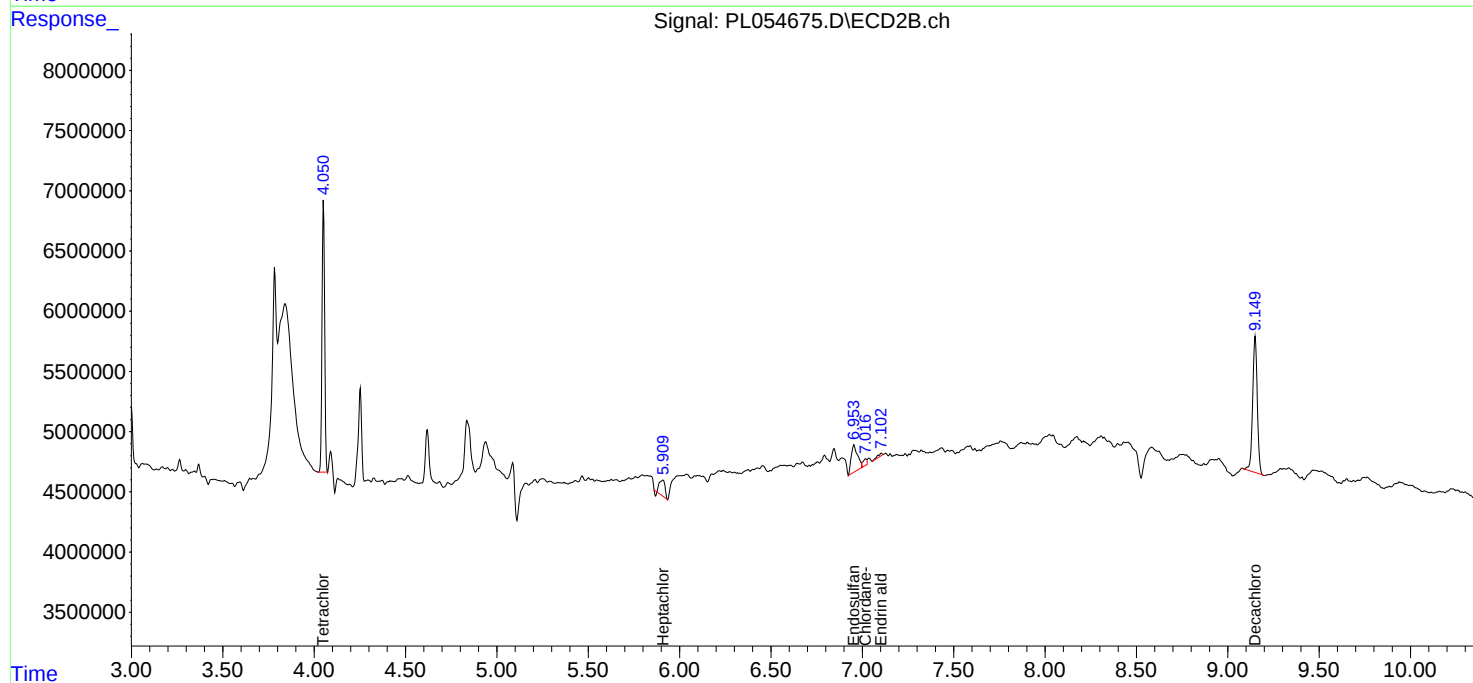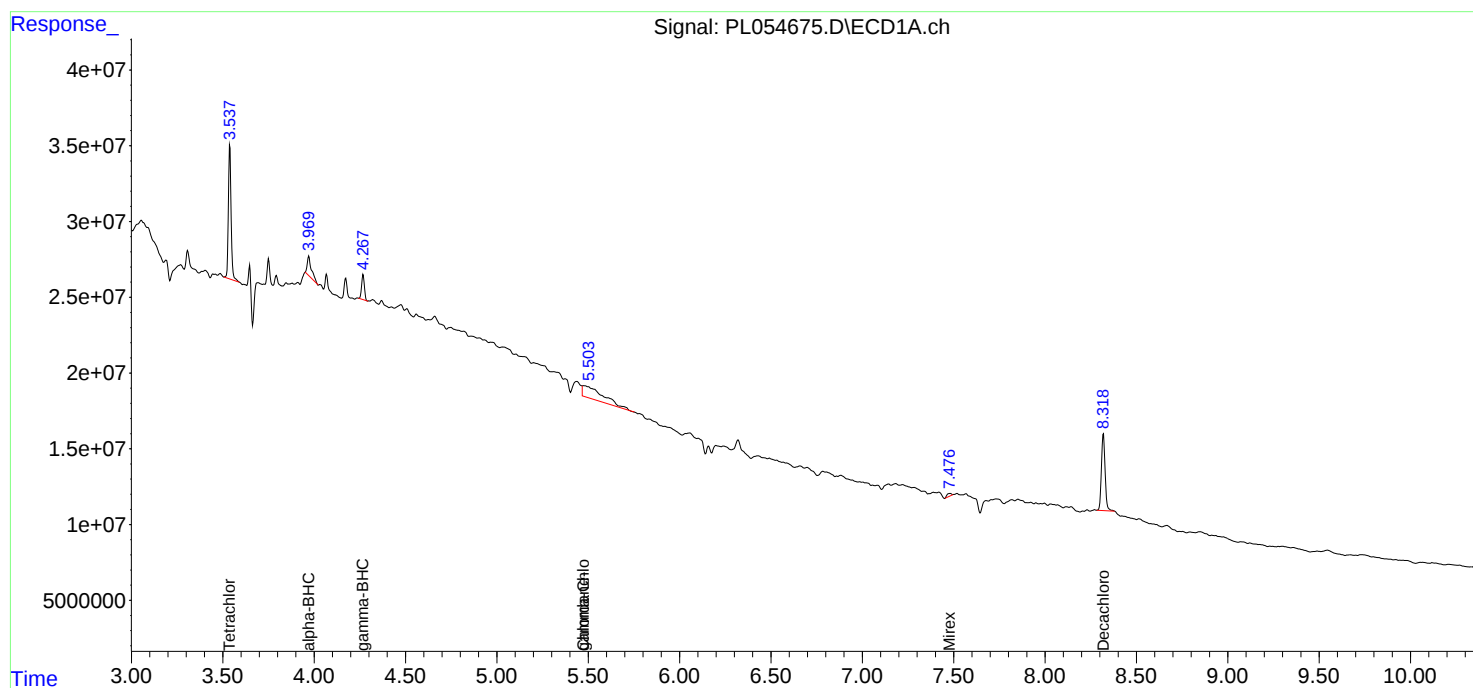


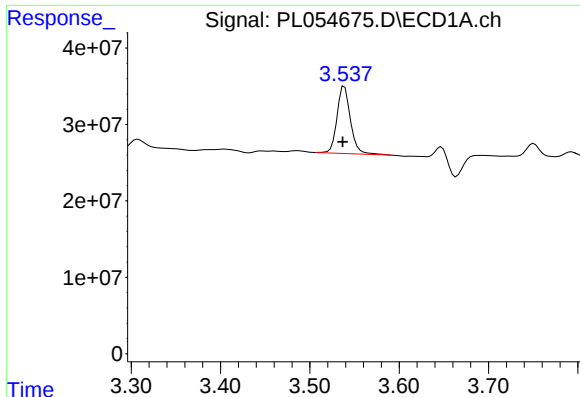

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.002 min
Response: 91505967
Conc: 7.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-3

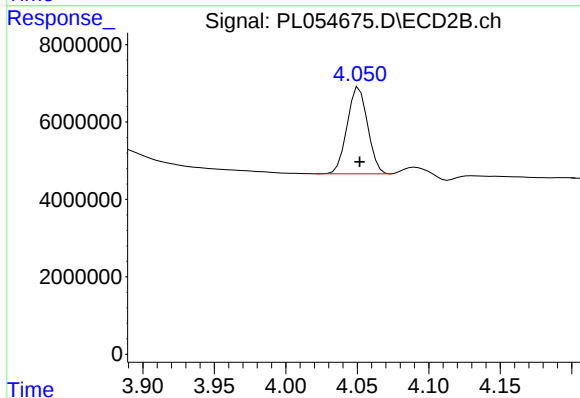


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 22304068
Conc: 8.74 ng/ml

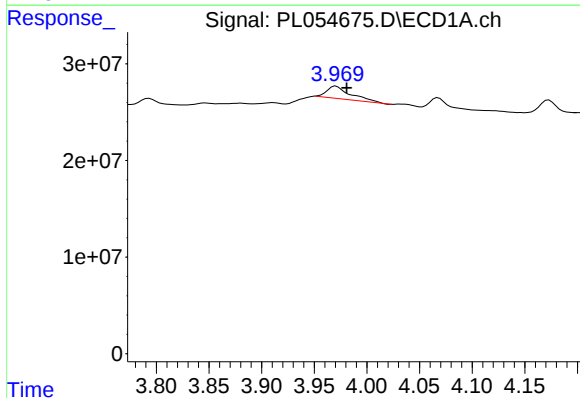


#2 alpha-BHC

R.T.: 3.971 min
Delta R.T.: -0.010 min
Response: 20756457
Conc: 1.09 ng/ml

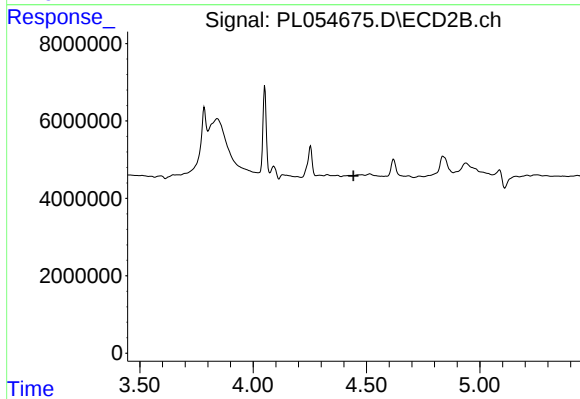

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.443 min
Response: 0
Conc: N.D.

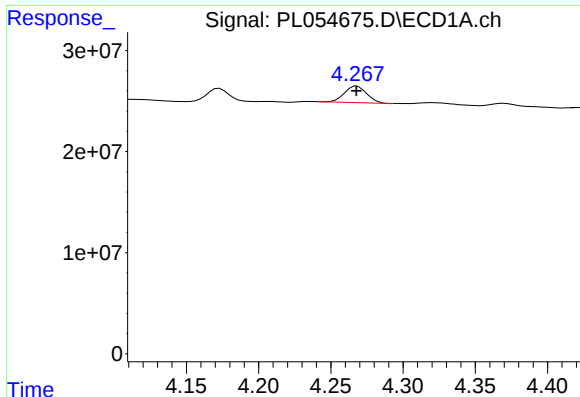

#3 gamma-BHC (Lindane)


R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 17511256
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-3

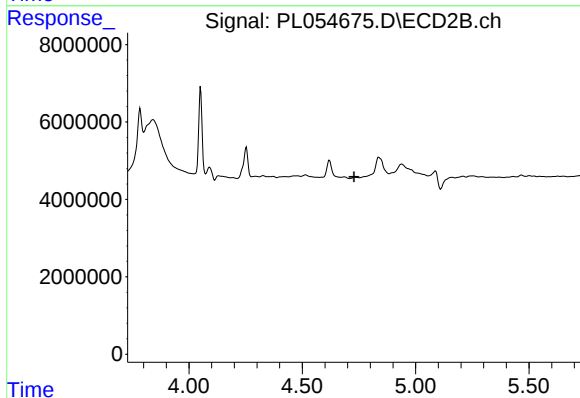


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.729 min
Response: 0
Conc: N.D.

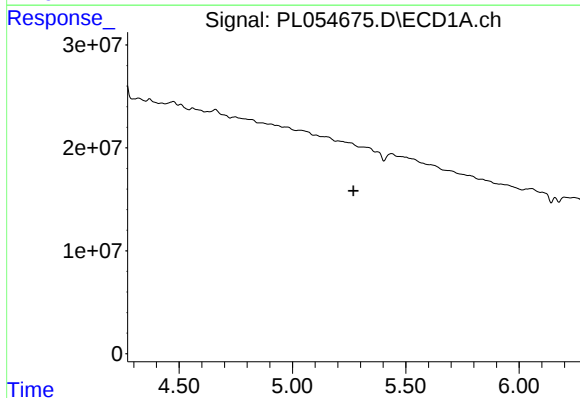


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.270 min
Response: 0
Conc: N.D.

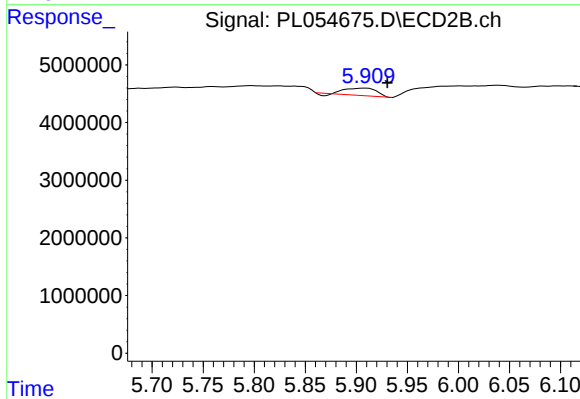

#8 Heptachlor epoxide


R.T.: 5.909 min
Delta R.T.: -0.021 min
Response: 2751828
Conc: 1.10 ng/ml

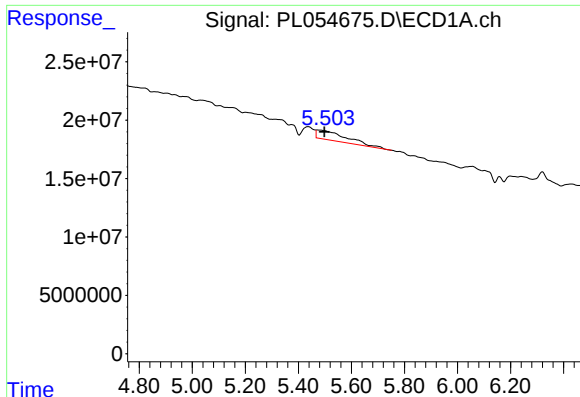

#10 gamma-Chlordane


R.T.: 5.473 min
Delta R.T.: -0.025 min
Response: 61264034
Conc: 4.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-3

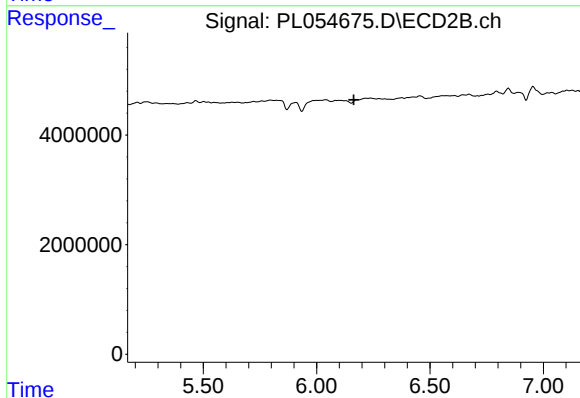


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

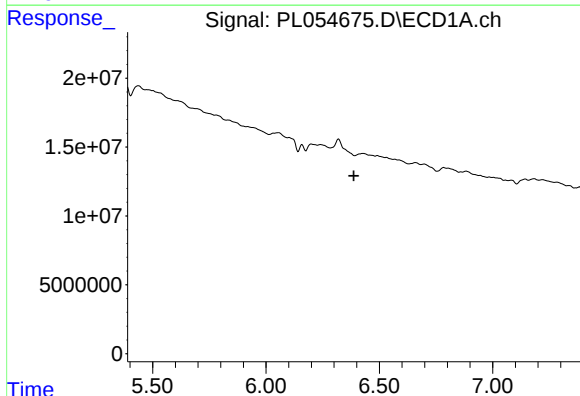


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.388 min
Response: 0
Conc: N.D.

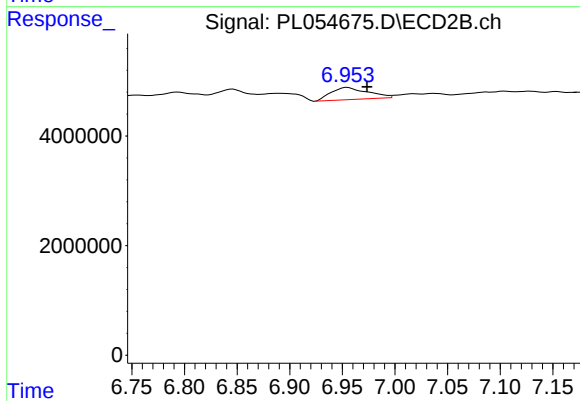

#15 Endosulfan II


R.T.: 6.955 min
Delta R.T.: -0.019 min
Response: 5360797
Conc: 2.28 ng/ml

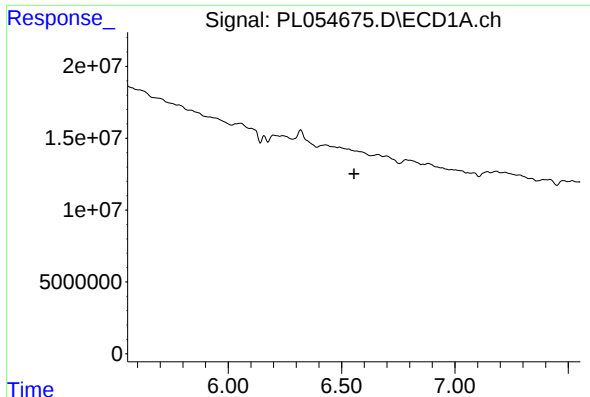

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TWP-3

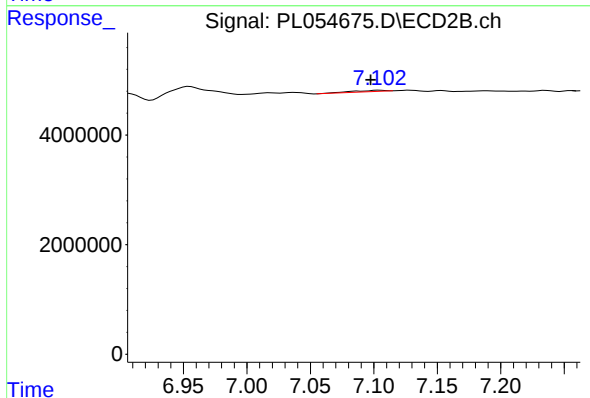


#18 Endrin aldehyde

R.T.: 7.104 min
Delta R.T.: 0.006 min
Response: 414440
Conc: 0.21 ng/ml

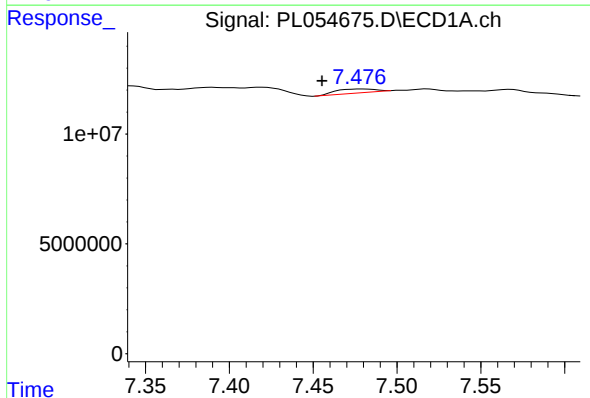


#22 Mirex

R.T.: 7.479 min
Delta R.T.: 0.023 min
Response: 2999031
Conc: 0.37 ng/ml

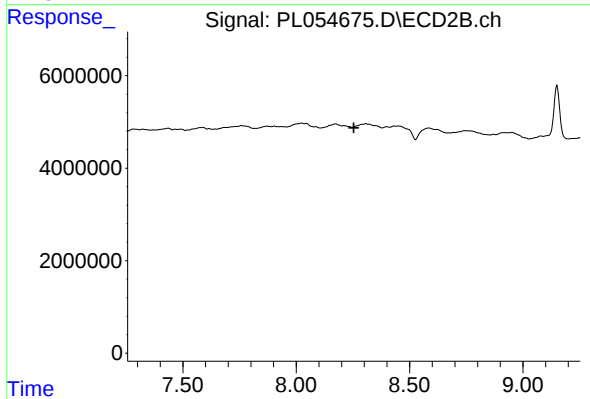

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 8.254 min
Response: 0
Conc: N.D.

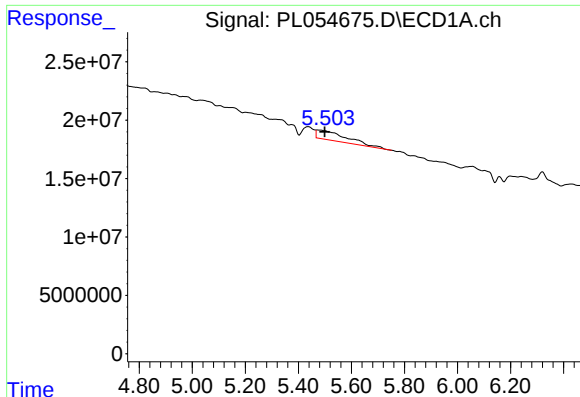

#25 Chlordane-3


R.T.: 5.473 min
Delta R.T.: -0.025 min
Response: 61264034
Conc: 47.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-3

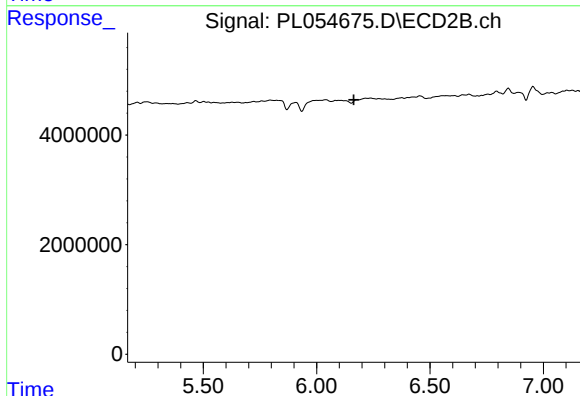


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.164 min
Response: 0
Conc: N.D.

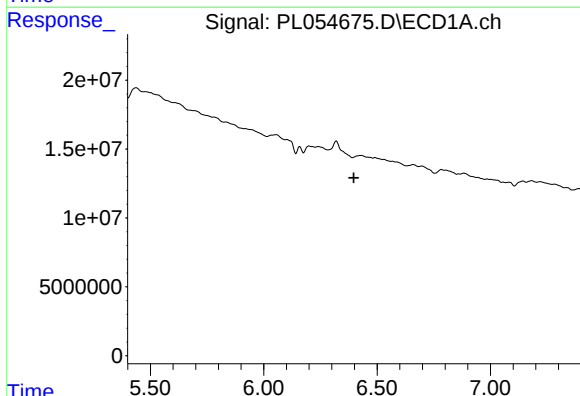


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.397 min
Response: 0
Conc: N.D.

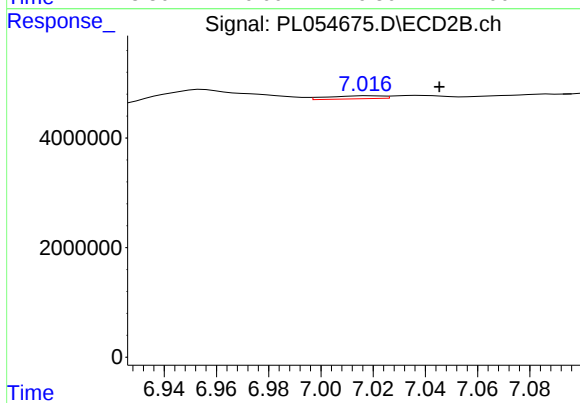

#27 Chlordane-5


R.T.: 7.018 min
Delta R.T.: -0.027 min
Response: 809490
Conc: 12.01 ng/ml

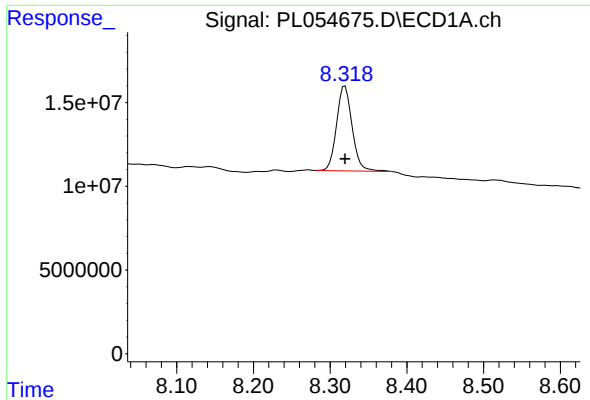

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 71355013
Conc: 7.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TWP-3

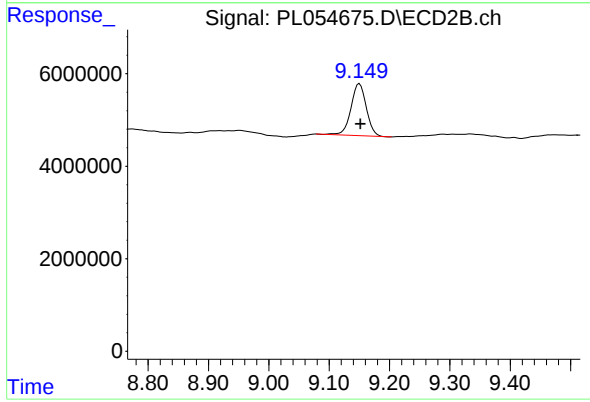

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: -0.001 min
Response: 19892026
Conc: 8.30 ng/ml