

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 17:21
 Operator : SG\AJ
 Sample : K6018-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-359

Manual Integrations
 APPROVED

Ankita
 11/27/2019 11:35:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 02:45:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	4.051	237.8E6	55578557	20.440	21.780
28) SA Decachlor...	8.319	9.150	152.6E6	40491545	15.931	16.890
Target Compounds						
10) B gamma-Chl...	5.497	6.163	110.9E6	25079048	7.314m	9.520 #
11) B alpha-Chl...	5.555	6.238	92045903	32693143	6.242m	12.451 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 17:21
Operator : SG\AJ
Sample : K6018-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ETGI-359


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 02:45:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

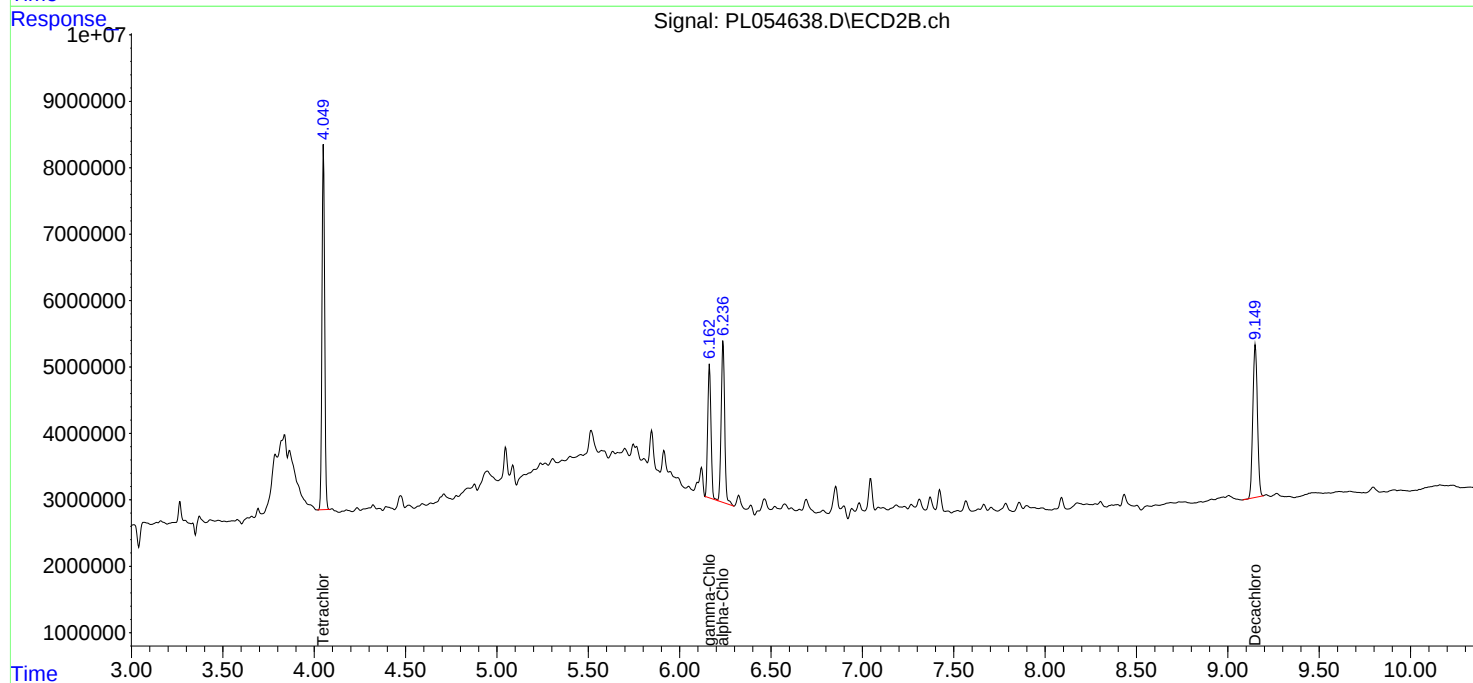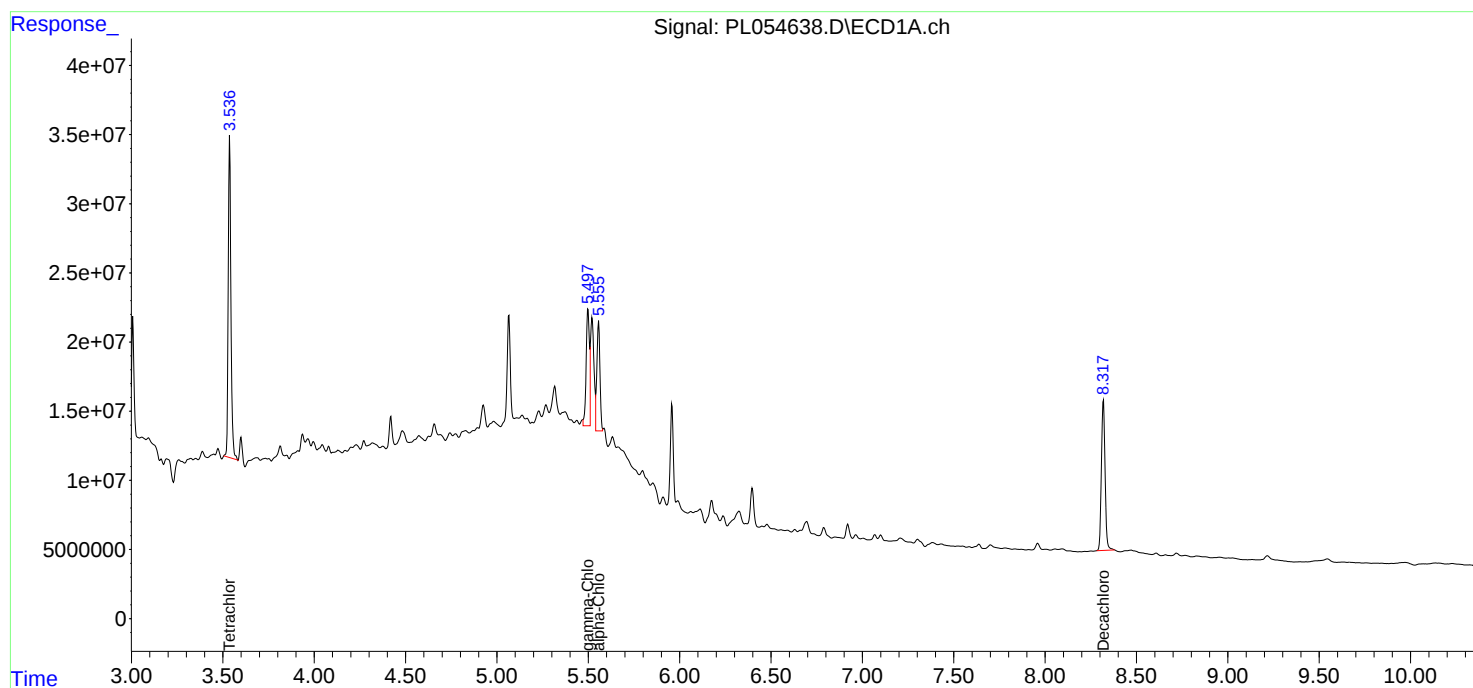

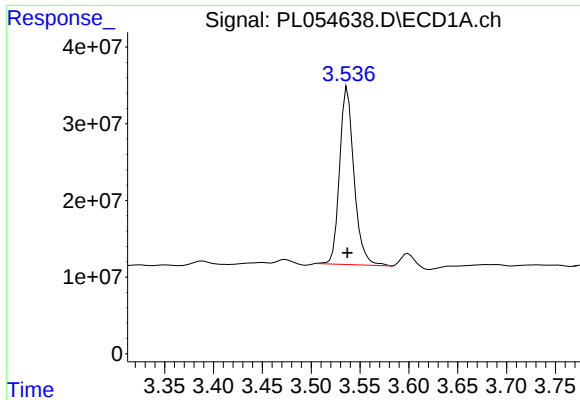


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 237800046
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-359


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:44 AM

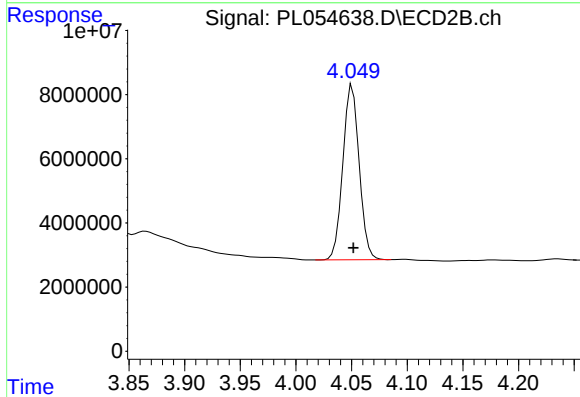


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 55578557
Conc: 21.78 ng/ml

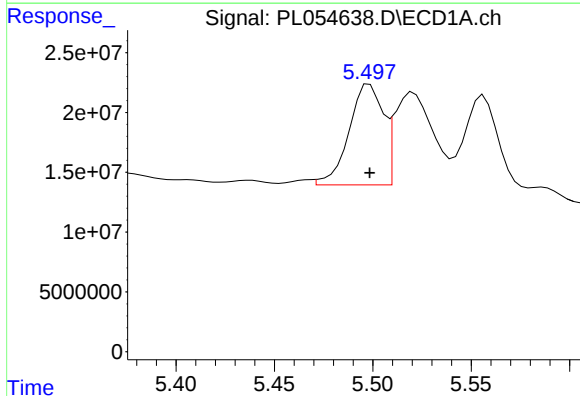


#10 gamma-Chlordane

R.T.: 5.497 min
Delta R.T.: -0.002 min
Response: 110917868
Conc: 7.31 ng/ml m

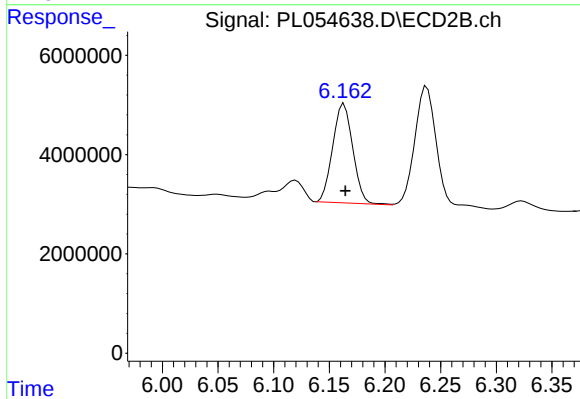

#10 gamma-Chlordane

R.T.: 6.163 min
Delta R.T.: -0.001 min
Response: 25079048
Conc: 9.52 ng/ml

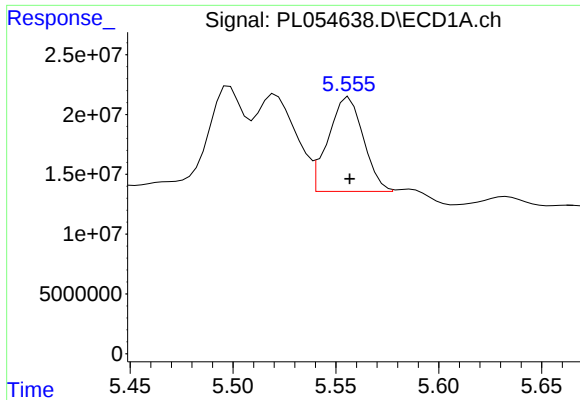


#11 alpha-Chlordane

R.T.: 5.555 min
Delta R.T.: -0.002 min
Response: 92045903
Conc: 6.24 ng/ml m

Instrument :
ECD_L
ClientSampleId :
ETGI-359


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:44 AM

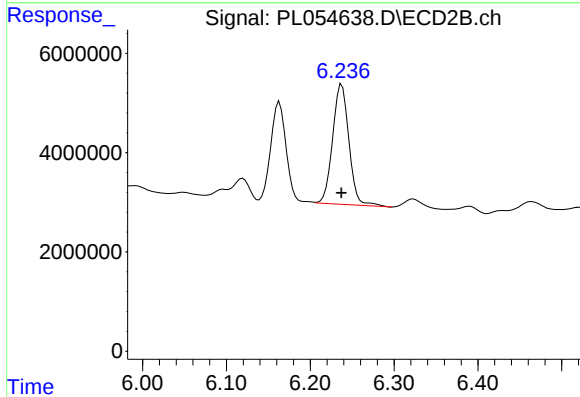


#11 alpha-Chlordane

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 32693143
Conc: 12.45 ng/ml

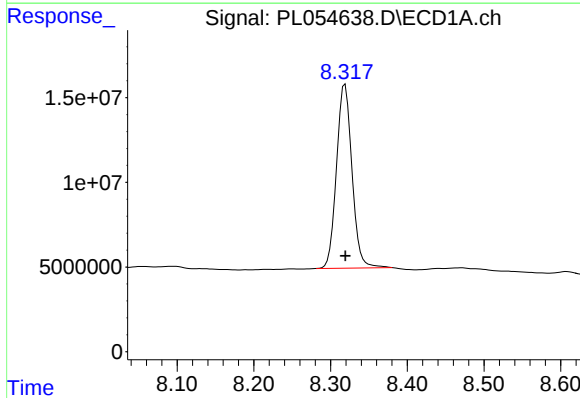

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 152555364
Conc: 15.93 ng/ml

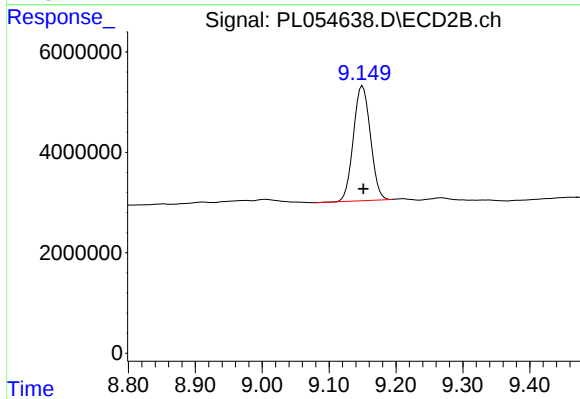

#28 Decachlorobiphenyl

R.T.: 9.150 min
Delta R.T.: -0.001 min
Response: 40491545
Conc: 16.89 ng/ml