

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 18:32
 Operator : SG\AJ
 Sample : K6022-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15-S

Manual Integrations
 APPROVED

Ankita
 11/27/2019 11:35:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 02:46:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.051	159.8E6	38292224	13.737	15.006
28)	SA Decachlor...	8.319	9.151	135.5E6	36483977	14.152	15.218
Target Compounds							
12)	B 4,4'-DDE	5.718	6.392	6949418	1722707	0.522m	0.696 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 18:32
Operator : SG\AJ
Sample : K6022-03
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 02:46:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

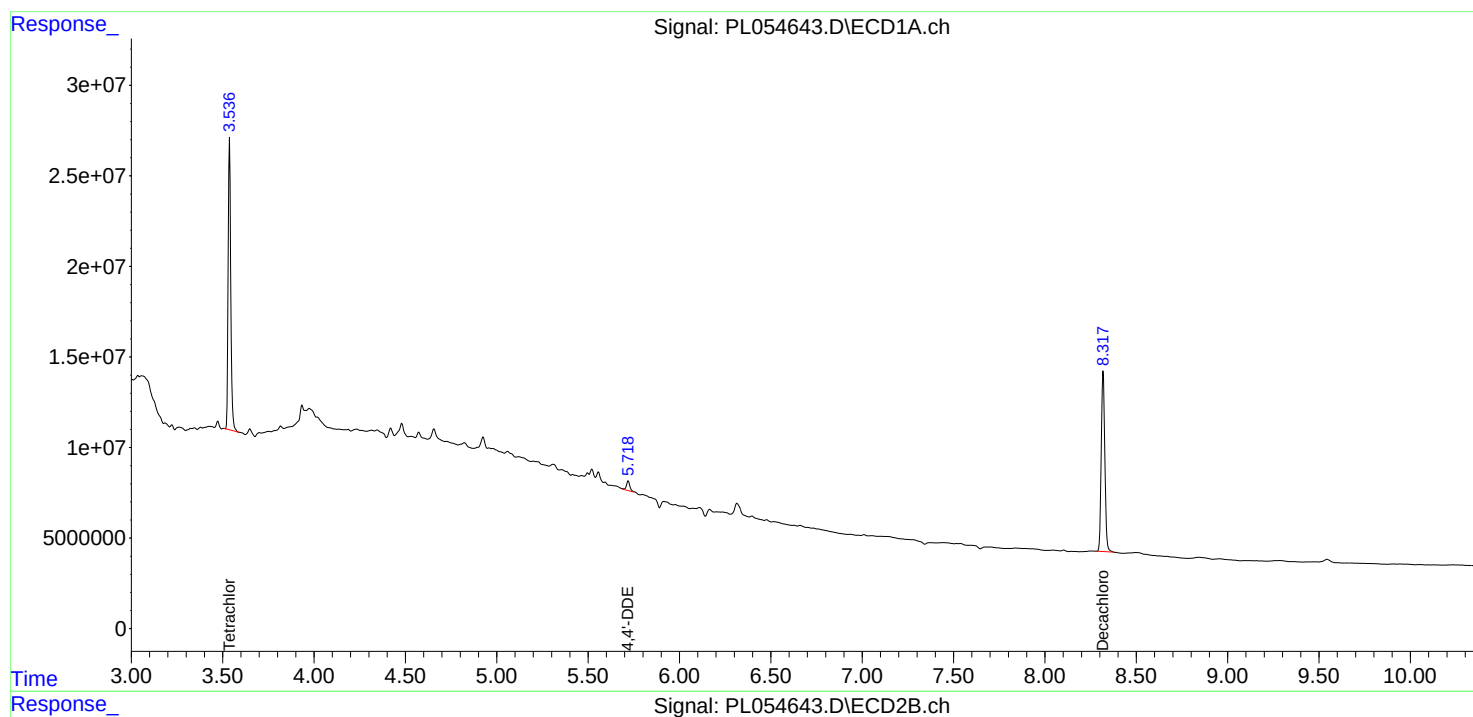

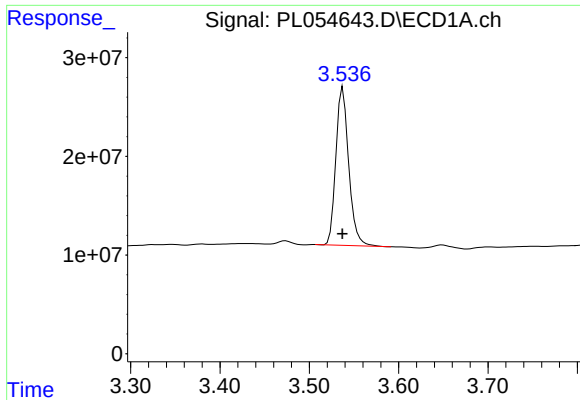


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 159813970
Conc: 13.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:53 AM

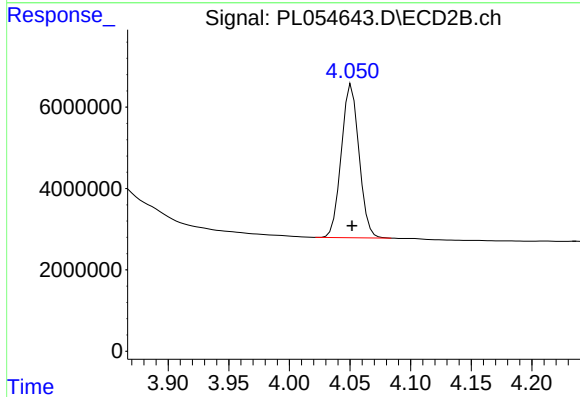


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 38292224
Conc: 15.01 ng/ml

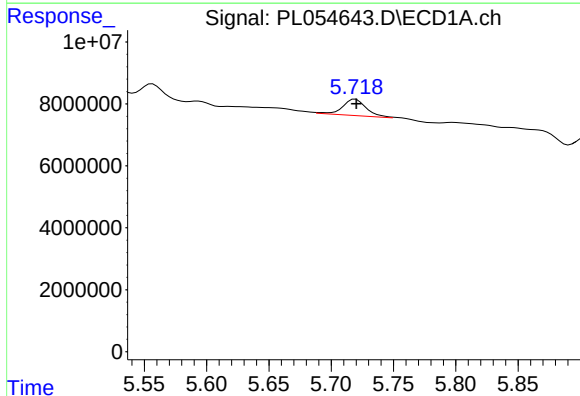


#12 4,4'-DDE

R.T.: 5.718 min
Delta R.T.: -0.002 min
Response: 6949418
Conc: 0.52 ng/ml m

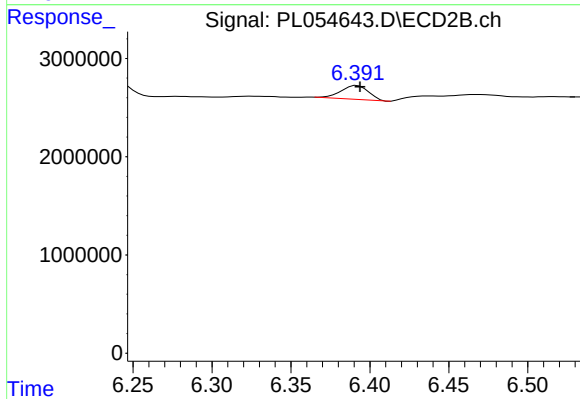

#12 4,4'-DDE

R.T.: 6.392 min
Delta R.T.: -0.002 min
Response: 1722707
Conc: 0.70 ng/ml

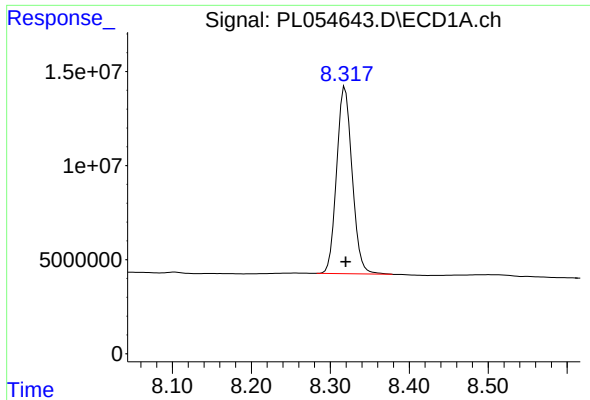


#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 135521588
Conc: 14.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S

Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:53 AM

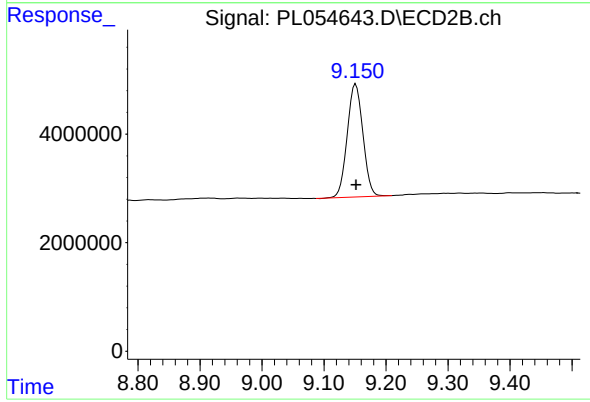

#28 Decachlorobiphenyl

R.T.: 9.151 min
Delta R.T.: 0.000 min
Response: 36483977
Conc: 15.22 ng/ml