

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
 Data File : PL054644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Nov 2019 18:46
 Operator : SG\AJ
 Sample : K6022-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-16-S

Manual Integrations
 APPROVED

Ankita
 11/27/2019 11:35:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 02:46:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	4.051	151.9E6	35678467	13.060	13.982
28)	SA Decachlor...	8.319	9.152	98094877	26506216	10.244	11.056
Target Compounds							
10)	B gamma-Chl...	5.499	6.165	11248321	5065456	0.742	1.923 #
11)	B alpha-Chl...	5.557	6.238	16893365	9949178	1.146	3.789m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112619\
Data File : PL054644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Nov 2019 18:46
Operator : SG\AJ
Sample : K6022-07
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-16-S


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 02:46:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

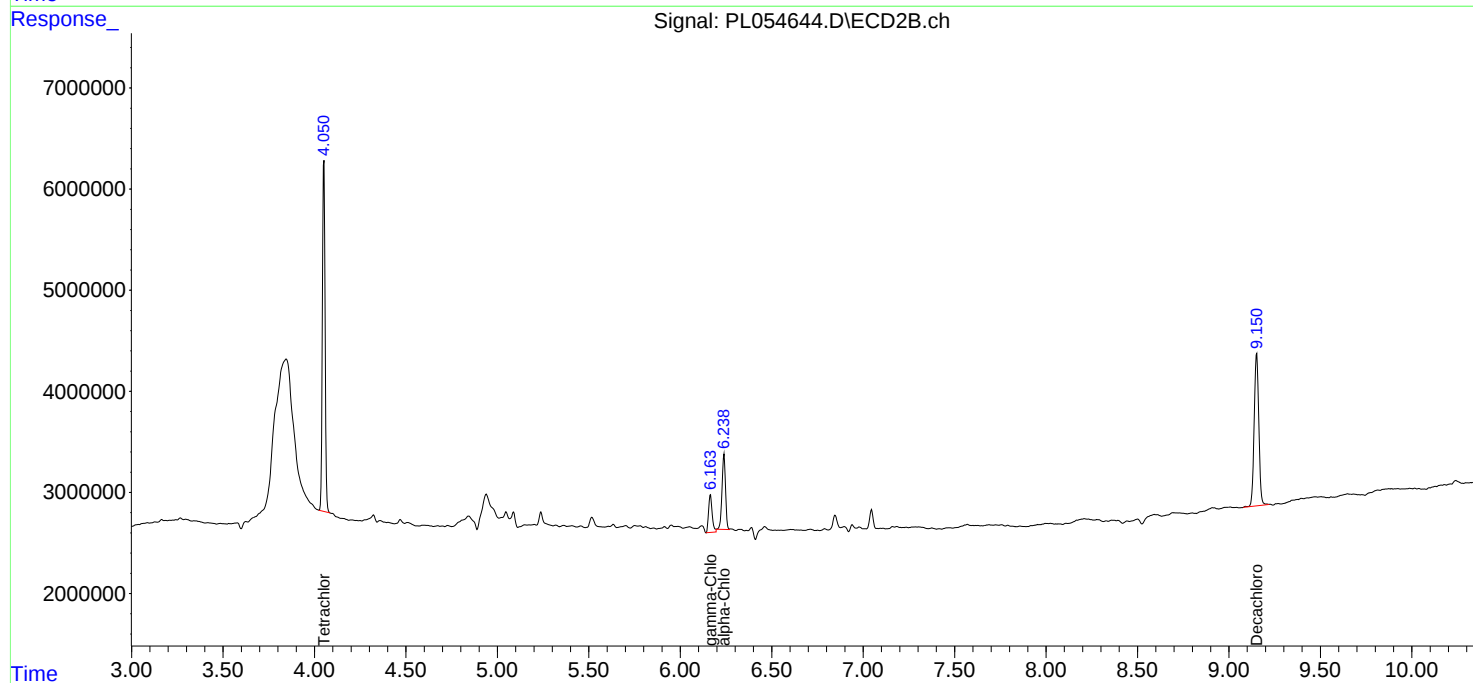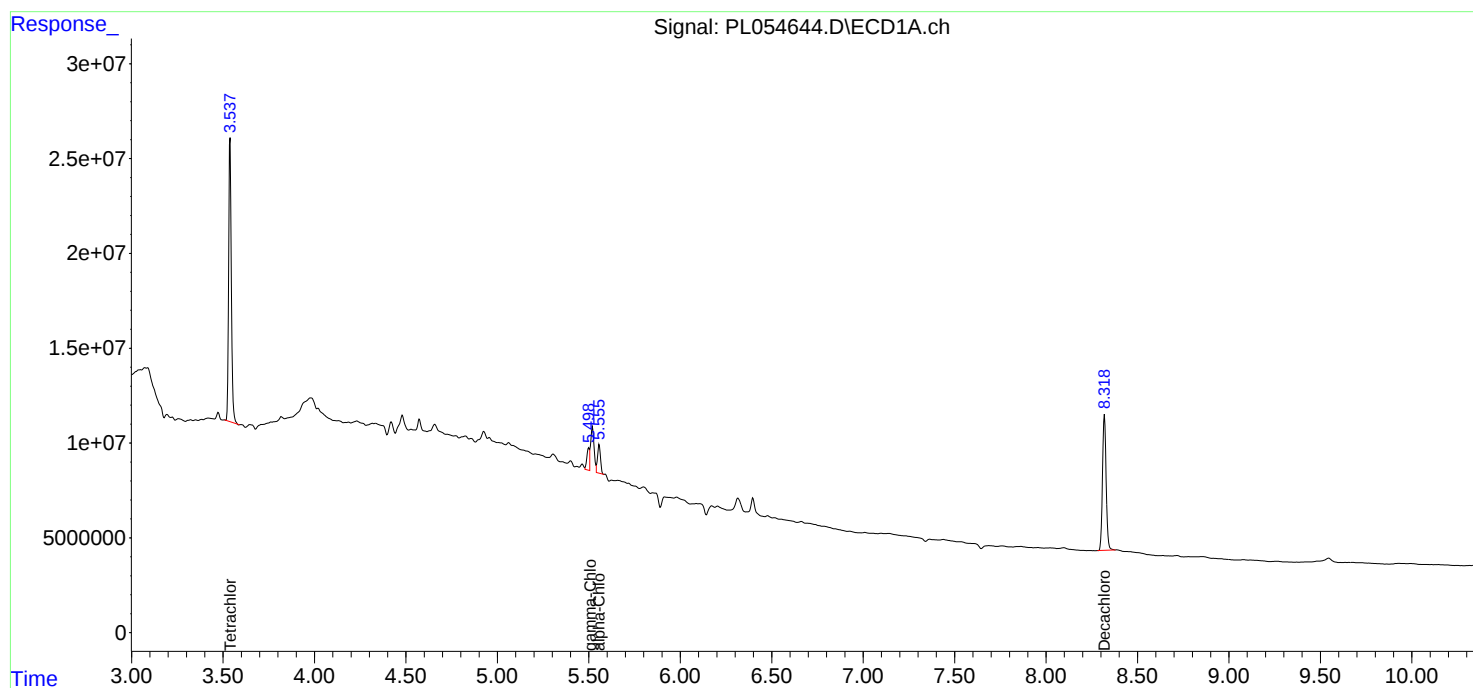

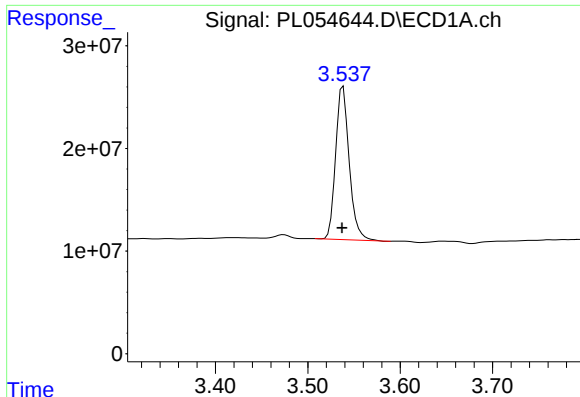


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: 0.001 min
Response: 151946187
Conc: 13.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-16-S


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:55 AM

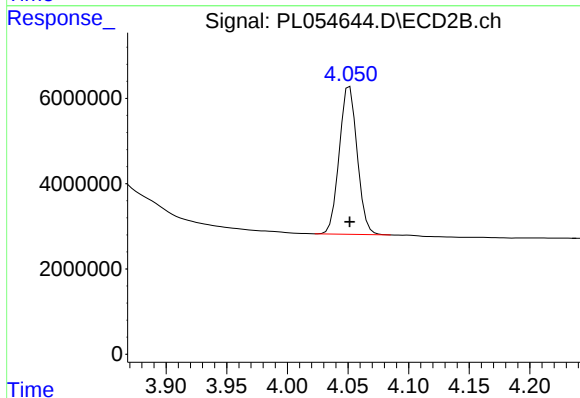


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 35678467
Conc: 13.98 ng/ml

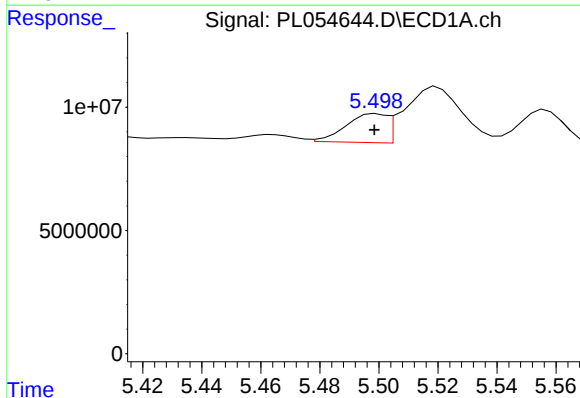


#10 gamma-Chlordane

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 11248321
Conc: 0.74 ng/ml

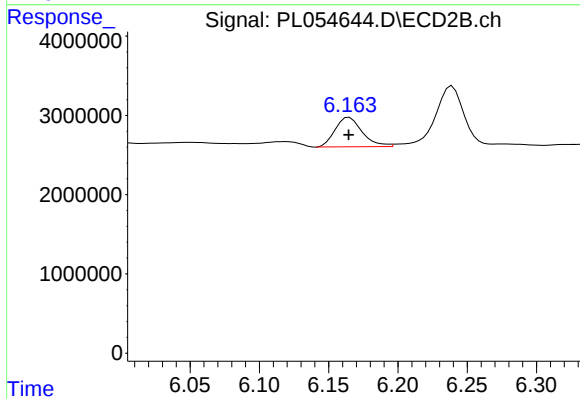

#10 gamma-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.000 min
Response: 5065456
Conc: 1.92 ng/ml

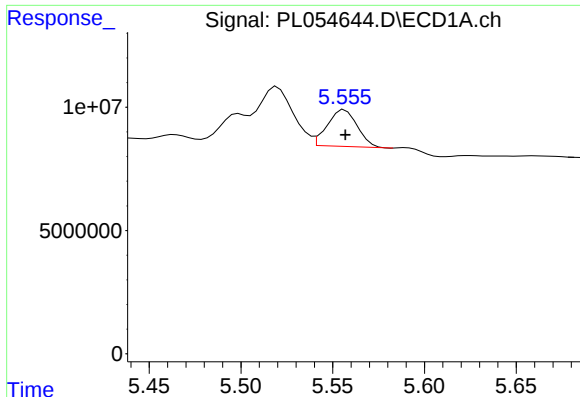


#11 alpha-Chlordane

R.T.: 5.557 min
Delta R.T.: 0.000 min
Response: 16893365
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-16-S


Manual Integrations
APPROVED

Ankita
11/27/2019 11:35:55 AM

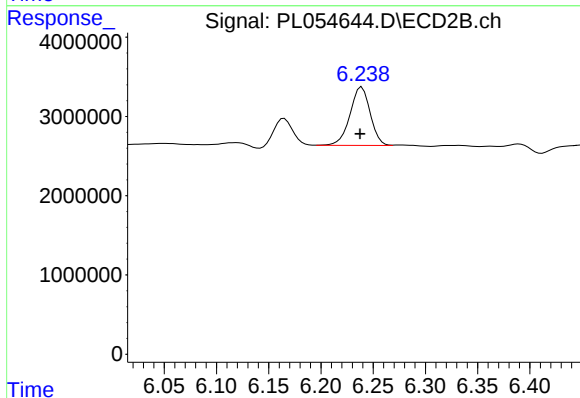


#11 alpha-Chlordane

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 9949178
Conc: 3.79 ng/ml m

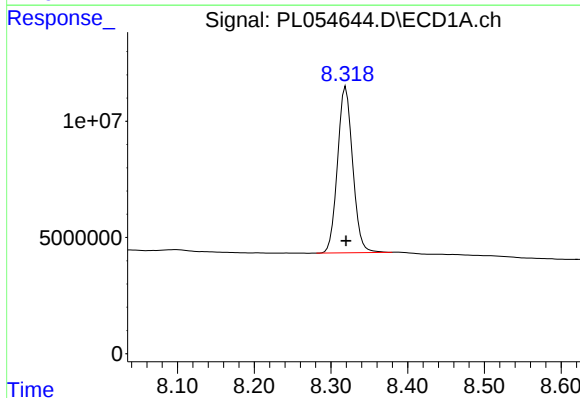

#28 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: 0.000 min
Response: 98094877
Conc: 10.24 ng/ml

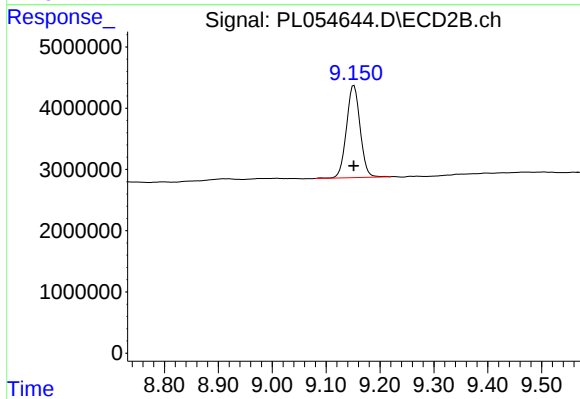

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 26506216
Conc: 11.06 ng/ml