

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
 Data File : PL042504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2018 10:44
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 27 12:22:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.102	126.7E6	65679996	21.539	22.836
28)	SA Decachlor...	8.209	9.239	118.6E6	47257281	18.821	19.594
Target Compounds							
2)	A alpha-BHC	0.000	4.451f	0	349471	N.D.	0.082 #
6)	B beta-BHC	4.402f	4.904f	3408352	341422	0.962	0.216 #
8)	B Heptachlo...	0.000	5.936f	0	1625946	N.D.	0.453 #
10)	B gamma-Chl...	5.368	0.000	2604442	0	0.342	N.D. #
23)	Chlordane-1	4.366	0.000	1815914	0	6.568	N.D. #
25)	Chlordane-3	5.368	0.000	2604442	0	2.971	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
Data File : PL042504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2018 10:44
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 27 12:22:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

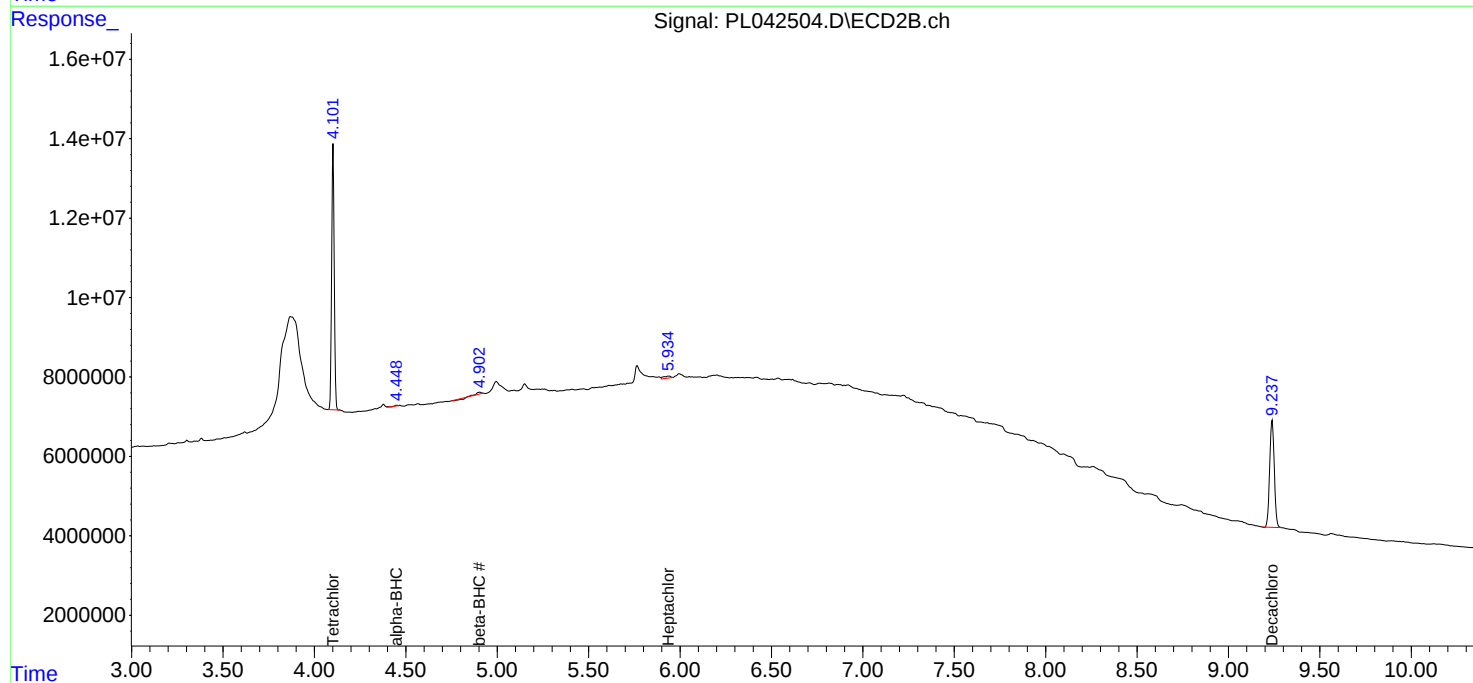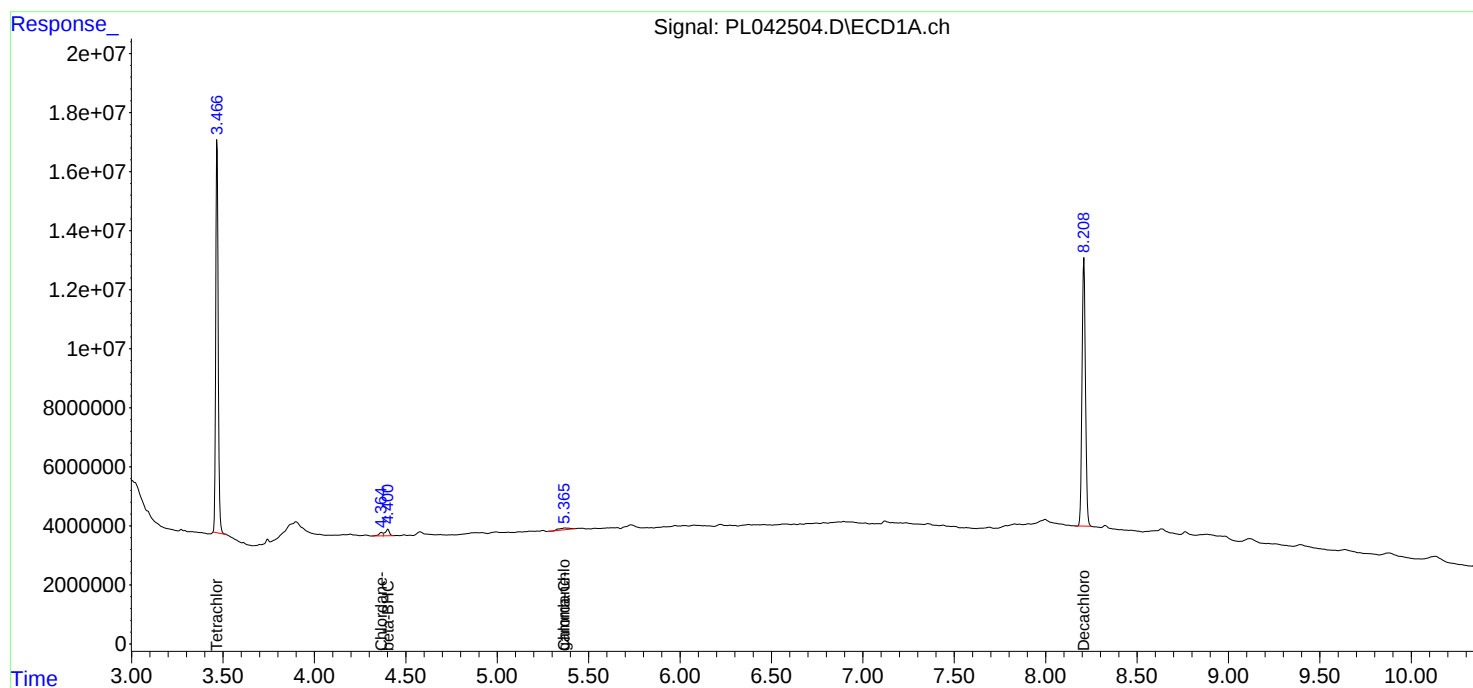


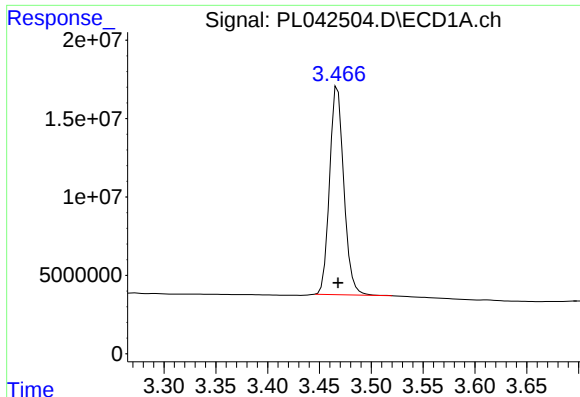

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 126726232
Conc: 21.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

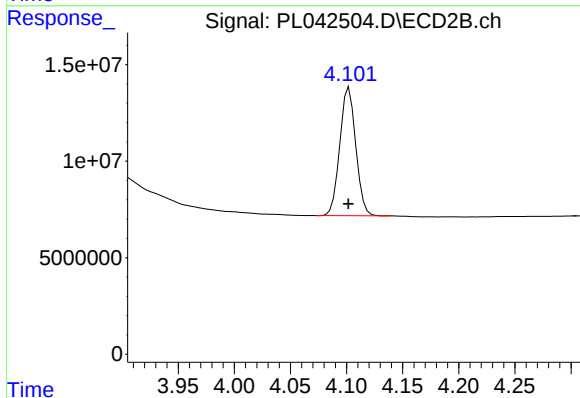


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 65679996
Conc: 22.84 ng/ml

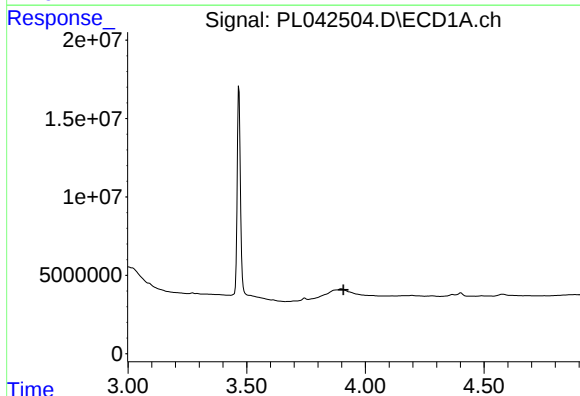


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

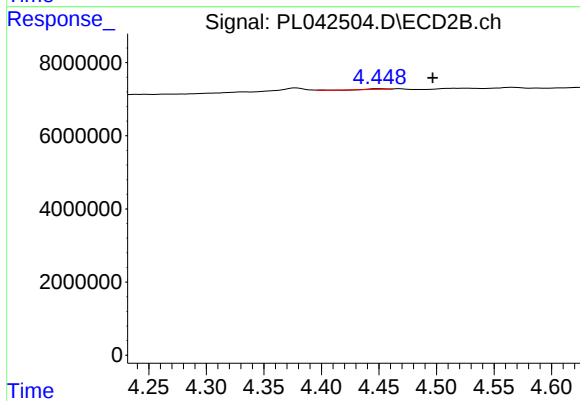

#2 alpha-BHC


R.T.: 4.451 min
Delta R.T.: -0.046 min
Response: 349471
Conc: 0.08 ng/ml

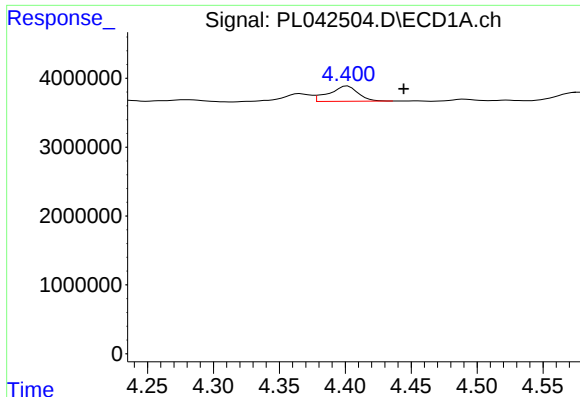

#6 beta-BHC


R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 3408352
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

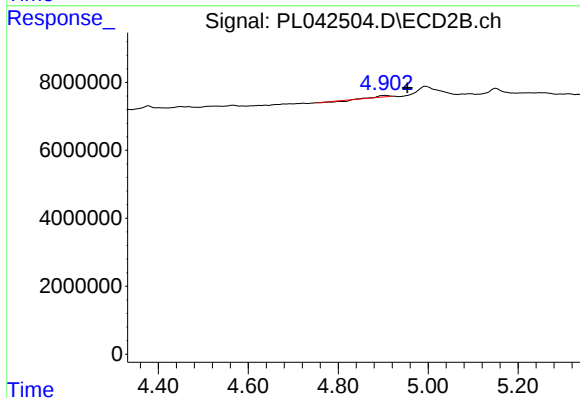


#6 beta-BHC

R.T.: 4.904 min
Delta R.T.: -0.049 min
Response: 341422
Conc: 0.22 ng/ml

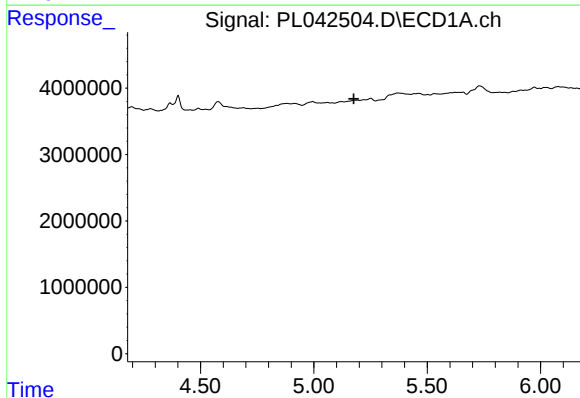


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

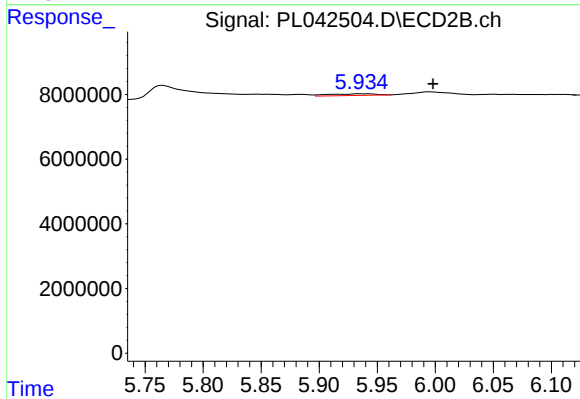

#8 Heptachlor epoxide


R.T.: 5.936 min
Delta R.T.: -0.063 min
Response: 1625946
Conc: 0.45 ng/ml

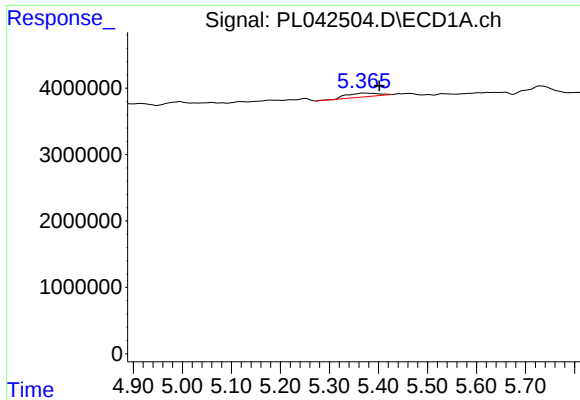

#10 gamma-Chlordane


R.T.: 5.368 min
Delta R.T.: -0.034 min
Response: 2604442
Conc: 0.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

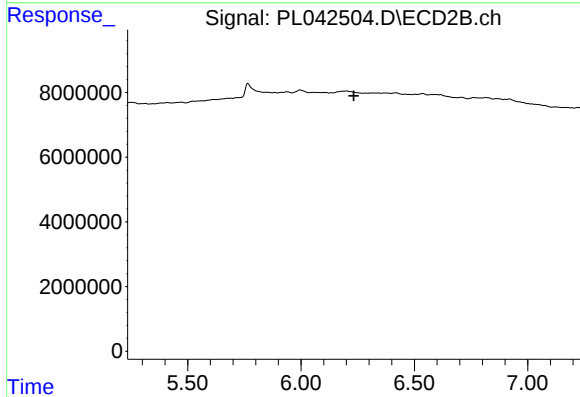


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

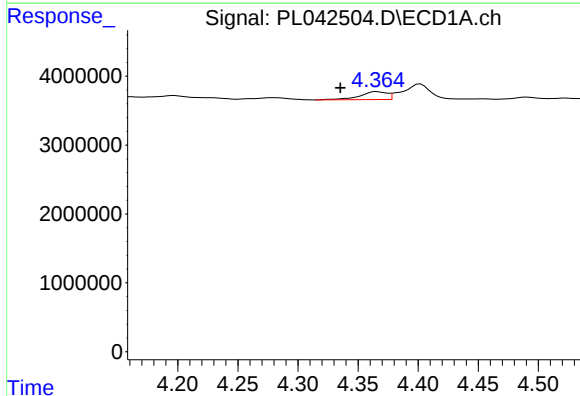


#23 Chlordane-1

R.T.: 4.366 min
Delta R.T.: 0.030 min
Response: 1815914
Conc: 6.57 ng/ml

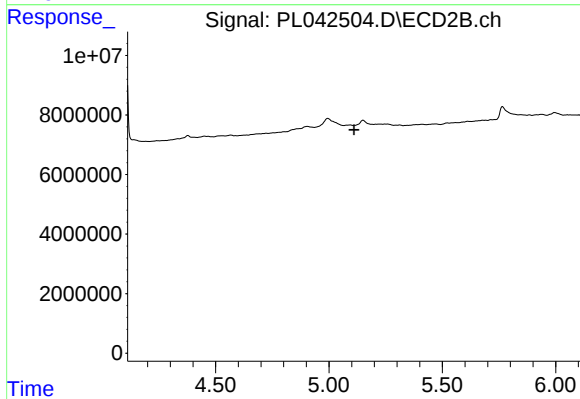

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

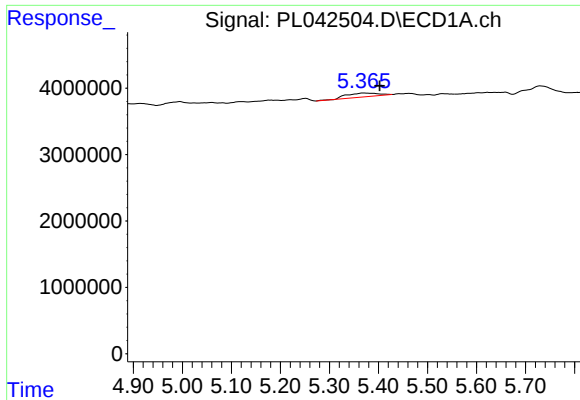

#25 Chlordane-3


R.T.: 5.368 min
Delta R.T.: -0.034 min
Response: 2604442
Conc: 2.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

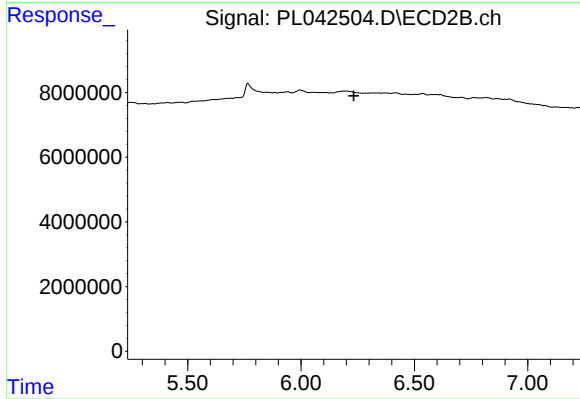


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.233 min
Response: 0
Conc: N.D.

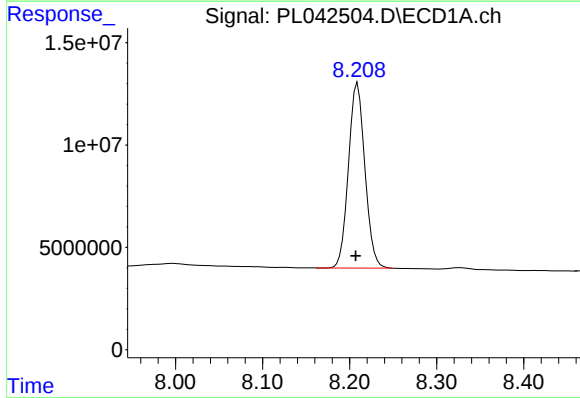

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 118609551
Conc: 18.82 ng/ml

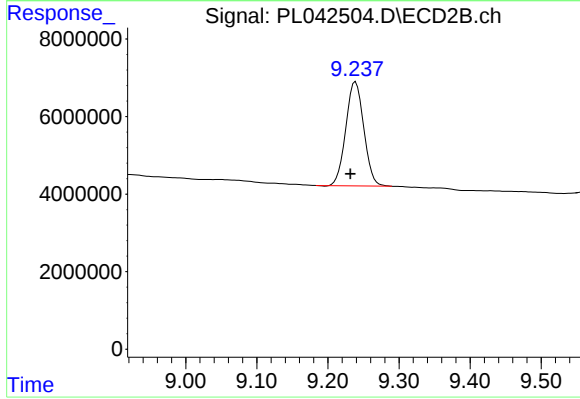

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 47257281
Conc: 19.59 ng/ml