

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
 Data File : PL042527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2018 21:18
 Operator : AJ\SJ
 Sample : PB115088TB
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 00:26:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.103	128.2E6	67928060	21.784	23.618
28)	SA Decachlor...	8.210	9.240	124.7E6	51155222	19.786	21.210
Target Compounds							
2)	A alpha-BHC	3.900	4.505	3536923	981425	0.392	0.229 #
6)	B beta-BHC	4.403f	0.000	7771025	0	2.193	N.D. #
8)	B Heptachlo...	0.000	5.999	0	1995237	N.D.	0.556 #
19)	B Endosulfa...	0.000	7.389	0	2603276	N.D.	0.936 #
20)	A Methoxychlor	0.000	7.652f	0	3590550	N.D.	2.633 #
23)	Chlordane-1	4.366	0.000	1913189	0	6.920	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
Data File : PL042527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2018 21:18
Operator : AJ\SJ
Sample : PB115088TB
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 00:26:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

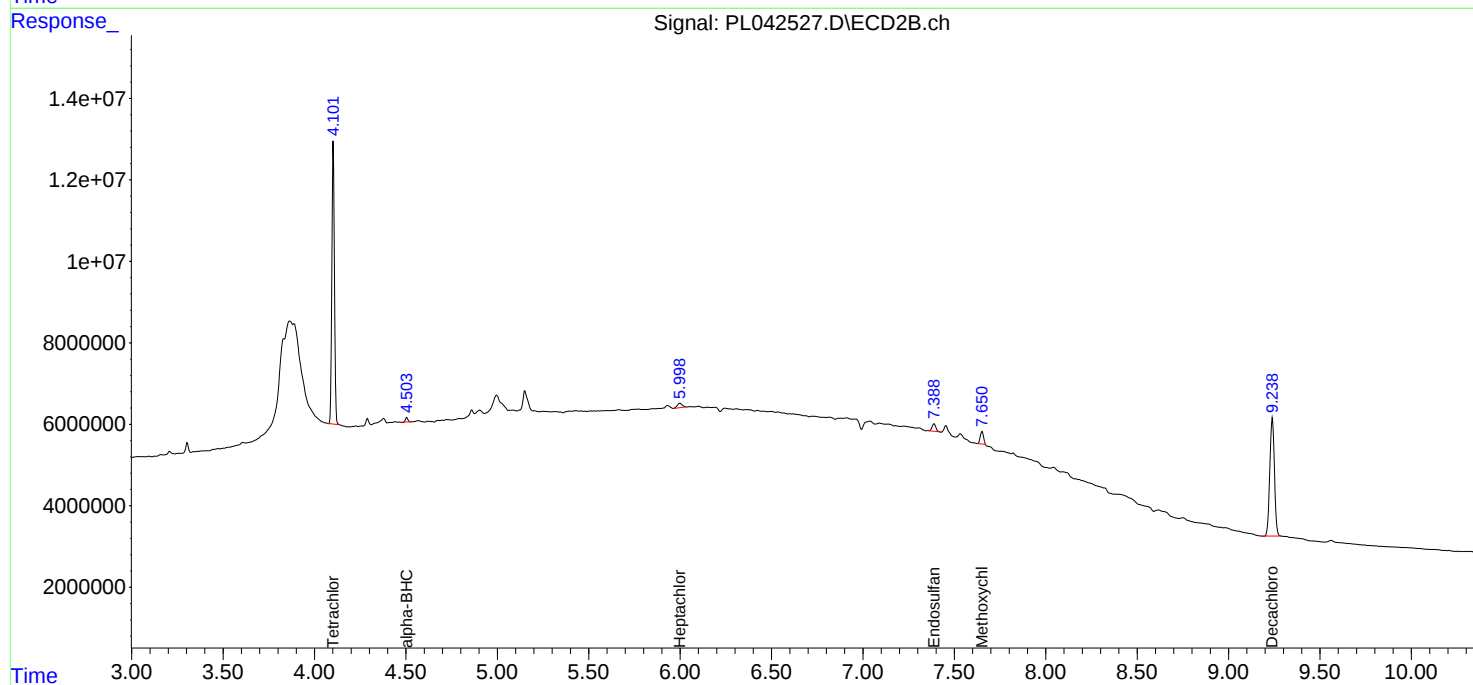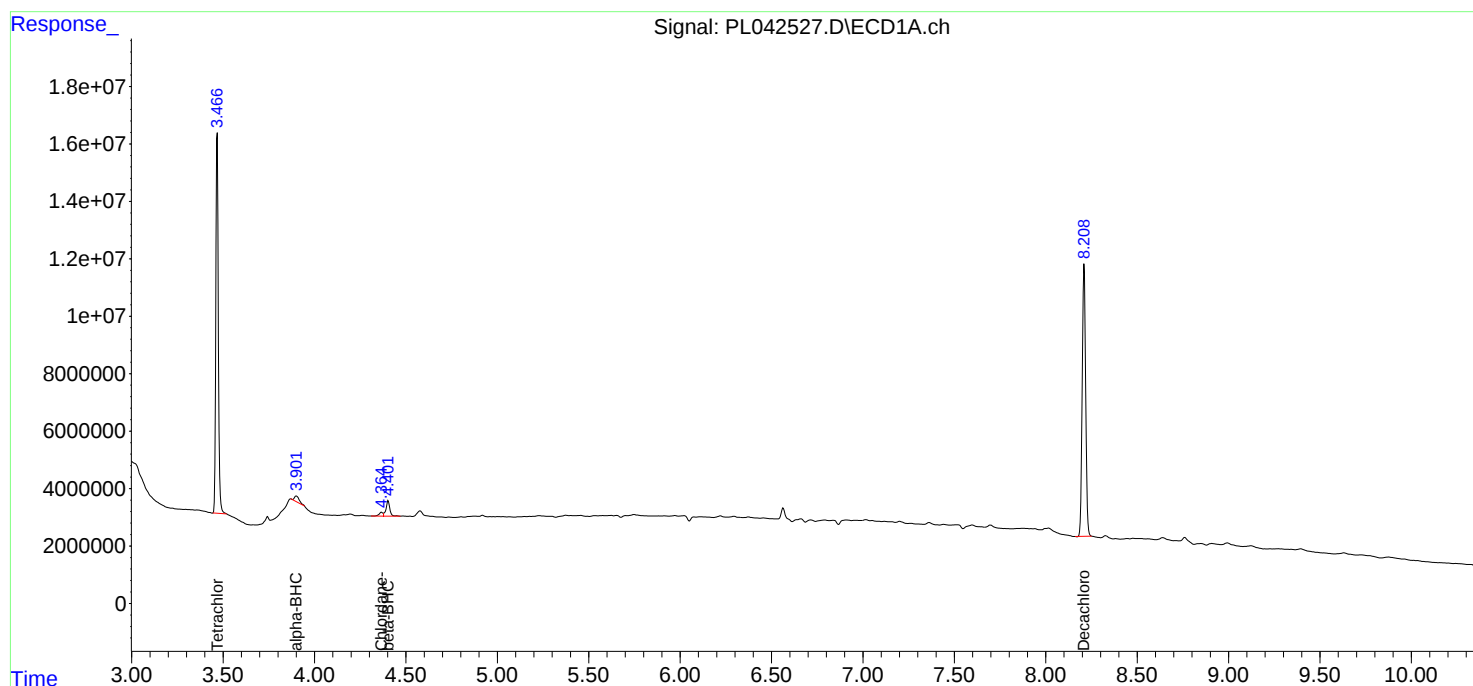


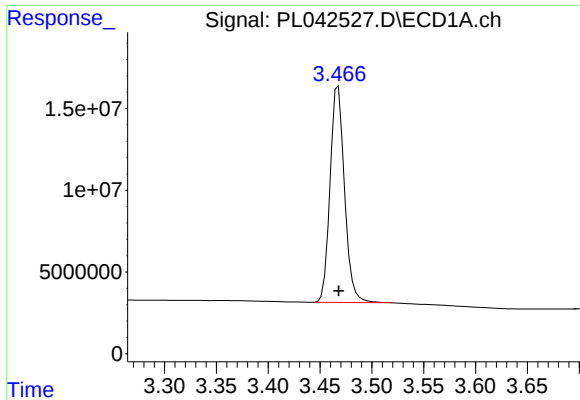

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 128165119
Conc: 21.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

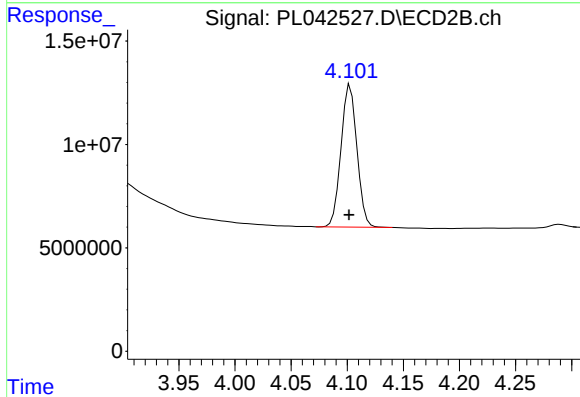


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 67928060
Conc: 23.62 ng/ml

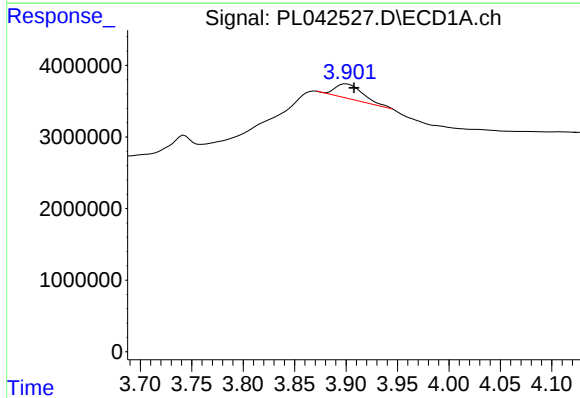


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: -0.008 min
Response: 3536923
Conc: 0.39 ng/ml

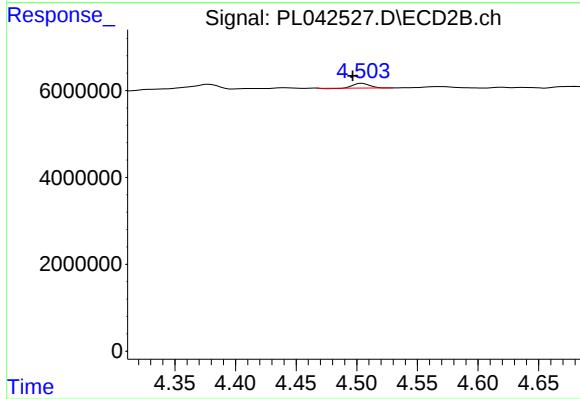

#2 alpha-BHC


R.T.: 4.505 min
Delta R.T.: 0.008 min
Response: 981425
Conc: 0.23 ng/ml

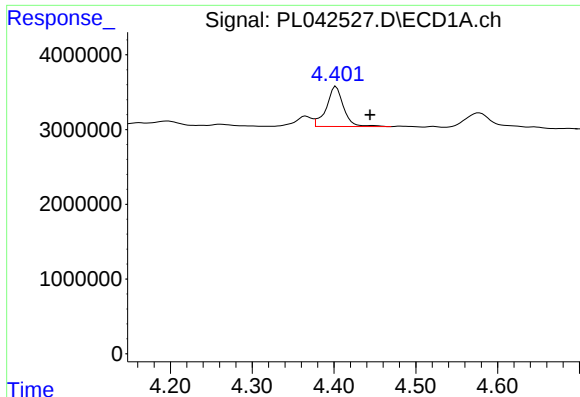

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: -0.042 min
Response: 7771025
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

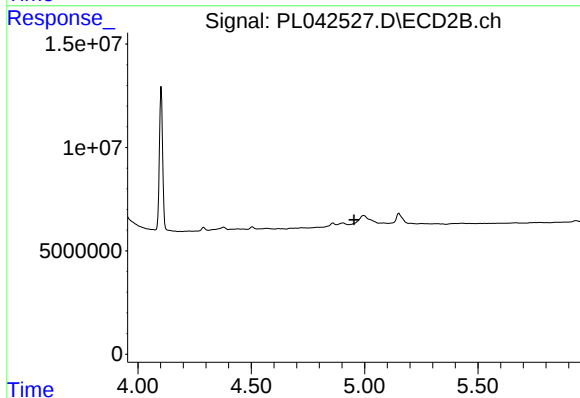


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

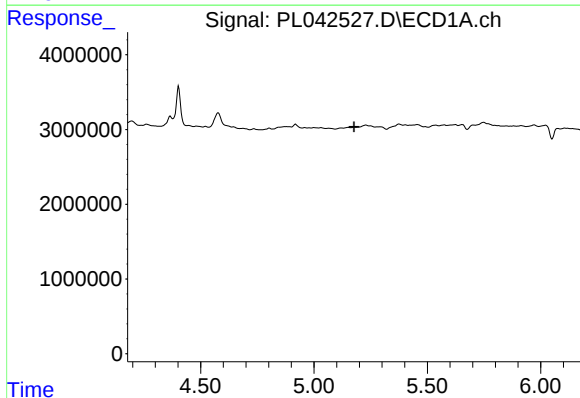


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

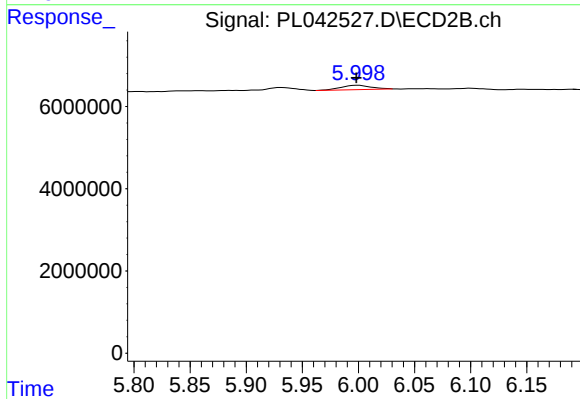

#8 Heptachlor epoxide


R.T.: 5.999 min
Delta R.T.: 0.001 min
Response: 1995237
Conc: 0.56 ng/ml

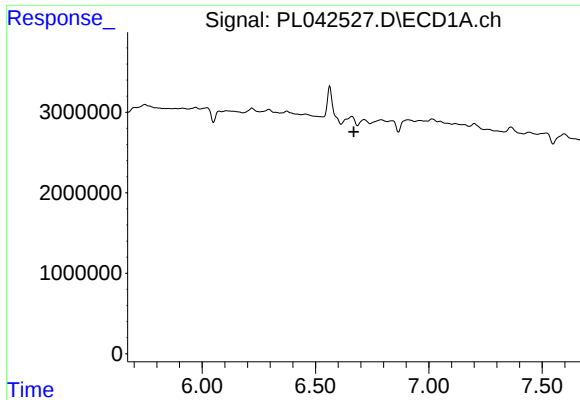

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

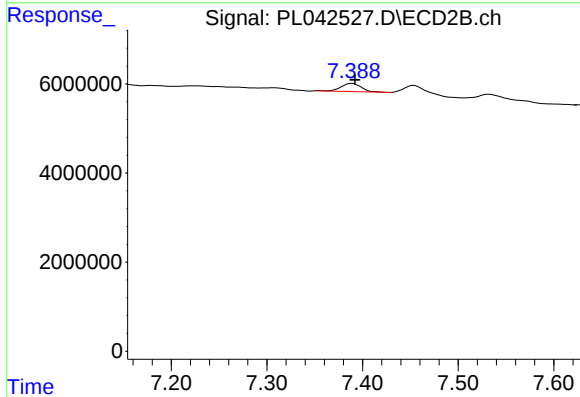


#19 Endosulfan Sulfate

R.T.: 7.389 min
Delta R.T.: -0.003 min
Response: 2603276
Conc: 0.94 ng/ml

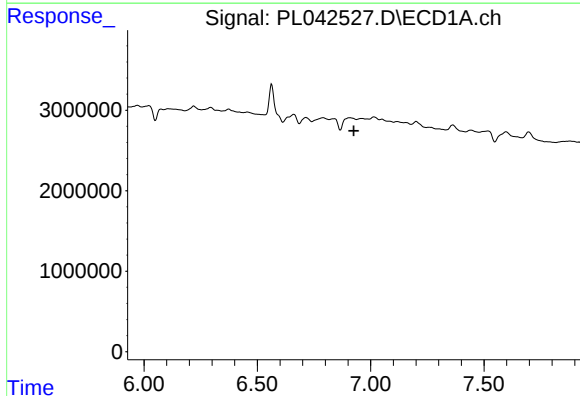


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.926 min
Response: 0
Conc: N.D.

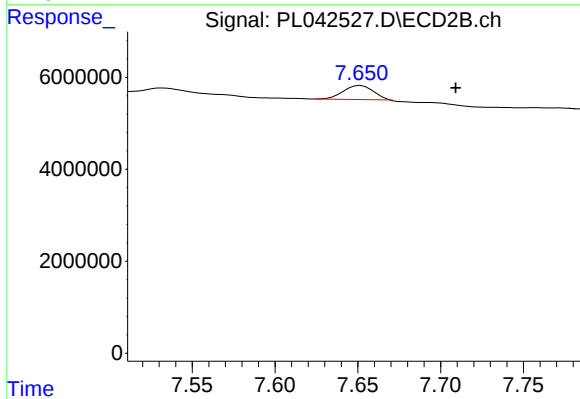

#20 Methoxychlor


R.T.: 7.652 min
Delta R.T.: -0.057 min
Response: 3590550
Conc: 2.63 ng/ml

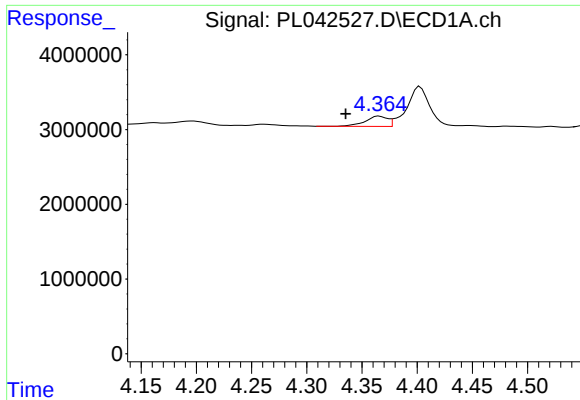

#23 Chlordane-1


R.T.: 4.366 min
Delta R.T.: 0.030 min
Response: 1913189
Conc: 6.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

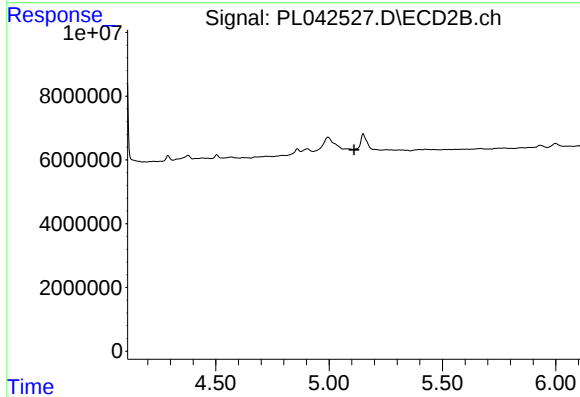


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

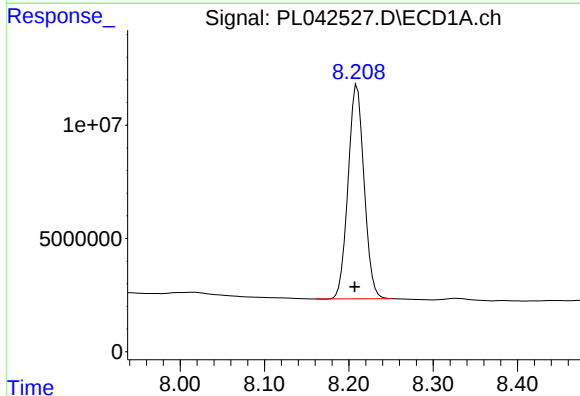

#28 Decachlorobiphenyl

R.T.: 8.210 min
Delta R.T.: 0.003 min
Response: 124692151
Conc: 19.79 ng/ml

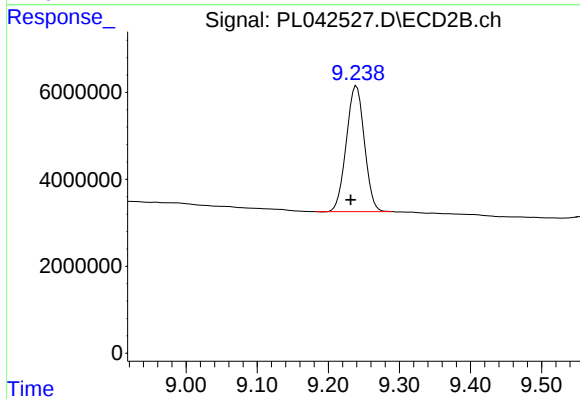

#28 Decachlorobiphenyl

R.T.: 9.240 min
Delta R.T.: 0.008 min
Response: 51155222
Conc: 21.21 ng/ml