

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
 Data File : PL042528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2018 21:32
 Operator : AJ\SJ
 Sample : J5770-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 00:26:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.103	111.6E6	59101543	18.969	20.549
28)	SA Decachlor...	8.209	9.239	111.2E6	45877314	17.640	19.022
Target Compounds							
2)	A alpha-BHC	0.000	4.448f	0	200281	N.D.	0.047 #
3)	MA gamma-BHC...	4.199	0.000	1419370	0	0.172	N.D. #
6)	B beta-BHC	4.402f	4.904f	24886576	1250471	7.025	0.793 #
8)	B Heptachlo...	5.245f	6.000	4523057	2773252	0.597	0.773 #
9)	A Endosulfan I	5.525	0.000	3359164	0	0.485	N.D. #
11)	B alpha-Chl...	5.525f	0.000	3359164	0	0.447	N.D. #
13)	MA Dieldrin	5.742	0.000	2918833	0	0.397	N.D. #
23)	Chlordane-1	4.402	0.000	24886576	0	90.014	N.D. #
26)	Chlordane-4	5.525	0.000	3359164	0	4.426	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
Data File : PL042528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2018 21:32
Operator : AJ\SJ
Sample : J5770-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 00:26:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

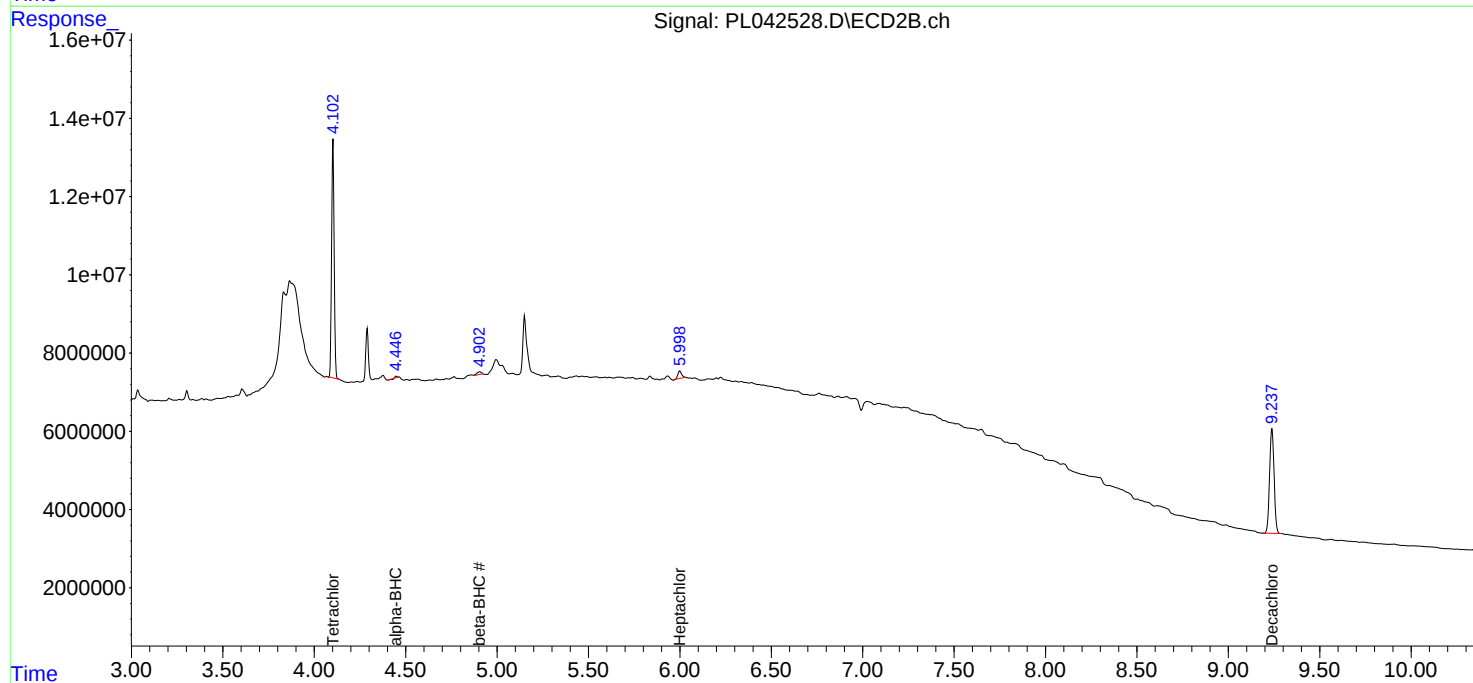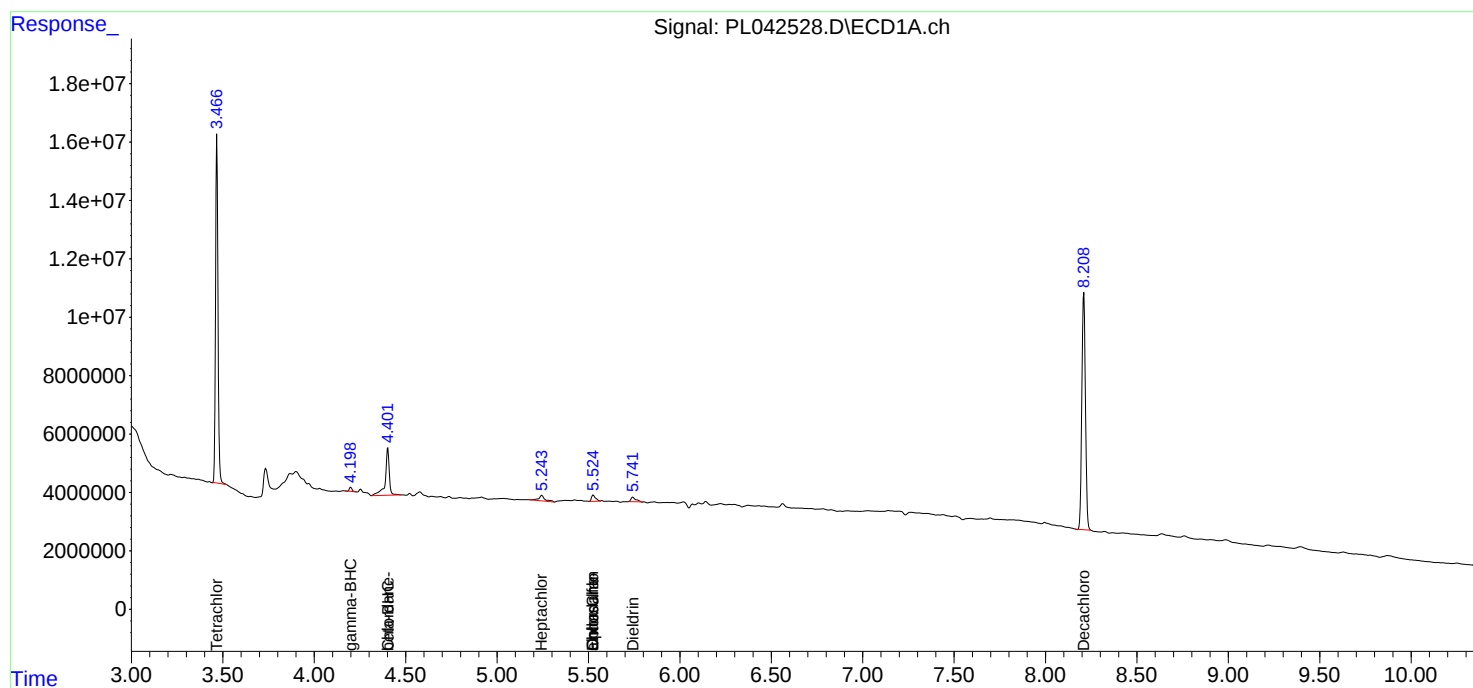


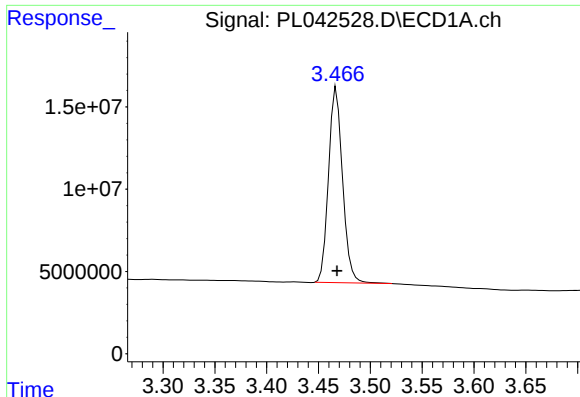

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 111600913
Conc: 18.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

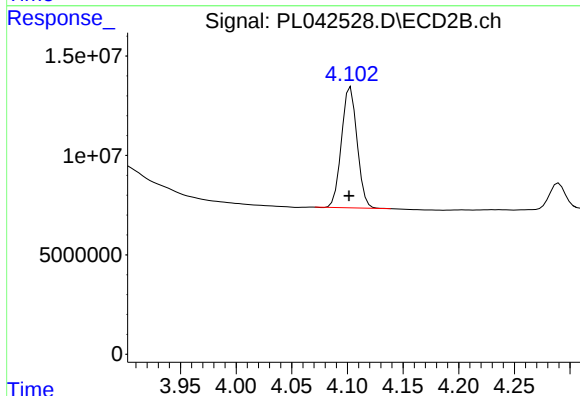


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 59101543
Conc: 20.55 ng/ml

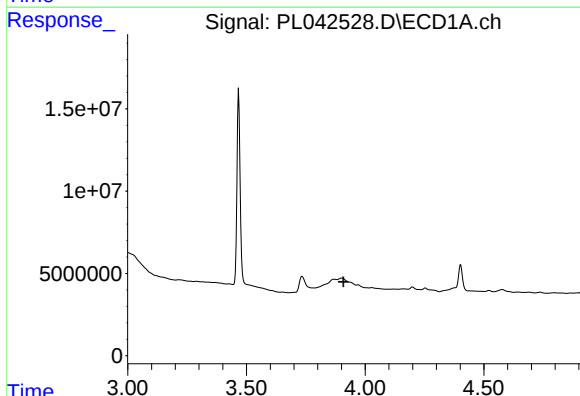


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.908 min
Response: 0
Conc: N.D.

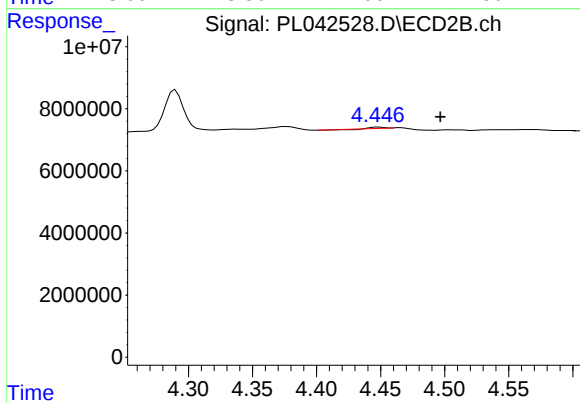

#2 alpha-BHC


R.T.: 4.448 min
Delta R.T.: -0.048 min
Response: 200281
Conc: 0.05 ng/ml

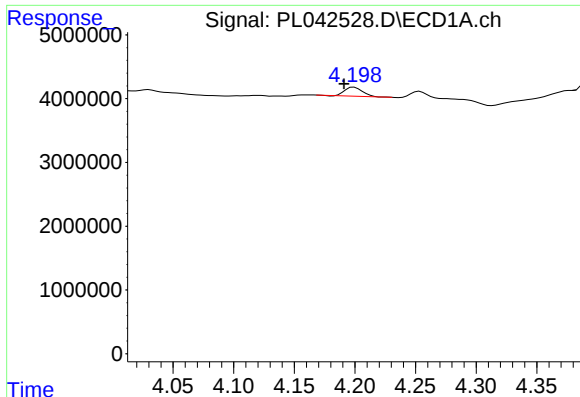

#3 gamma-BHC (Lindane)


R.T.: 4.199 min
Delta R.T.: 0.008 min
Response: 1419370
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

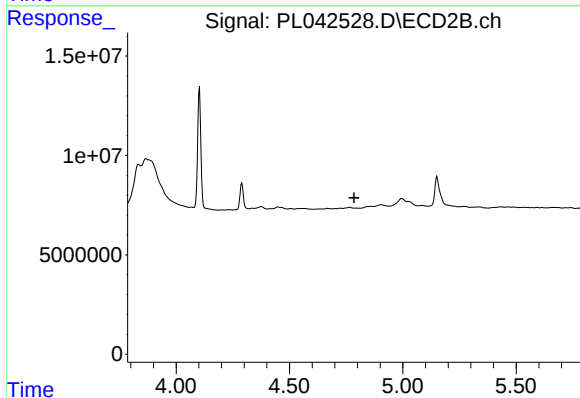


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

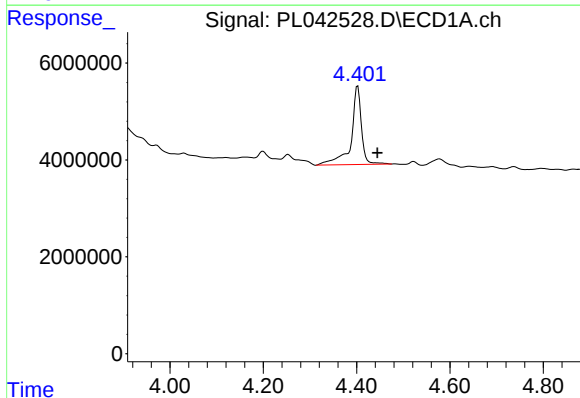


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 24886576
Conc: 7.02 ng/ml

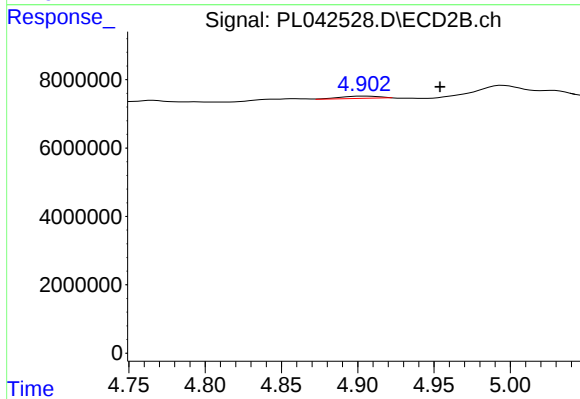

#6 beta-BHC


R.T.: 4.904 min
Delta R.T.: -0.050 min
Response: 1250471
Conc: 0.79 ng/ml

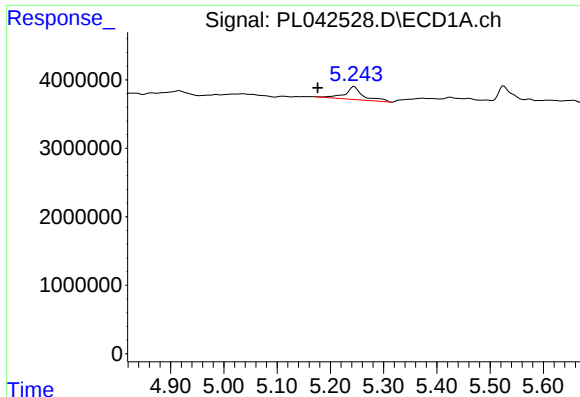

#8 Heptachlor epoxide


R.T.: 5.245 min
Delta R.T.: 0.068 min
Response: 4523057
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

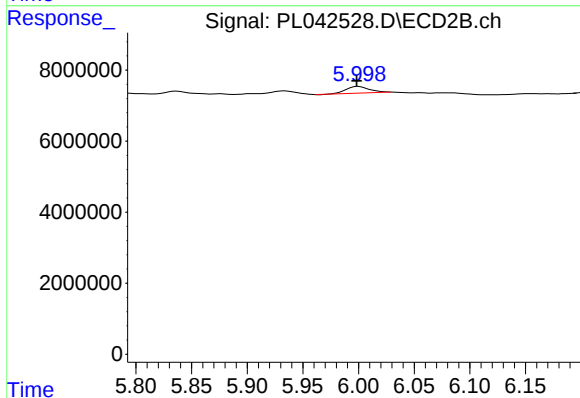


#8 Heptachlor epoxide

R.T.: 6.000 min
Delta R.T.: 0.001 min
Response: 2773252
Conc: 0.77 ng/ml

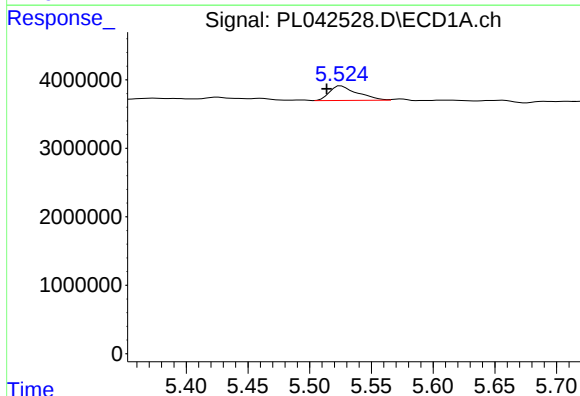


#9 Endosulfan I

R.T.: 5.525 min
Delta R.T.: 0.012 min
Response: 3359164
Conc: 0.49 ng/ml

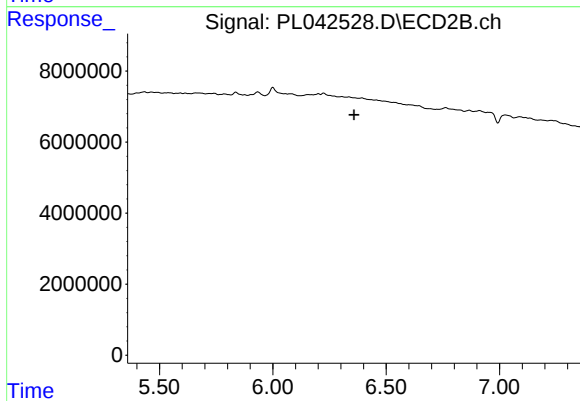

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.358 min
Response: 0
Conc: N.D.

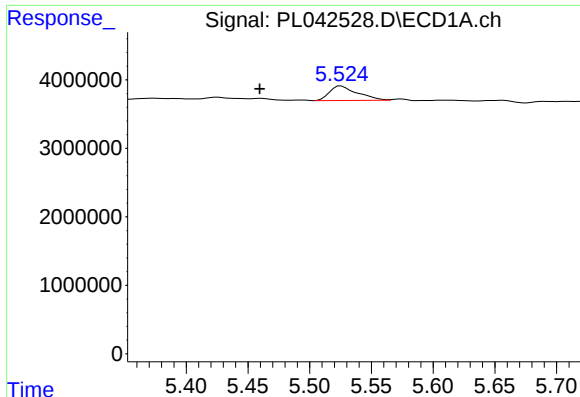

#11 alpha-Chlordane


R.T.: 5.525 min
Delta R.T.: 0.066 min
Response: 3359164
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

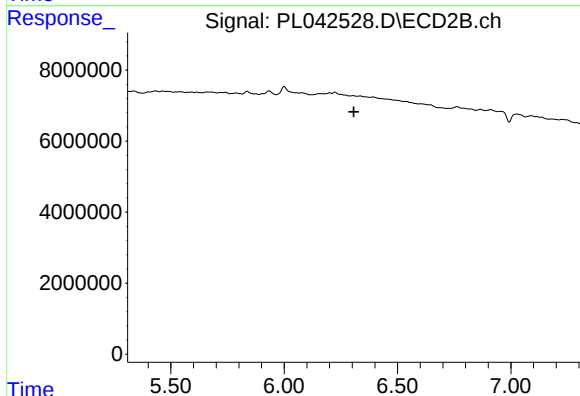


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

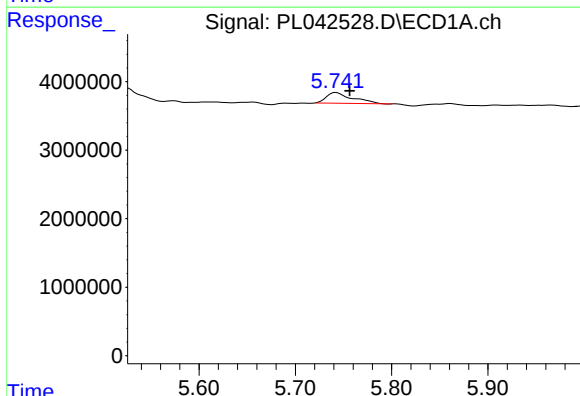


#13 Dieldrin

R.T.: 5.742 min
Delta R.T.: -0.014 min
Response: 2918833
Conc: 0.40 ng/ml

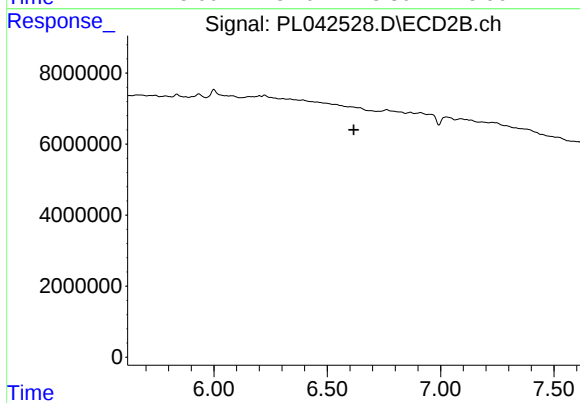

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

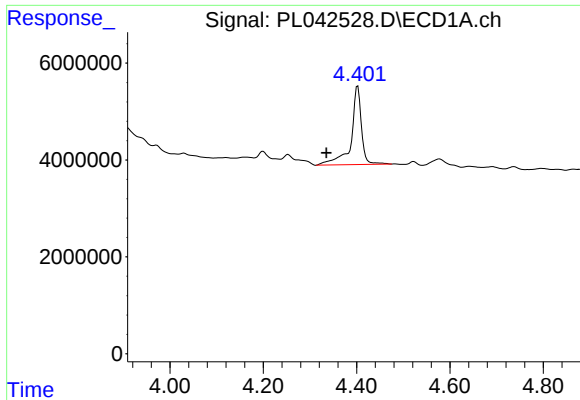

#23 Chlordane-1


R.T.: 4.402 min
Delta R.T.: 0.067 min
Response: 24886576
Conc: 90.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

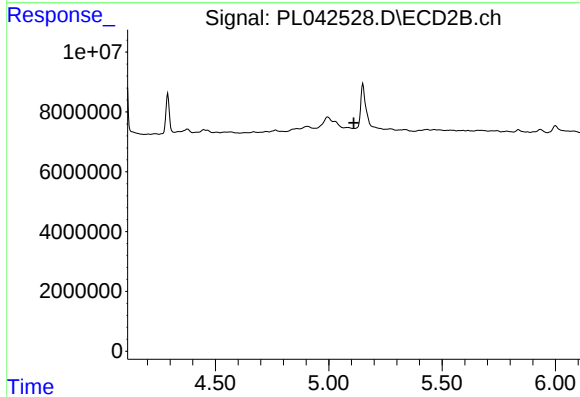


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

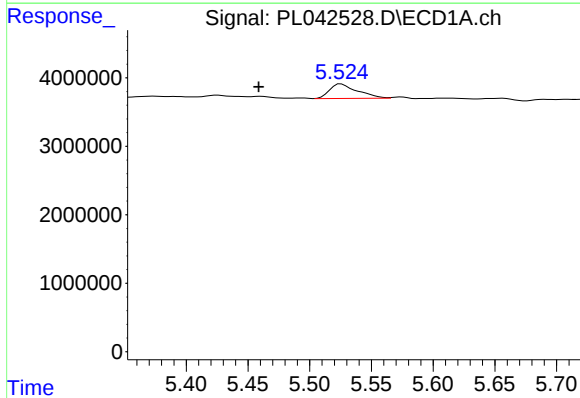


#26 Chlordane-4

R.T.: 5.525 min
Delta R.T.: 0.067 min
Response: 3359164
Conc: 4.43 ng/ml

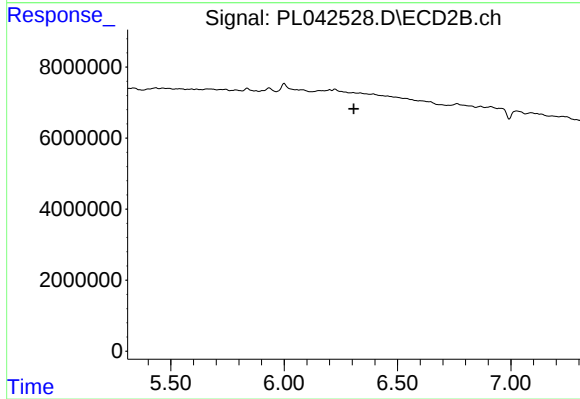

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

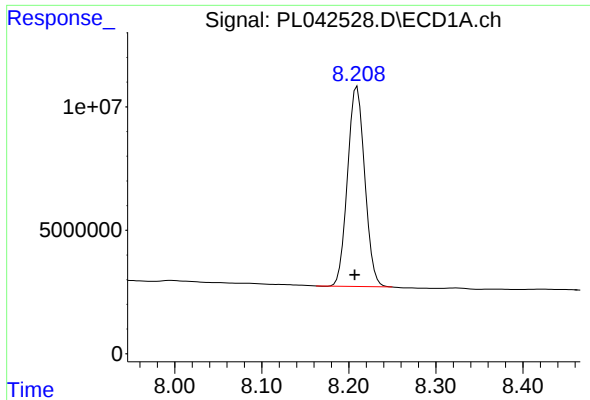

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.003 min
Response: 111171405
Conc: 17.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

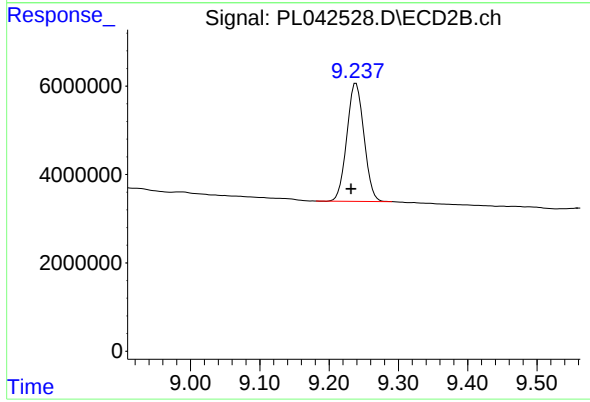

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 45877314
Conc: 19.02 ng/ml