

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
 Data File : PL042532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2018 22:29
 Operator : AJ\SJ
 Sample : J5774-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 00:27:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.468	4.103	116.8E6	61532694	19.860	21.394
28)	SA Decachlor...	8.209	9.239	114.2E6	46923426	18.113	19.455
Target Compounds							
6)	B beta-BHC	4.402f	4.905f	11149895	1525952	3.147	0.967 #
8)	B Heptachlo...	0.000	5.998	0	2065472	N.D.	0.576 #
13)	MA Dieldrin	5.744	0.000	2277548	0	0.310	N.D. #
15)	B Endosulfa...	6.235f	0.000	1931705	0	0.309	N.D. #
23)	Chlordane-1	4.402	0.000	11149895	0	40.329	N.D. #
27)	Chlordane-5	6.235	0.000	1931705	0	6.483	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112718\
Data File : PL042532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2018 22:29
Operator : AJ\SJ
Sample : J5774-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 00:27:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

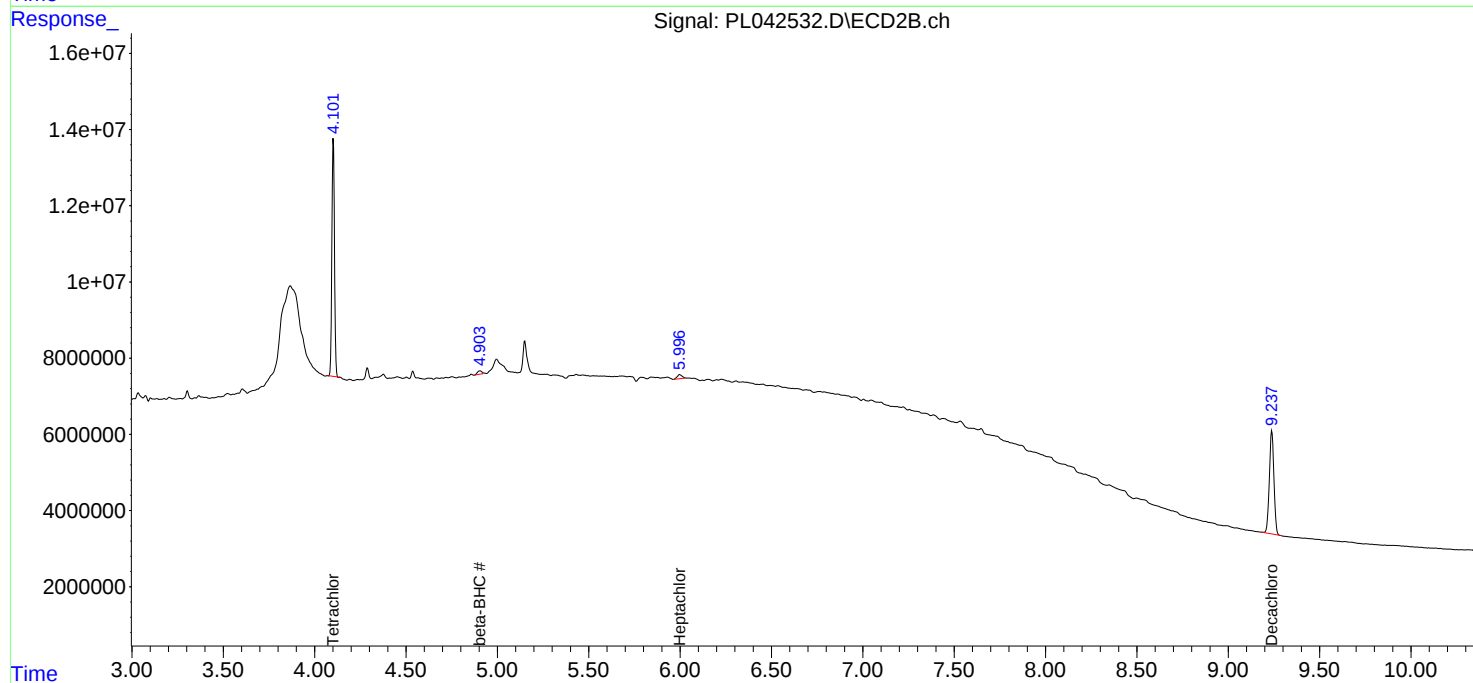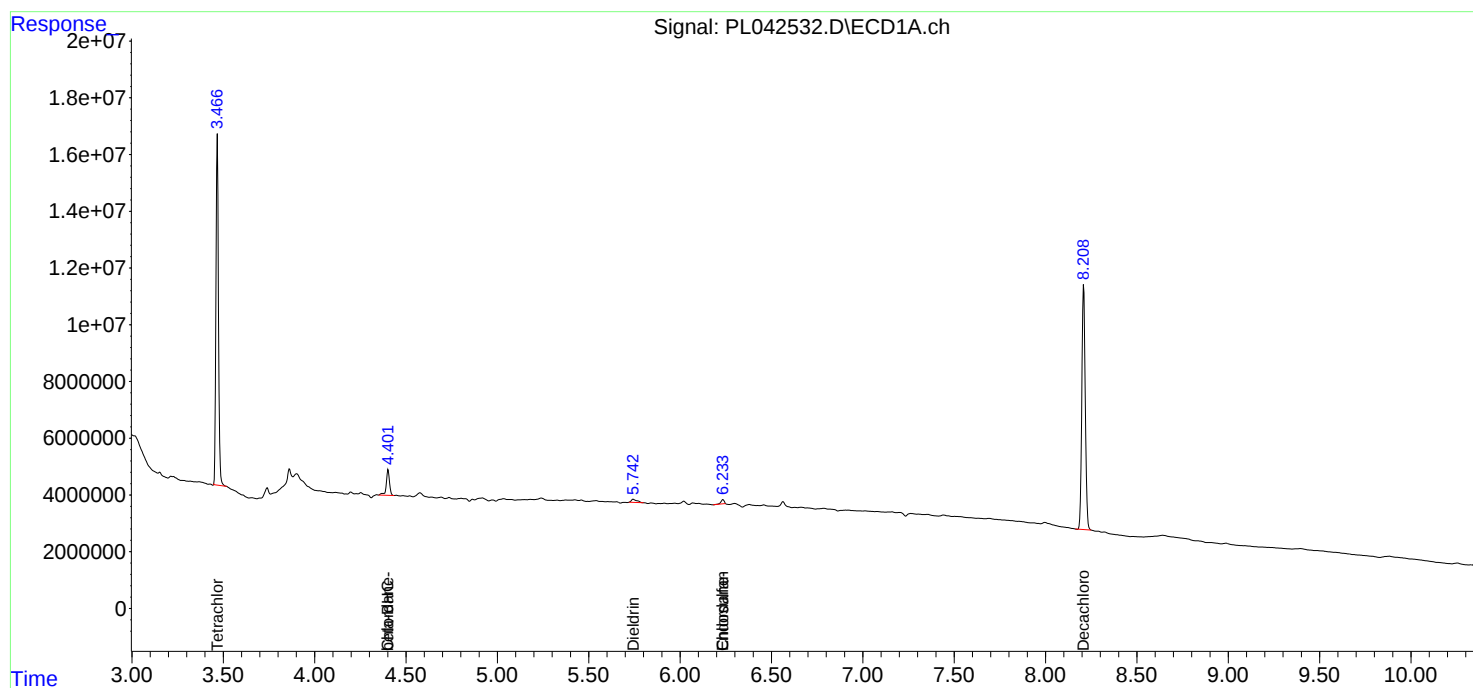


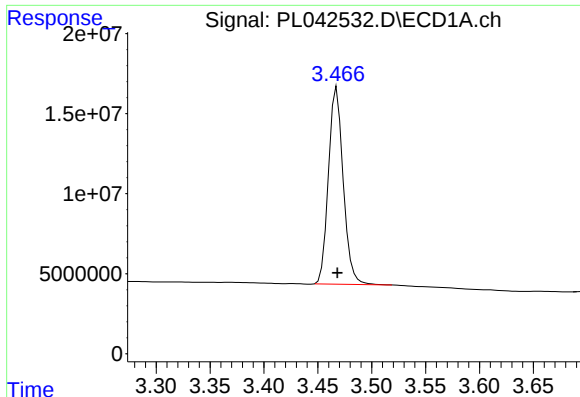

#1 Tetrachloro-m-xylene


R.T.: 3.468 min
Delta R.T.: 0.000 min
Response: 116844040
Conc: 19.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

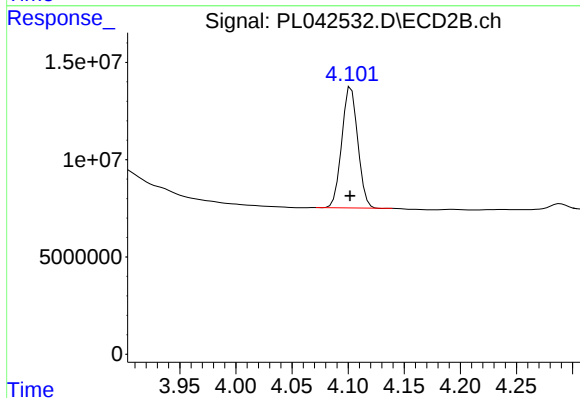


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.001 min
Response: 61532694
Conc: 21.39 ng/ml

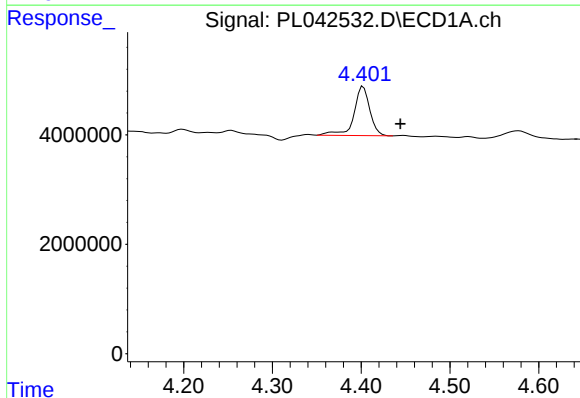


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 11149895
Conc: 3.15 ng/ml

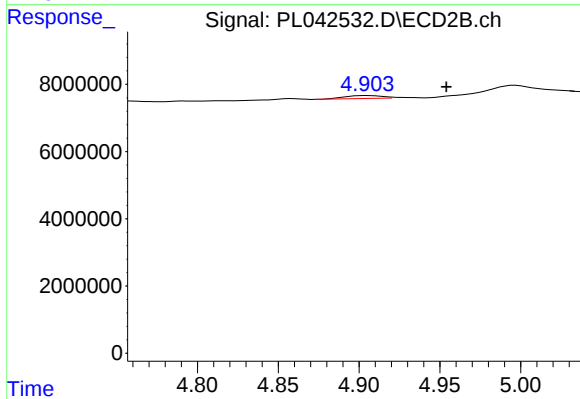

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.049 min
Response: 1525952
Conc: 0.97 ng/ml

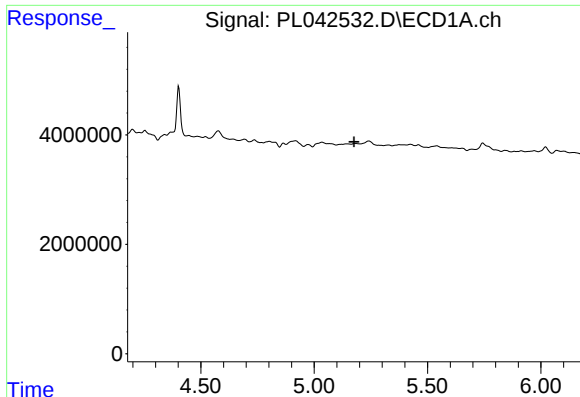

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

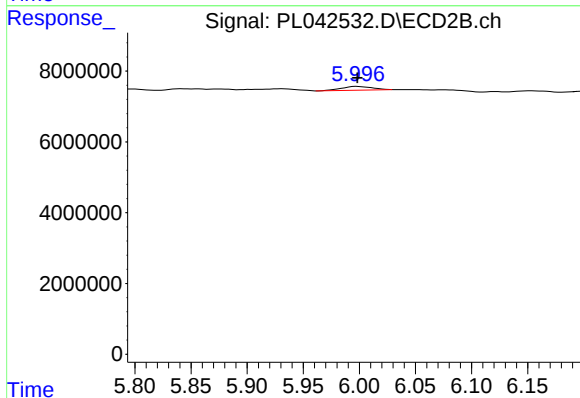


#8 Heptachlor epoxide

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 2065472
Conc: 0.58 ng/ml

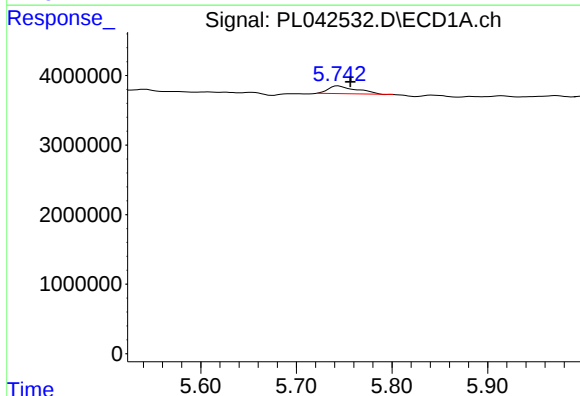


#13 Dieldrin

R.T.: 5.744 min
Delta R.T.: -0.013 min
Response: 2277548
Conc: 0.31 ng/ml

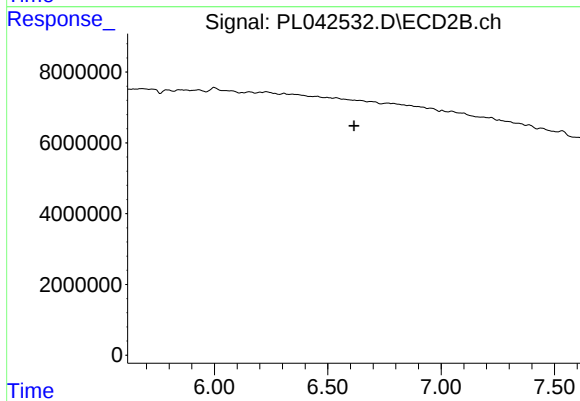

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

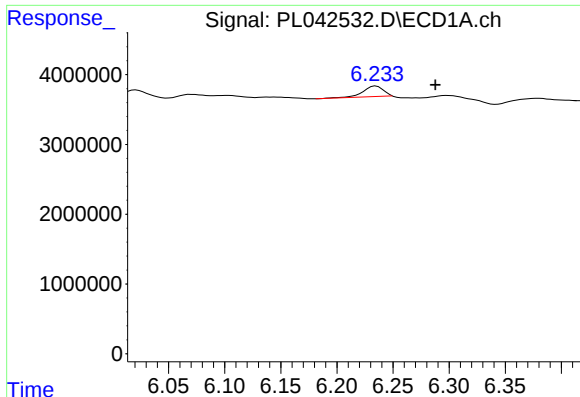

#15 Endosulfan II


R.T.: 6.235 min
Delta R.T.: -0.053 min
Response: 1931705
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

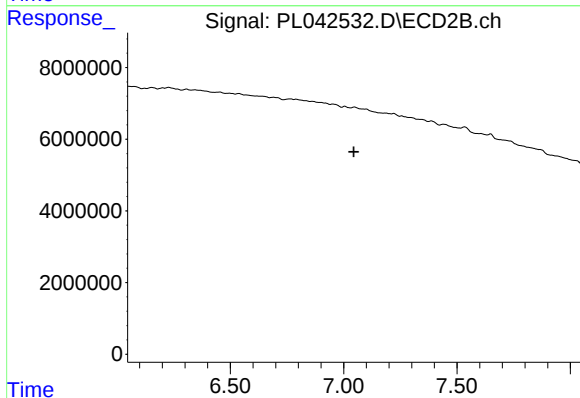


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

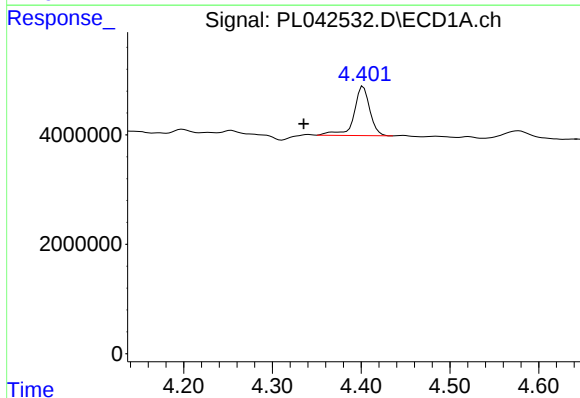


#23 Chlordane-1

R.T.: 4.402 min
Delta R.T.: 0.067 min
Response: 11149895
Conc: 40.33 ng/ml

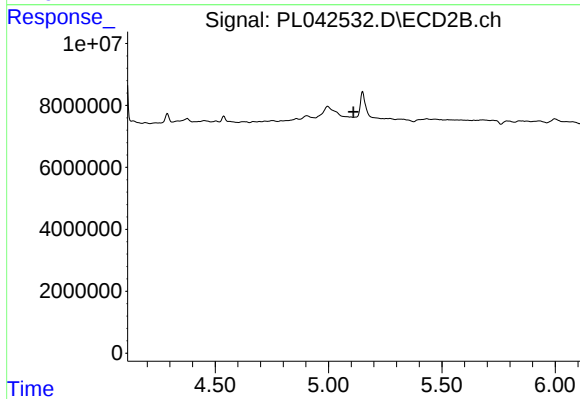

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

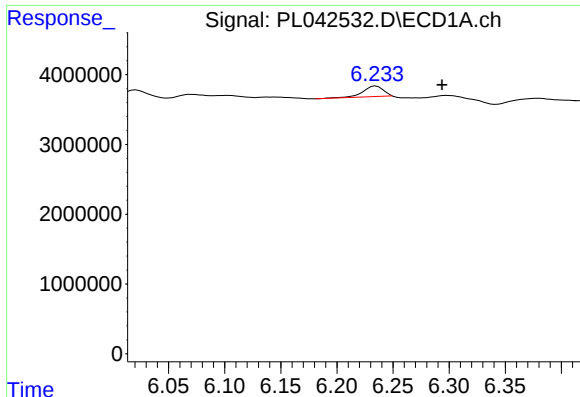

#27 Chlordane-5


R.T.: 6.235 min
Delta R.T.: -0.059 min
Response: 1931705
Conc: 6.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

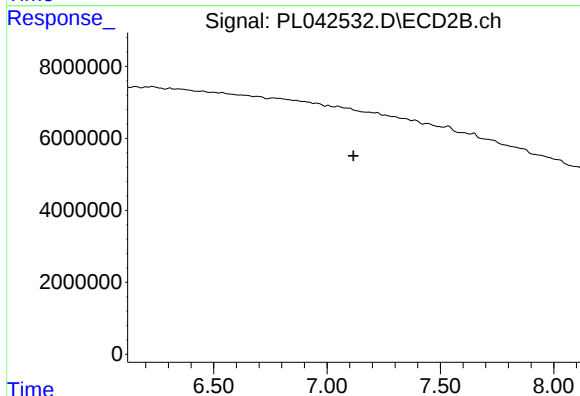


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

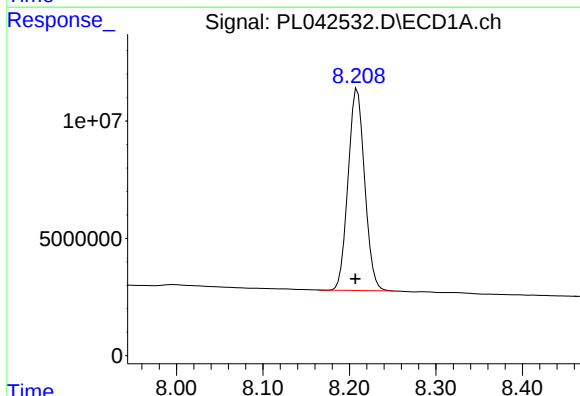

#28 Decachlorobiphenyl

R.T.: 8.209 min
Delta R.T.: 0.002 min
Response: 114150861
Conc: 18.11 ng/ml

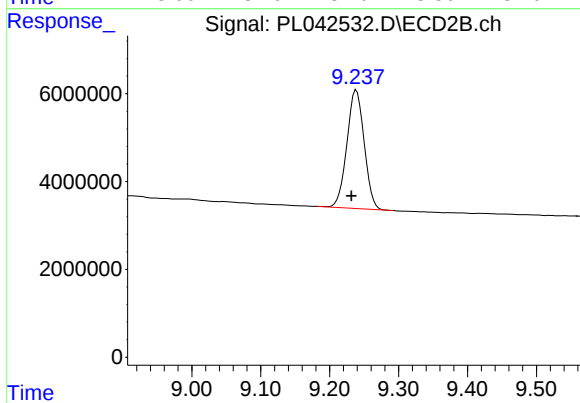

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 46923426
Conc: 19.46 ng/ml