

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112719\
 Data File : PL054691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Nov 2019 12:42
 Operator : SG\AJ
 Sample : K6016-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-627

Manual Integrations
 APPROVED

Ankita
 12/2/2019 1:11:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 28 00:14:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 27 01:19:55 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	4.050	782.5E6	64380154	67.261	25.229m#
28)	SA Decachlor...	8.320	9.152	62401615	18406781	6.516	7.678m
Target Compounds							
4)	MA Heptachlor	4.579	5.235	152.8E6	52774367	8.666	17.487m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112719\
Data File : PL054691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Nov 2019 12:42
Operator : SG\AJ
Sample : K6016-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
12/2/2019 1:11:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 28 00:14:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112619.M
Quant Title : GC Extractables
QLast Update : Wed Nov 27 01:19:55 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

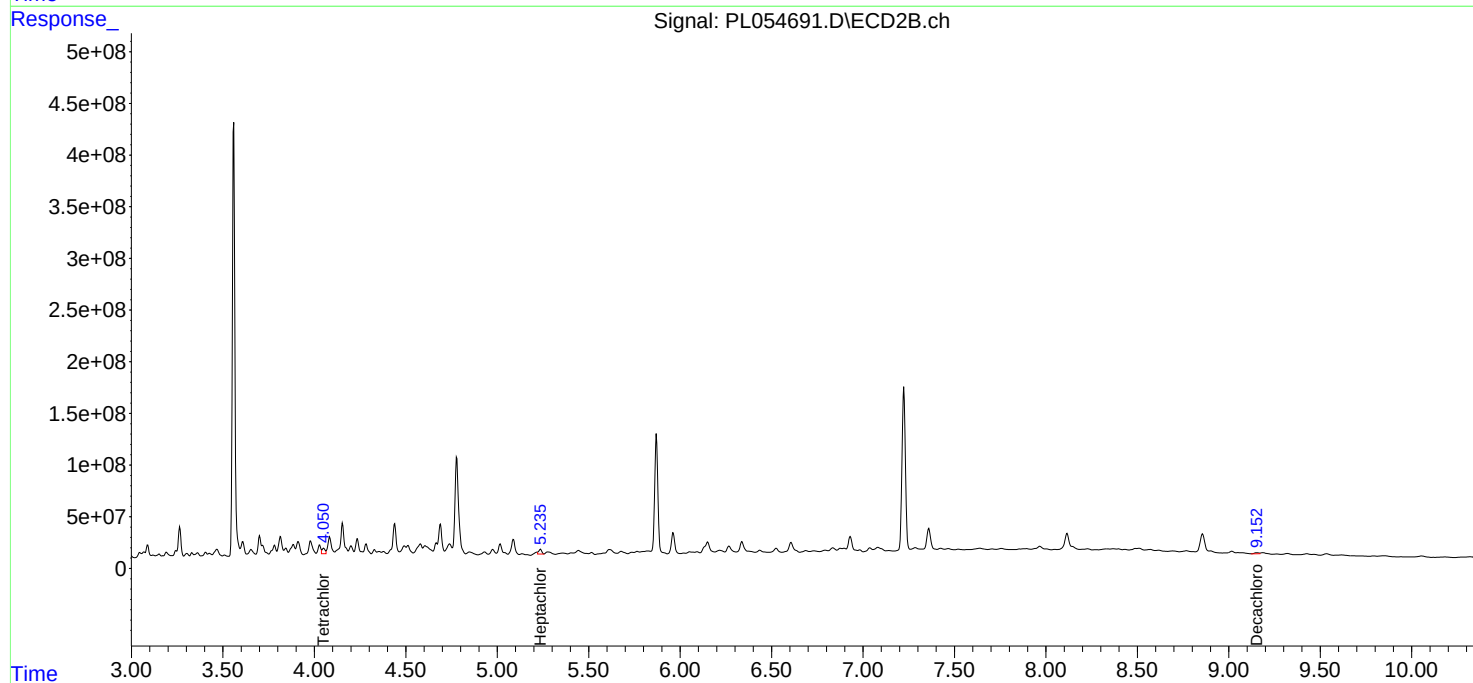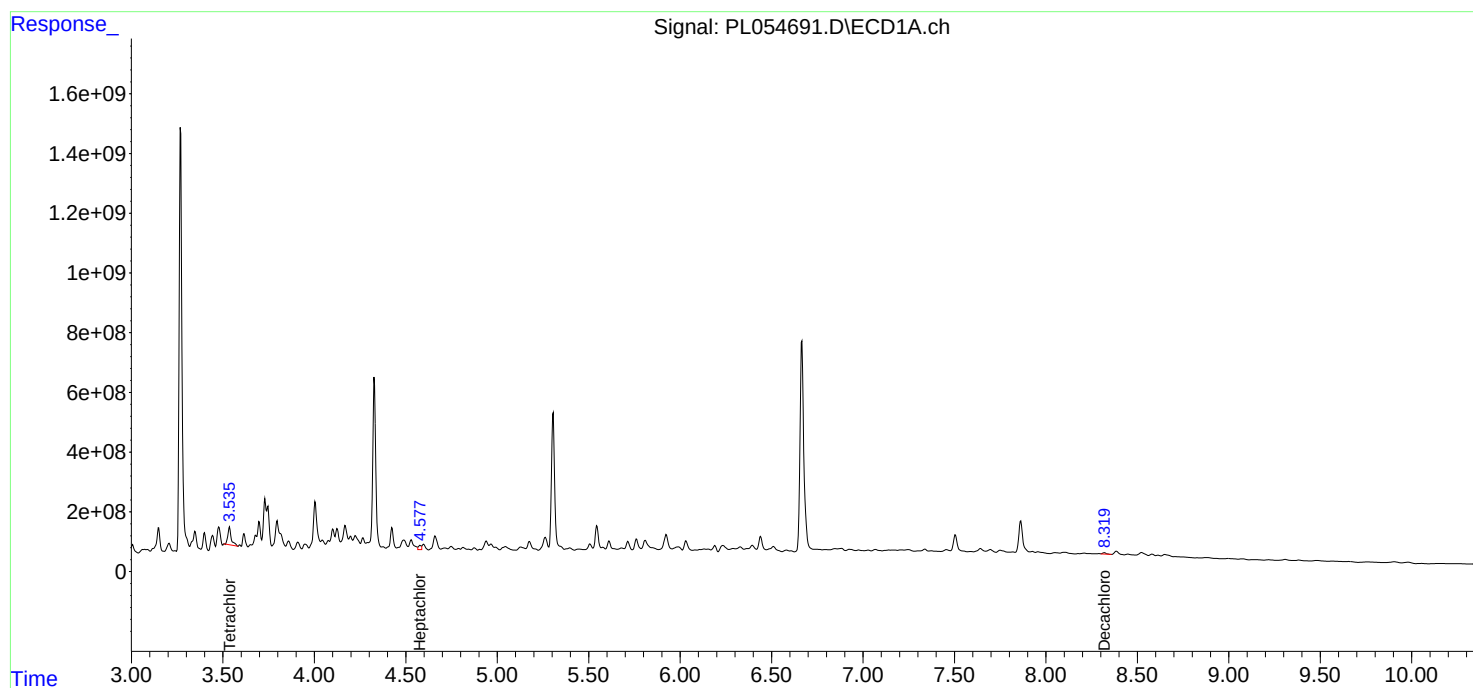

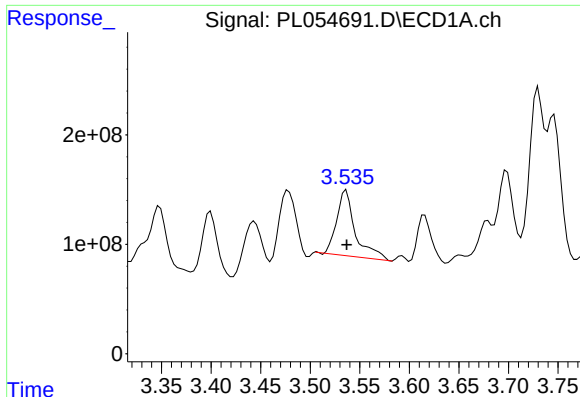


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.000 min
Response: 782524213
Conc: 67.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627


Manual Integrations
APPROVED

Ankita
12/2/2019 1:11:29 PM

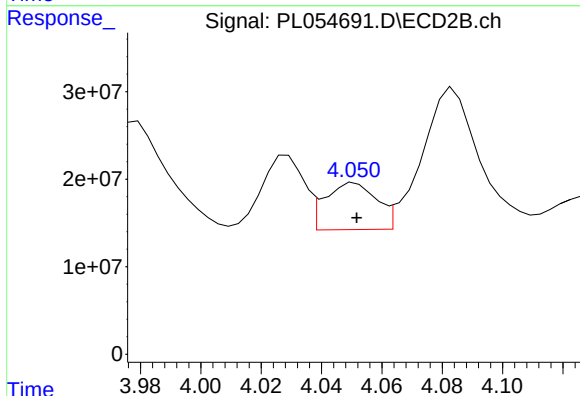


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 64380154
Conc: 25.23 ng/ml m

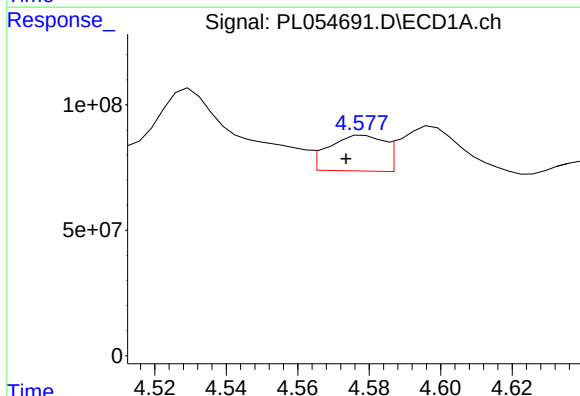


#4 Heptachlor

R.T.: 4.579 min
Delta R.T.: 0.005 min
Response: 152810500
Conc: 8.67 ng/ml

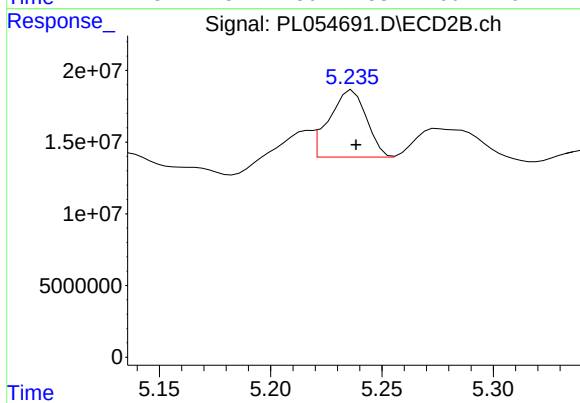

#4 Heptachlor

R.T.: 5.235 min
Delta R.T.: -0.003 min
Response: 52774367
Conc: 17.49 ng/ml m

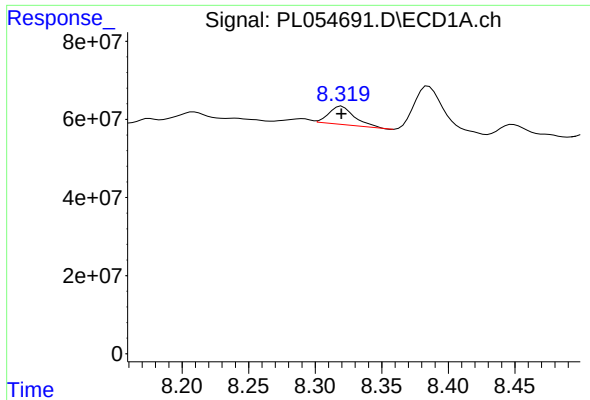


#28 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 62401615
Conc: 6.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-627

Manual Integrations
APPROVED

Ankita
12/2/2019 1:11:29 PM

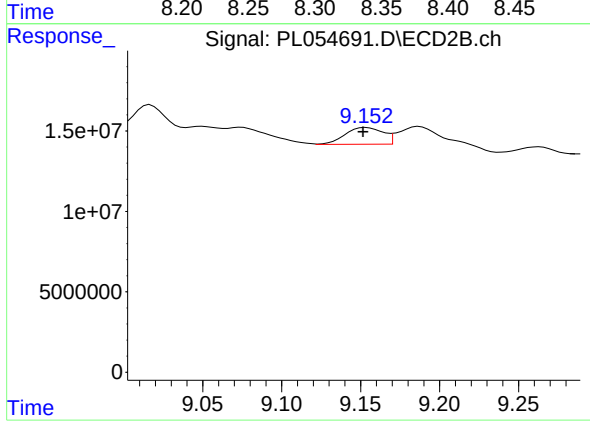

#28 Decachlorobiphenyl

R.T.: 9.152 min
Delta R.T.: 0.000 min
Response: 18406781
Conc: 7.68 ng/ml m