

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
 Data File : PL042544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2018 13:15
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 00:05:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.102	124.6E6	59595110	21.170	20.721
28)	SA Decachlor...	8.219	9.242	122.7E6	47719801	19.474	19.786
Target Compounds							
3)	MA gamma-BHC...	0.000	4.808	0	1102326	N.D.	0.279 #
6)	B beta-BHC	4.412f	0.000	2578433	0	0.728	N.D. #
8)	B Heptachlo...	0.000	5.956f	0	523966	N.D.	0.146 #
9)	A Endosulfan I	0.000	6.316f	0	12385401	N.D.	3.922 #
10)	B gamma-Chl...	5.353f	6.178f	4081072	9434833	0.535	2.771 #
11)	B alpha-Chl...	0.000	6.316	0	12385401	N.D.	3.704 #
14)	MA Endrin	0.000	6.770f	0	2730467	N.D.	0.991 #
18)	B Endrin al...	0.000	7.123f	0	457713	N.D.	0.200 #
19)	B Endosulfa...	6.701	0.000	1824668	0	0.292	N.D. #
25)	Chlordane-3	5.353	6.178	4081072	9434833	4.656	20.077 #
26)	Chlordane-4	0.000	6.316	0	12385401	N.D.	22.636 #
27)	Chlordane-5	0.000	7.123	0	457713	N.D.	4.758 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
Data File : PL042544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2018 13:15
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:05:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

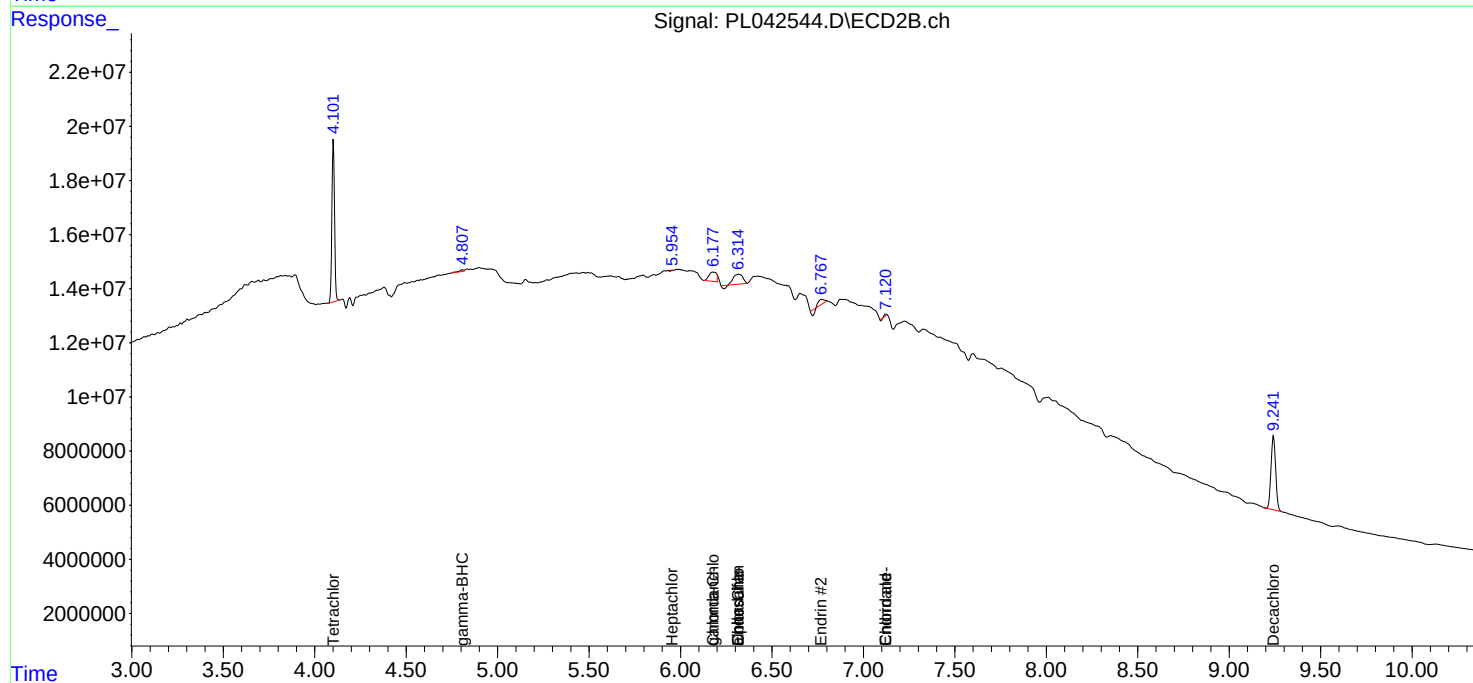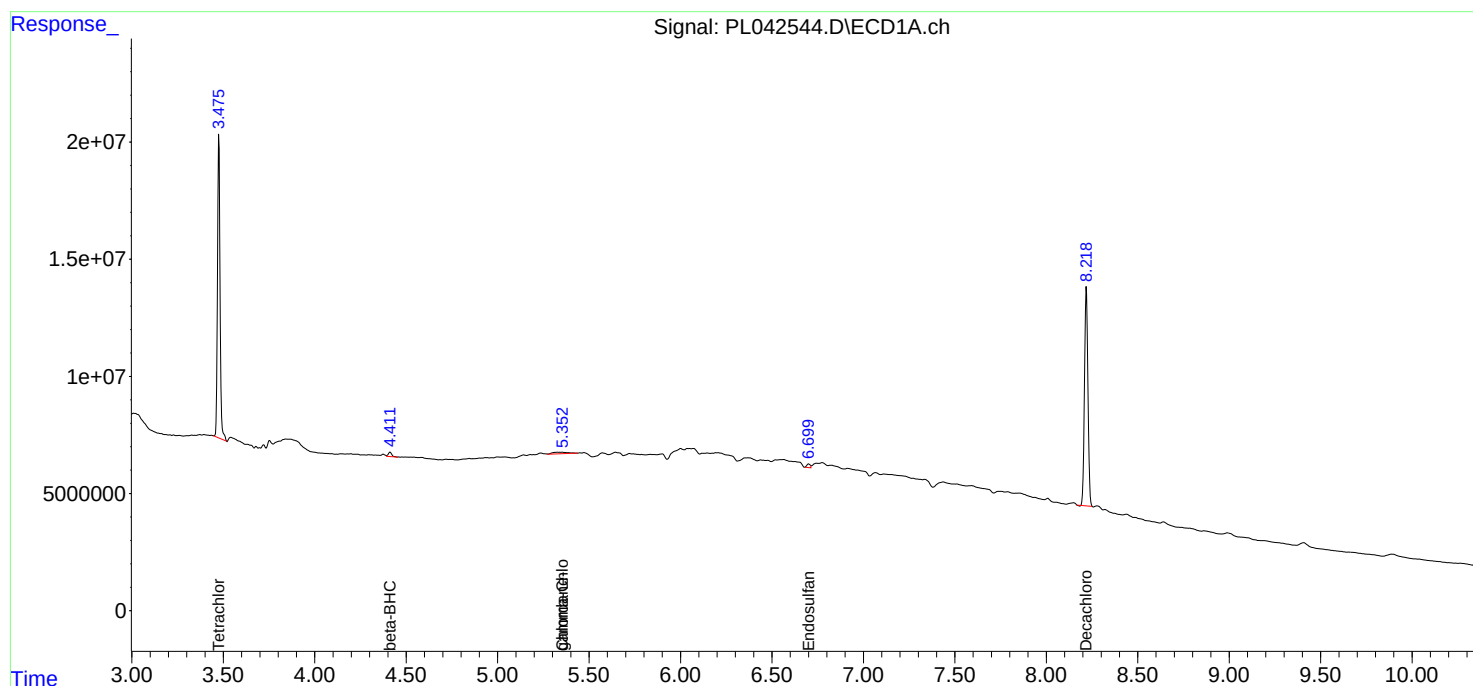


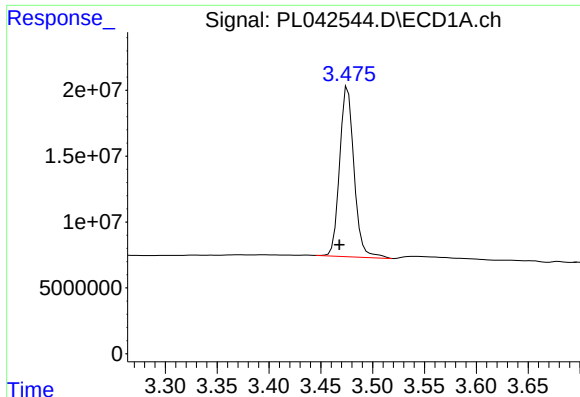

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.008 min
Response: 124554550
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

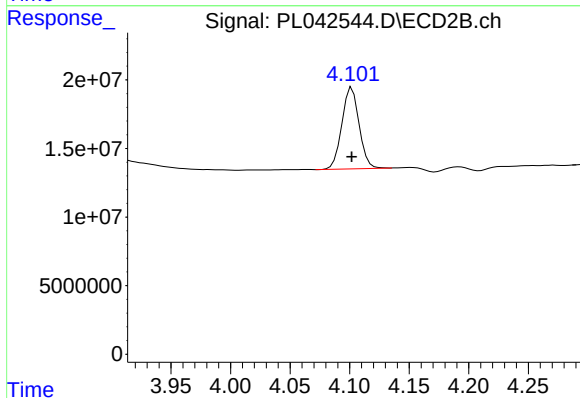


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 59595110
Conc: 20.72 ng/ml

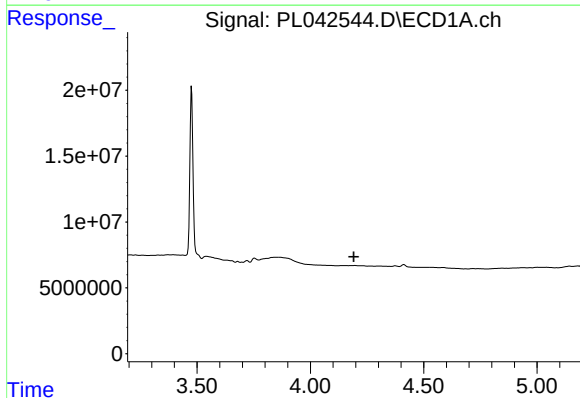


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.191 min
Response: 0
Conc: N.D.

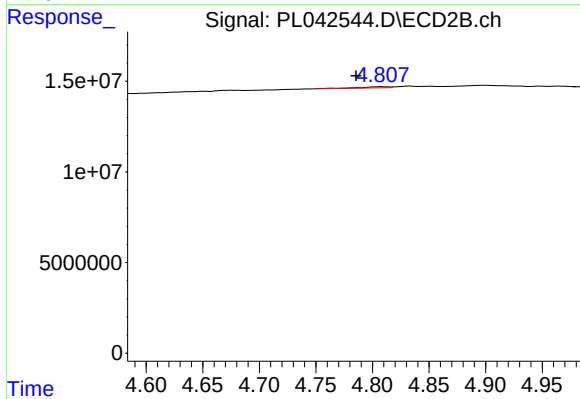

#3 gamma-BHC (Lindane)


R.T.: 4.808 min
Delta R.T.: 0.023 min
Response: 1102326
Conc: 0.28 ng/ml

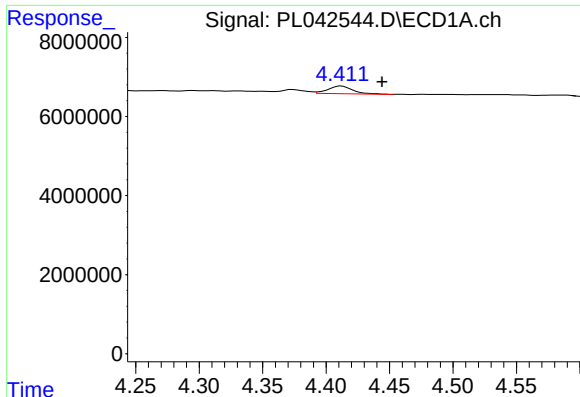

#6 beta-BHC


R.T.: 4.412 min
Delta R.T.: -0.032 min
Response: 2578433
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

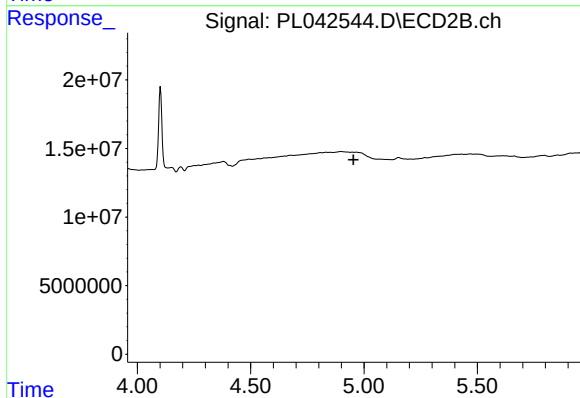


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

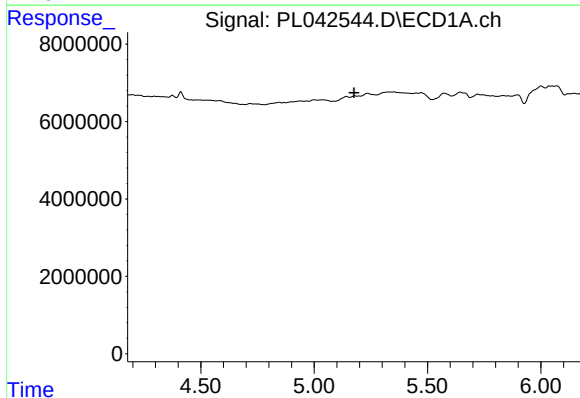


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

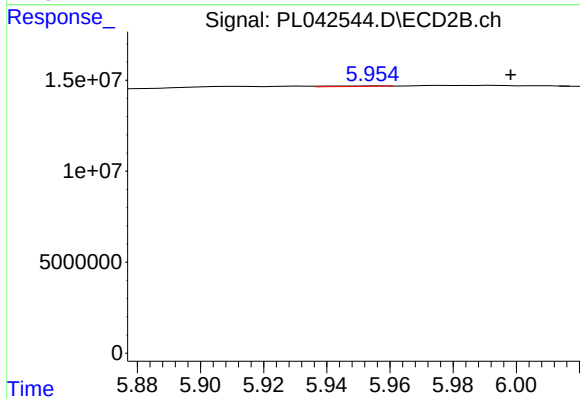

#8 Heptachlor epoxide


R.T.: 5.956 min
Delta R.T.: -0.042 min
Response: 523966
Conc: 0.15 ng/ml

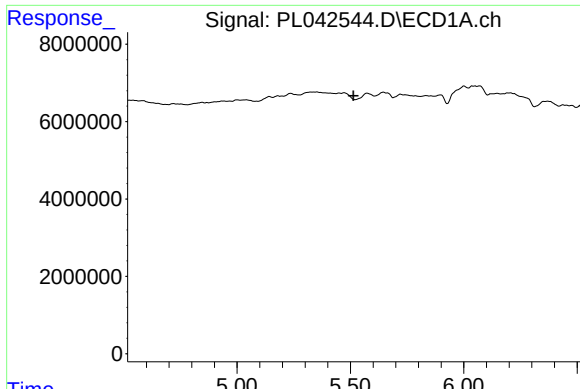

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.514 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

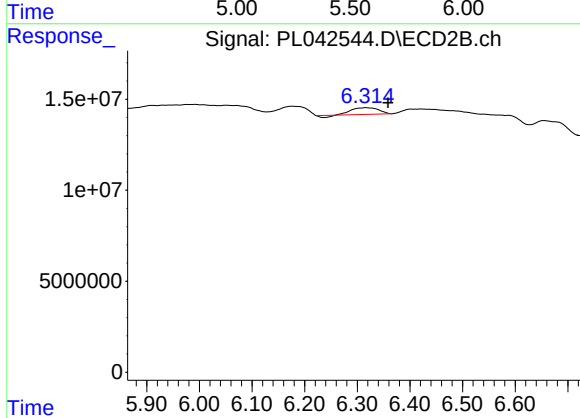


#9 Endosulfan I

R.T.: 6.316 min
Delta R.T.: -0.043 min
Response: 12385401
Conc: 3.92 ng/ml

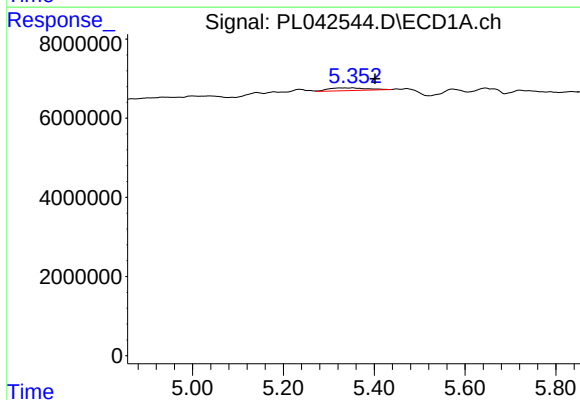


#10 gamma-Chlordane

R.T.: 5.353 min
Delta R.T.: -0.049 min
Response: 4081072
Conc: 0.54 ng/ml

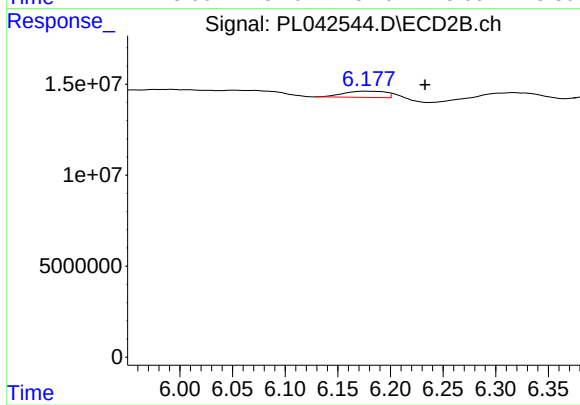

#10 gamma-Chlordane


R.T.: 6.178 min
Delta R.T.: -0.055 min
Response: 9434833
Conc: 2.77 ng/ml

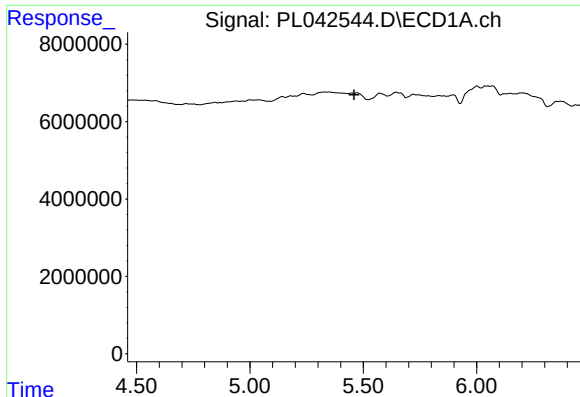

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

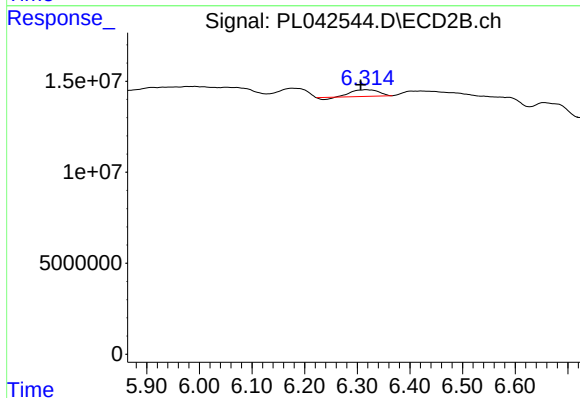


#11 alpha-Chlordane

R.T.: 6.316 min
Delta R.T.: 0.009 min
Response: 12385401
Conc: 3.70 ng/ml

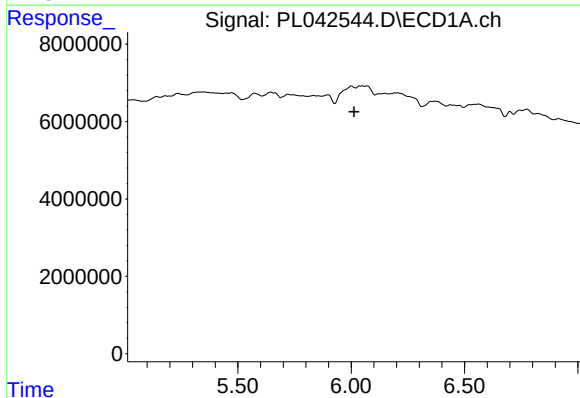


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.013 min
Response: 0
Conc: N.D.

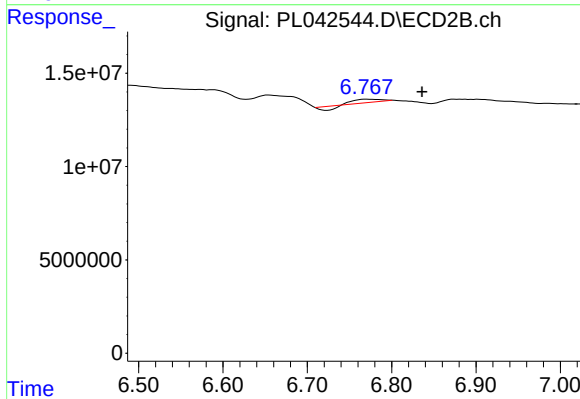

#14 Endrin


R.T.: 6.770 min
Delta R.T.: -0.066 min
Response: 2730467
Conc: 0.99 ng/ml

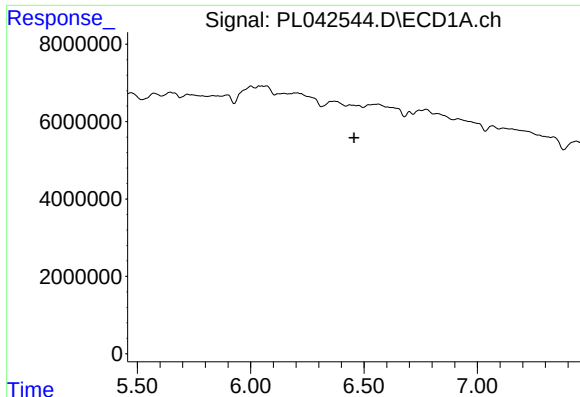

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.456 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

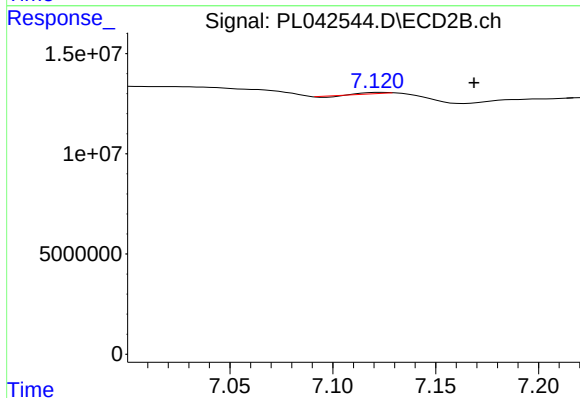


#18 Endrin aldehyde

R.T.: 7.123 min
Delta R.T.: -0.046 min
Response: 457713
Conc: 0.20 ng/ml

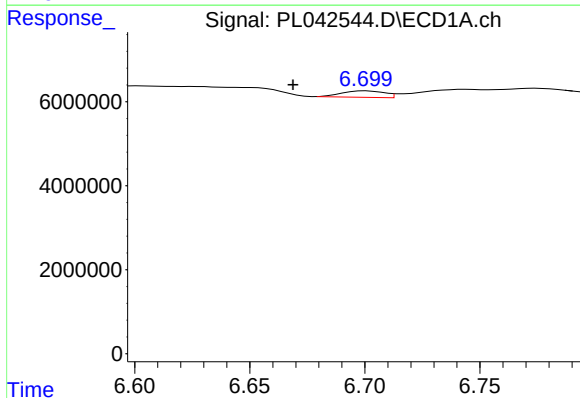


#19 Endosulfan Sulfate

R.T.: 6.701 min
Delta R.T.: 0.032 min
Response: 1824668
Conc: 0.29 ng/ml

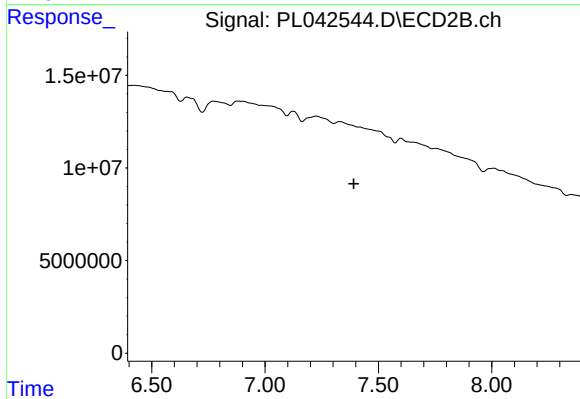

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.392 min
Response: 0
Conc: N.D.

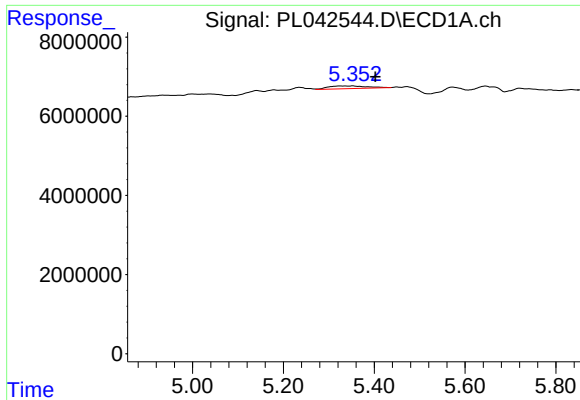

#25 Chlordane-3


R.T.: 5.353 min
Delta R.T.: -0.049 min
Response: 4081072
Conc: 4.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

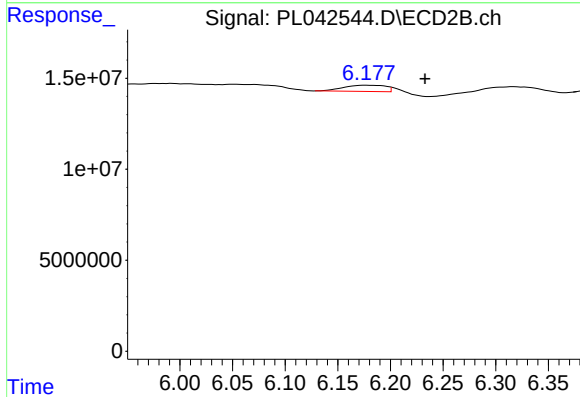


#25 Chlordane-3

R.T.: 6.178 min
Delta R.T.: -0.055 min
Response: 9434833
Conc: 20.08 ng/ml

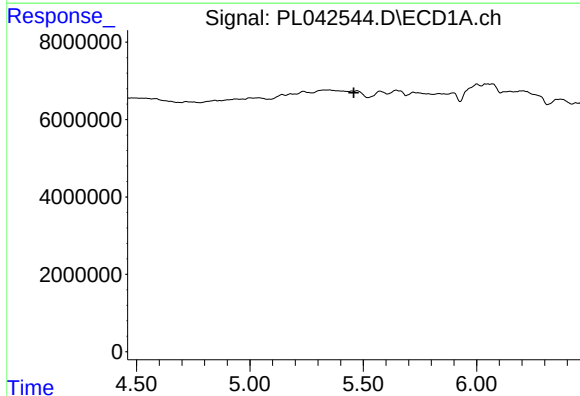


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

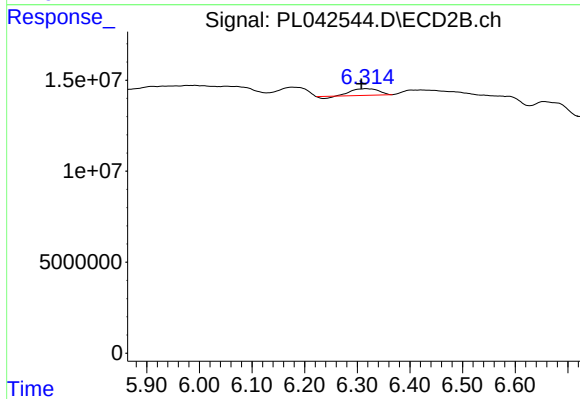

#26 Chlordane-4


R.T.: 6.316 min
Delta R.T.: 0.008 min
Response: 12385401
Conc: 22.64 ng/ml

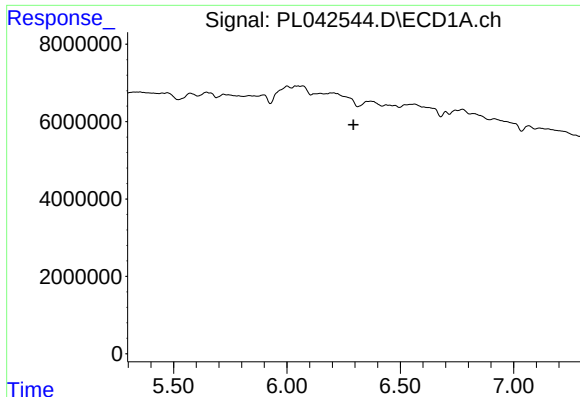

#27 Chloroform


R.T.: 0.000 min
Exp R.T.: 6.294 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

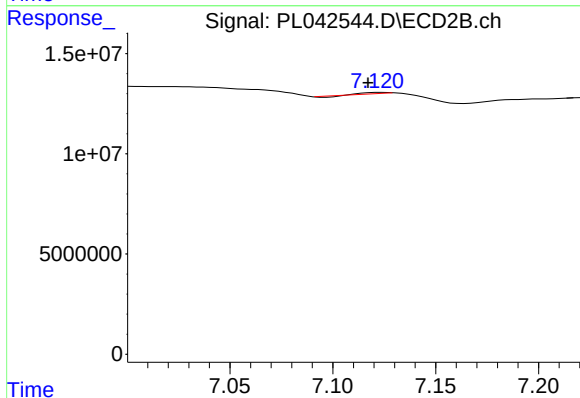


#27 Chloroform

R.T.: 7.123 min
Delta R.T.: 0.006 min
Response: 457713
Conc: 4.76 ng/ml

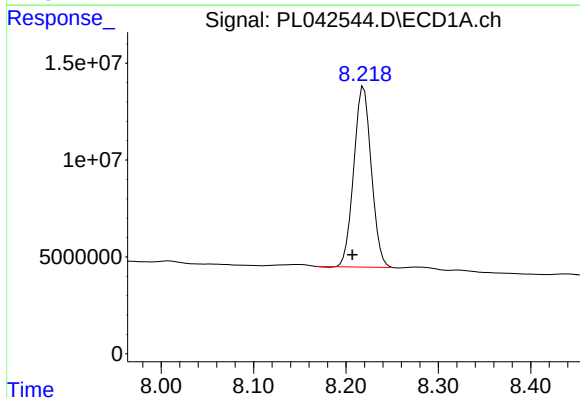

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: 0.012 min
Response: 122724930
Conc: 19.47 ng/ml

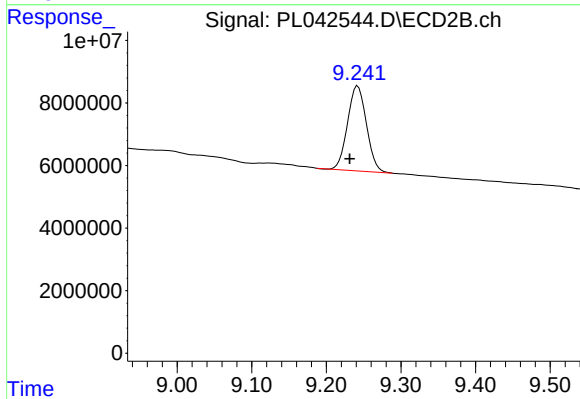

#28 Decachlorobiphenyl

R.T.: 9.242 min
Delta R.T.: 0.011 min
Response: 47719801
Conc: 19.79 ng/ml