

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
 Data File : PL042560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2018 18:02
 Operator : AJ\SJ
 Sample : J6079-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 00:09:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	104.7E6	54670354	17.804	19.008
28)	SA Decachlor...	8.207	9.237	90899370	35290273	14.424	14.632
Target Compounds							
2)	A alpha-BHC	3.900	0.000	4530109	0	0.502	N.D. #
4)	MA Heptachlor	4.518	0.000	1042002	0	0.120	N.D. #
6)	B beta-BHC	4.402f	0.000	5362632	0	1.514	N.D. #
8)	B Heptachlo...	5.235f	0.000	5235380	0	0.691	N.D. #
12)	B 4,4'-DDE	5.626	0.000	3282042	0	0.501	N.D. #
14)	MA Endrin	6.068f	0.000	1304141	0	0.199	N.D. #
15)	B Endosulfa...	6.234f	0.000	1230353	0	0.197	N.D. #
16)	A 4,4'-DDD	6.165	0.000	615221	0	0.116	N.D. #
17)	MA 4,4'-DDT	6.375	0.000	1785935	0	0.321	N.D. #
23)	Chlordane-1	4.360	0.000	2814383	0	10.180	N.D. #
27)	Chlordane-5	6.234	0.000	1230353	0	4.129	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
Data File : PL042560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2018 18:02
Operator : AJ\SJ
Sample : J6079-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:09:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

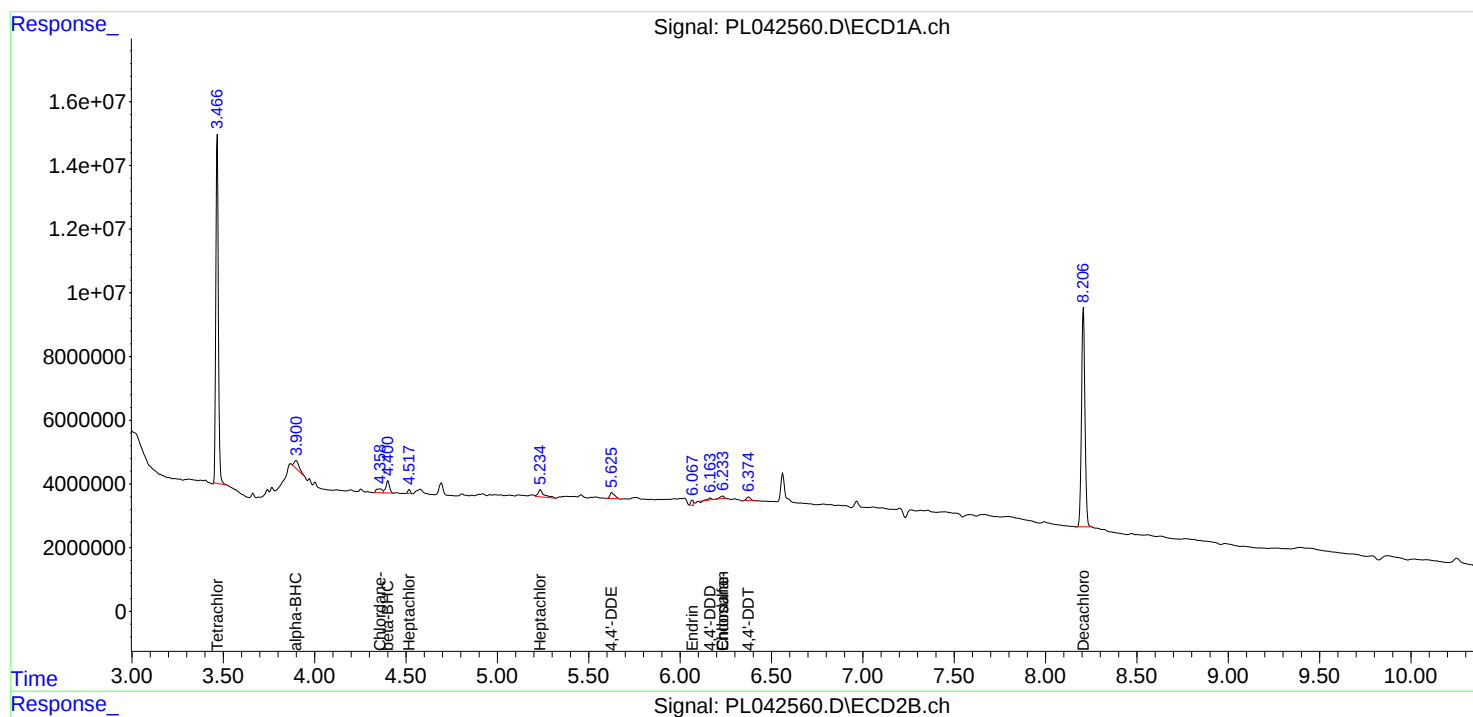


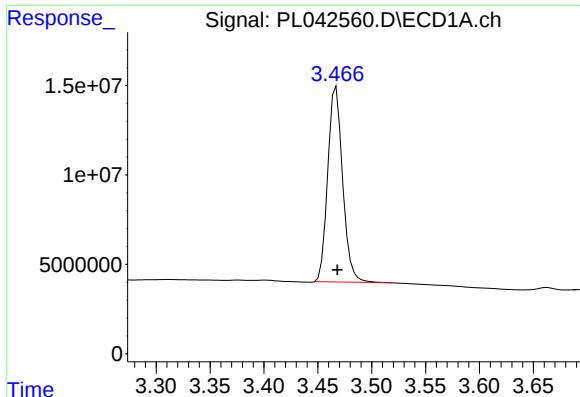

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 104748460
Conc: 17.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

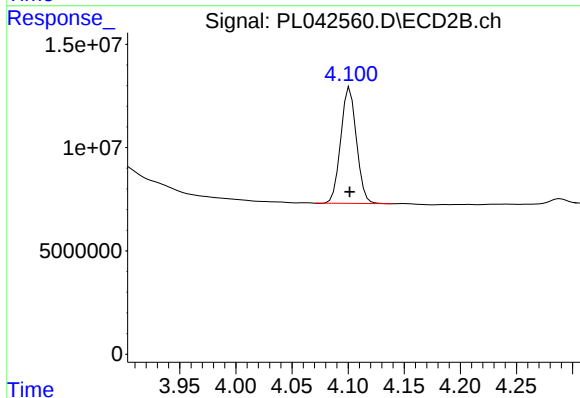


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 54670354
Conc: 19.01 ng/ml

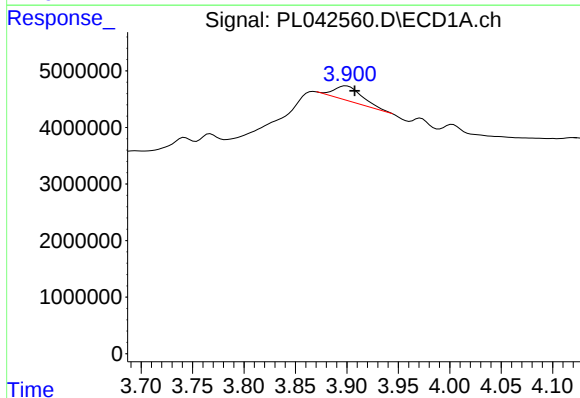


#2 alpha-BHC

R.T.: 3.900 min
Delta R.T.: -0.008 min
Response: 4530109
Conc: 0.50 ng/ml

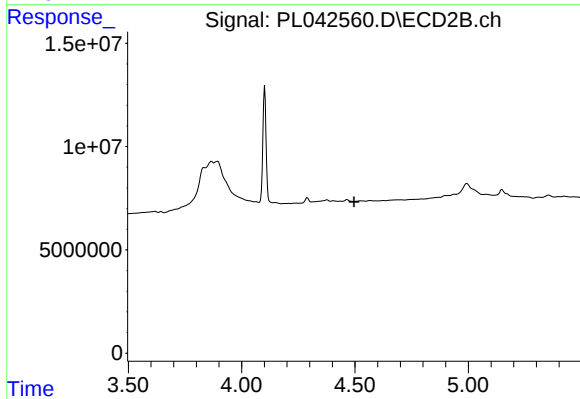

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

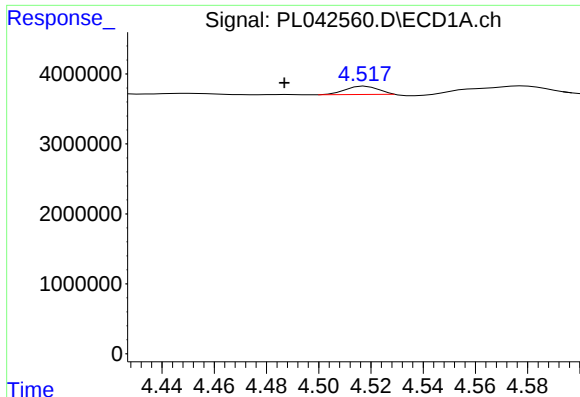

#4 Heptachlor


R.T.: 4.518 min
Delta R.T.: 0.031 min
Response: 1042002
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

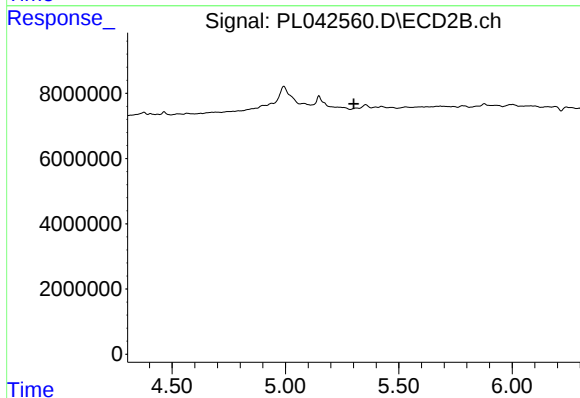


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.301 min
Response: 0
Conc: N.D.

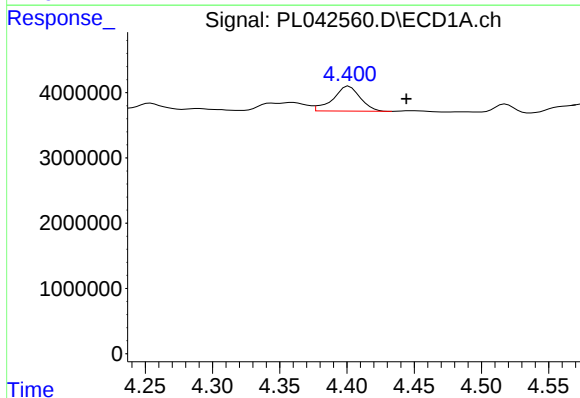


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 5362632
Conc: 1.51 ng/ml

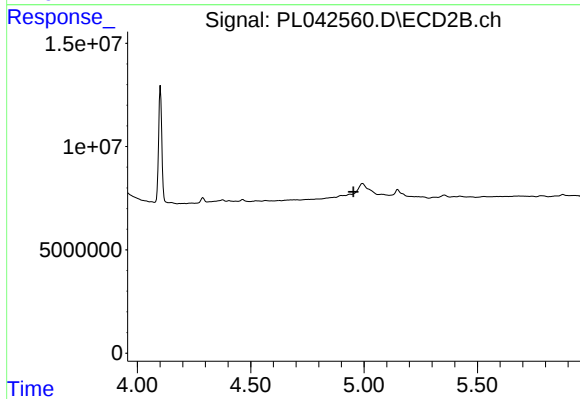

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

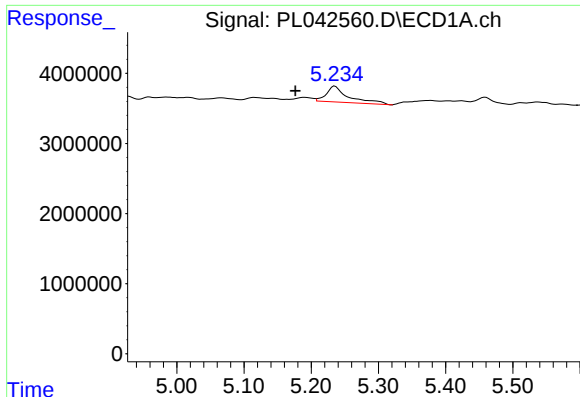

#8 Heptachlor epoxide


R.T.: 5.235 min
Delta R.T.: 0.059 min
Response: 5235380
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

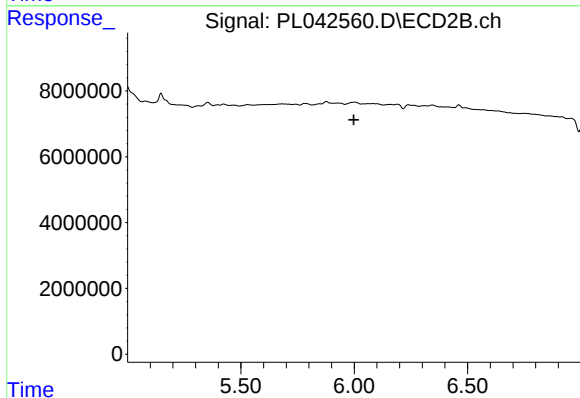


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.998 min
Response: 0
Conc: N.D.

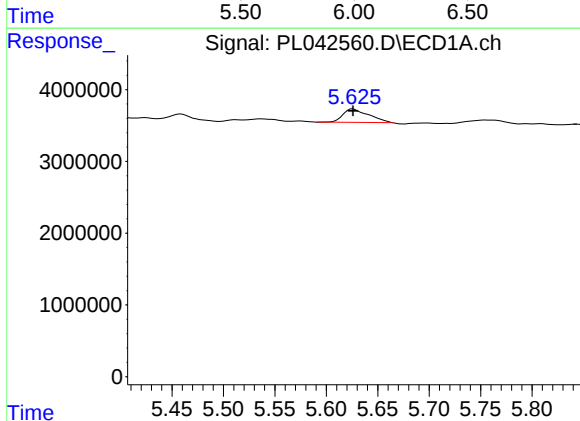


#12 4,4'-DDE

R.T.: 5.626 min
Delta R.T.: 0.000 min
Response: 3282042
Conc: 0.50 ng/ml

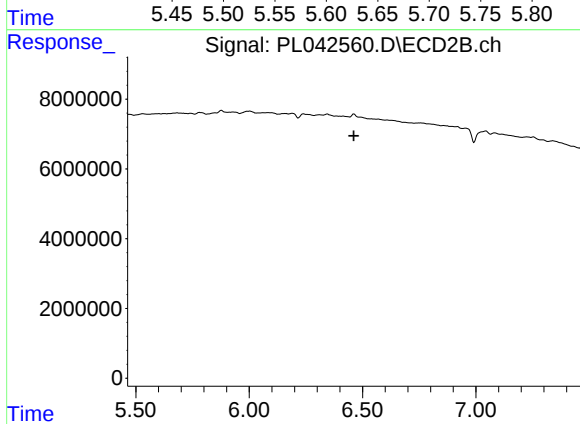

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

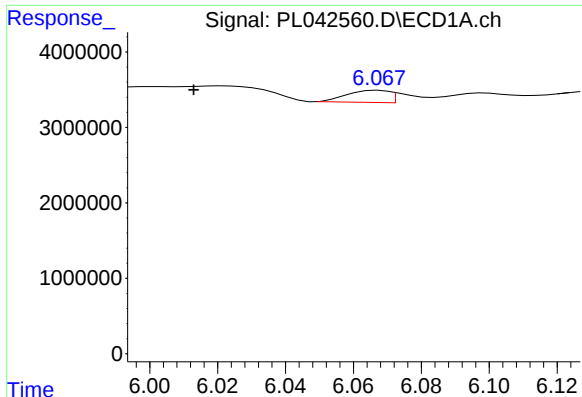

#14 Endrin


R.T.: 6.068 min
Delta R.T.: 0.055 min
Response: 1304141
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

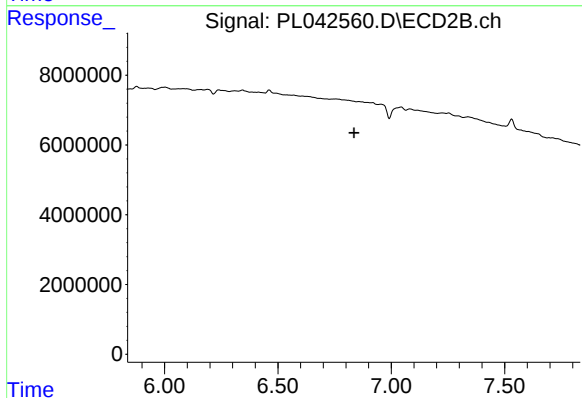


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

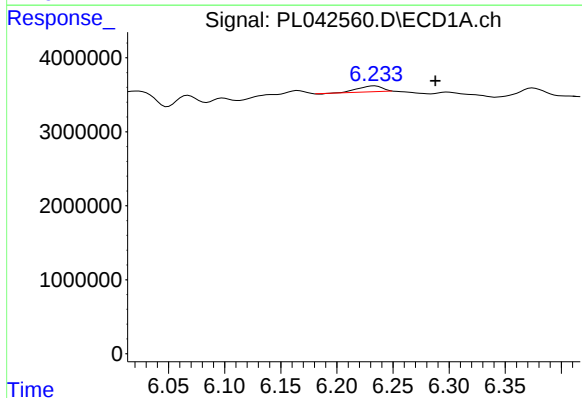


#15 Endosulfan II

R.T.: 6.234 min
Delta R.T.: -0.054 min
Response: 1230353
Conc: 0.20 ng/ml

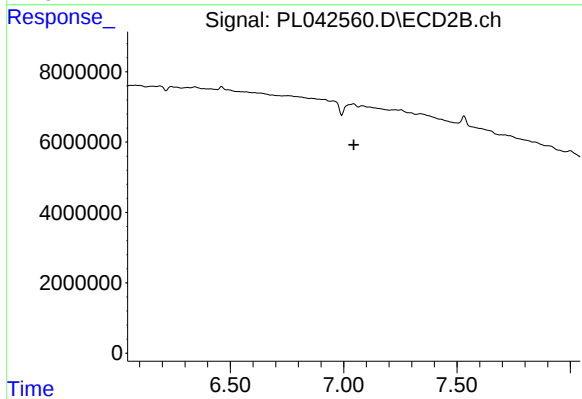

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

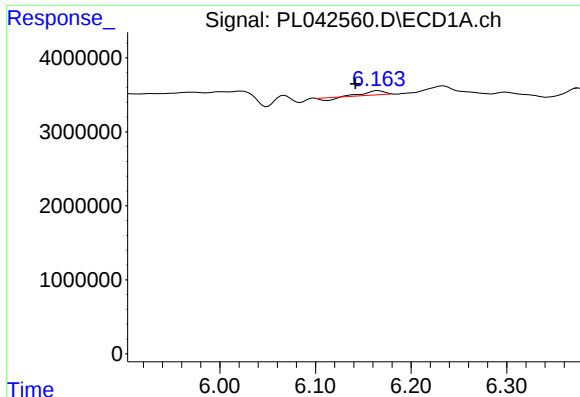

#16 4,4'-DDD


R.T.: 6.165 min
Delta R.T.: 0.024 min
Response: 615221
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

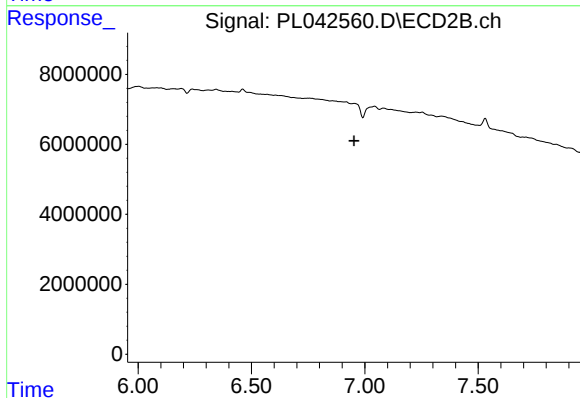


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.953 min
Response: 0
Conc: N.D.

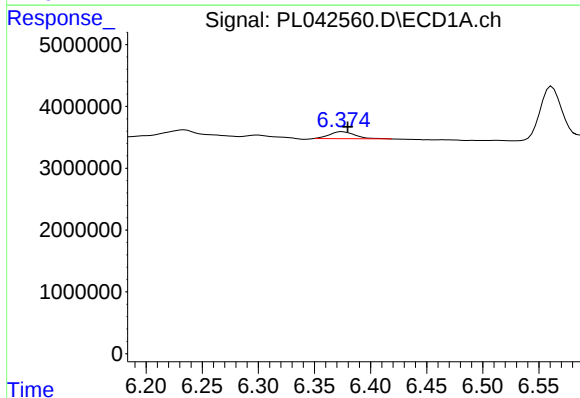


#17 4,4'-DDT

R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 1785935
Conc: 0.32 ng/ml

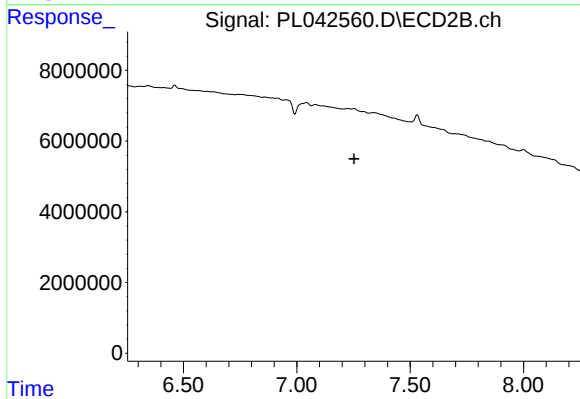

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

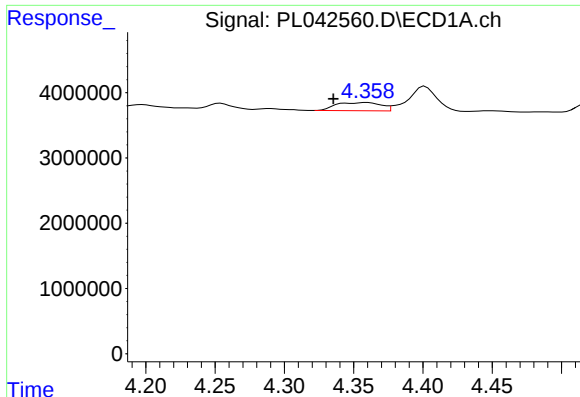

#23 Chlordane-1


R.T.: 4.360 min
Delta R.T.: 0.024 min
Response: 2814383
Conc: 10.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

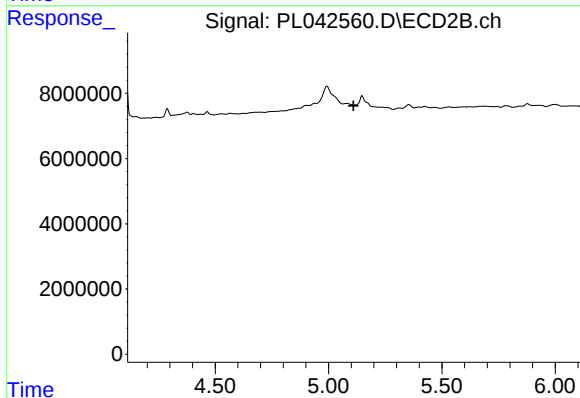


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

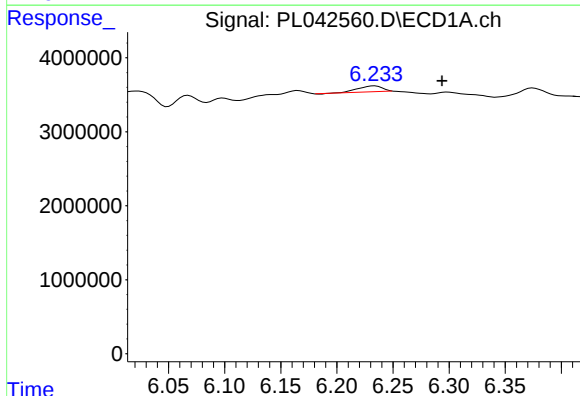


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: -0.060 min
Response: 1230353
Conc: 4.13 ng/ml

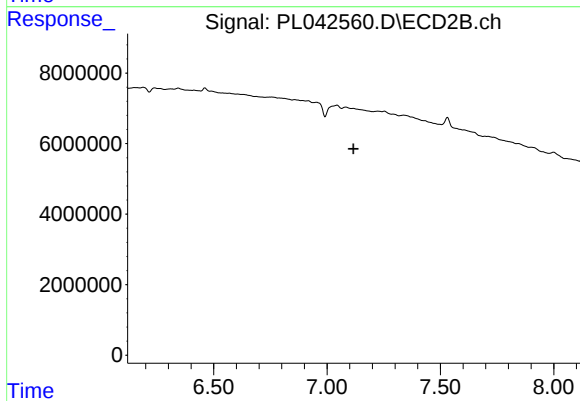

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

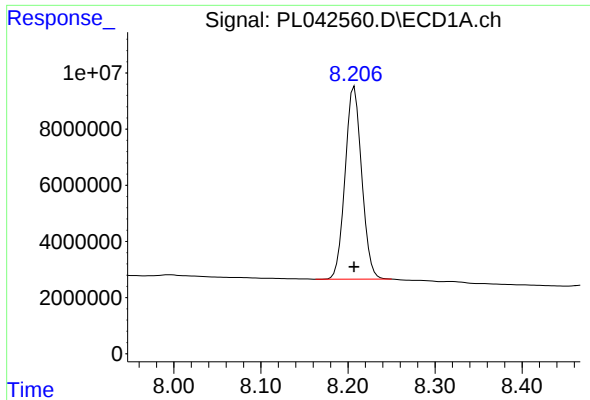

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 90899370
Conc: 14.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

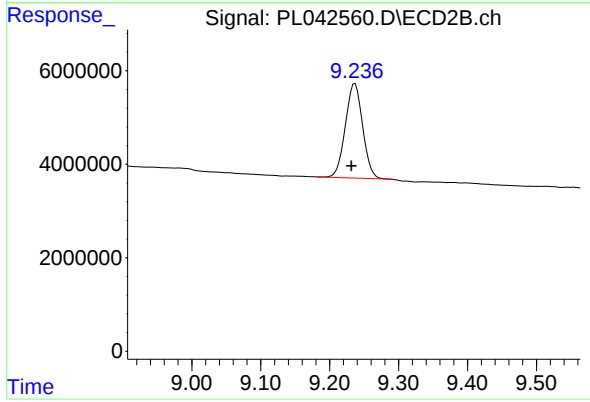

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.005 min
Response: 35290273
Conc: 14.63 ng/ml