

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
 Data File : PL042570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2018 20:23
 Operator : AJ\SJ
 Sample : PB115126BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 00:14:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	132.9E6	69621821	22.585	24.207
28)	SA Decachlor...	8.208	9.237	138.2E6	55732391	21.929	23.108
Target Compounds							
2)	A alpha-BHC	3.901	4.504	3301648	1118711	0.366	0.261 #
6)	B beta-BHC	4.403f	0.000	5265228	0	1.486	N.D. #
8)	B Heptachlo...	0.000	6.000	0	1868805	N.D.	0.521 #
19)	B Endosulfa...	6.655	7.388	3526248	3710538	0.565	1.334 #
20)	A Methoxychlor	0.000	7.650f	0	4611001	N.D.	3.382 #
23)	Chlordane-1	4.403	0.000	5265228	0	19.044	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
Data File : PL042570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2018 20:23
Operator : AJ\SJ
Sample : PB115126BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:14:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

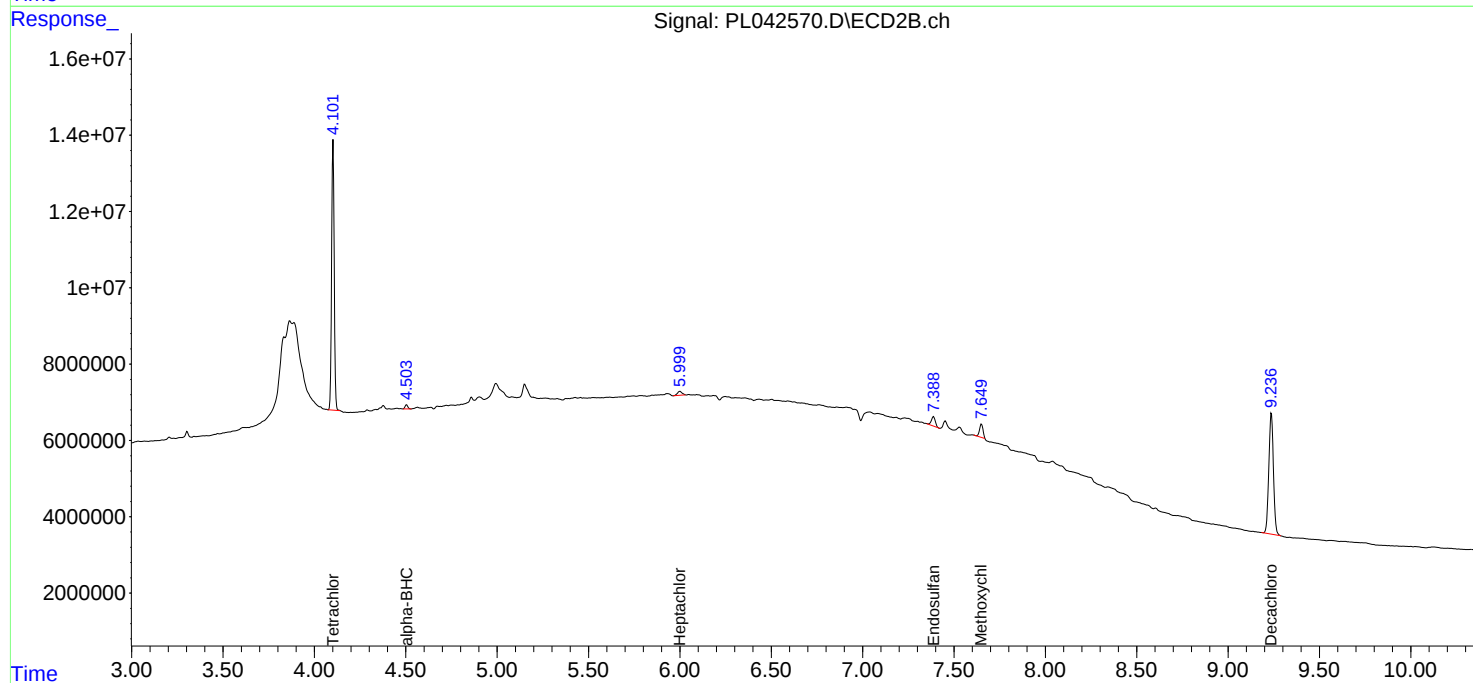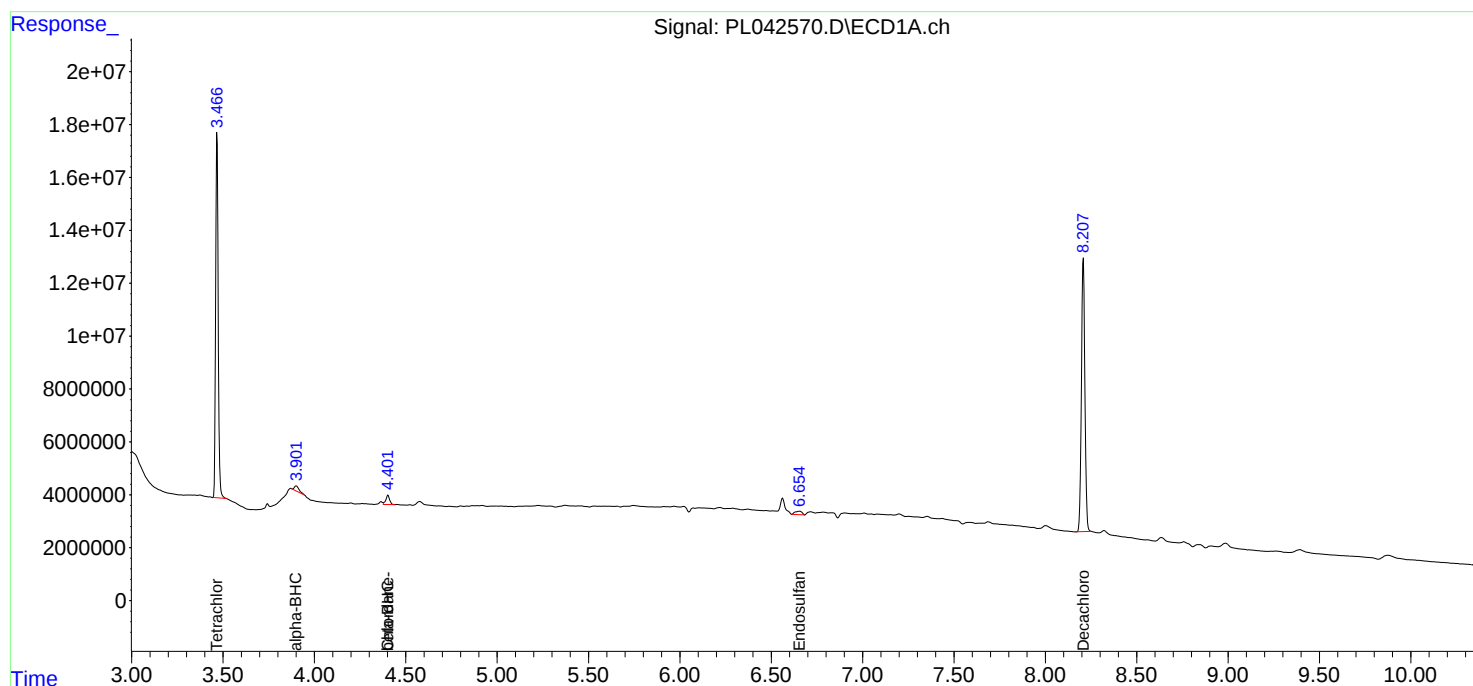


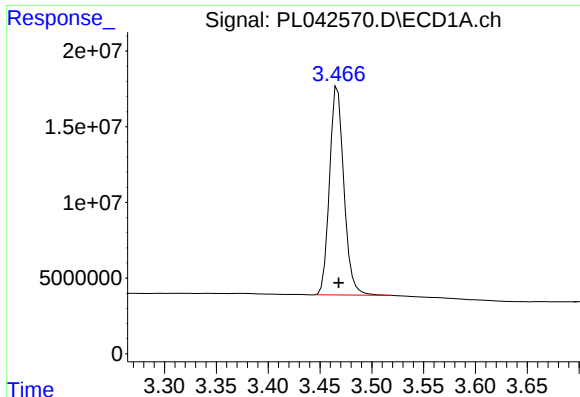

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 132875703
Conc: 22.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

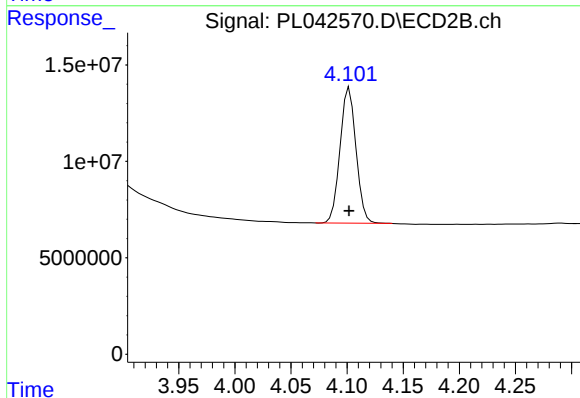


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 69621821
Conc: 24.21 ng/ml

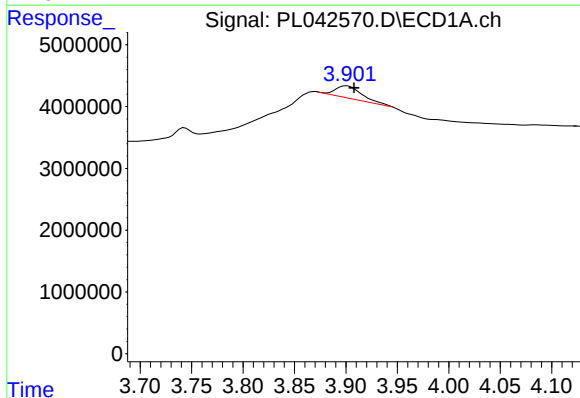


#2 alpha-BHC

R.T.: 3.901 min
Delta R.T.: -0.007 min
Response: 3301648
Conc: 0.37 ng/ml

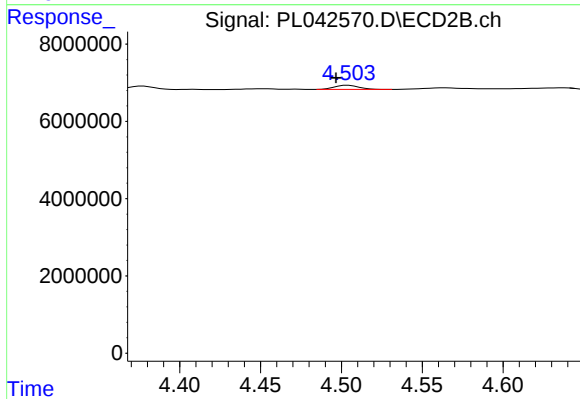

#2 alpha-BHC


R.T.: 4.504 min
Delta R.T.: 0.008 min
Response: 1118711
Conc: 0.26 ng/ml

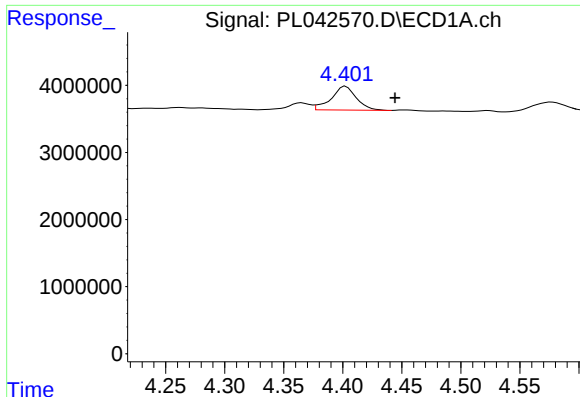

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: -0.042 min
Response: 5265228
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

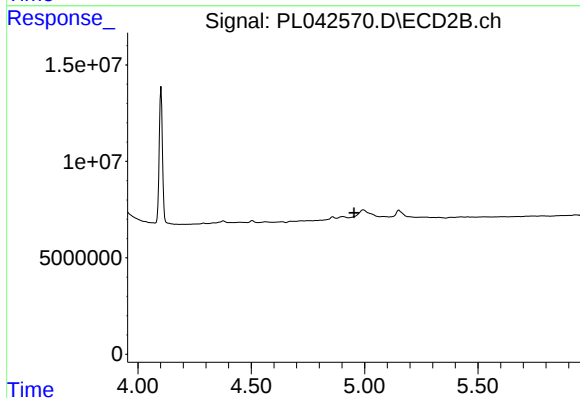


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

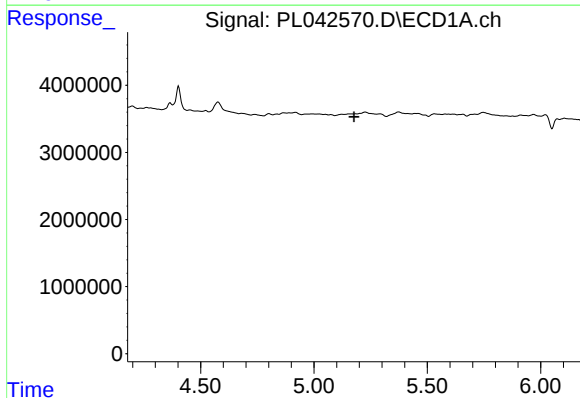


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.177 min
Response: 0
Conc: N.D.

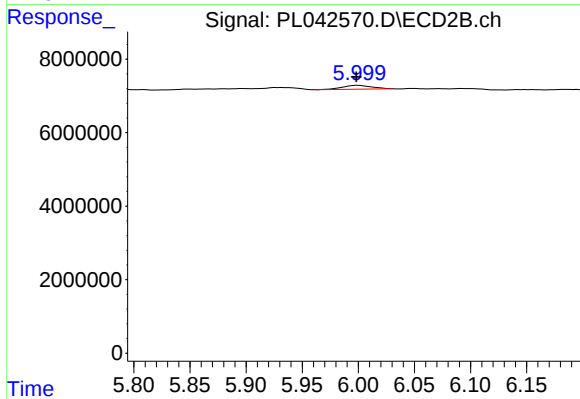

#8 Heptachlor epoxide


R.T.: 6.000 min
Delta R.T.: 0.002 min
Response: 1868805
Conc: 0.52 ng/ml

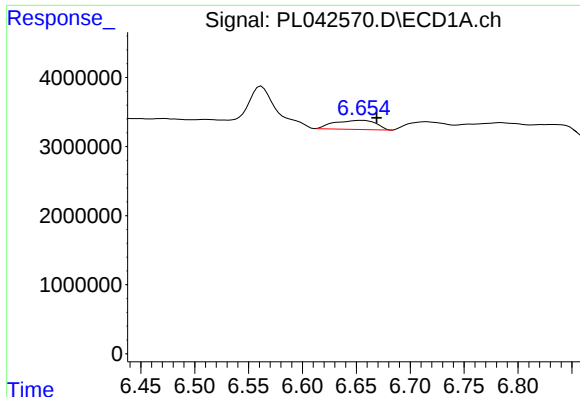

#19 Endosulfan Sulfate


R.T.: 6.655 min
Delta R.T.: -0.014 min
Response: 3526248
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

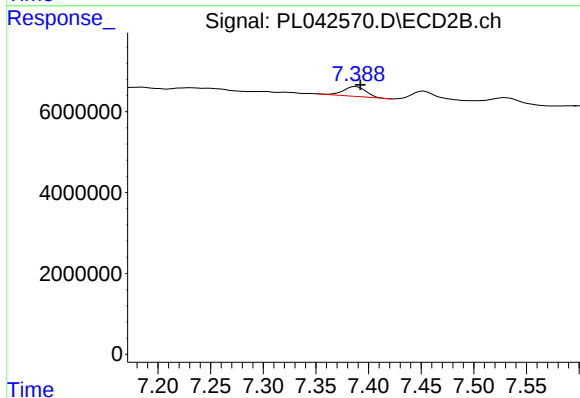


#19 Endosulfan Sulfate

R.T.: 7.388 min
Delta R.T.: -0.004 min
Response: 3710538
Conc: 1.33 ng/ml

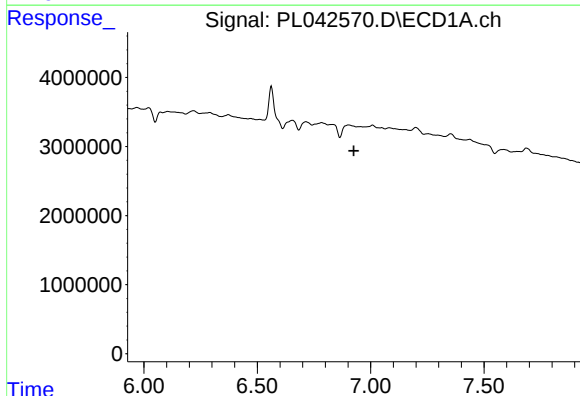


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.926 min
Response: 0
Conc: N.D.

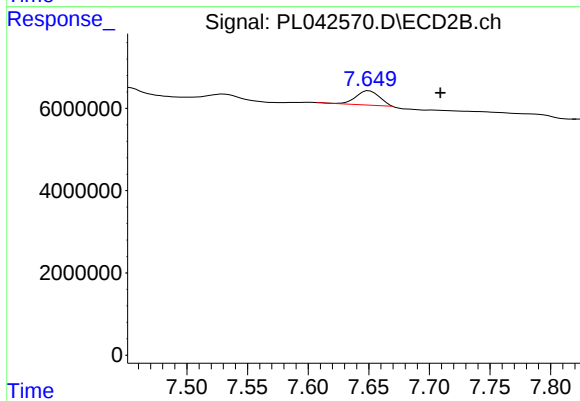

#20 Methoxychlor


R.T.: 7.650 min
Delta R.T.: -0.059 min
Response: 4611001
Conc: 3.38 ng/ml

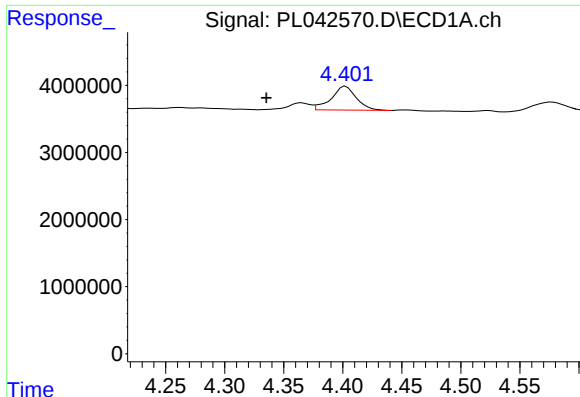

#23 Chlordane-1


R.T.: 4.403 min
Delta R.T.: 0.067 min
Response: 5265228
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

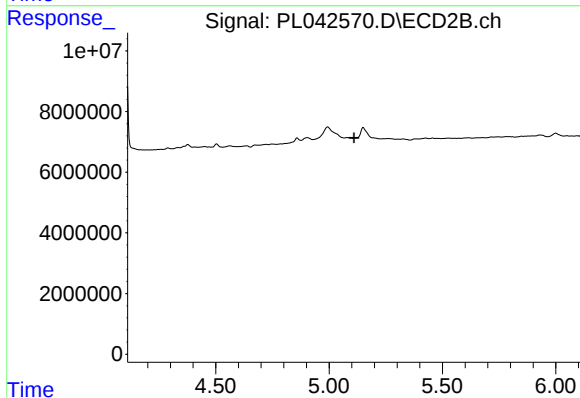


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

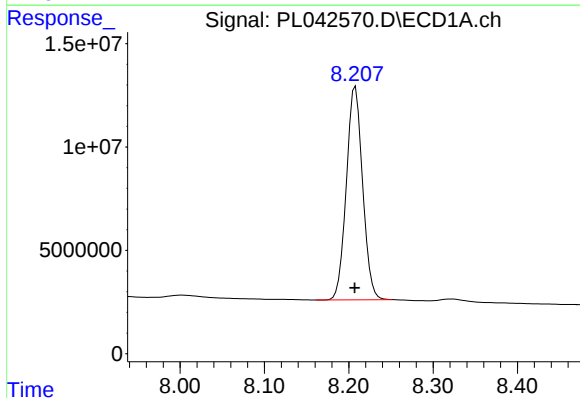

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 138196306
Conc: 21.93 ng/ml

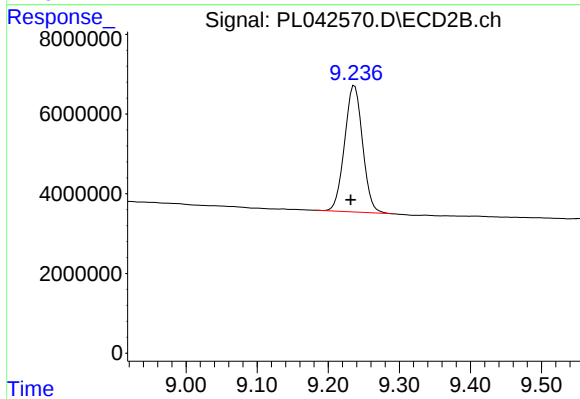

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.005 min
Response: 55732391
Conc: 23.11 ng/ml