

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
 Data File : PL042574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Nov 2018 21:20
 Operator : AJ\SJ
 Sample : J6060-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 00:14:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	97668837	51258108	16.601	17.822
2)	SA Decachlor...	8.207	9.237	110.0E6	43406816	17.455	17.997
Target Compounds							
2)	A alpha-BHC	3.893	0.000	3085673	0	0.342	N.D. #
5)	MB Aldrin	4.727	0.000	6414946	0	0.790	N.D. #
6)	B beta-BHC	4.402f	0.000	45901491	0	12.956	N.D. #
9)	A Endosulfan I	5.460f	0.000	925243	0	0.134	N.D. #
10)	B gamma-Chl...	5.371	6.235	2364213	-290754	0.310	N.D. #
11)	B alpha-Chl...	5.460	0.000	925243	0	0.123	N.D. #
15)	B Endosulfa...	6.232f	0.000	1795558	0	0.287	N.D. #
17)	MA 4,4'-DDT	6.383	0.000	2710997	0	0.487	N.D. #
23)	Chlordane-1	4.324	0.000	2326887	0	8.416	N.D. #
25)	Chlordane-3	5.371	6.235	2364213	-290754	2.697	N.D. #
26)	Chlordane-4	5.460	0.000	925243	0	1.219	N.D. #
27)	Chlordane-5	6.232	0.000	1795558	0	6.026	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112818\
Data File : PL042574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Nov 2018 21:20
Operator : AJ\SJ
Sample : J6060-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 00:14:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

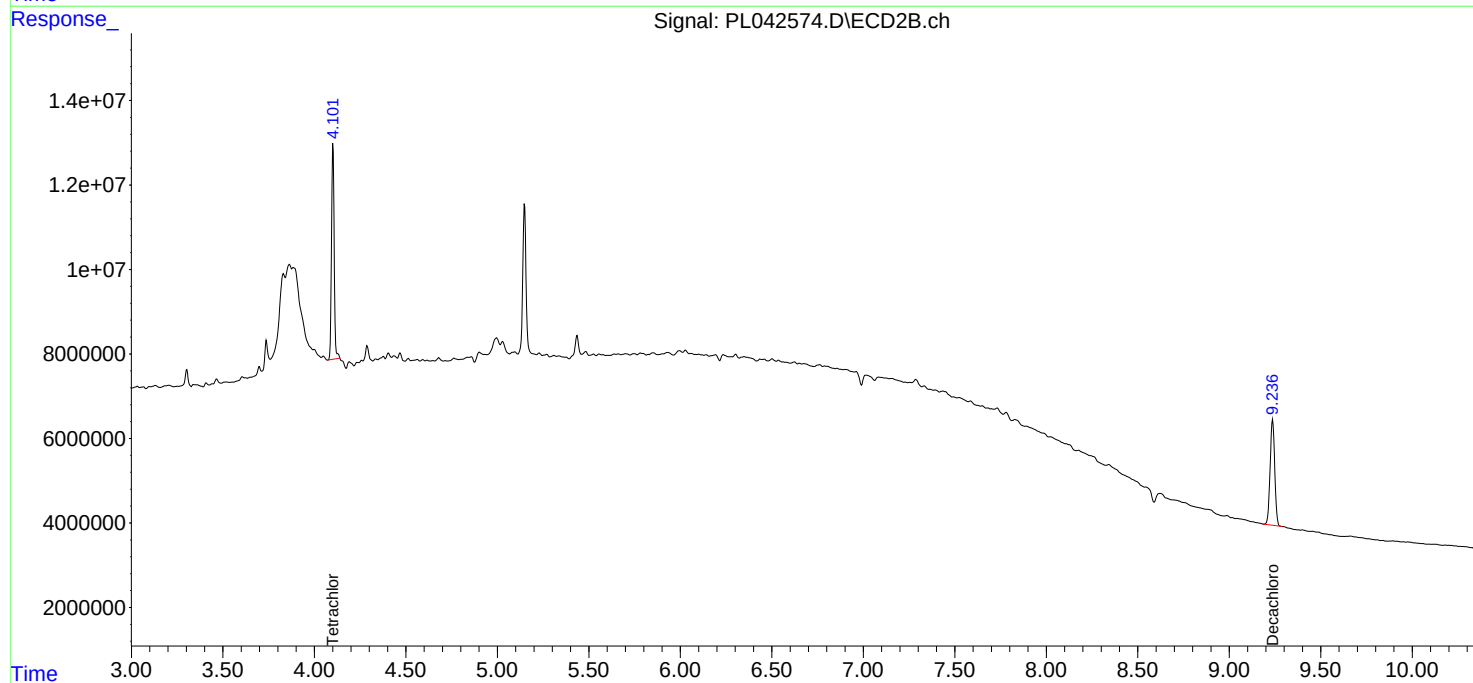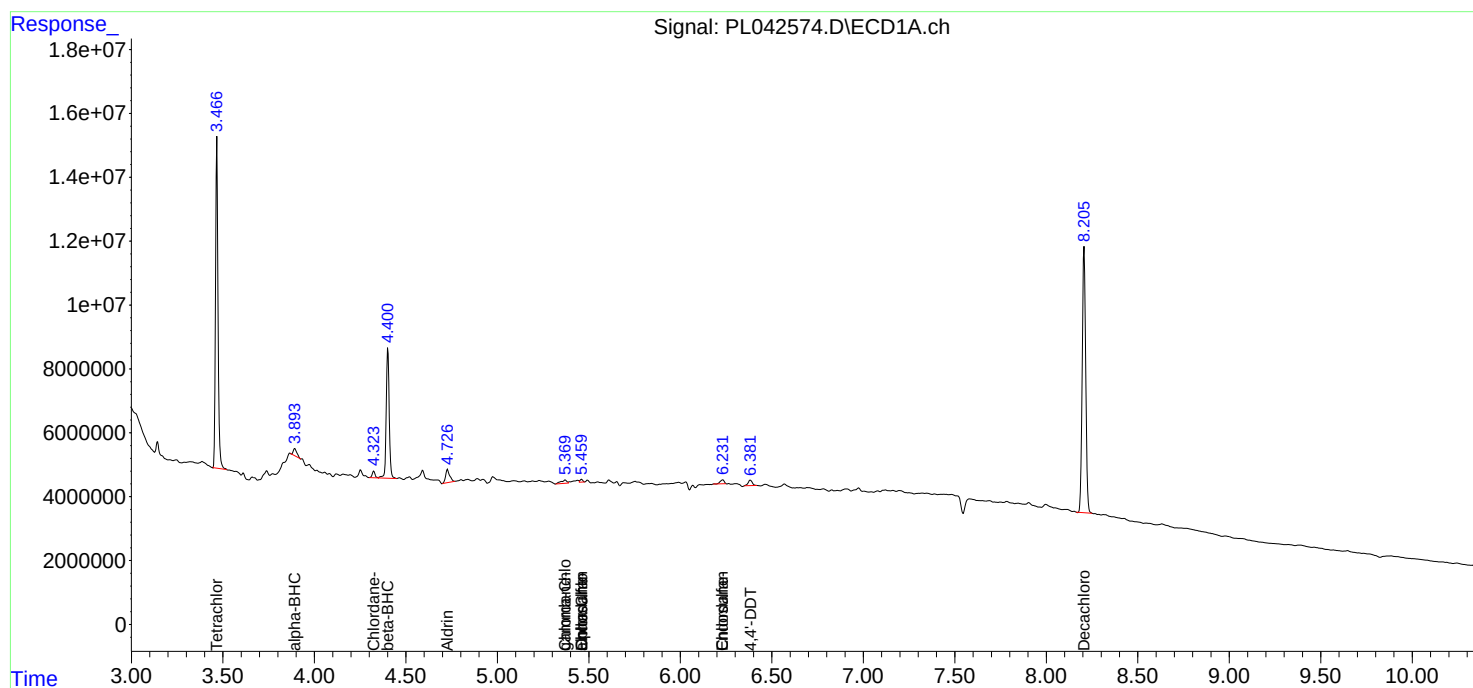


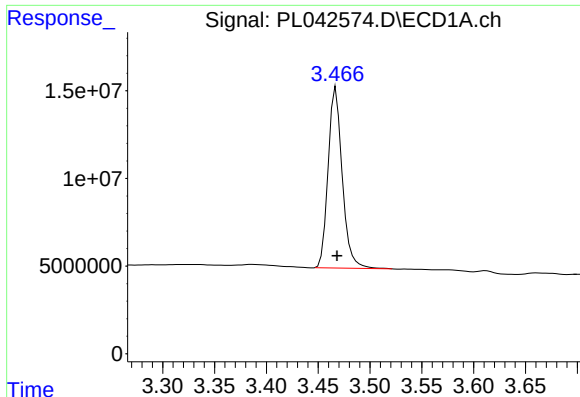

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 97668837
Conc: 16.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

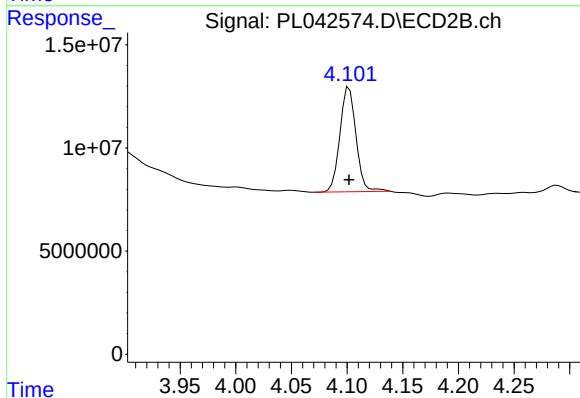


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 51258108
Conc: 17.82 ng/ml

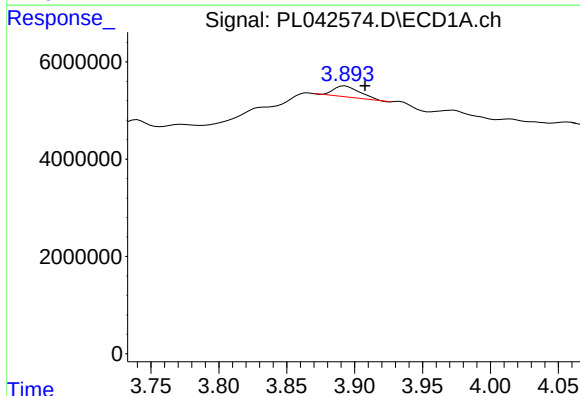


#2 alpha-BHC

R.T.: 3.893 min
Delta R.T.: -0.015 min
Response: 3085673
Conc: 0.34 ng/ml

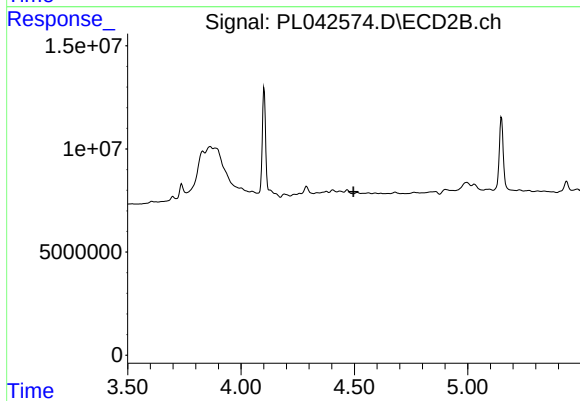

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

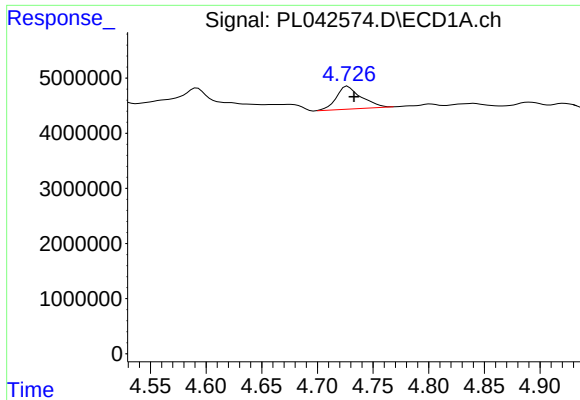

#5 Aldrin


R.T.: 4.727 min
Delta R.T.: -0.006 min
Response: 6414946
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

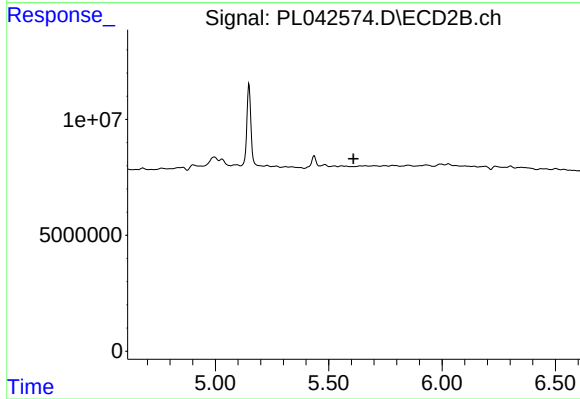


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.610 min
Response: 0
Conc: N.D.

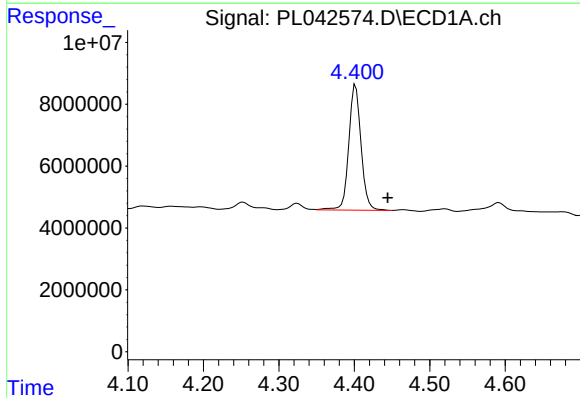


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.042 min
Response: 45901491
Conc: 12.96 ng/ml

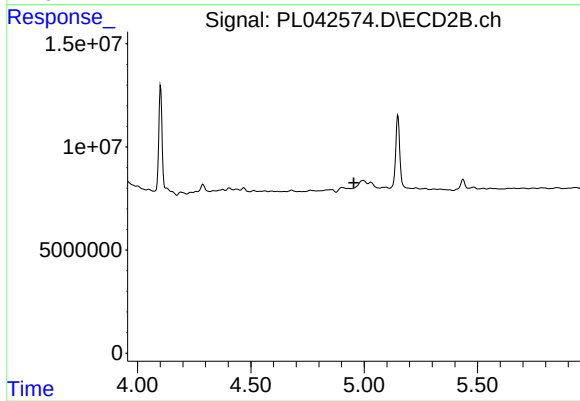

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

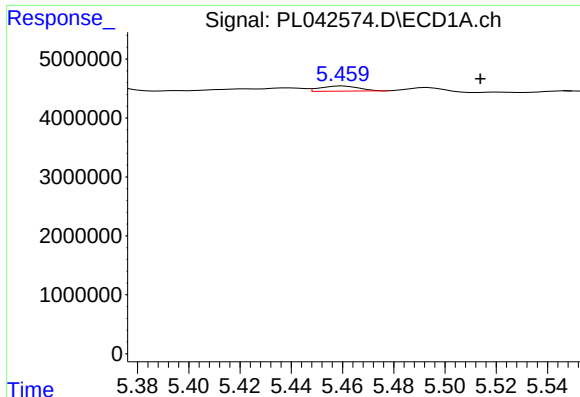

#9 Endosulfan I


R.T.: 5.460 min
Delta R.T.: -0.054 min
Response: 925243
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

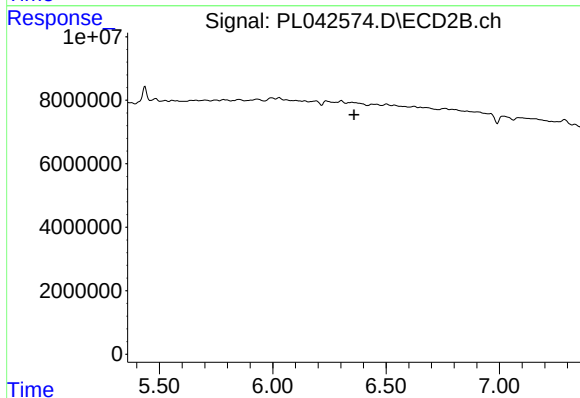


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

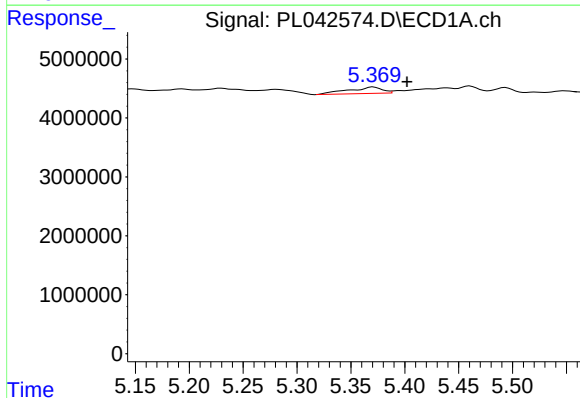


#10 gamma-Chlordane

R.T.: 5.371 min
Delta R.T.: -0.031 min
Response: 2364213
Conc: 0.31 ng/ml

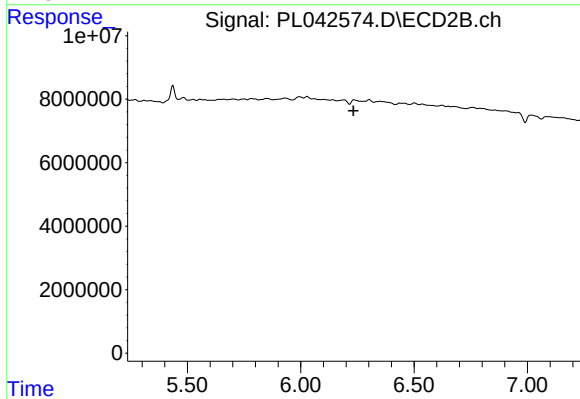

#10 gamma-Chlordane


R.T.: 6.235 min
Delta R.T.: 0.002 min
Response: -290754
Conc: N.D.

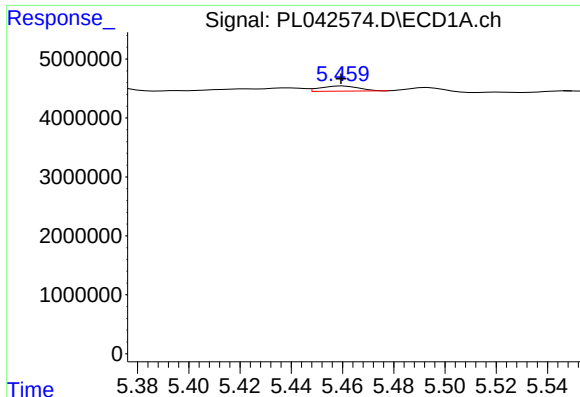

#11 alpha-Chlordane


R.T.: 5.460 min
Delta R.T.: 0.000 min
Response: 925243
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

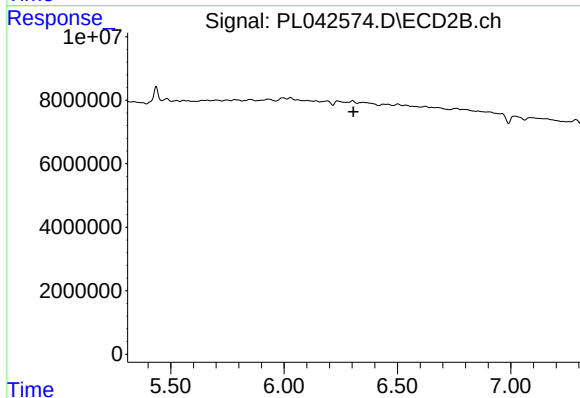


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

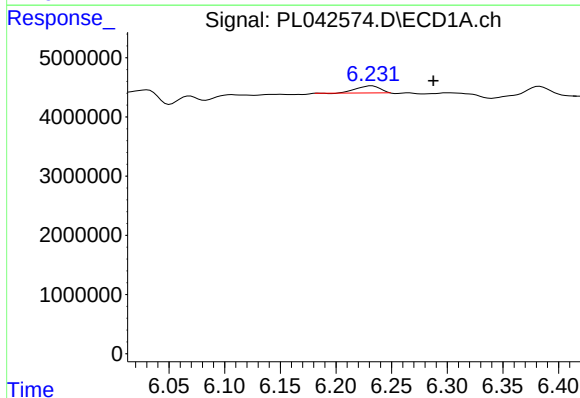


#15 Endosulfan II

R.T.: 6.232 min
Delta R.T.: -0.055 min
Response: 1795558
Conc: 0.29 ng/ml

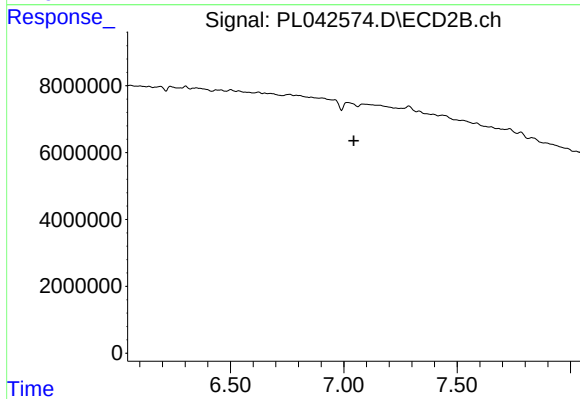

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

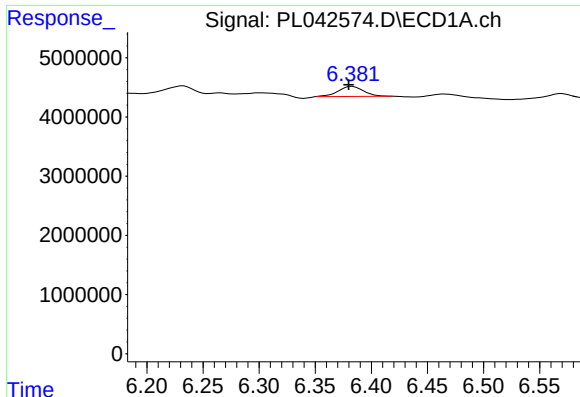

#17 4,4'-DDT


R.T.: 6.383 min
Delta R.T.: 0.003 min
Response: 2710997
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

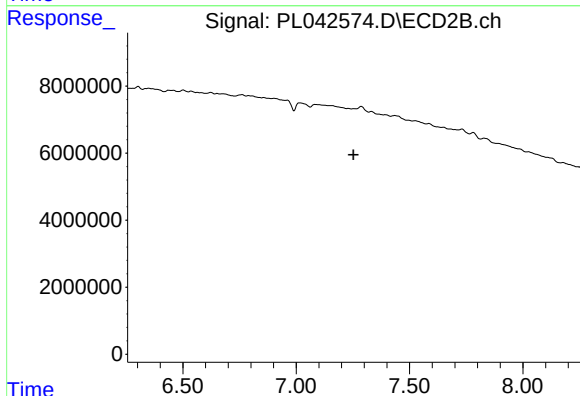


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

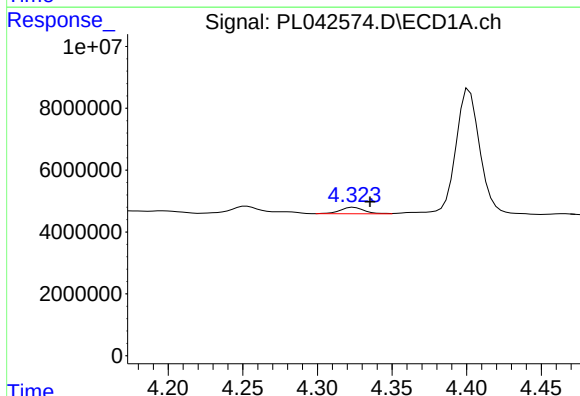


#23 Chlordane-1

R.T.: 4.324 min
Delta R.T.: -0.011 min
Response: 2326887
Conc: 8.42 ng/ml

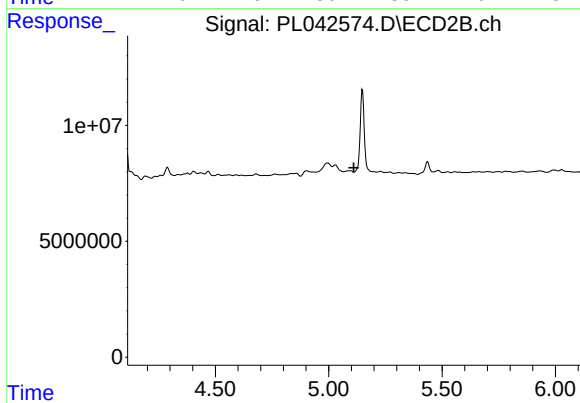

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

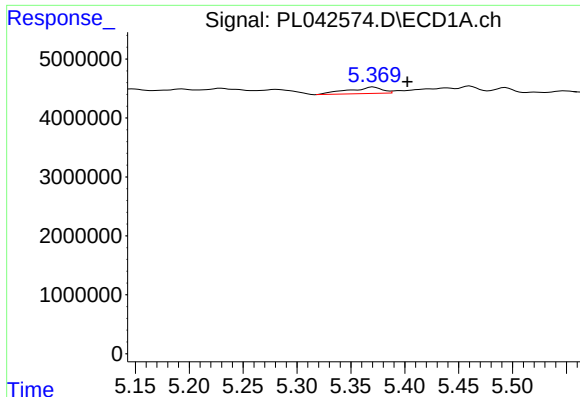

#25 Chlordane-3


R.T.: 5.371 min
Delta R.T.: -0.032 min
Response: 2364213
Conc: 2.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

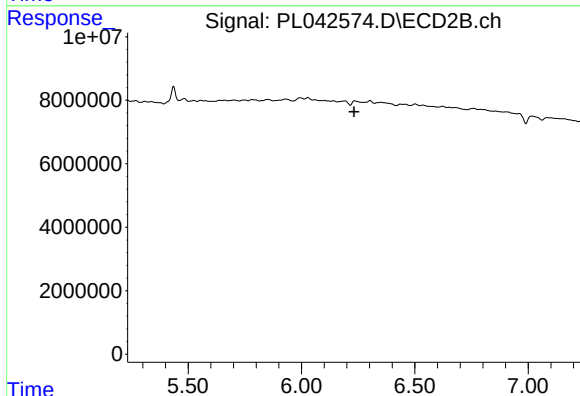


#25 Chlordane-3

R.T.: 6.235 min
Delta R.T.: 0.002 min
Response: -290754
Conc: N.D.

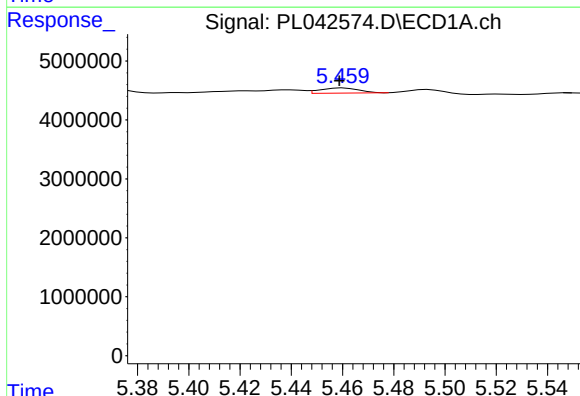


#26 Chlordane-4

R.T.: 5.460 min
Delta R.T.: 0.002 min
Response: 925243
Conc: 1.22 ng/ml

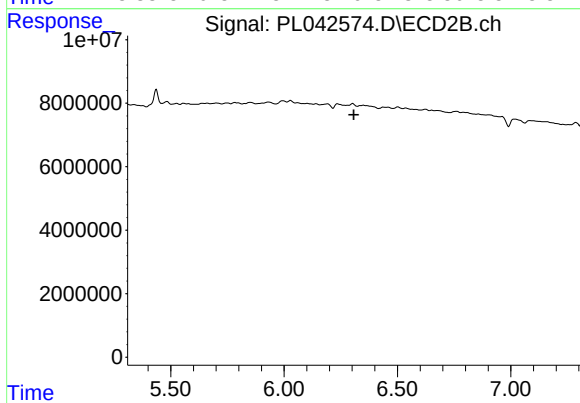

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.308 min
Response: 0
Conc: N.D.

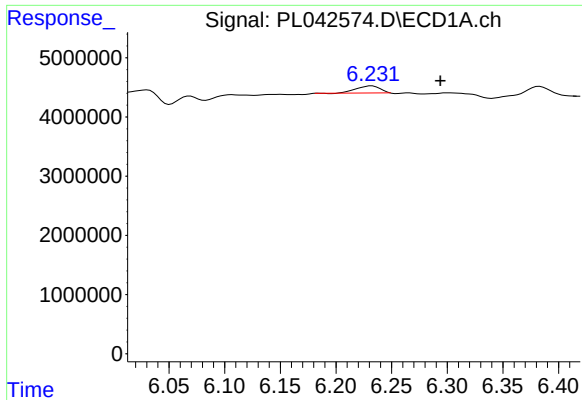

#27 Chlordane-5


R.T.: 6.232 min
Delta R.T.: -0.061 min
Response: 1795558
Conc: 6.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

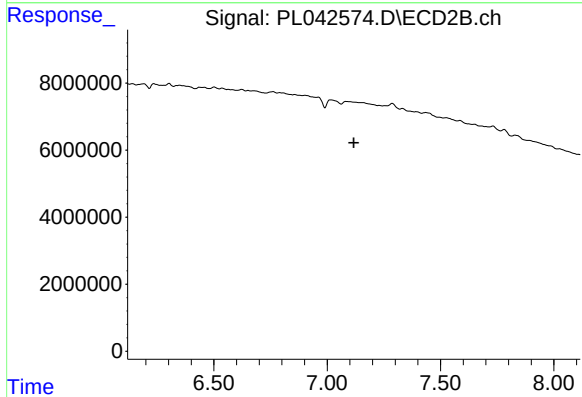


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

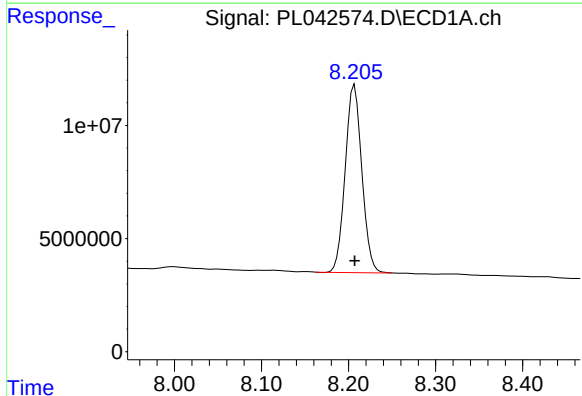

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 110002002
Conc: 17.45 ng/ml

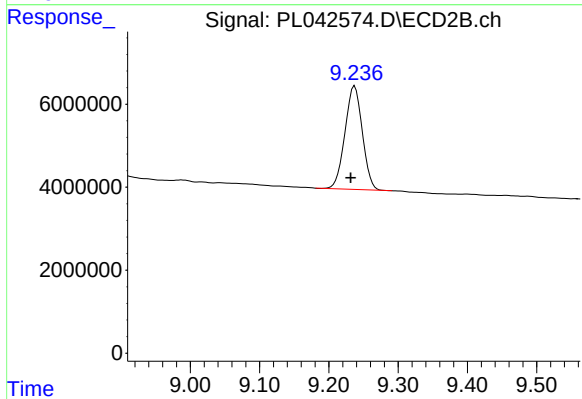

#28 Decachlorobiphenyl

R.T.: 9.237 min
Delta R.T.: 0.006 min
Response: 43406816
Conc: 18.00 ng/ml