

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 16:04
 Operator : AJ\SJ
 Sample : J5768-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 23:53:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.101	58404333	31415656	9.927	10.923
28)	SA Decachlor...	8.205	9.233	60926676	22474078	9.668	9.318
Target Compounds							
6)	B beta-BHC	4.401f	4.904f	6384294	2810813	1.802	1.782
9)	A Endosulfan I	5.458f	0.000	780532	0	0.113	N.D. #
11)	B alpha-Chl...	5.458	0.000	780532	0	0.104	N.D. #
23)	Chlordane-1	4.401	0.000	6384294	0	23.092	N.D. #
26)	Chlordane-4	5.458	0.000	780532	0	1.028	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 16:04
Operator : AJ\SJ
Sample : J5768-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 23:53:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

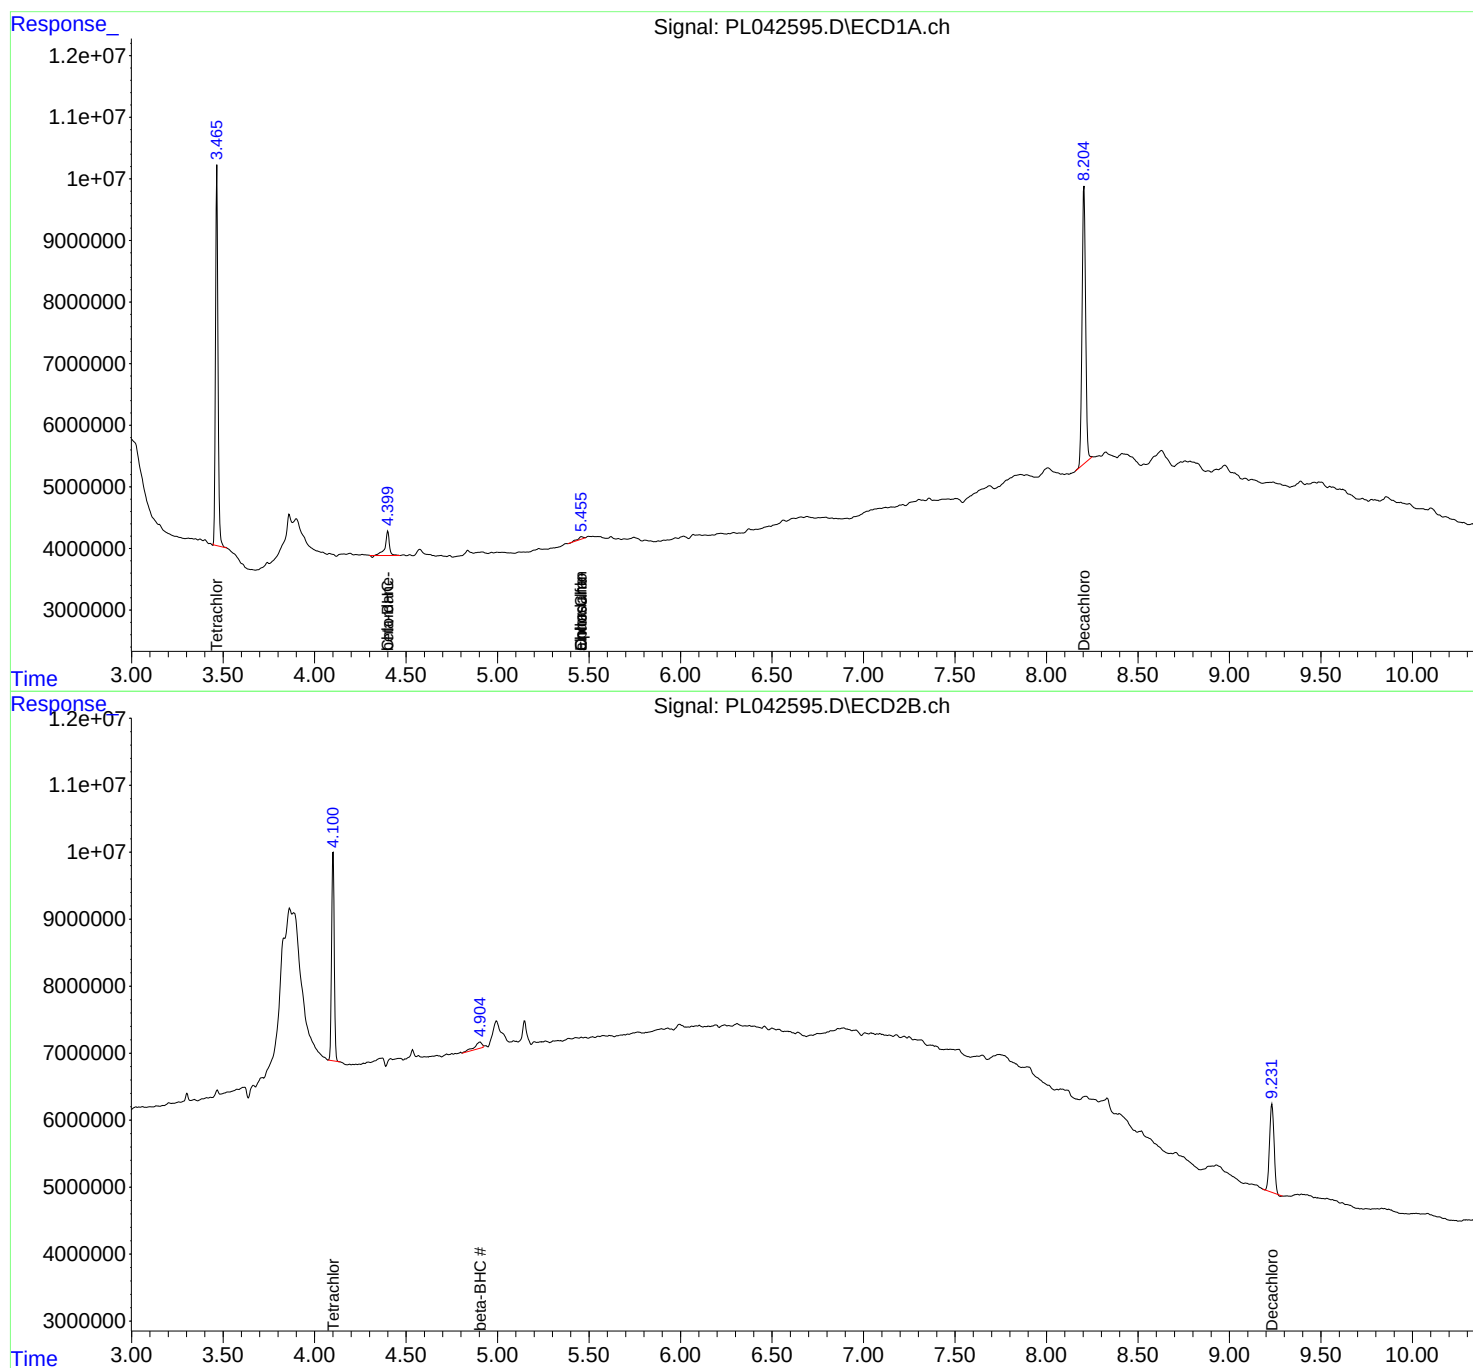


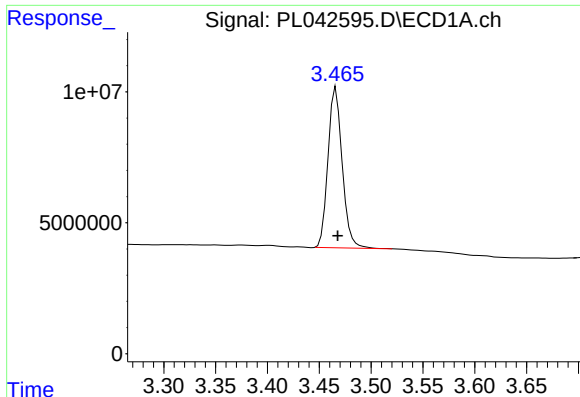

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 58404333
Conc: 9.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

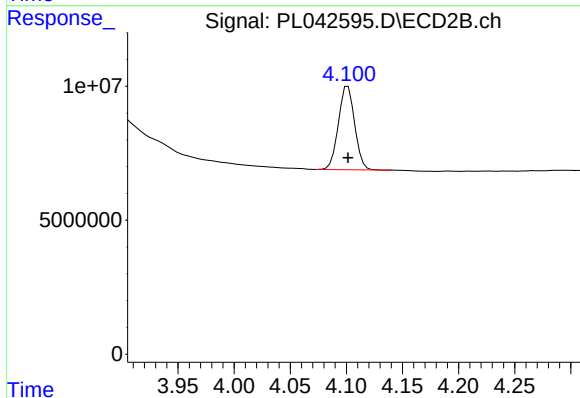


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 31415656
Conc: 10.92 ng/ml

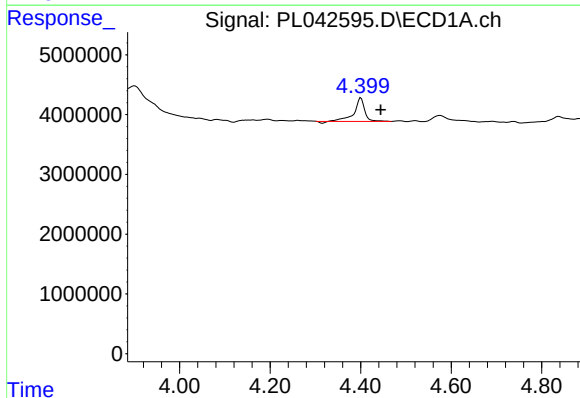


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.044 min
Response: 6384294
Conc: 1.80 ng/ml

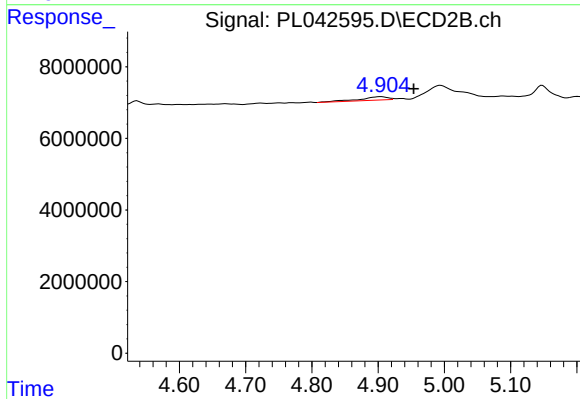

#6 beta-BHC


R.T.: 4.904 min
Delta R.T.: -0.049 min
Response: 2810813
Conc: 1.78 ng/ml

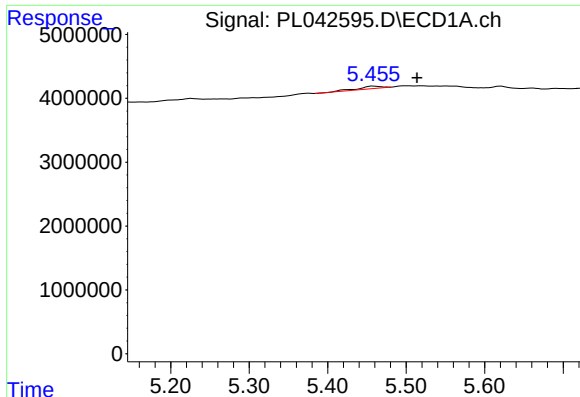

#9 Endosulfan I


R.T.: 5.458 min
Delta R.T.: -0.056 min
Response: 780532
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

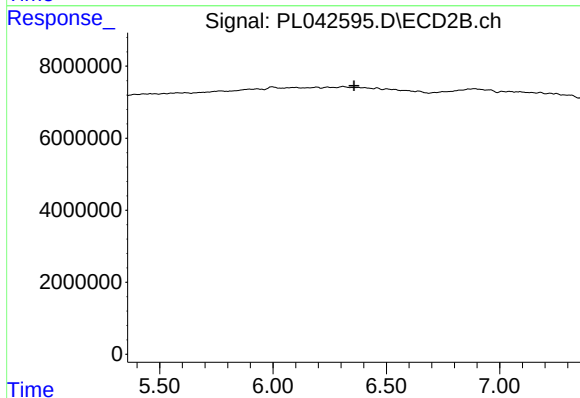


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

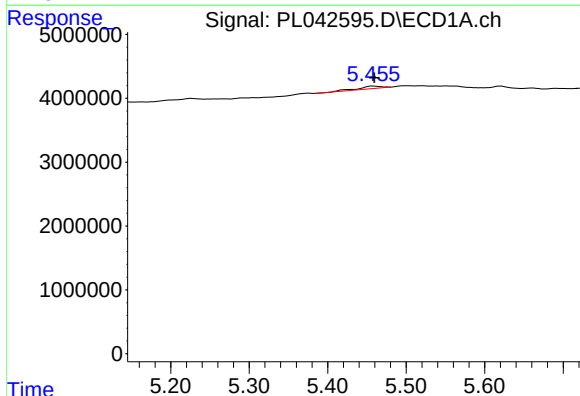


#11 alpha-Chlordane

R.T.: 5.458 min
Delta R.T.: -0.002 min
Response: 780532
Conc: 0.10 ng/ml

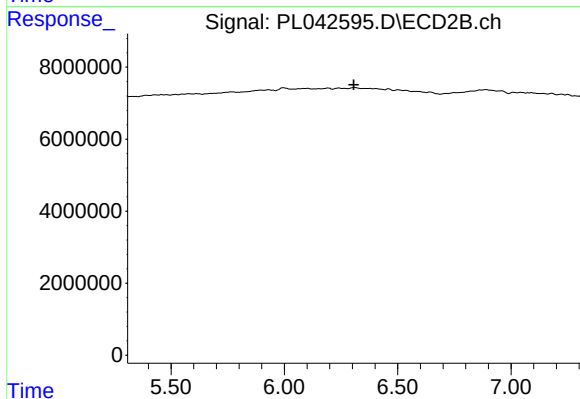

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.307 min
Response: 0
Conc: N.D.

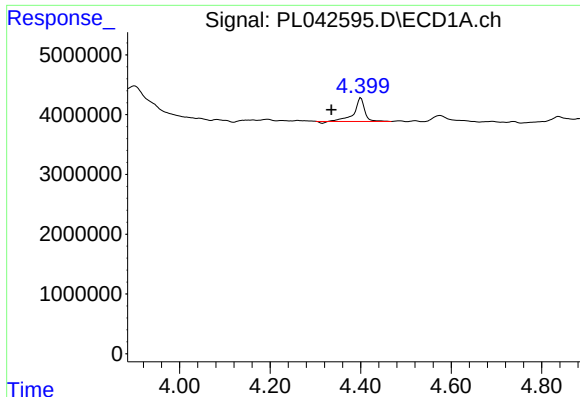

#23 Chlordane-1


R.T.: 4.401 min
Delta R.T.: 0.065 min
Response: 6384294
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

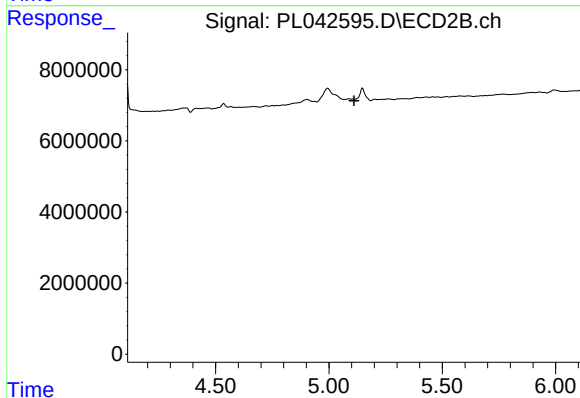


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

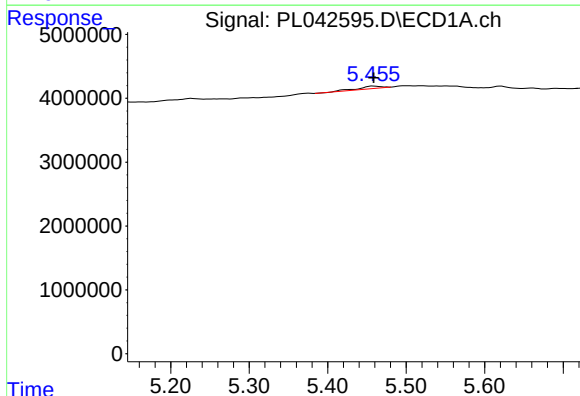


#26 Chlordane-4

R.T.: 5.458 min
Delta R.T.: 0.000 min
Response: 780532
Conc: 1.03 ng/ml

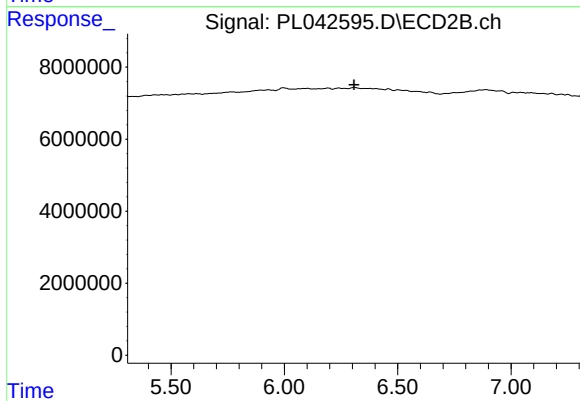

#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.308 min
Response: 0
Conc: N.D.

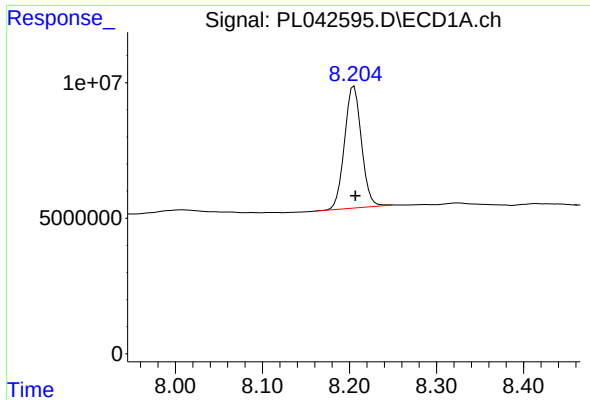

#28 Decachlorobiphenyl


R.T.: 8.205 min

Delta R.T.: -0.002 min

Response: 60926676

Conc: 9.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

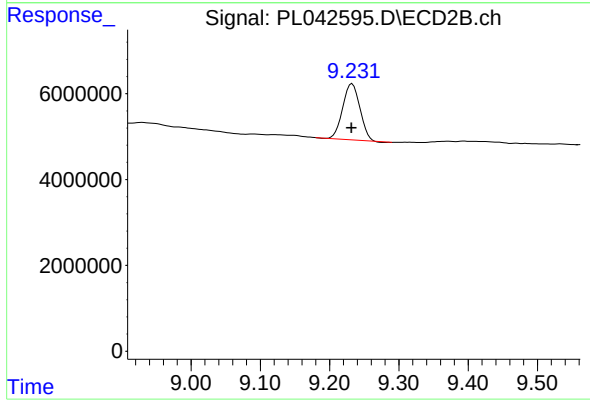

#28 Decachlorobiphenyl

R.T.: 9.233 min

Delta R.T.: 0.001 min

Response: 22474078

Conc: 9.32 ng/ml