

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 17:15
 Operator : AJ\SJ
 Sample : PB115162BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 23:55:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.466	4.101	97203969	51827328	16.522	18.020
28) SA Decachlor...	8.205	9.233	94657779	36759066	15.020	15.241
Target Compounds						
6) B beta-BHC	4.400f	0.000	4337922	0	1.224	N.D. #
23) Chlordane-1	4.400	0.000	4337922	0	15.690	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 17:15
Operator : AJ\SJ
Sample : PB115162BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 23:55:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

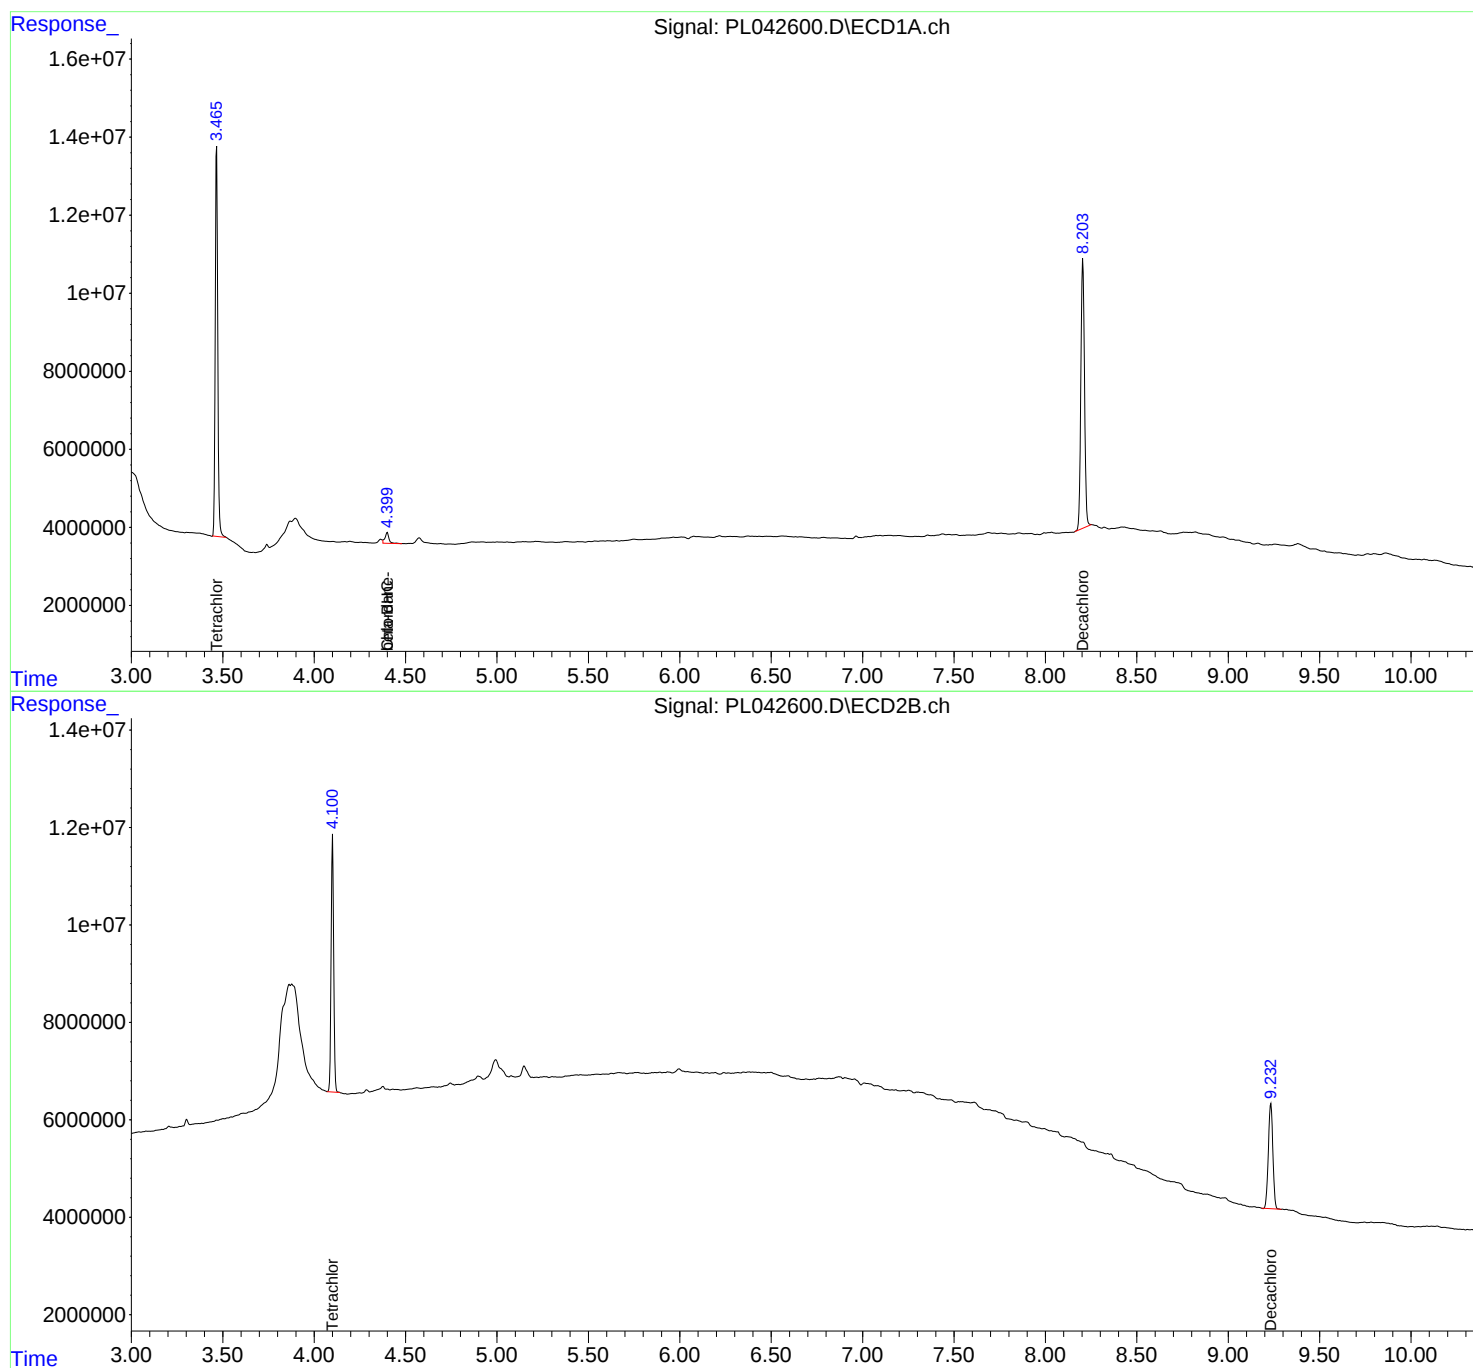


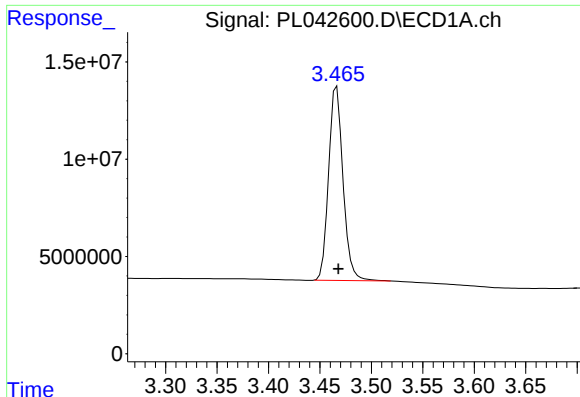

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 97203969
Conc: 16.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

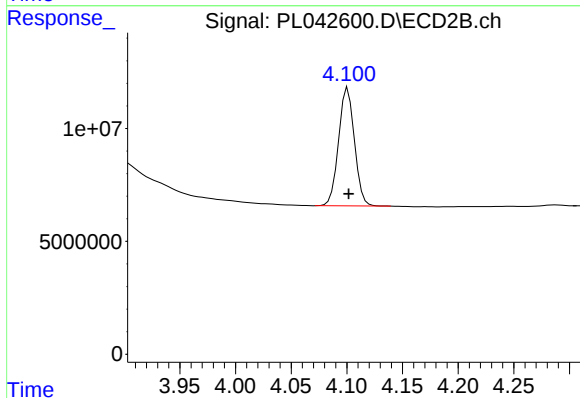


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 51827328
Conc: 18.02 ng/ml

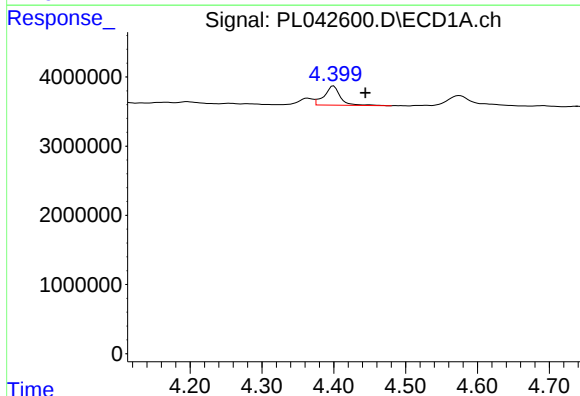


#6 beta-BHC

R.T.: 4.400 min
Delta R.T.: -0.044 min
Response: 4337922
Conc: 1.22 ng/ml

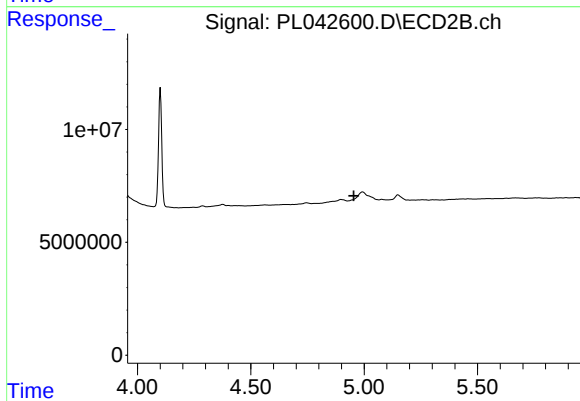

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.954 min
Response: 0
Conc: N.D.

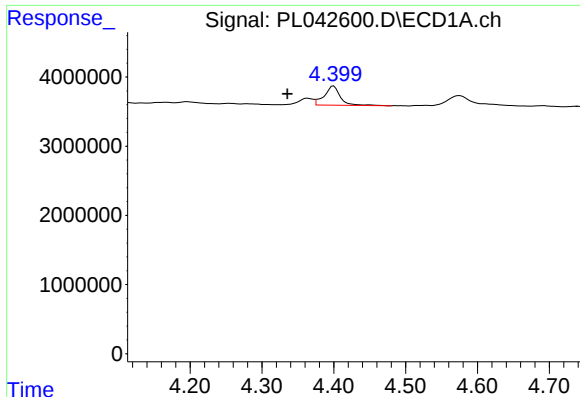

#23 Chlordane-1


R.T.: 4.400 min
Delta R.T.: 0.064 min
Response: 4337922
Conc: 15.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

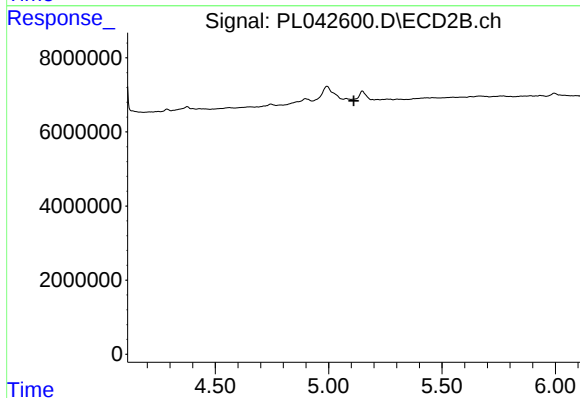


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

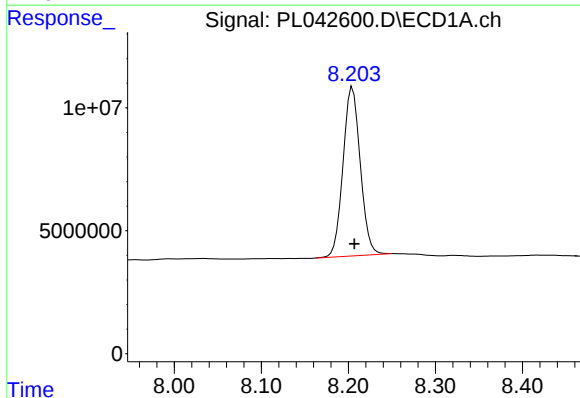

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 94657779
Conc: 15.02 ng/ml

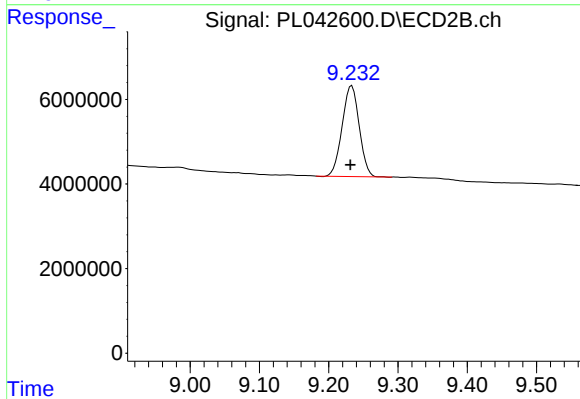

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 36759066
Conc: 15.24 ng/ml