

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 20:32
 Operator : AJ\SJ
 Sample : J5768-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 00:01:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.101	107.2E6	56934131	18.223	19.795
28)	SA Decachlor...	8.204	9.233	102.6E6	41060085	16.277	17.024
Target Compounds							
3)	MA gamma-BHC...	4.197	4.766	9273358	1194376	1.125	0.302 #
6)	B beta-BHC	4.401f	4.910f	13374902	989633	3.775	0.627 #
8)	B Heptachlo...	5.242f	0.000	5071009	0	0.669	N.D. #
9)	A Endosulfan I	5.541	0.000	3260620	0	0.471	N.D. #
10)	B gamma-Chl...	0.000	6.164f	0	2049863	N.D.	0.602 #
13)	MA Dieldrin	5.739	0.000	3250804	0	0.442	N.D. #
15)	B Endosulfa...	6.297	0.000	2631646	0	0.421	N.D. #
23)	Chlordane-1	4.368	0.000	5747515	0	20.789	N.D. #
25)	Chlordane-3	0.000	6.164	0	2049863	N.D.	4.362 #
27)	Chlordane-5	6.297	0.000	2631646	0	8.832	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 20:32
Operator : AJ\SJ
Sample : J5768-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 00:01:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

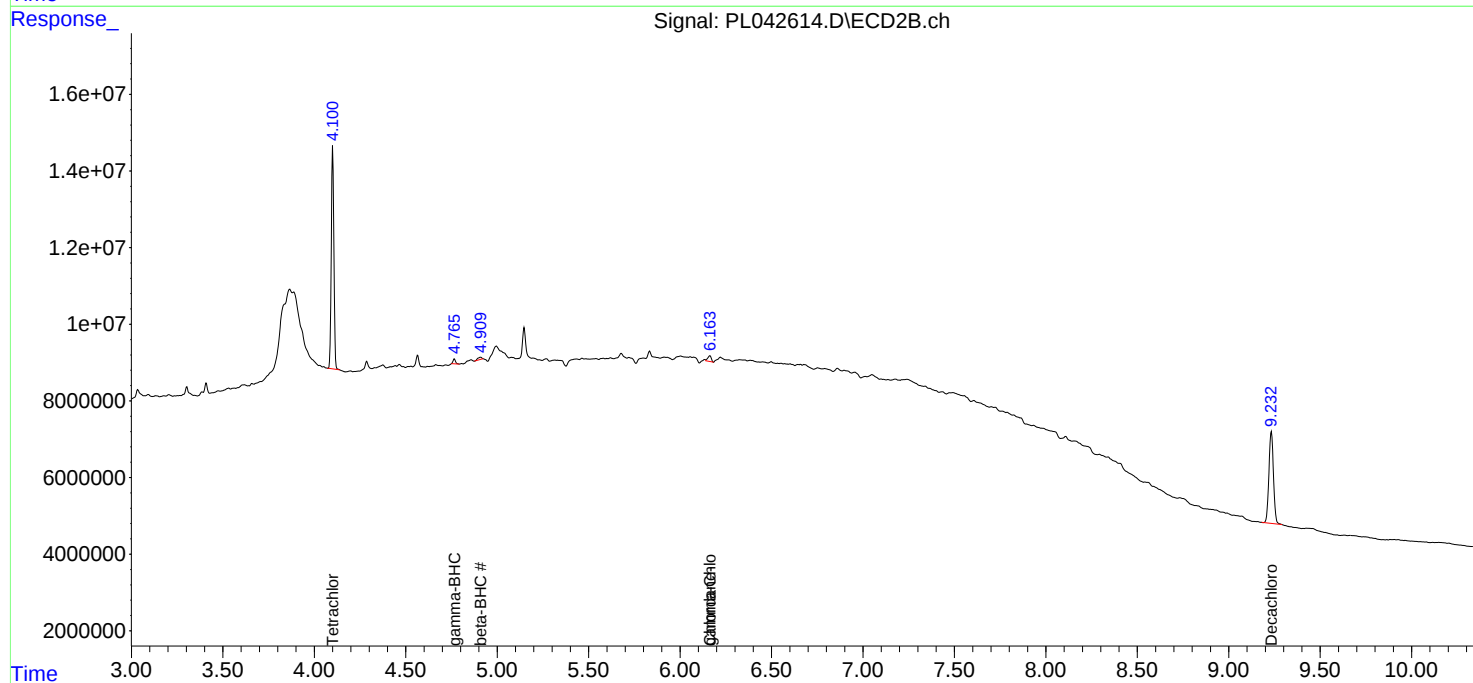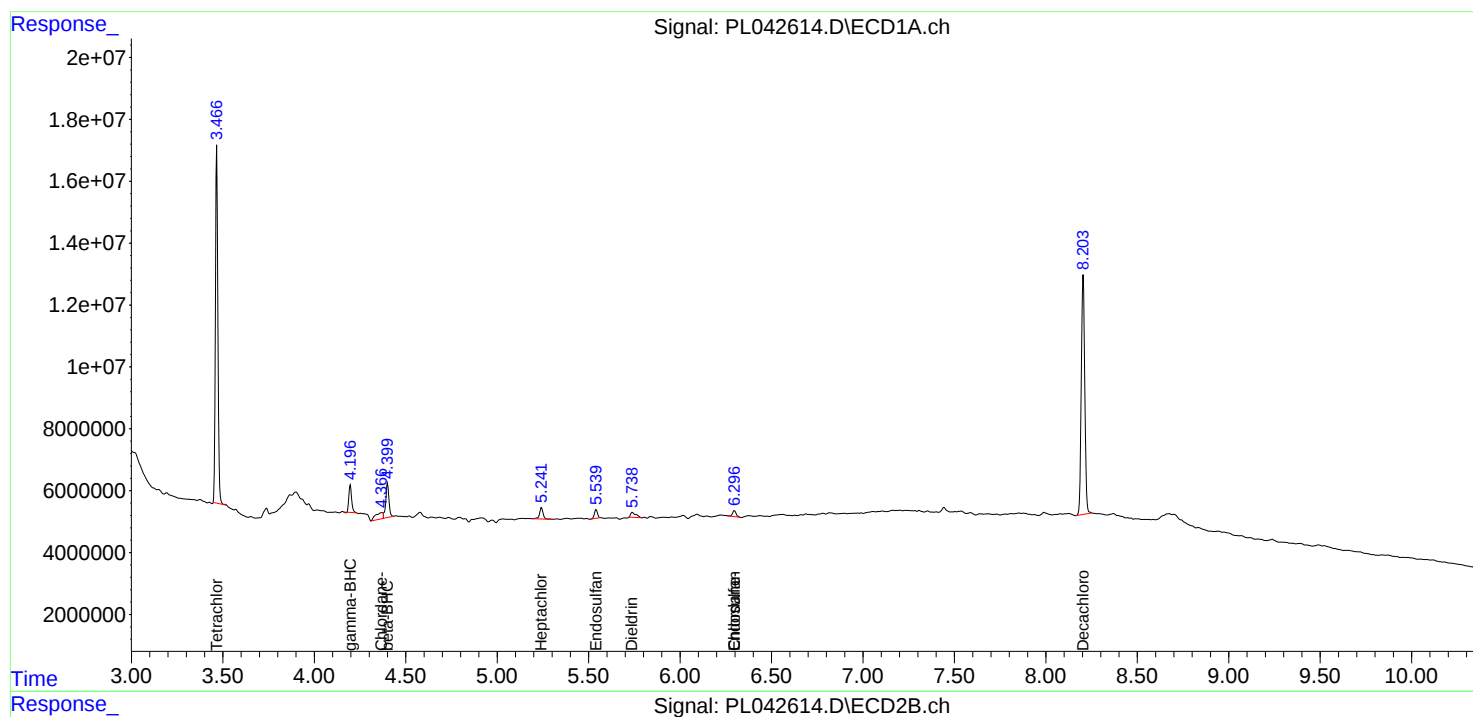


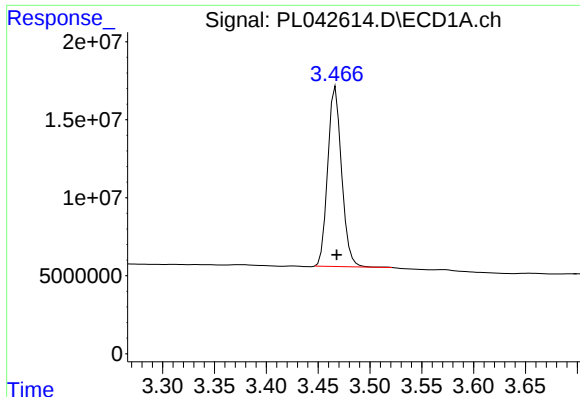

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 107217008
Conc: 18.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

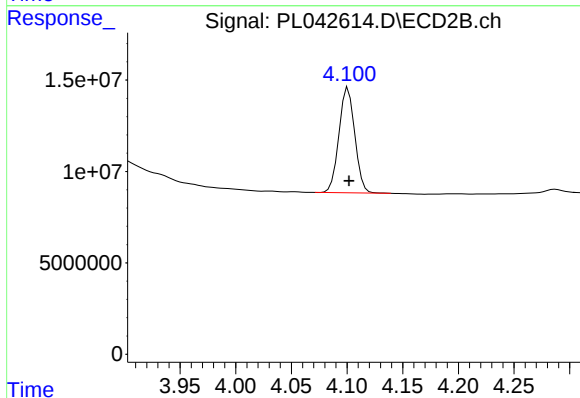


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 56934131
Conc: 19.80 ng/ml

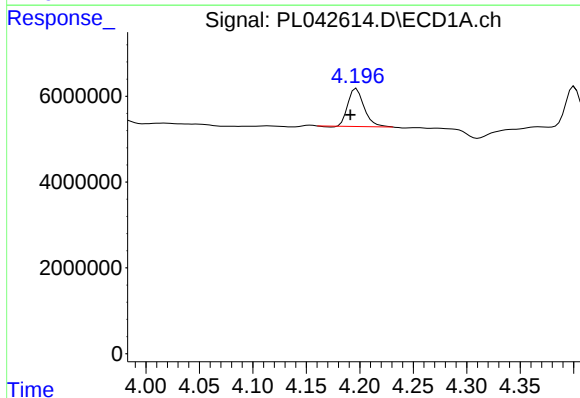


#3 gamma-BHC (Lindane)

R.T.: 4.197 min
Delta R.T.: 0.006 min
Response: 9273358
Conc: 1.13 ng/ml

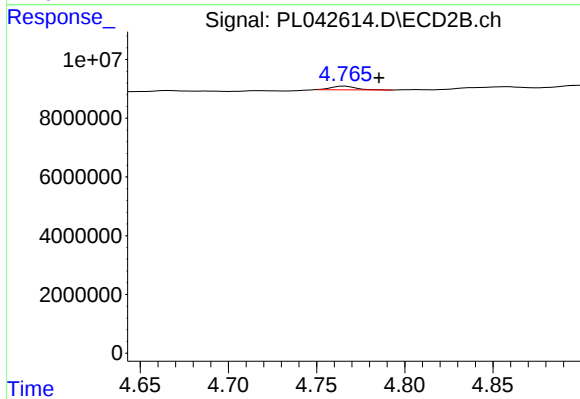

#3 gamma-BHC (Lindane)


R.T.: 4.766 min
Delta R.T.: -0.019 min
Response: 1194376
Conc: 0.30 ng/ml

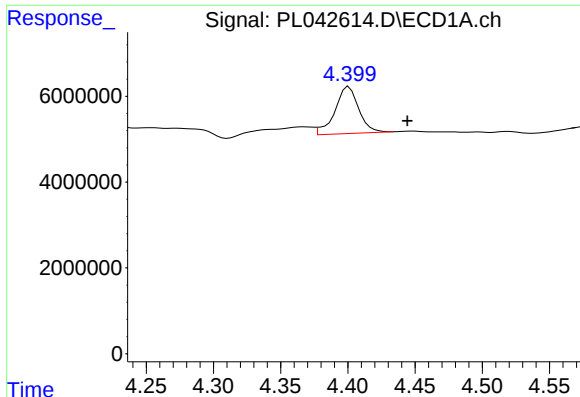

#6 beta-BHC


R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 13374902
Conc: 3.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

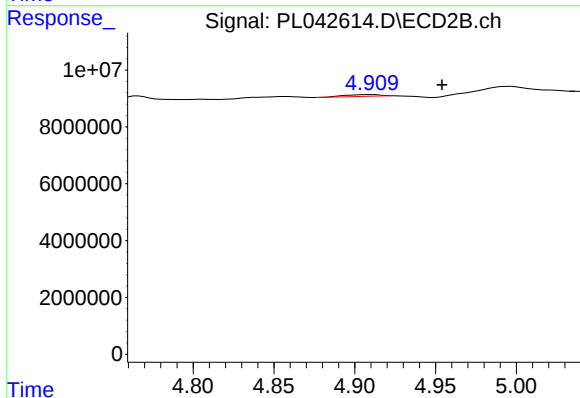


#6 beta-BHC

R.T.: 4.910 min
Delta R.T.: -0.044 min
Response: 989633
Conc: 0.63 ng/ml

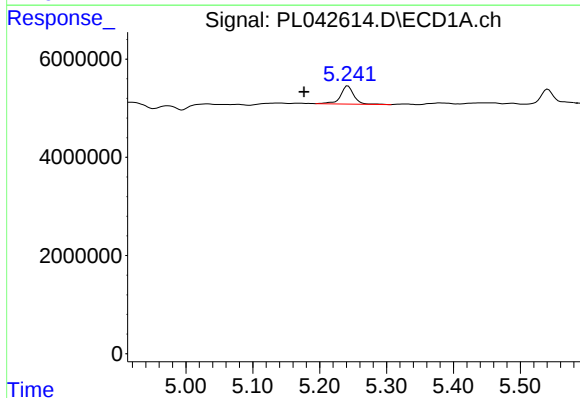


#8 Heptachlor epoxide

R.T.: 5.242 min
Delta R.T.: 0.066 min
Response: 5071009
Conc: 0.67 ng/ml

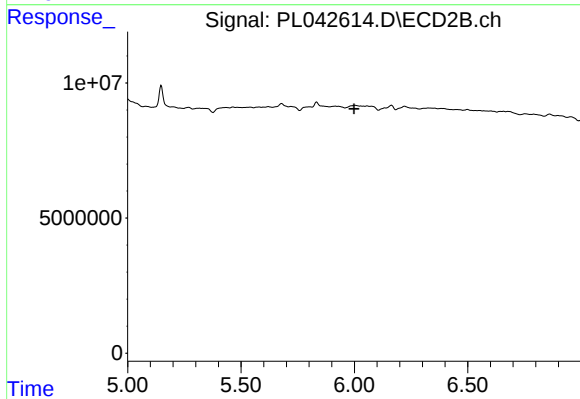

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.998 min
Response: 0
Conc: N.D.

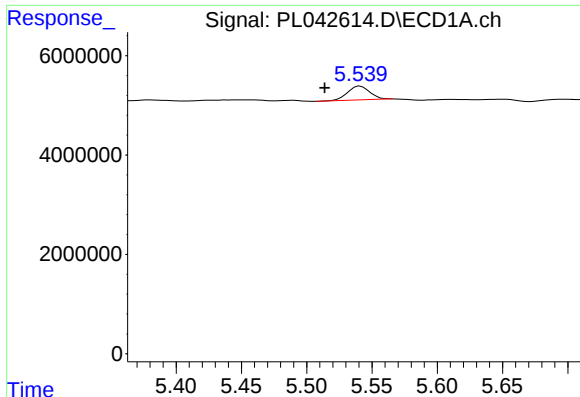

#9 Endosulfan I


R.T.: 5.541 min
Delta R.T.: 0.027 min
Response: 3260620
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

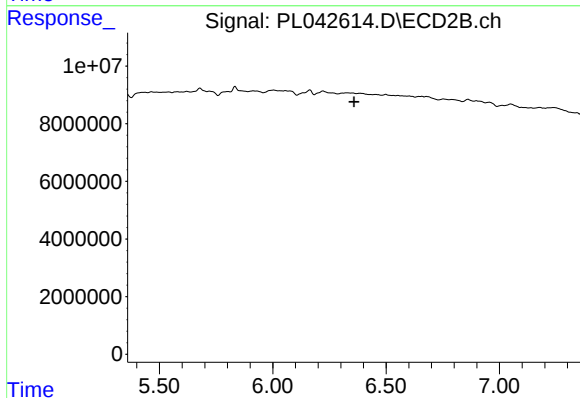


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.358 min
Response: 0
Conc: N.D.

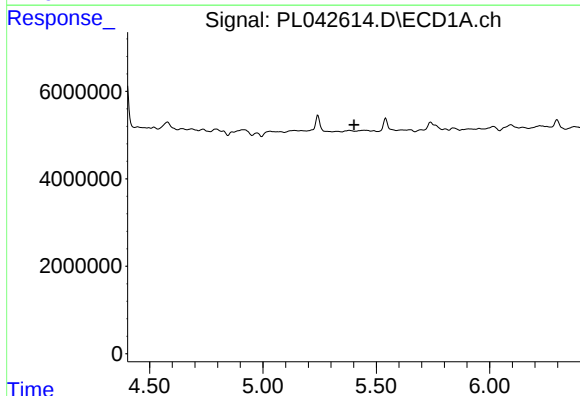


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

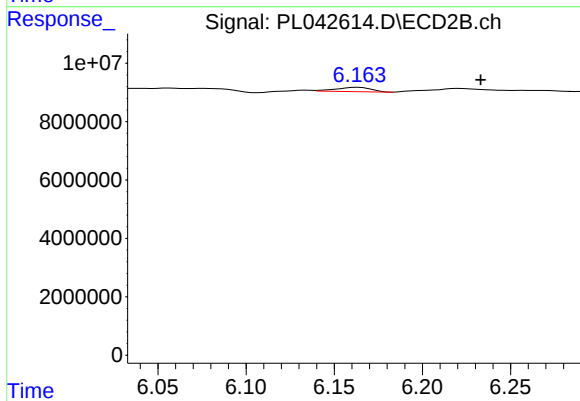

#10 gamma-Chlordane


R.T.: 6.164 min
Delta R.T.: -0.069 min
Response: 2049863
Conc: 0.60 ng/ml

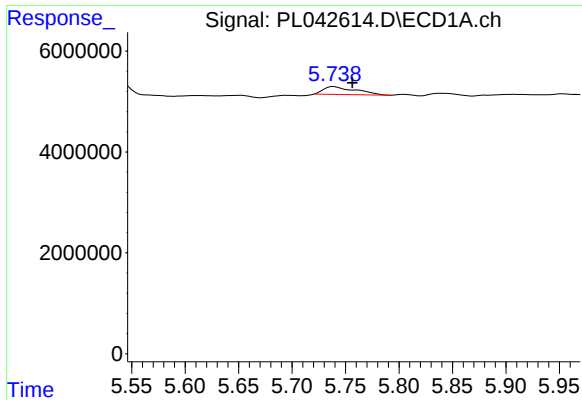

#13 Dieldrin


R.T.: 5.739 min
Delta R.T.: -0.017 min
Response: 3250804
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

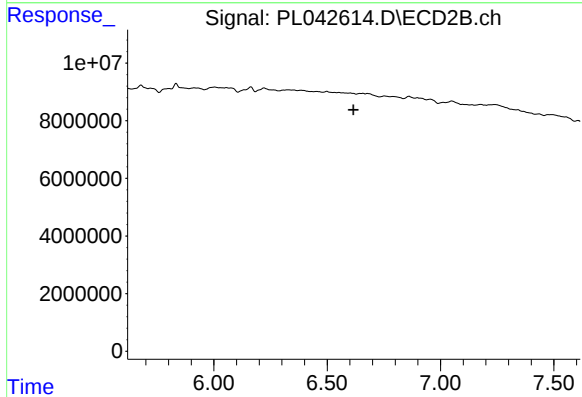


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.617 min
Response: 0
Conc: N.D.

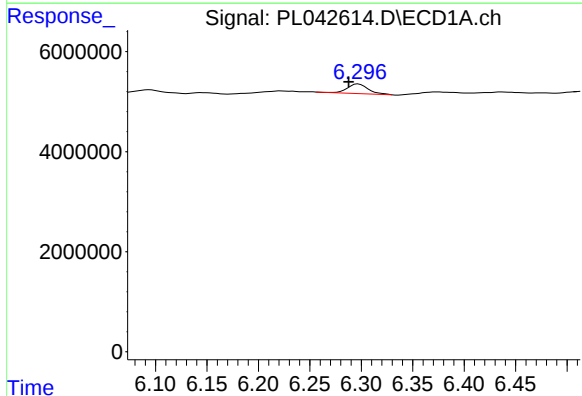


#15 Endosulfan II

R.T.: 6.297 min
Delta R.T.: 0.010 min
Response: 2631646
Conc: 0.42 ng/ml

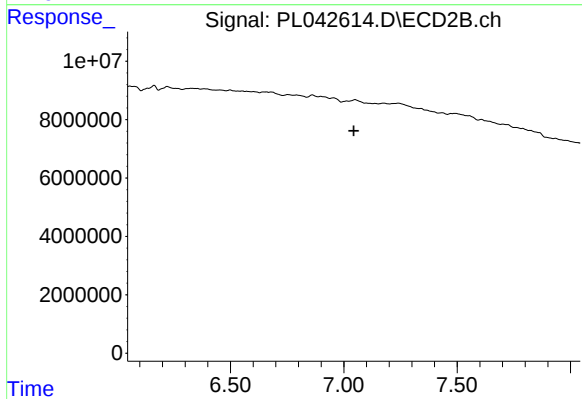

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.044 min
Response: 0
Conc: N.D.

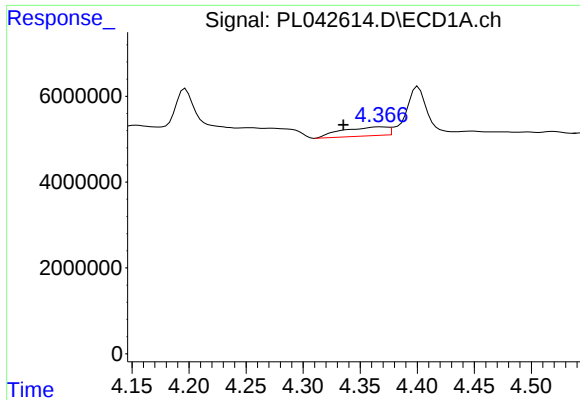

#23 Chlordane-1


R.T.: 4.368 min
Delta R.T.: 0.032 min
Response: 5747515
Conc: 20.79 ng/ml

Instrument :
ECD_L
ClientSampleId :

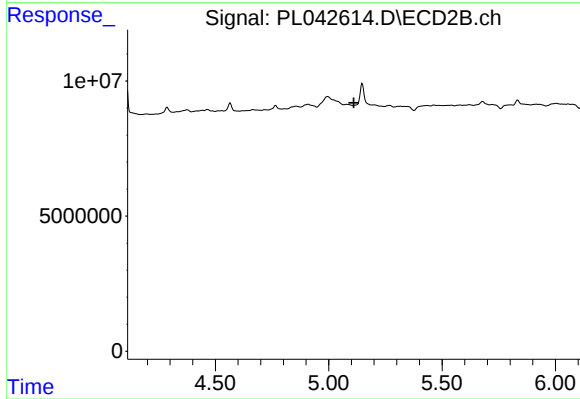


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

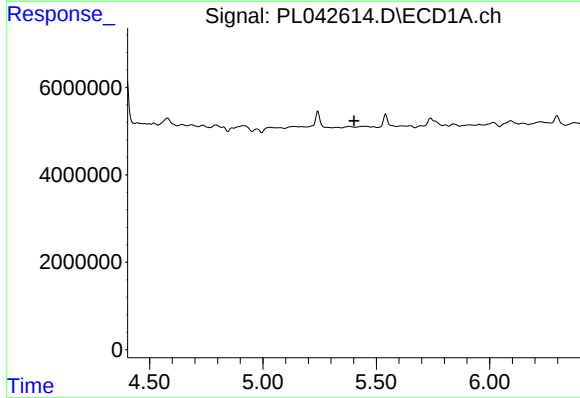


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

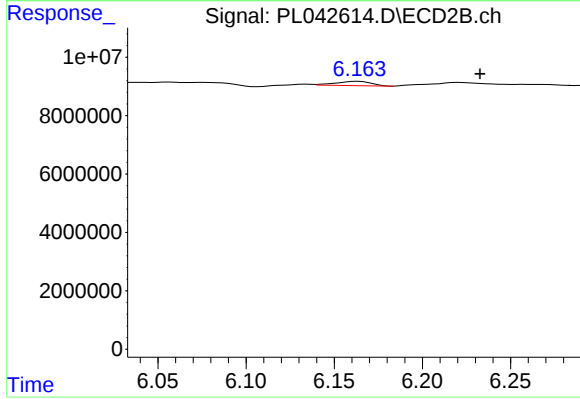

#25 Chlordane-3


R.T.: 6.164 min
Delta R.T.: -0.069 min
Response: 2049863
Conc: 4.36 ng/ml

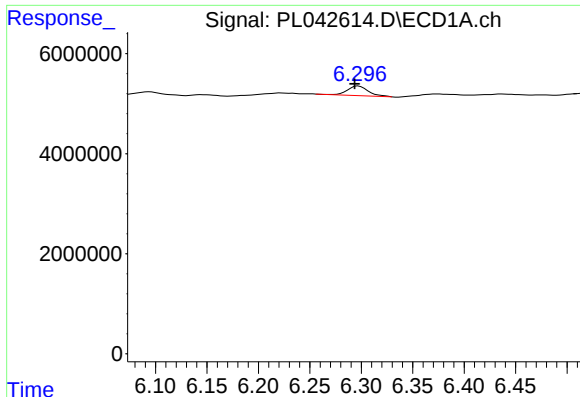

#27 Chlordane-5


R.T.: 6.297 min
Delta R.T.: 0.004 min
Response: 2631646
Conc: 8.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

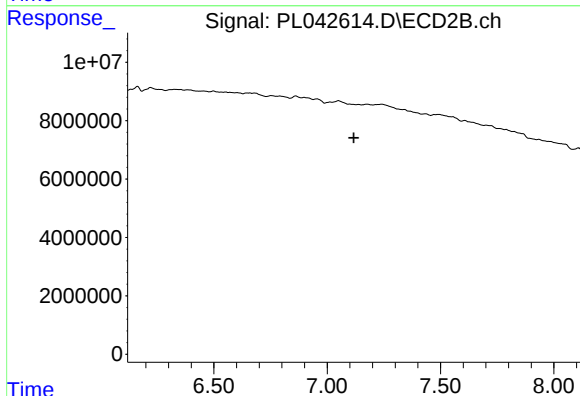


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

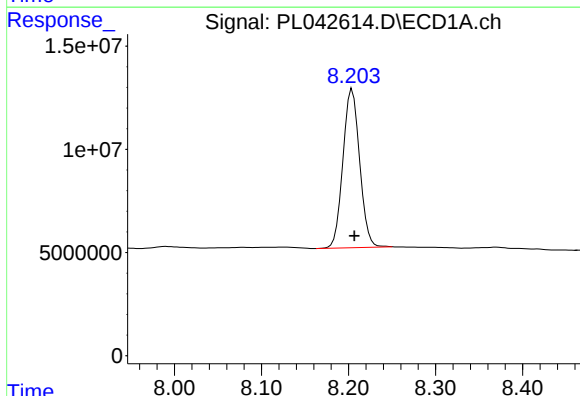

#28 Decachlorobiphenyl

R.T.: 8.204 min
Delta R.T.: -0.003 min
Response: 102577799
Conc: 16.28 ng/ml

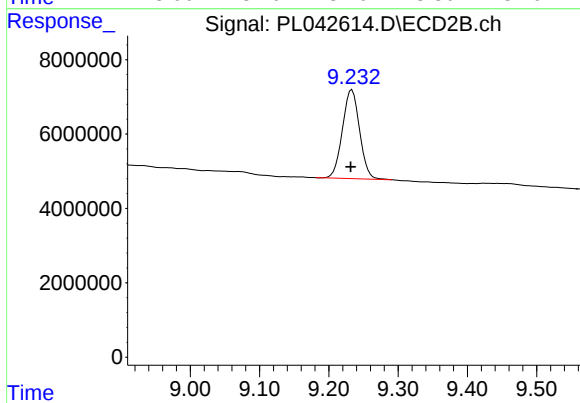

#28 Decachlorobiphenyl

R.T.: 9.233 min
Delta R.T.: 0.002 min
Response: 41060085
Conc: 17.02 ng/ml