

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
 Data File : PL042615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Nov 2018 20:46
 Operator : AJ\SJ
 Sample : J5767-24
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 30 00:01:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	116.2E6	61468583	19.755	21.372
28)	SA Decachlor...	8.205	9.234	111.7E6	44656823	17.729	18.516
Target Compounds							
2)	A alpha-BHC	3.905	0.000	4265929	0	0.473	N.D. #
3)	MA gamma-BHC...	4.196	0.000	5667055	0	0.688	N.D. #
6)	B beta-BHC	4.401f	4.905f	9260278	983298	2.614	0.623 #
8)	B Heptachlo...	0.000	5.997	0	3858287	N.D.	1.076 #
13)	MA Dieldrin	5.740	0.000	2363120	0	0.321	N.D. #
15)	B Endosulfa...	6.297	7.050	5926264	2120218	0.948	0.768
19)	B Endosulfa...	6.675	0.000	2172055	0	0.348	N.D. #
23)	Chlordane-1	4.367	0.000	3284364	0	11.880	N.D. #
27)	Chlordane-5	6.297	7.050	5926264	2120218	19.889	22.041


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL112918\
Data File : PL042615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Nov 2018 20:46
Operator : AJ\SJ
Sample : J5767-24
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 30 00:01:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

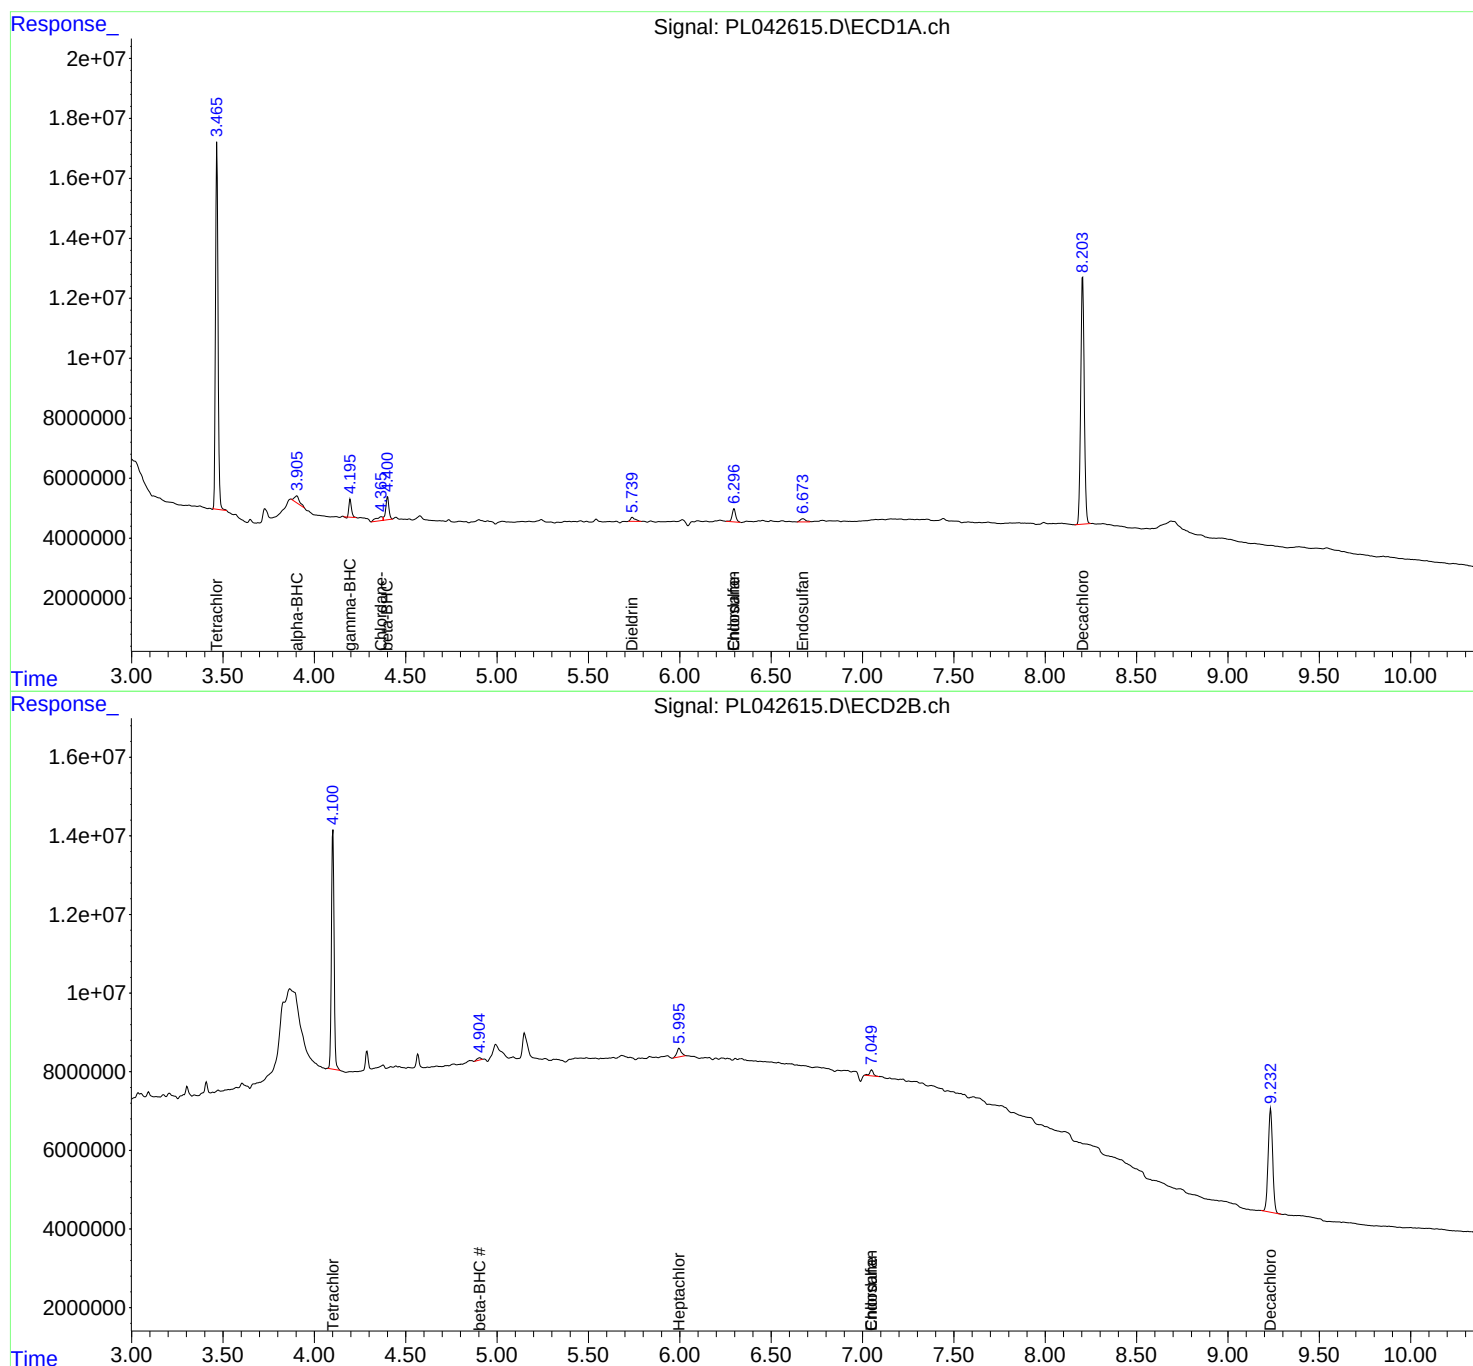


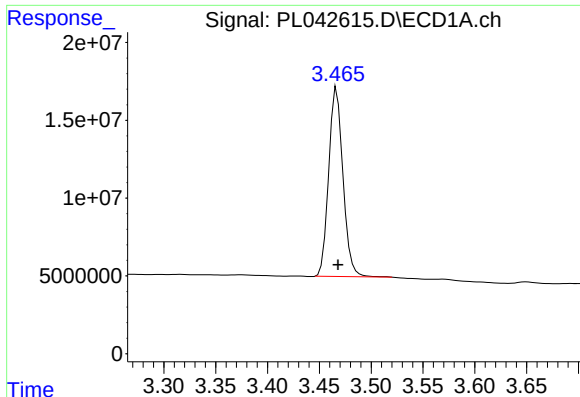

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: -0.001 min
Response: 116228902
Conc: 19.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

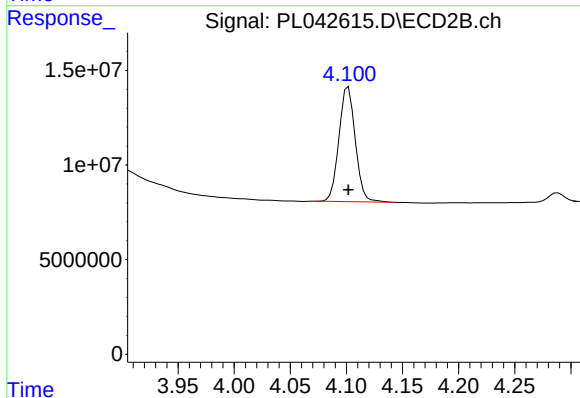


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 61468583
Conc: 21.37 ng/ml

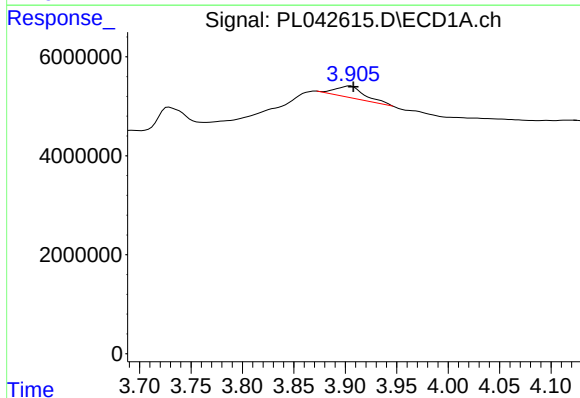


#2 alpha-BHC

R.T.: 3.905 min
Delta R.T.: -0.003 min
Response: 4265929
Conc: 0.47 ng/ml

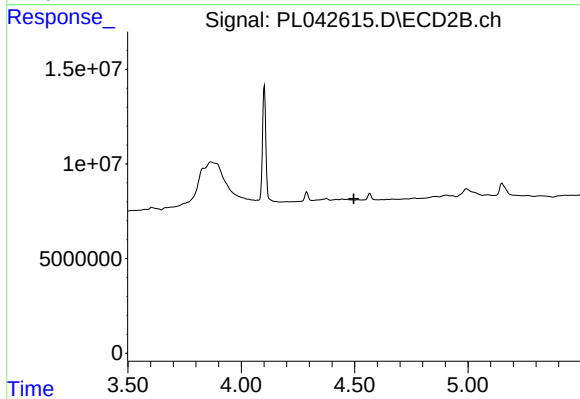

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.497 min
Response: 0
Conc: N.D.

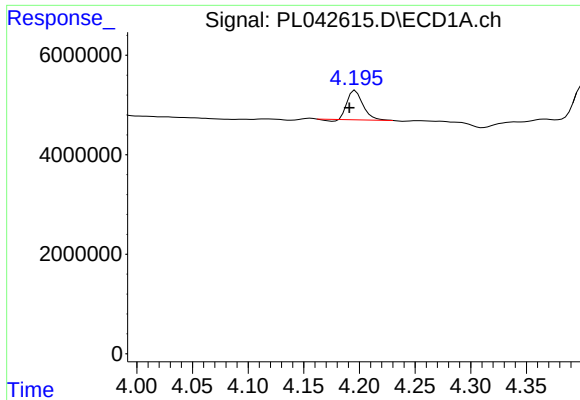

#3 gamma-BHC (Lindane)


R.T.: 4.196 min
Delta R.T.: 0.005 min
Response: 5667055
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

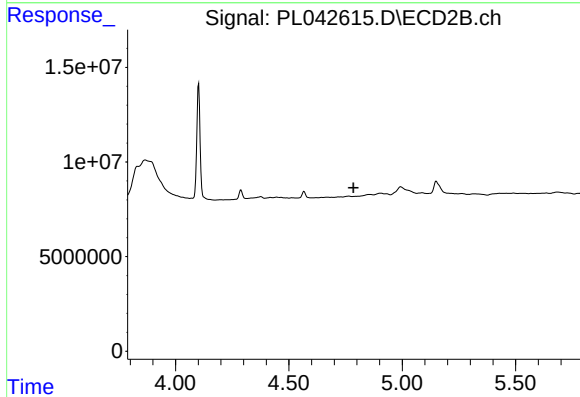


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

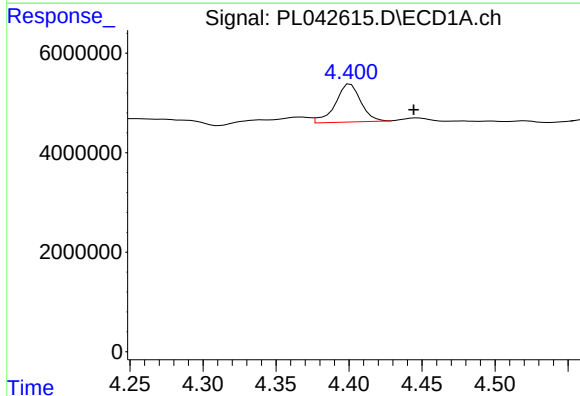


#6 beta-BHC

R.T.: 4.401 min
Delta R.T.: -0.043 min
Response: 9260278
Conc: 2.61 ng/ml

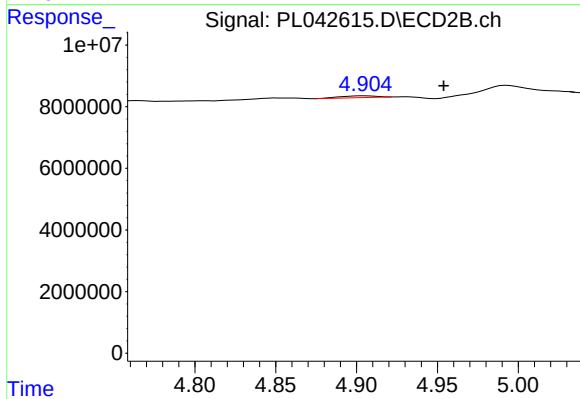

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.049 min
Response: 983298
Conc: 0.62 ng/ml

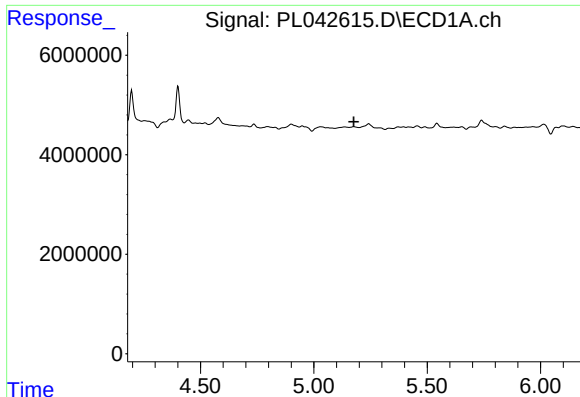

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

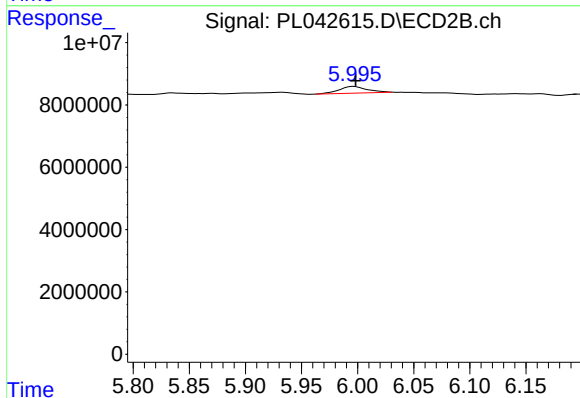


#8 Heptachlor epoxide

R.T.: 5.997 min
Delta R.T.: -0.002 min
Response: 3858287
Conc: 1.08 ng/ml

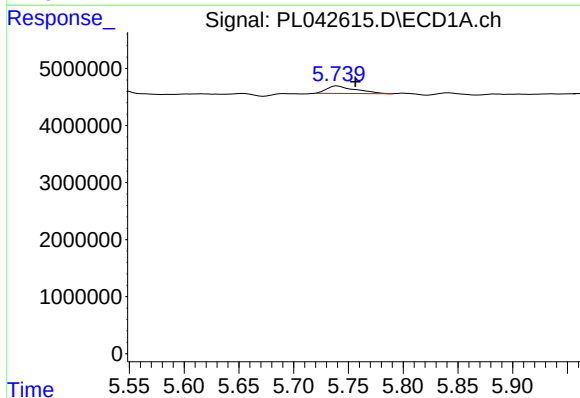


#13 Dieldrin

R.T.: 5.740 min
Delta R.T.: -0.016 min
Response: 2363120
Conc: 0.32 ng/ml

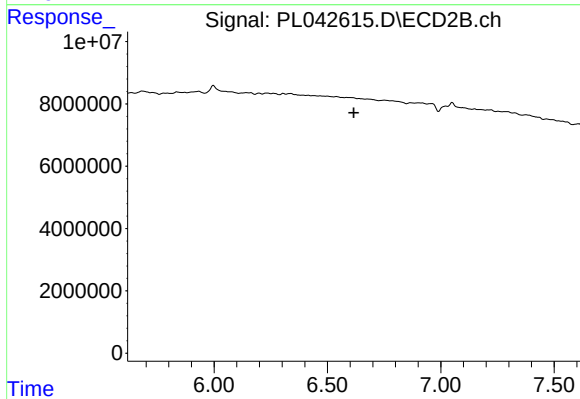

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

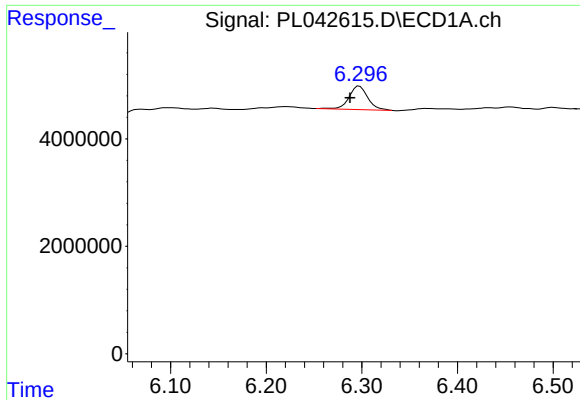

#15 Endosulfan II


R.T.: 6.297 min
Delta R.T.: 0.010 min
Response: 5926264
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

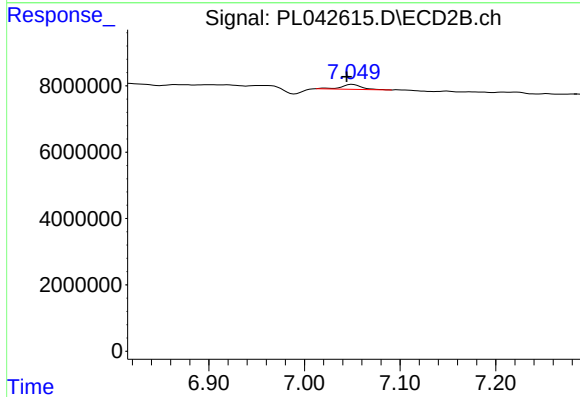


#15 Endosulfan II

R.T.: 7.050 min
Delta R.T.: 0.006 min
Response: 2120218
Conc: 0.77 ng/ml

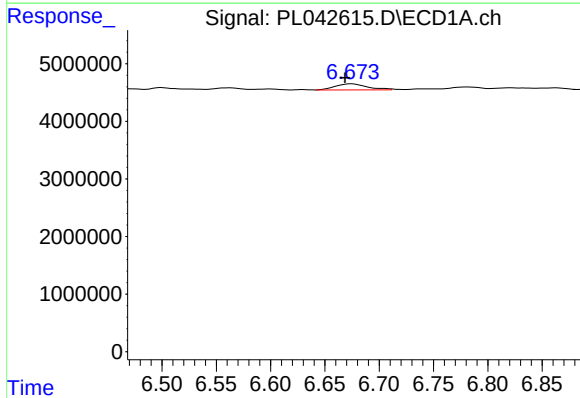


#19 Endosulfan Sulfate

R.T.: 6.675 min
Delta R.T.: 0.006 min
Response: 2172055
Conc: 0.35 ng/ml

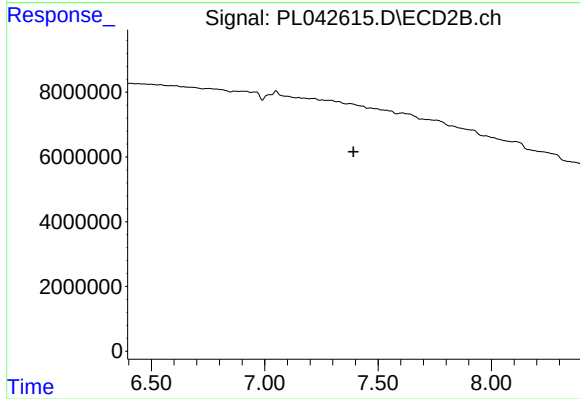

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

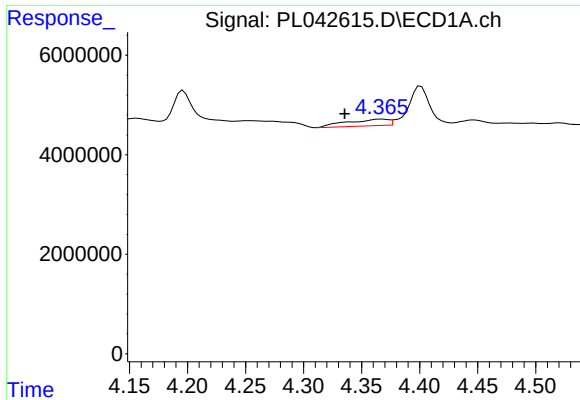

#23 Chlordane-1


R.T.: 4.367 min
Delta R.T.: 0.031 min
Response: 3284364
Conc: 11.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

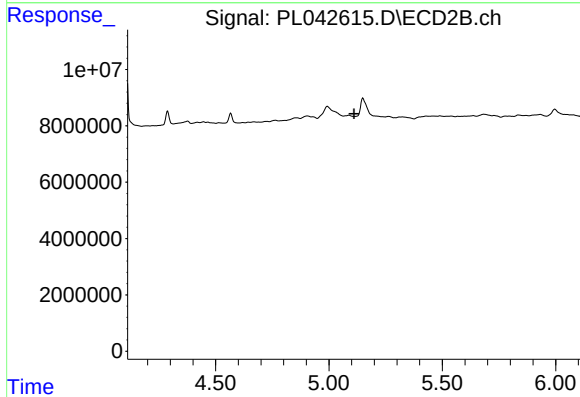


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

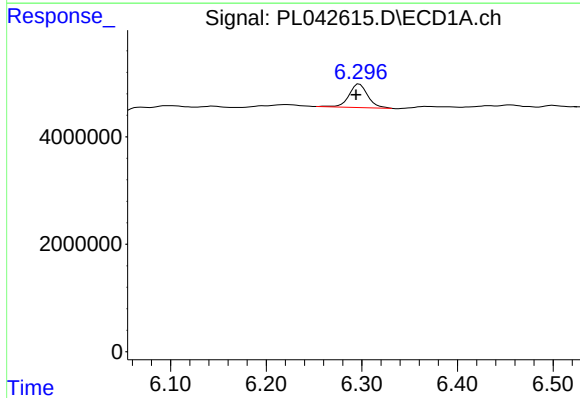


#27 Chlordane-5

R.T.: 6.297 min
Delta R.T.: 0.004 min
Response: 5926264
Conc: 19.89 ng/ml

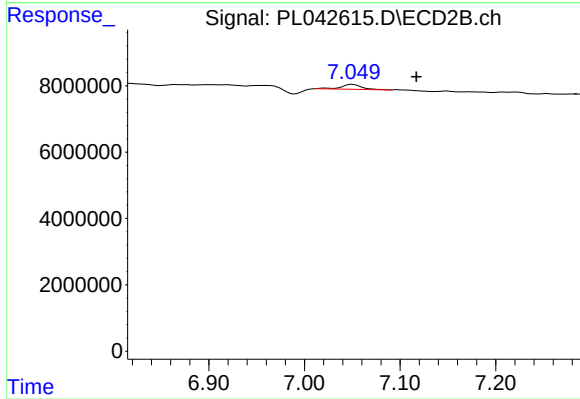

#27 Chlordane-5


R.T.: 7.050 min
Delta R.T.: -0.067 min
Response: 2120218
Conc: 22.04 ng/ml

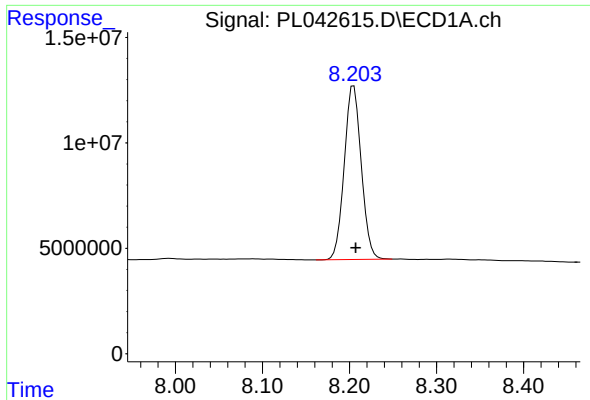

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 111732172
Conc: 17.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

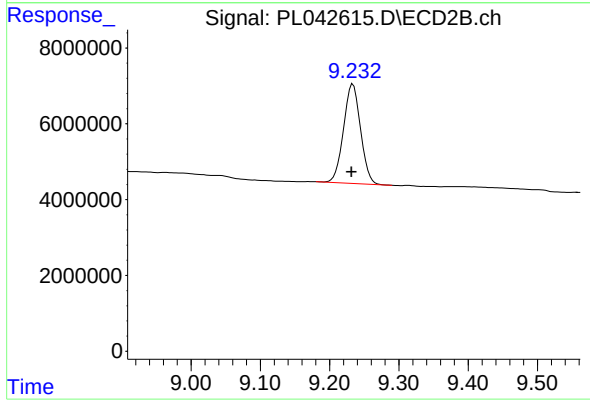

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 44656823
Conc: 18.52 ng/ml